

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020229.D
 Acq On : 07 May 2024 12:03
 Operator : MA/JU
 Sample : P2368-23
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y4

Quant Time: May 07 23:05:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 06 12:26:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	95760	20.000	ng/u1	0.02
20) Naphthalene-d8	10.393	136	404775	20.000	ng/u1	0.02
38) Acenaphthene-d10	14.287	164	275927	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.128	188	612789	20.000	ng/u1	-0.01
79) Chrysene-d12	21.639	240	575135	20.000	ng/u1	0.00
88) Perylene-d12	24.992	264	543610	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	8631	3.807	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.805	99	222933	27.108	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	6.975	67	133099	26.643	ng/u1	0.02
11) 2-Chlorophenol-d4	7.158	132	167867	28.554	ng/u1	0.02
15) 4-Methylphenol-d8	8.334	113	183366	27.579	ng/u1	0.02
21) Nitrobenzene-d5	8.781	128	89577	29.553	ng/u1	0.02
24) 2-Nitrophenol-d4	9.493	143	105977	30.532	ng/u1	0.02
28) 2,4-Dichlorophenol-d3	10.022	165	235444	37.171	ng/u1	0.01
31) 4-Chloroaniline-d4	10.552	131	158170	17.842	ng/u1	0.02
46) Dimethylphthalate-d6	13.704	166	676635	33.580	ng/u1	0.00
49) Acenaphthylene-d8	13.981	160	743248	33.391	ng/u1	0.00
54) 4-Nitrophenol-d4	14.551	143	116157	37.508	ng/u1	0.00
60) Fluorene-d10	15.310	176	594549	35.376	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.469	200	98992	25.457	ng/u1	0.00
73) Anthracene-d10	17.234	188	960778	36.243	ng/u1	0.00
81) Pyrene-d10	19.639	212	1217194	36.205	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.774	264	983140	37.404	ng/u1	0.01
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.769	266	995402	214.212	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020229.D
Acq On : 07 May 2024 12:03
Operator : MA/JU
Sample : P2368-23
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y4

Quant Time: May 07 23:05:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 06 12:26:12 2024
Response via : Initial Calibration

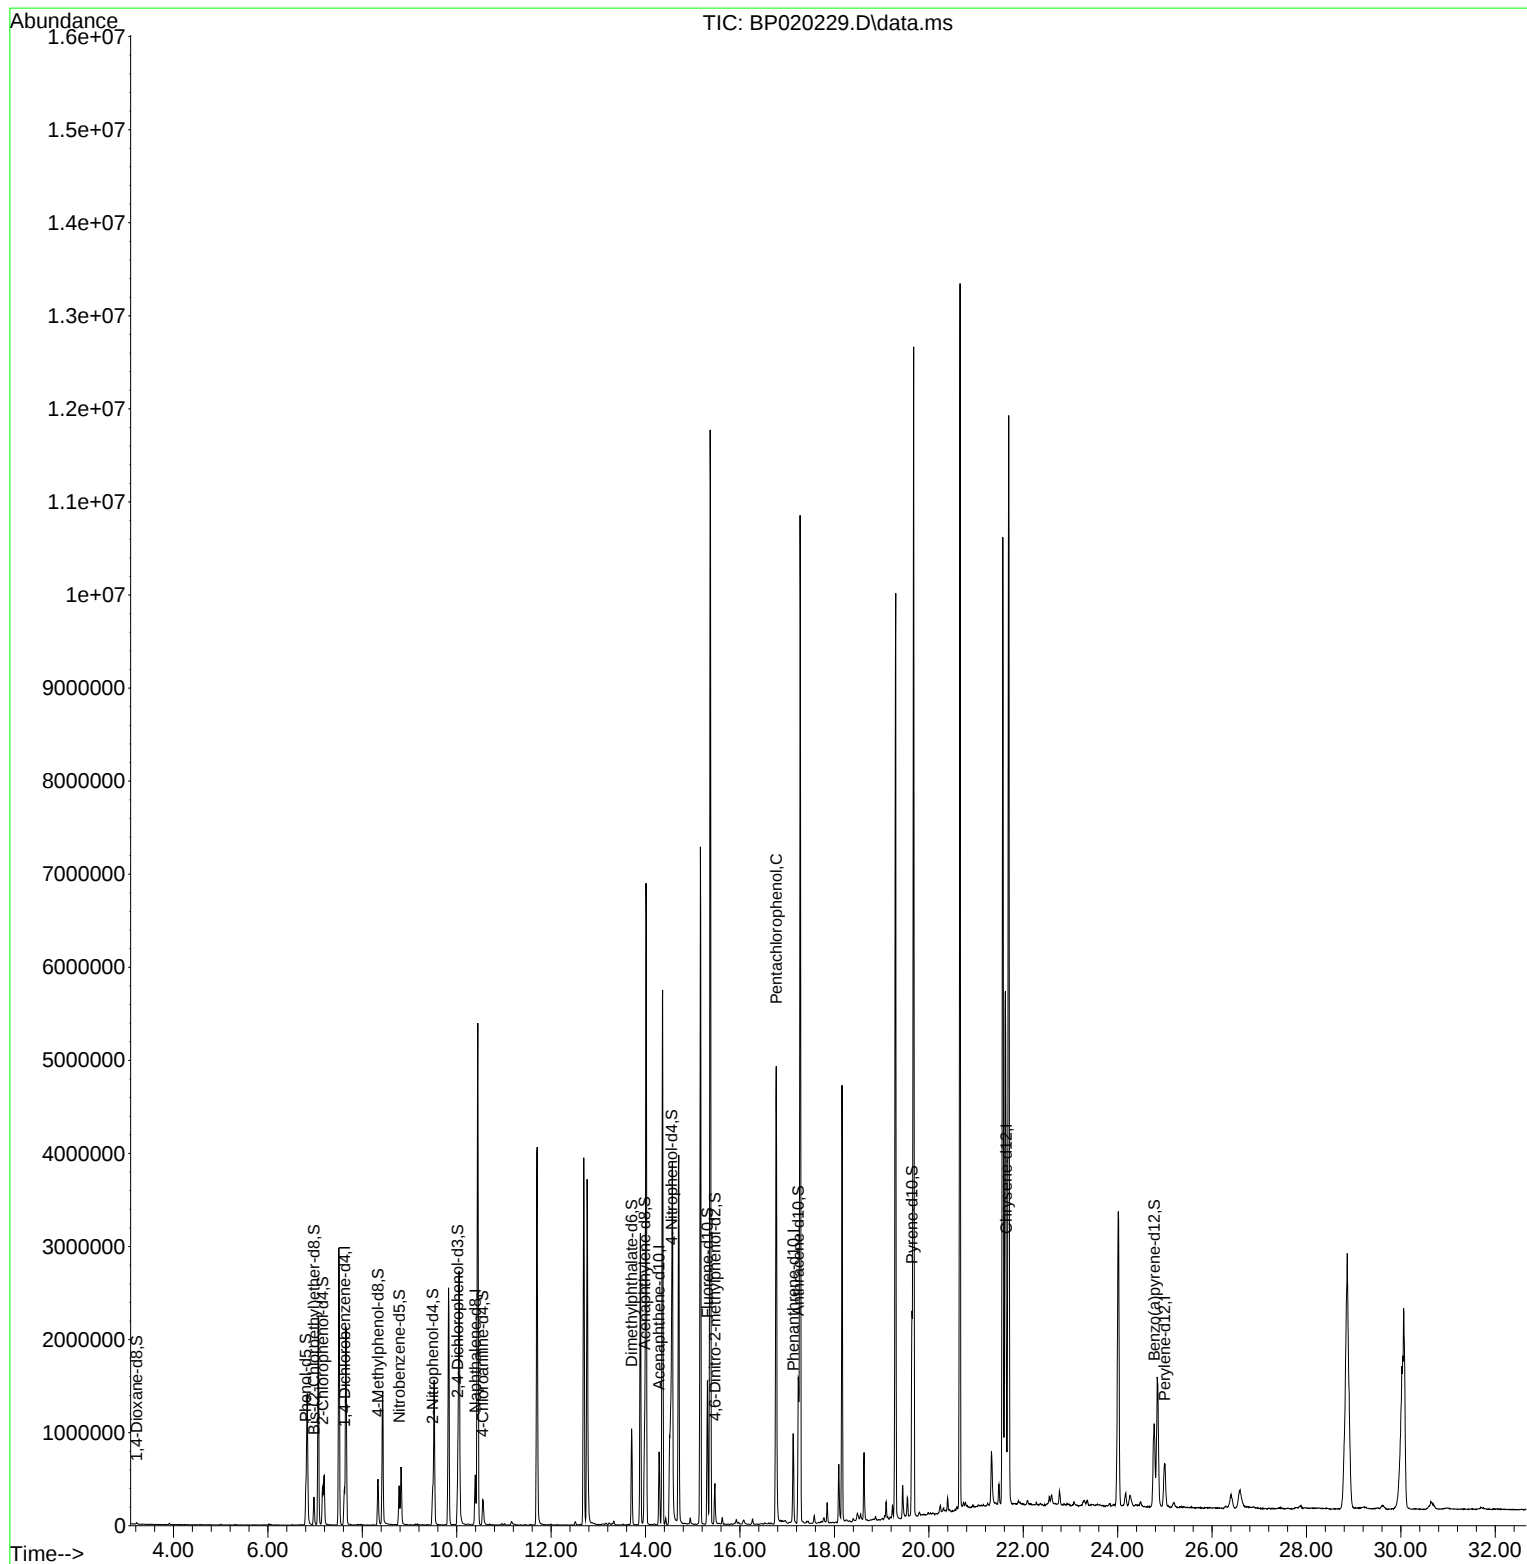

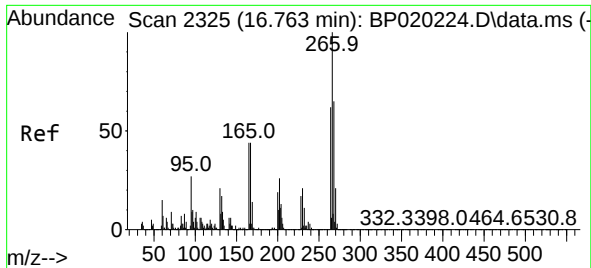

#71
 Pentachlorophenol
 Concen: 214.212 ng/ul
 RT: 16.769 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP020229.D
 Acq: 07 May 2024 12:03

Instrument :
 BNA_P
 ClientSampleId :
 A43Y4

Tgt Ion:266 Resp: 995402
 Ion Ratio Lower Upper
 266 100
 264 62.6 49.8 74.6
 268 63.6 50.4 75.6

