

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020200.D
 Acq On : 06 May 2024 09:59
 Operator : MA/JU
 Sample : PB160579BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK579

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	30	rVB	25967	40102	1.38%	0.130%
2	3.617	87	90	109	rBV	278029	536047	18.51%	1.735%
3	3.911	137	140	146	rVB5	7586	11769	0.41%	0.038%
4	6.805	624	632	651	rVV	374056	744813	25.72%	2.411%
5	6.975	654	661	680	rVB	316014	567134	19.58%	1.836%
6	7.158	685	692	711	rBV	463193	750240	25.91%	2.429%
7	7.616	763	770	785	rBV	408168	754411	26.05%	2.442%
8	8.328	882	891	913	rBV	433443	890709	30.76%	2.883%
9	8.781	959	968	982	rBV	403884	744329	25.70%	2.409%
10	9.493	1081	1089	1107	rBV	341062	653537	22.57%	2.116%
11	10.028	1173	1180	1203	rBV	430898	907328	31.33%	2.937%
12	10.393	1234	1242	1254	rBV	655471	1100760	38.01%	3.563%
13	10.551	1261	1269	1297	rBV	397217	958218	33.09%	3.102%
14	12.028	1514	1520	1525	rBV2	6245	12655	0.44%	0.041%
15	13.175	1706	1715	1721	rBV5	8432	15797	0.55%	0.051%
16	13.710	1799	1806	1824	rBV	1068624	1608490	55.54%	5.207%
17	13.987	1846	1853	1867	rBV2	1109990	1741004	60.12%	5.636%
18	14.298	1898	1906	1918	rBV	1021768	1622564	56.03%	5.252%
19	14.557	1944	1950	1964	rBV	239198	623202	21.52%	2.017%
20	15.316	2072	2079	2091	rBV	1345490	2221384	76.71%	7.191%
21	15.475	2099	2106	2118	rBV	423304	807675	27.89%	2.615%
22	16.139	2212	2219	2223	rBV10	3965	6181	0.21%	0.020%
23	16.922	2347	2352	2360	rVB3	3716	7982	0.28%	0.026%
24	17.139	2380	2389	2398	rBV	1344437	2113422	72.98%	6.841%
25	17.233	2399	2405	2427	rVB2	1583013	2495095	86.16%	8.077%
26	19.180	2732	2736	2742	rVB3	23180	35739	1.23%	0.116%
27	19.263	2746	2750	2757	rVB2	14603	24346	0.84%	0.079%
28	19.633	2806	2813	2826	rBV	2104613	2895888	100.00%	9.374%
29	21.621	3144	3151	3162	rBV2	1173062	2115456	73.05%	6.848%
30	24.739	3672	3681	3695	rVB	768039	2130139	73.56%	6.896%
31	24.980	3712	3722	3736	rVB	560149	1755205	60.61%	5.682%




Sum of corrected areas: 30891621

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020200.D
Acq On : 06 May 2024 09:59
Operator : MA/JU
Sample : PB160579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

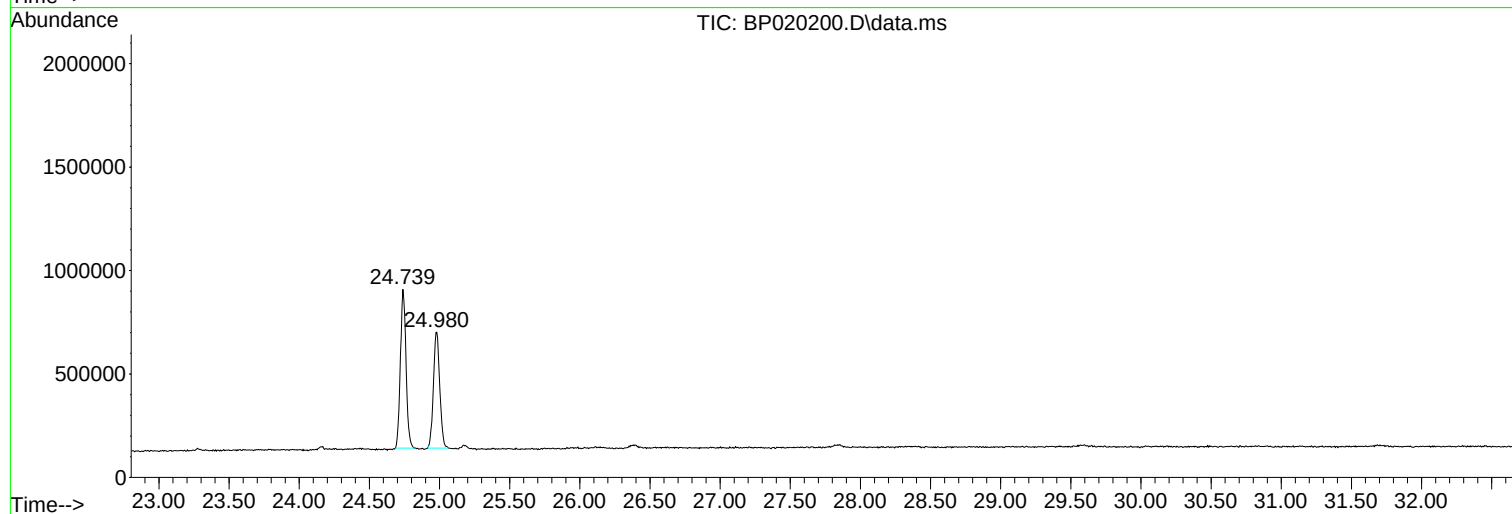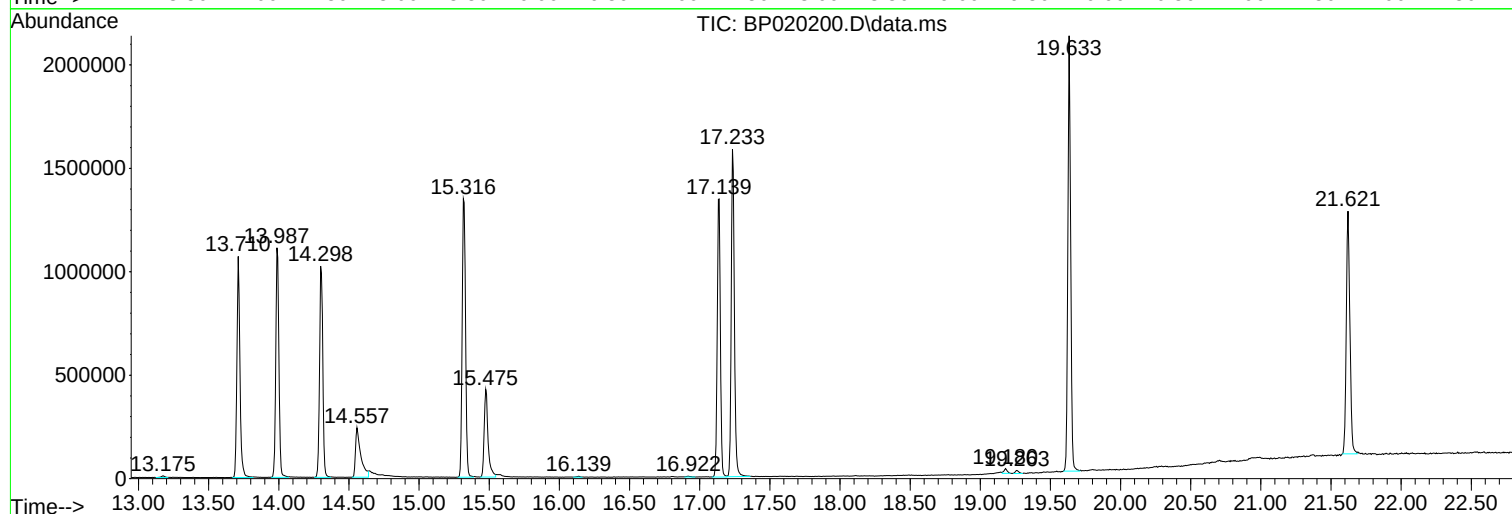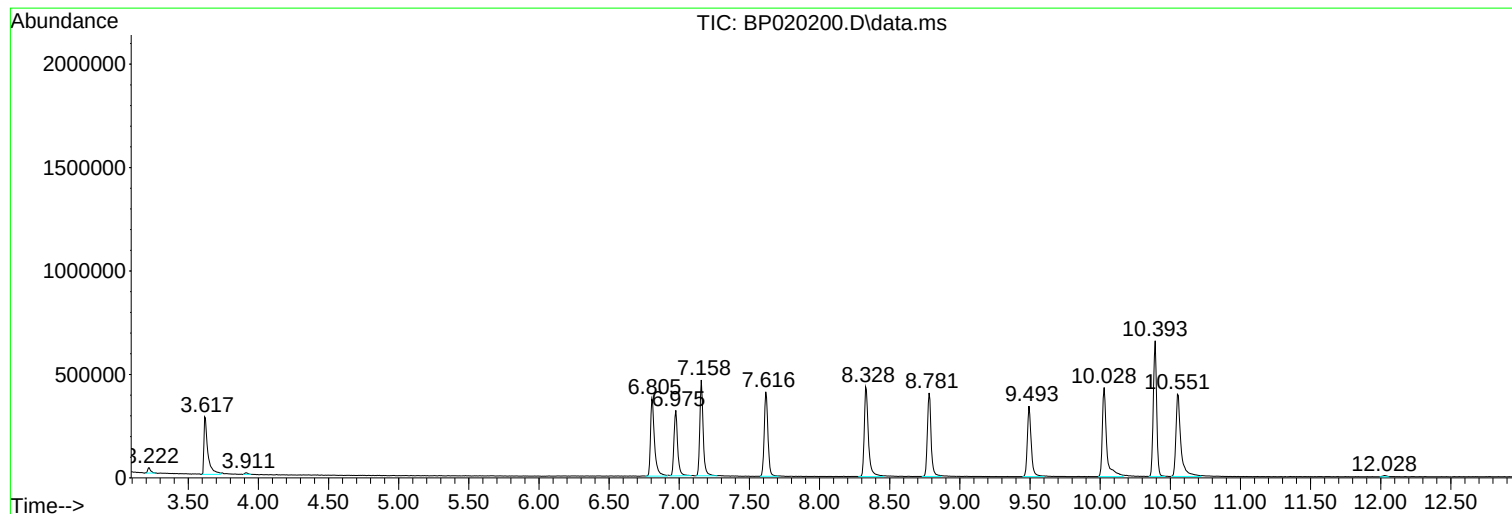

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020200.D
Acq On : 06 May 2024 09:59
Operator : MA/JU
Sample : PB160579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020200.D
Acq On : 06 May 2024 09:59
Operator : MA/JU
Sample : PB160579BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK579

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------