

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020211.D
 Acq On : 06 May 2024 18:03
 Operator : MA/JU
 Sample : PB160744BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK744

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	34	rVB	20067	37972	1.60%	0.158%
2	3.617	87	90	110	rBV	209723	421653	17.78%	1.760%
3	3.911	135	140	149	rVB2	12999	21770	0.92%	0.091%
4	6.811	625	633	648	rBV	277679	578890	24.41%	2.416%
5	6.975	654	661	675	rBV	226111	410802	17.32%	1.714%
6	7.158	686	692	708	rBV	307064	569409	24.01%	2.376%
7	7.622	763	771	783	rBV	271990	503086	21.21%	2.100%
8	8.328	883	891	915	rBV	374613	734275	30.96%	3.064%
9	8.781	960	968	985	rBV	313903	609728	25.71%	2.545%
10	9.499	1082	1090	1110	rBV	279806	530046	22.35%	2.212%
11	10.028	1173	1180	1213	rBV	302499	741329	31.25%	3.094%
12	10.393	1234	1242	1255	rBV	364065	718073	30.27%	2.997%
13	10.557	1262	1270	1282	rBV	357740	854602	36.03%	3.567%
14	12.034	1514	1521	1531	rBV5	4216	10427	0.44%	0.044%
15	13.175	1708	1715	1721	rBV5	5730	11122	0.47%	0.046%
16	13.710	1798	1806	1826	rBV	700772	1206615	50.87%	5.036%
17	13.981	1843	1852	1866	rBV	786971	1315576	55.46%	5.490%
18	14.293	1897	1905	1921	rBV	634940	1013636	42.73%	4.230%
19	14.557	1943	1950	1970	rBV3	145192	550838	23.22%	2.299%
20	15.310	2071	2078	2093	rBV	1006483	1671592	70.47%	6.976%
21	15.463	2098	2104	2119	rBV	303307	591767	24.95%	2.470%
22	15.563	2119	2121	2130	rVB8	8363	14890	0.63%	0.062%
23	16.116	2212	2215	2220	rBV6	2514	3671	0.15%	0.015%
24	16.916	2346	2351	2354	rBV6	1931	3834	0.16%	0.016%
25	17.122	2378	2386	2396	rBV	866346	1287729	54.29%	5.374%
26	17.228	2396	2404	2423	rVB2	1085923	1909134	80.49%	7.968%
27	18.104	2548	2553	2560	rBV2	3635	8296	0.35%	0.035%
28	19.175	2731	2735	2743	rVB7	14224	24081	1.02%	0.101%
29	19.263	2745	2750	2756	rVB2	11143	19631	0.83%	0.082%
30	19.633	2806	2813	2827	rBV	1524675	2372007	100.00%	9.899%
31	21.622	3145	3151	3166	rBV2	793427	1516587	63.94%	6.329%
32	24.757	3674	3684	3701	rVB	854660	2254032	95.03%	9.407%
33	24.986	3714	3723	3740	rVB	504025	1444083	60.88%	6.027%




Sum of corrected areas: 23961183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020211.D
Acq On : 06 May 2024 18:03
Operator : MA/JU
Sample : PB160744BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

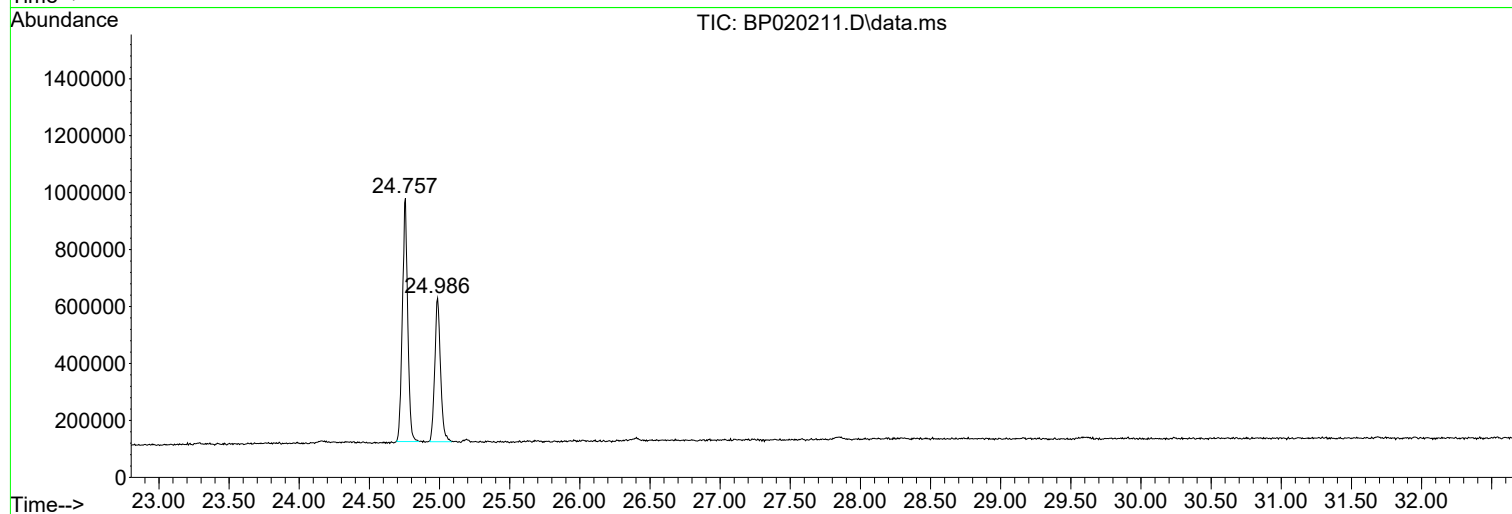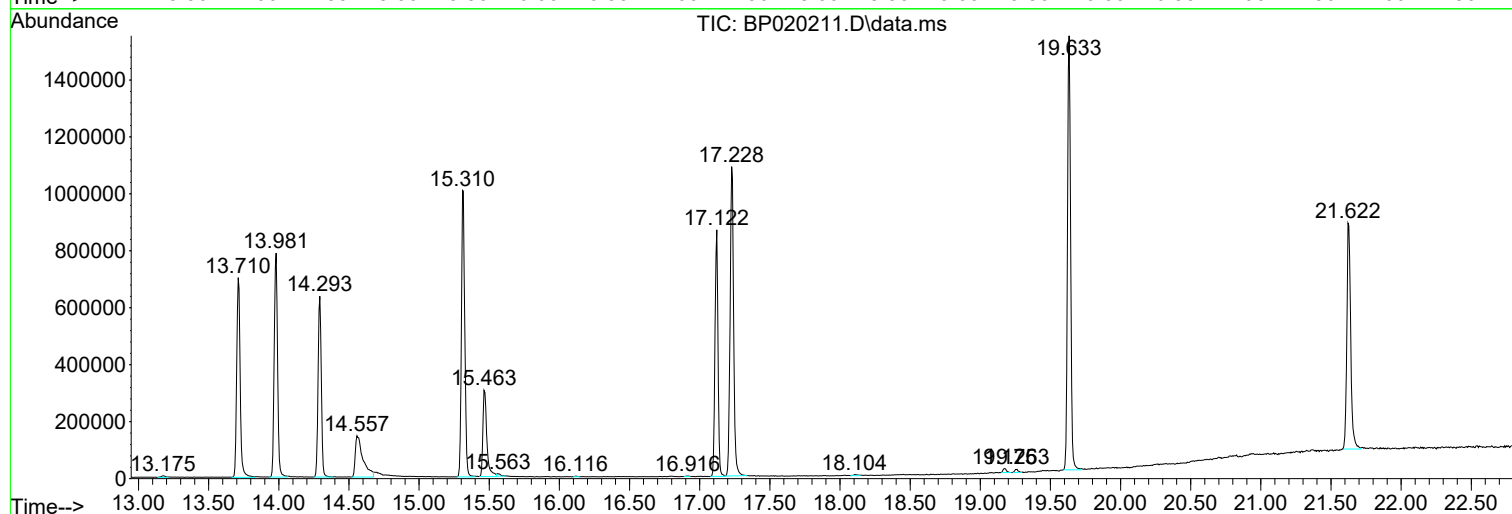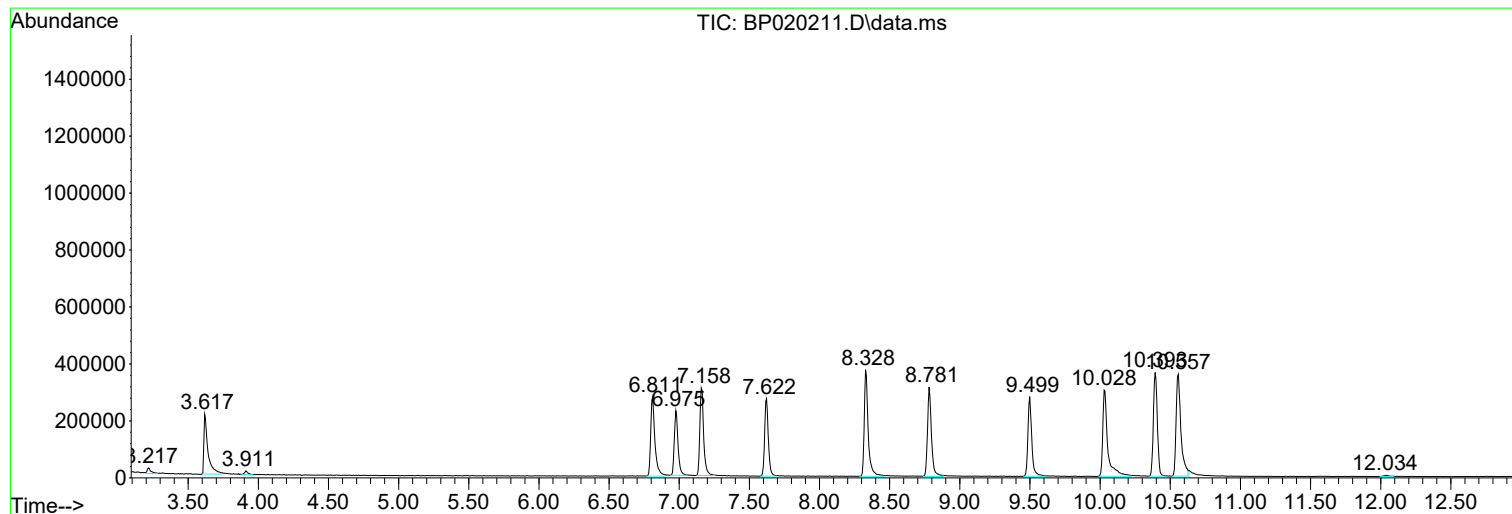

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020211.D
Acq On : 06 May 2024 18:03
Operator : MA/JU
Sample : PB160744BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020211.D
Acq On : 06 May 2024 18:03
Operator : MA/JU
Sample : PB160744BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------