

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
 Data File : BP020225.D
 Acq On : 07 May 2024 08:22
 Operator : MA/JU
 Sample : PB160715BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK715

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	16	20	31	rVB	25126	43116	1.43%	0.132%
2	3.605	84	88	114	rBV	316683	590734	19.60%	1.803%
3	3.899	134	138	143	rVB	14745	22888	0.76%	0.070%
4	4.311	204	208	210	rBV4	4112	5899	0.20%	0.018%
5	6.781	621	628	648	rBV	379829	771612	25.60%	2.355%
6	6.952	650	657	675	rVB	310339	562478	18.66%	1.717%
7	7.134	681	688	705	rVB	425844	757472	25.13%	2.312%
8	7.599	758	767	780	rBV	455691	737933	24.48%	2.252%
9	8.305	879	887	910	rBV	498596	965907	32.04%	2.948%
10	8.757	957	964	982	rBV	423475	790546	26.23%	2.413%
11	9.469	1076	1085	1111	rBV	369287	725104	24.05%	2.213%
12	10.004	1167	1176	1197	rBV	469422	991850	32.90%	3.027%
13	10.375	1231	1239	1251	rBV	598937	1080396	35.84%	3.297%
14	10.534	1256	1266	1287	rBV	540123	1217714	40.40%	3.716%
15	11.998	1507	1515	1519	rBV5	7157	15190	0.50%	0.046%
16	13.163	1706	1713	1719	rBV3	10005	16260	0.54%	0.050%
17	13.698	1796	1804	1816	rBV	1056083	1666272	55.28%	5.085%
18	13.969	1840	1850	1863	rBV	1231415	1825158	60.55%	5.570%
19	14.281	1895	1903	1912	rBV	1028640	1577585	52.33%	4.815%
20	14.539	1939	1947	1979	rBV	252398	878909	29.16%	2.682%
21	15.304	2069	2077	2092	rBV	1585436	2284762	75.79%	6.973%
22	15.457	2095	2103	2115	rBV	531605	869861	28.86%	2.655%
23	15.551	2117	2119	2125	rVB5	9950	14783	0.49%	0.045%
24	15.886	2171	2176	2179	rBV6	2059	3523	0.12%	0.011%
25	16.116	2211	2215	2221	rVB7	4323	7370	0.24%	0.022%
26	16.786	2325	2329	2333	rVB7	3816	6113	0.20%	0.019%
27	16.898	2343	2348	2351	rBV5	3630	6537	0.22%	0.020%
28	17.122	2378	2386	2396	rBV	1253357	1993013	66.12%	6.082%
29	17.222	2396	2403	2417	rVV	1765756	2608437	86.53%	7.961%
30	17.557	2455	2460	2462	rBV5	2392	4472	0.15%	0.014%
31	17.886	2512	2516	2519	rVB5	3425	4523	0.15%	0.014%
32	18.086	2544	2550	2558	rVV7	19106	37019	1.23%	0.113%
33	18.586	2631	2635	2636	rBV4	3314	3858	0.13%	0.012%
34	19.175	2731	2735	2740	rBV2	25181	35229	1.17%	0.108%
35	19.251	2744	2748	2752	rBV	21947	36511	1.21%	0.111%
36	19.439	2777	2780	2784	rBV4	12793	19497	0.65%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020225.D
Acq On : 07 May 2024 08:22
Operator : MA/JU
Sample : PB160715BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK715

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Title : SVOA CALIBRATION

37	19.633	2807	2813	2825	rBV	2194320	3014444	100.00%	9.200%
38	21.633	3147	3153	3160	rBV2	1279553	2062520	68.42%	6.295%
39	23.945	3543	3546	3547	rBV2	35125	45517	1.51%	0.139%
40	24.768	3677	3686	3698	rVB2	878591	2541089	84.30%	7.755%
41	25.004	3717	3726	3740	rVB	636228	1924558	63.84%	5.874%




Sum of corrected areas: 32766659

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020225.D
Acq On : 07 May 2024 08:22
Operator : MA/JU
Sample : PB160715BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

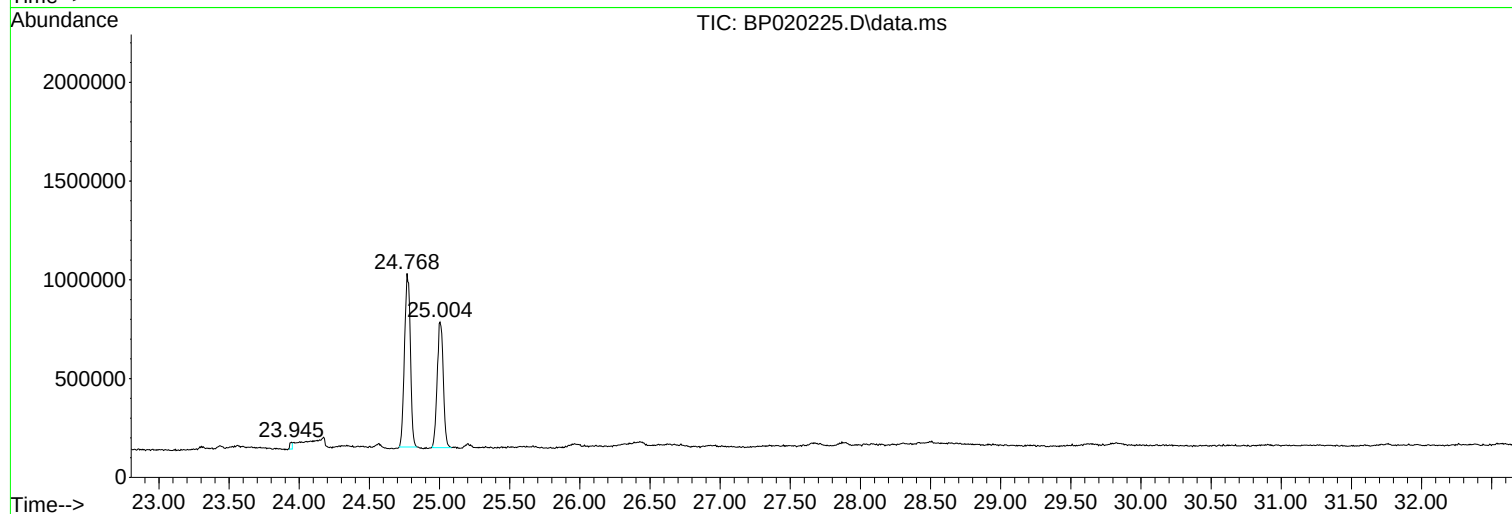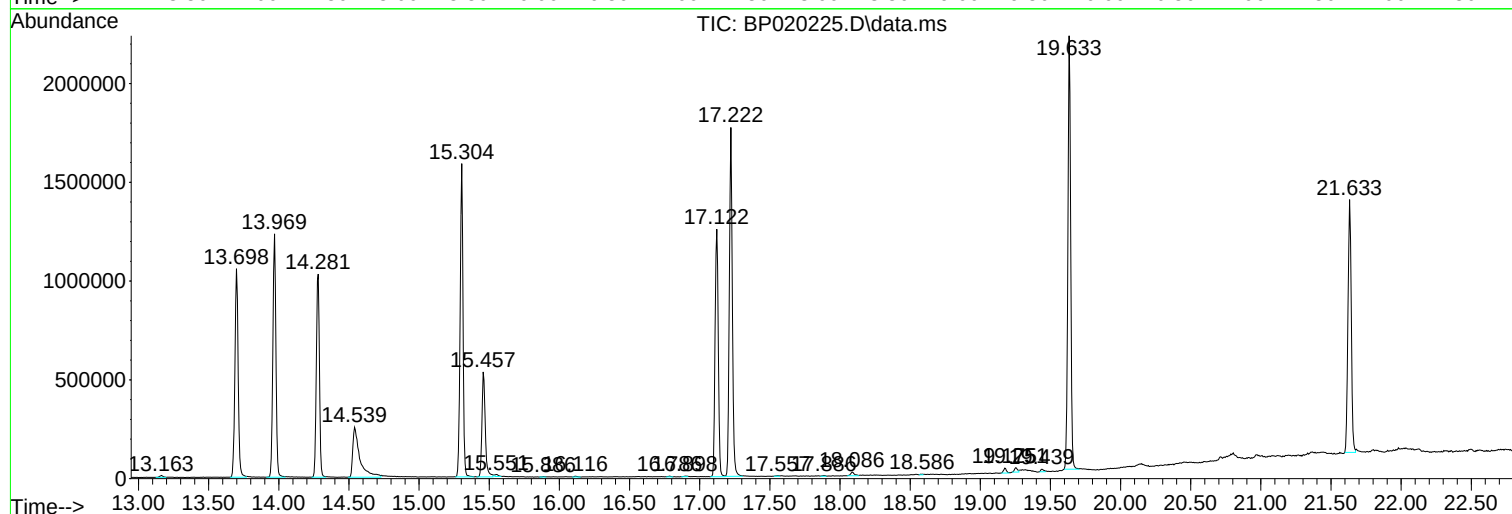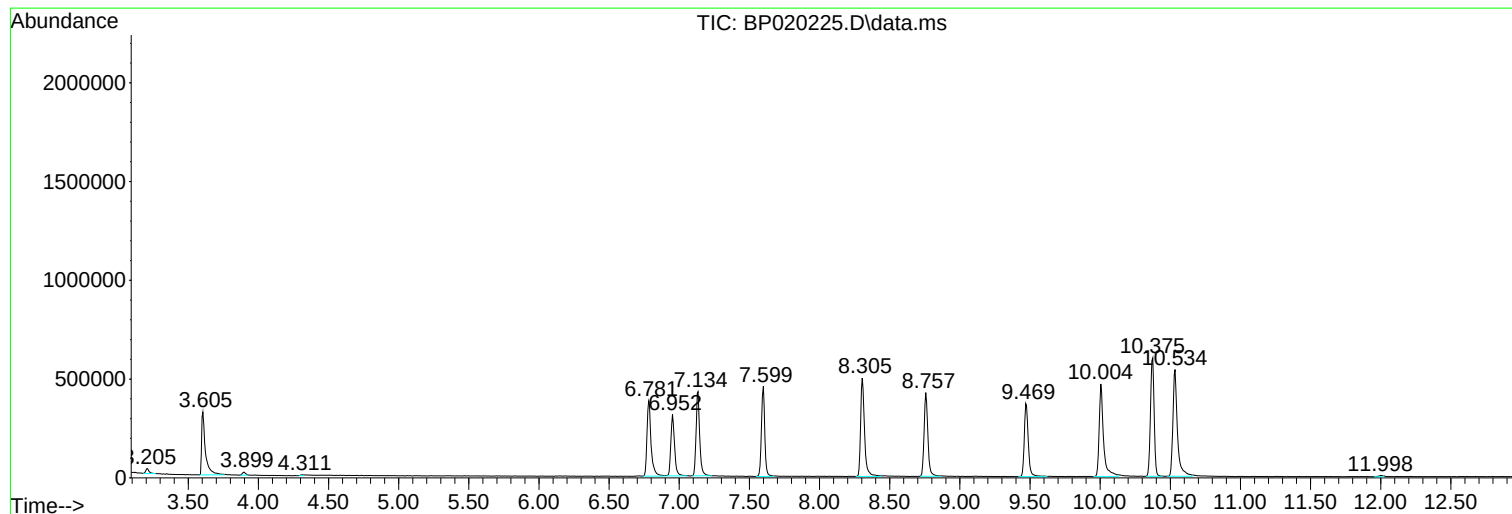

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020225.D
Acq On : 07 May 2024 08:22
Operator : MA/JU
Sample : PB160715BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050624\
Data File : BP020225.D
Acq On : 07 May 2024 08:22
Operator : MA/JU
Sample : PB160715BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK715

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc