
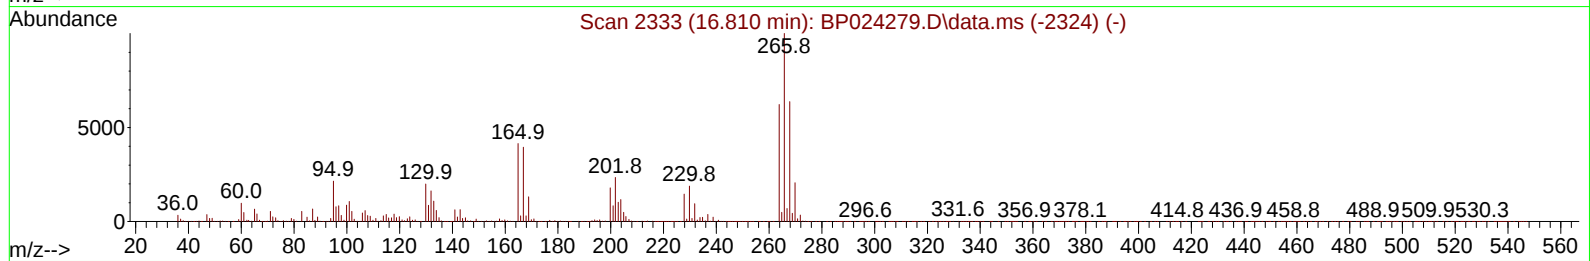
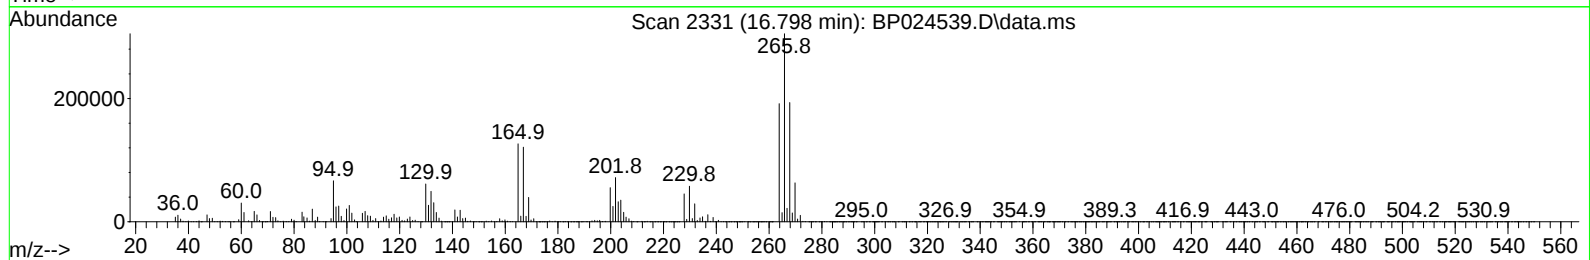


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050625\
Data File : BP024539.D
Acq On : 06 May 2025 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 13:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

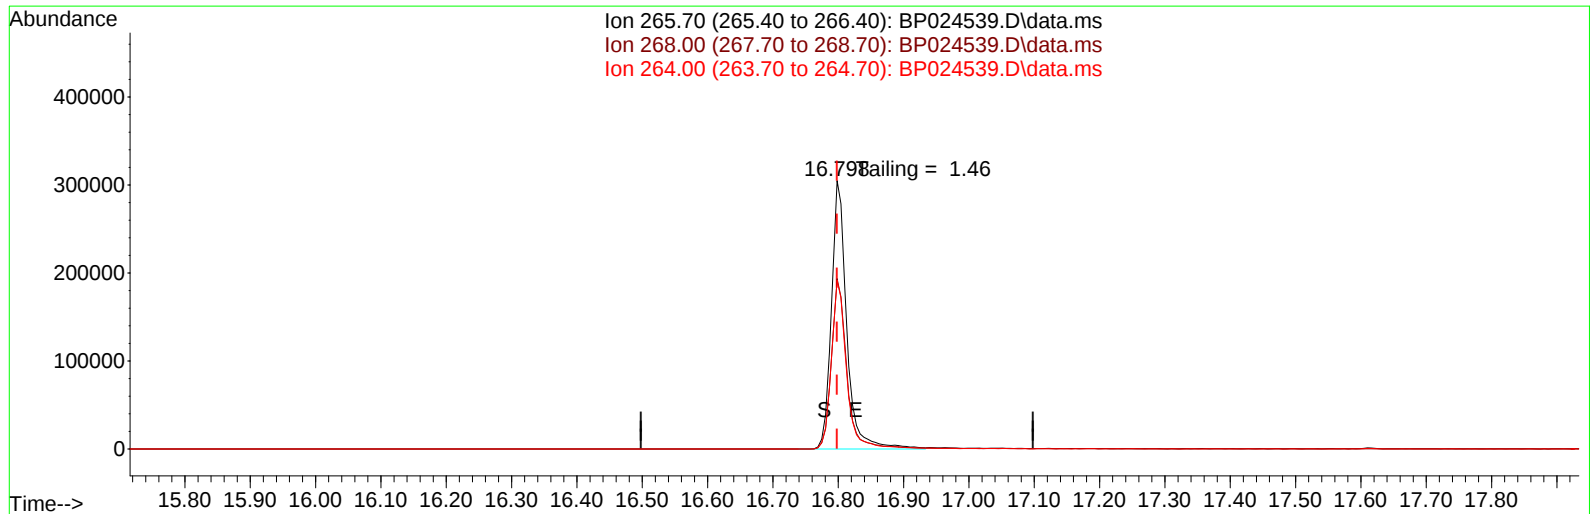

TIC: BP024539.D\data.ms

(70) Pentachlorophenol (C)




16.798min (+ 0.000) 36682.01 ng

response 497194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.43
264.00	62.20	62.84
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050625\  
Data File : BP024539.D  
Acq On    : 06 May 2025  09:37  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 06 13:41:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

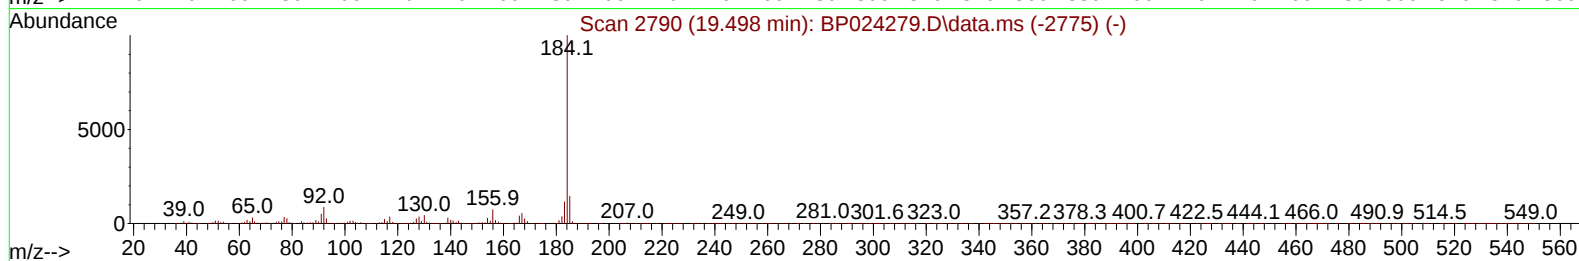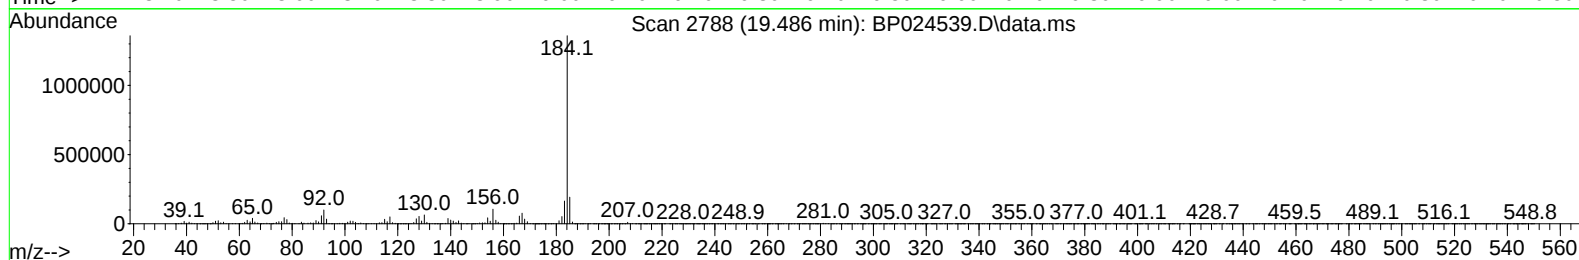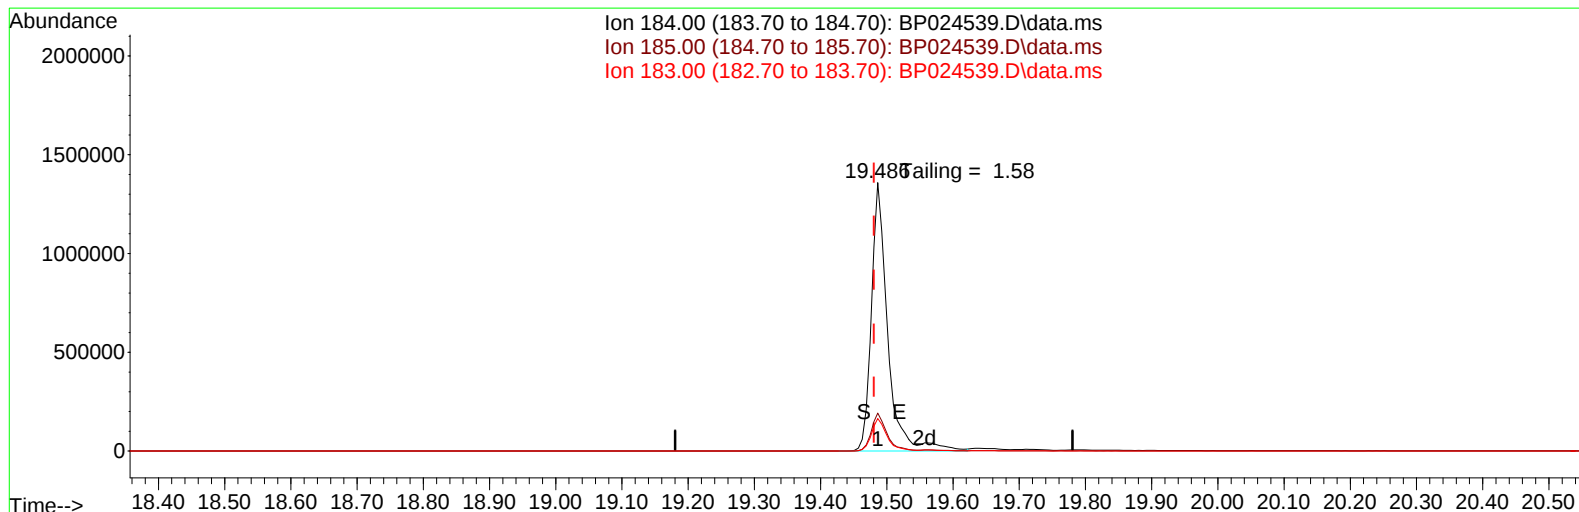

TIC: BP024539.D\data.ms

(77) Benzidine

19.486min (+ 0.006) 48697.69 ng

response **2219755**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.50	14.17
--------	-------	-------

183.00	11.50	12.11
--------	-------	-------

0.00 0.00 0.00