
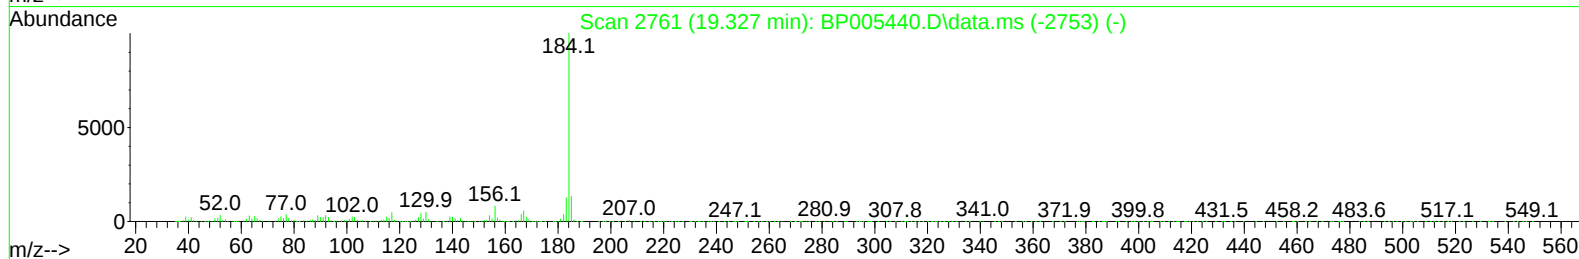
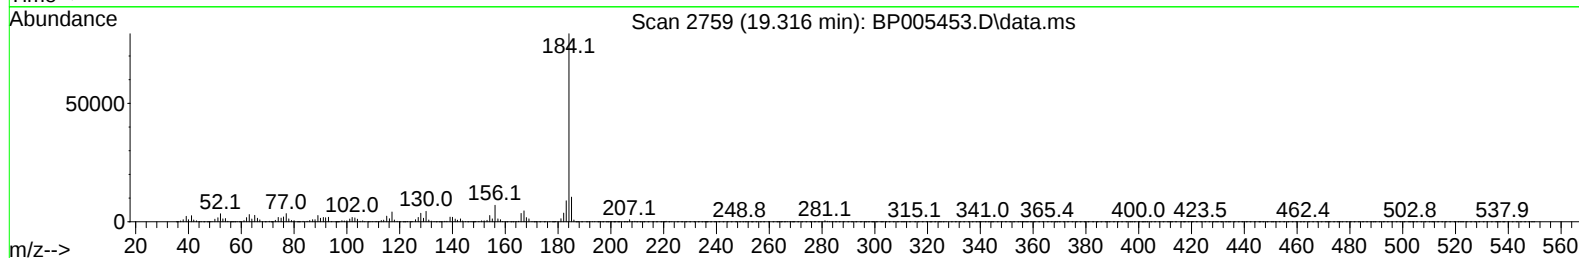


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050721\
Data File : BP005453.D
Acq On : 07 May 2021 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:25:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 19:00:25 2021
Response via : Initial Calibration

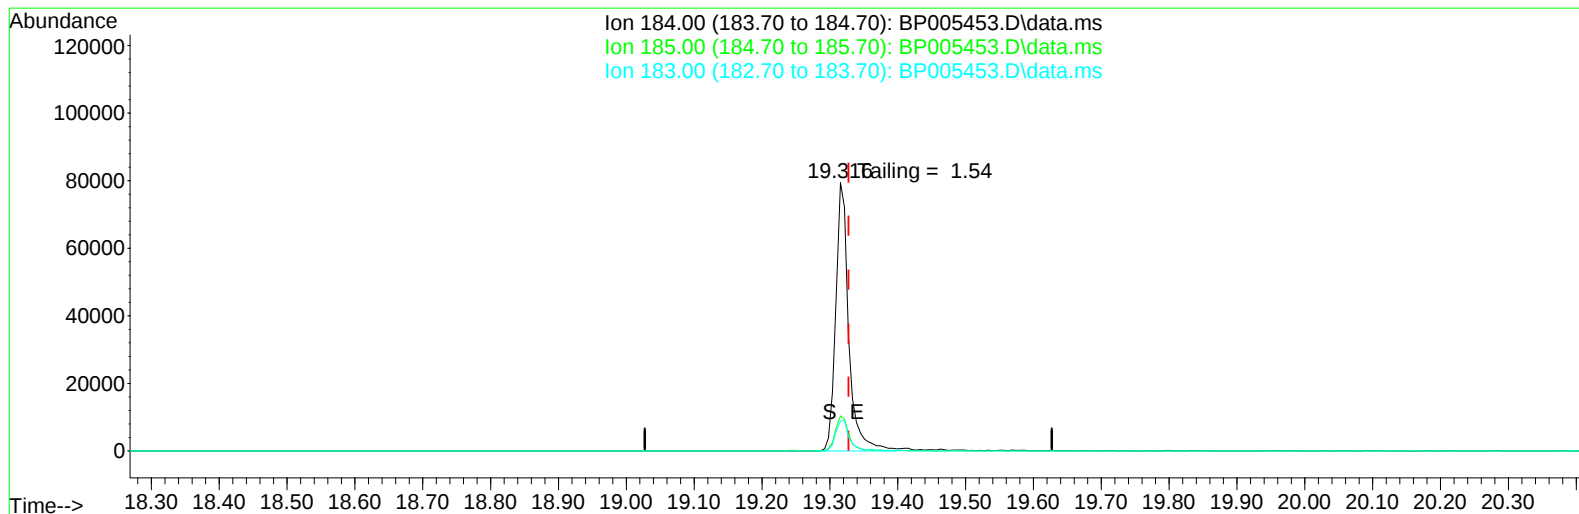

TIC: BP005453.D\data.ms

(77) Benzidine




19.316min (-0.012) 75255.77 ng

response 106003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.10
183.00	12.30	11.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050721\
 Data File : BP005453.D
 Acq On : 07 May 2021 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:25:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 19:00:25 2021
 Response via : Initial Calibration

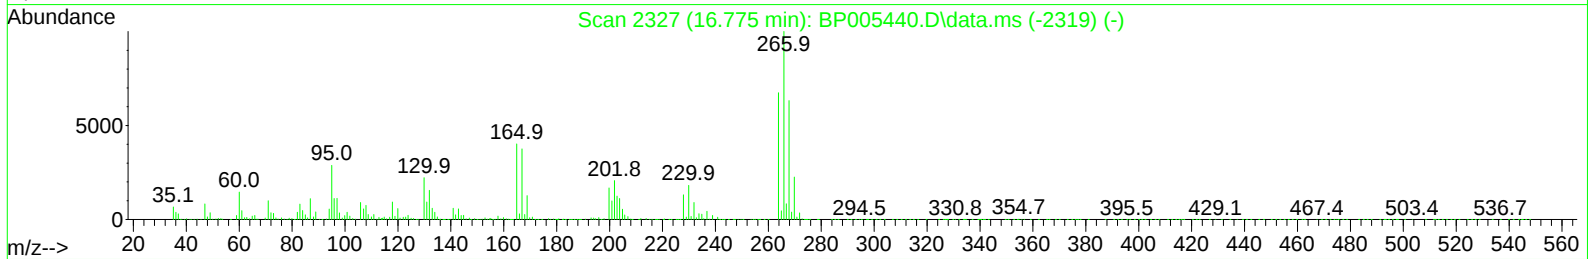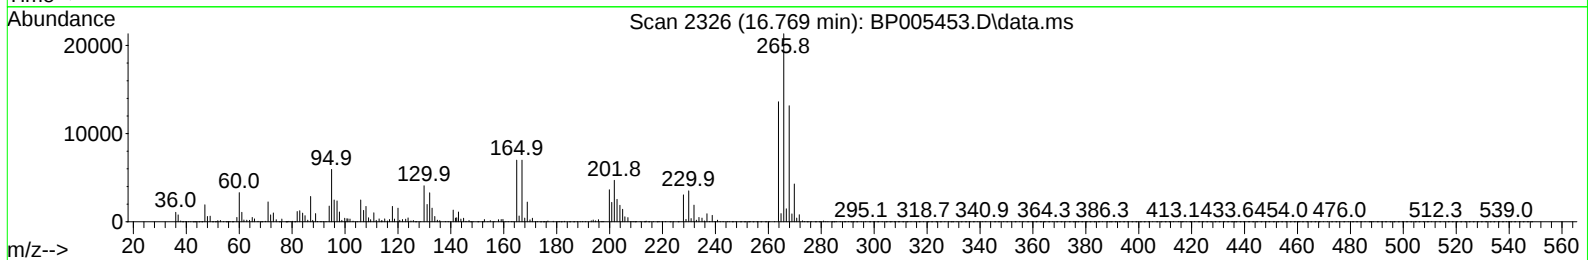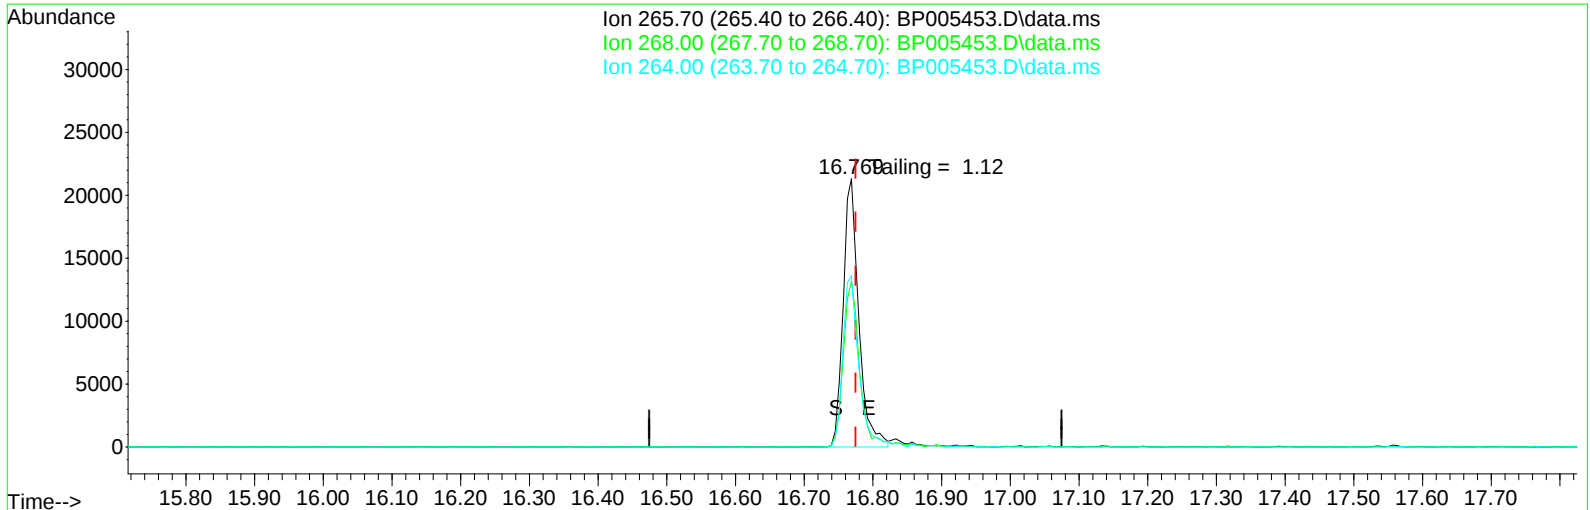

TIC: BP005453.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 400650.29 ng

response 33666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.73
264.00	67.10	63.85
0.00	0.00	0.00