
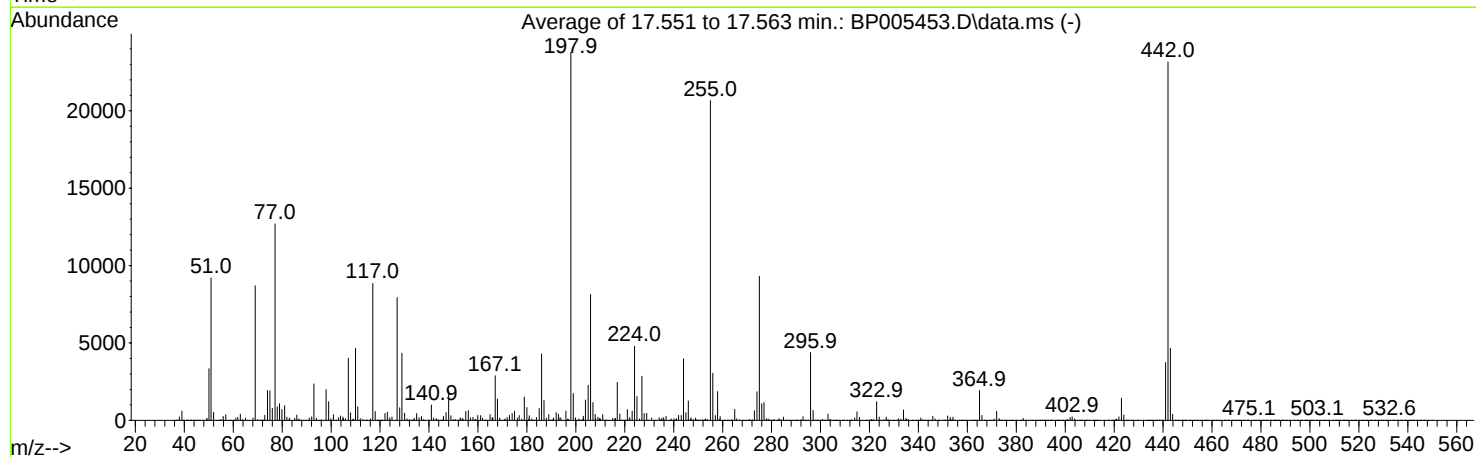


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050721\
 Data File : BP005453.D
 Acq On : 07 May 2021 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 07 12:37:06 2021

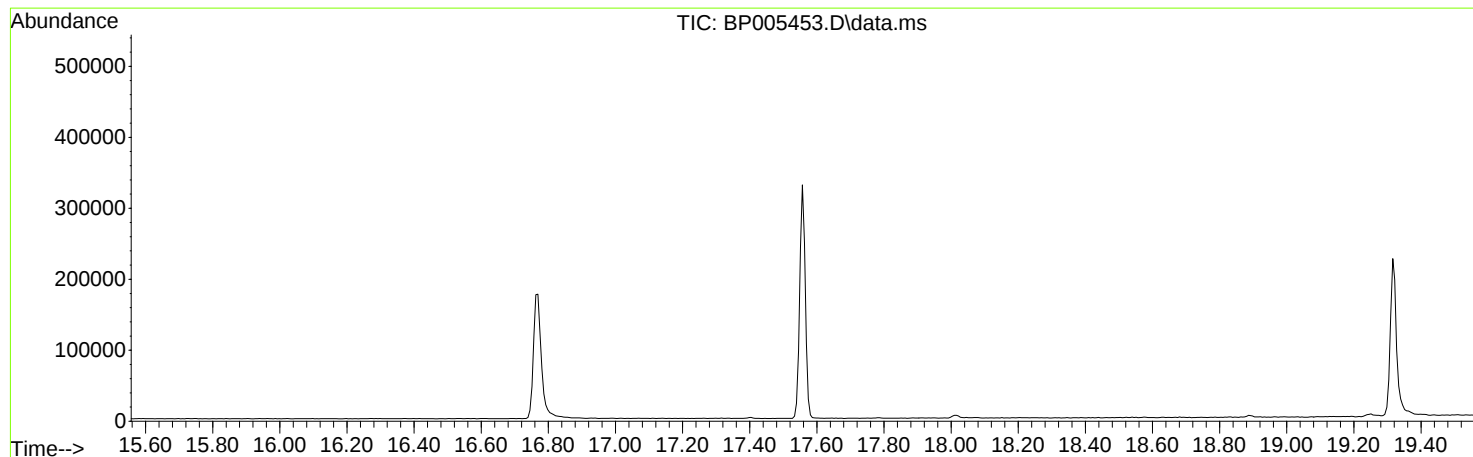

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	9197	PASS
68	69	0.00	2	1.7	151	PASS
69	198	0.00	100	36.6	8699	PASS
70	69	0.00	2	0.7	63	PASS
127	198	10	80	33.4	7937	PASS
197	198	0.00	2	0.4	84	PASS
198	198	100	100	100.0	23767	PASS
199	198	5	9	7.3	1742	PASS
275	198	10	60	39.2	9313	PASS
365	198	1	100	8.1	1927	PASS
441	198	0.01	100	15.7	3731	PASS
442	442	100	100	100.0	23155	PASS
443	442	15	24	20.1	4654	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/7/2021	BNA_P	<u>BP005453.D</u>
Compound Name	Response	Retention Time
DDT	95302	20.51
DDD	779	20.09
DDE	288	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1067	96369	1.11

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050721\
 Data File : BP005453.D
 Acq On : 07 May 2021 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 07 12:25:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 05 19:00:25 2021
 Response via : Initial Calibration

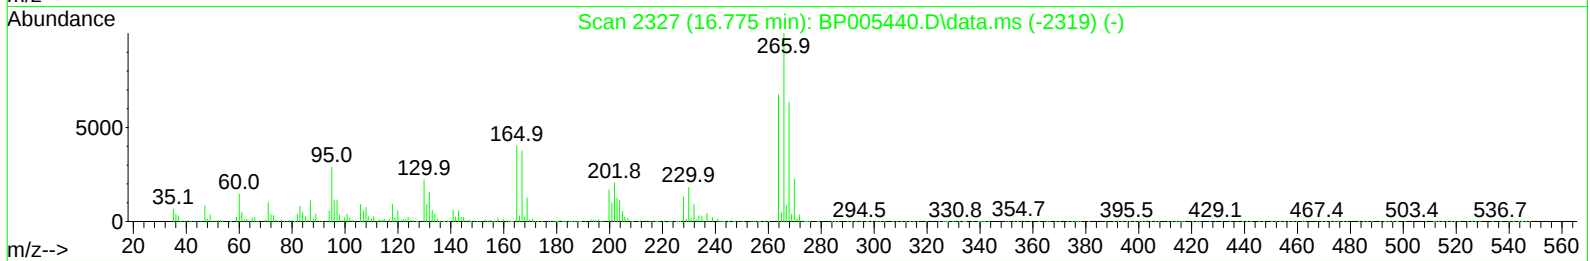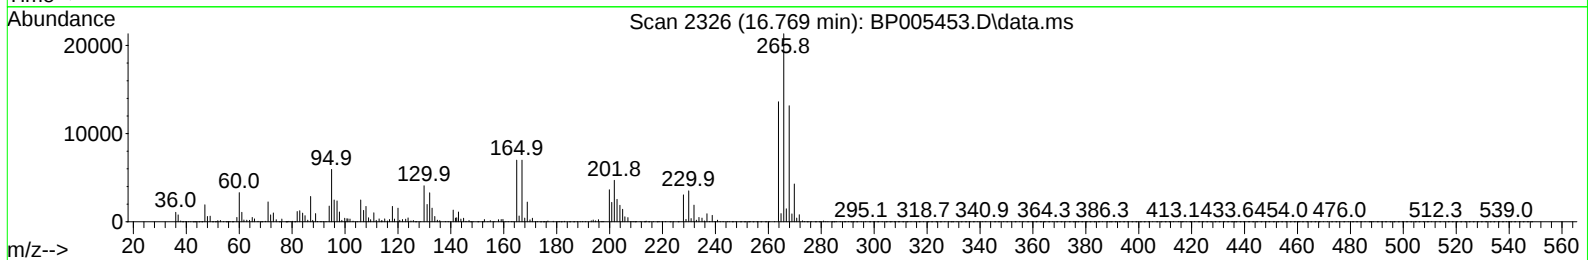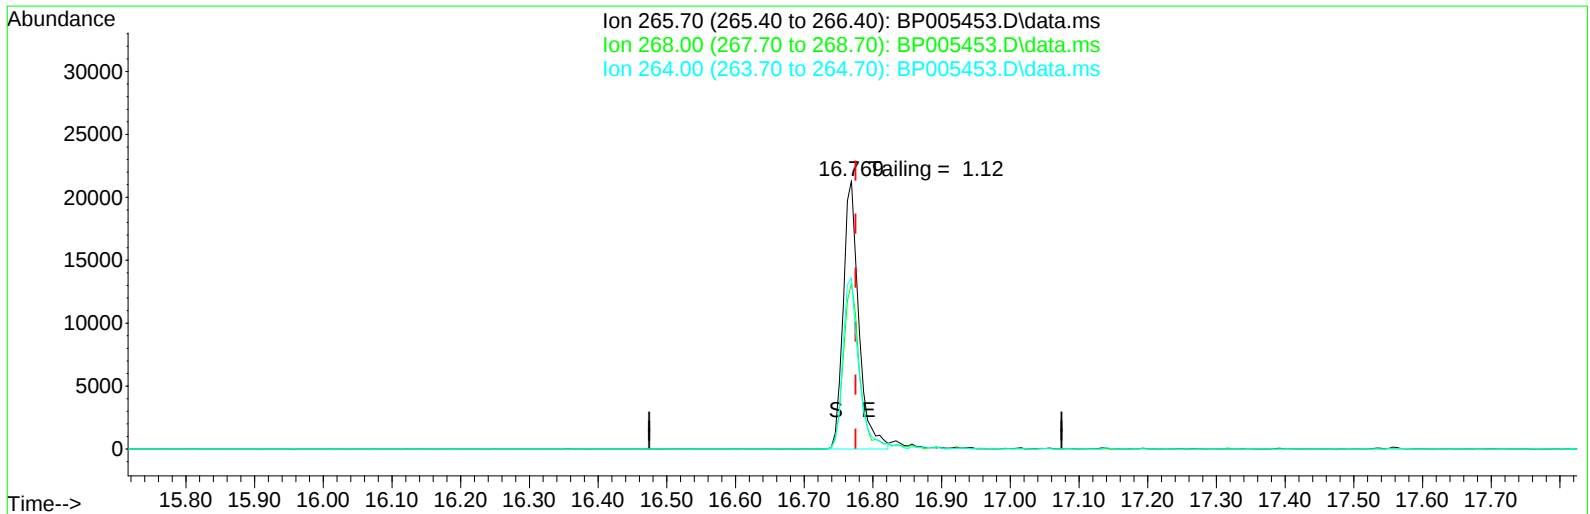

TIC: BP005453.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 400650.29 ng




response 33666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	61.73
264.00	67.10	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050721\
Data File : BP005453.D
Acq On : 07 May 2021 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 07 12:25:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 05 19:00:25 2021
Response via : Initial Calibration

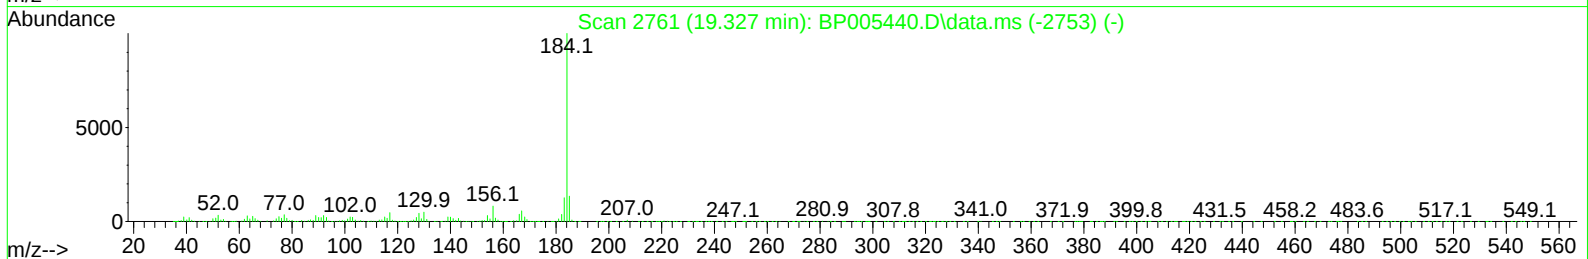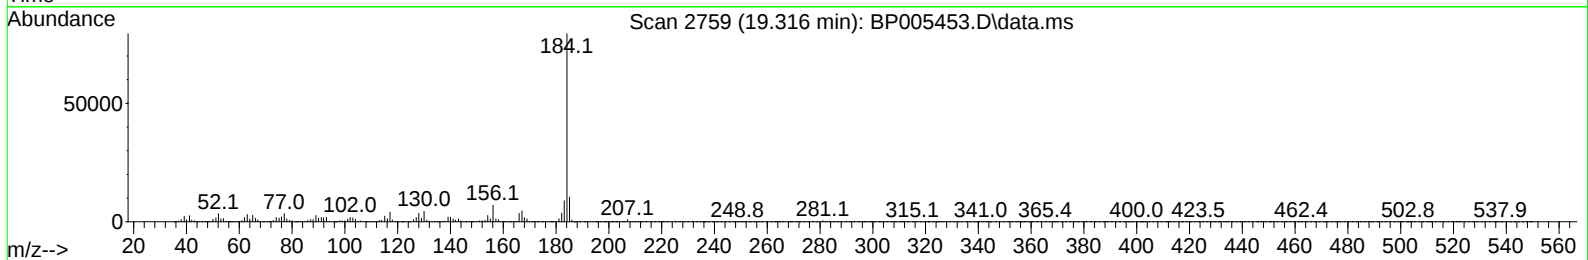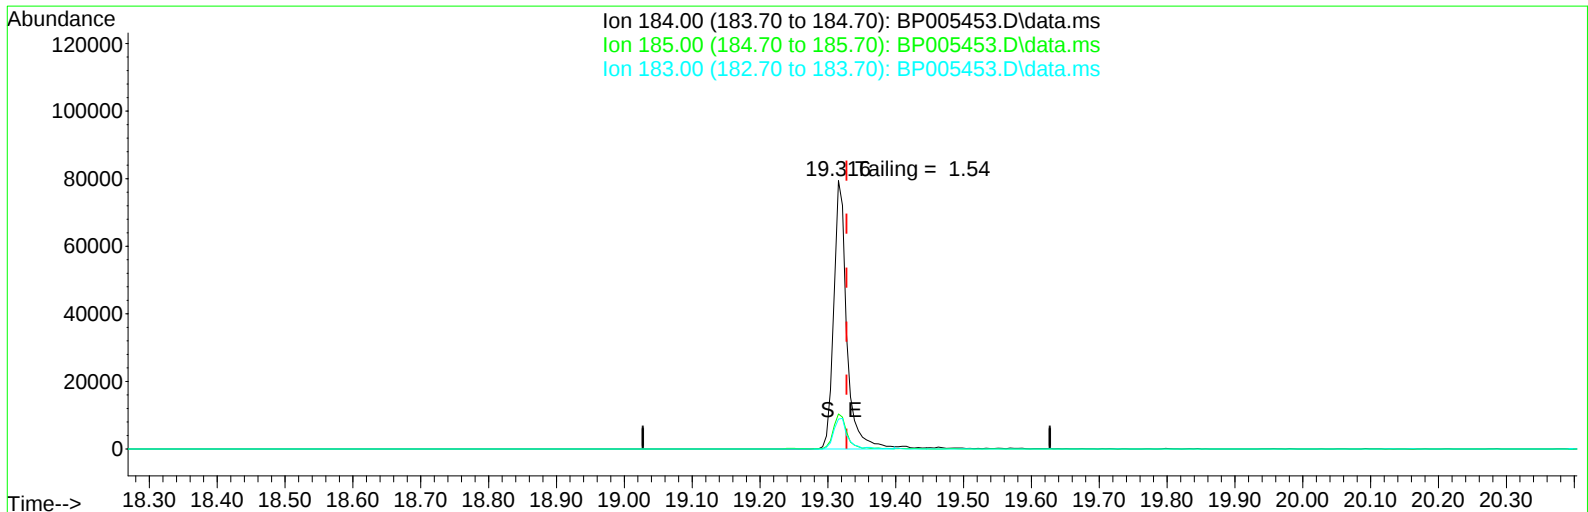

TIC: BP005453.D\data.ms

(77) Benzidine

19.316min (-0.012) 75255.77 ng

response 106003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.10
183.00	12.30	11.18
0.00	0.00	0.00