




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014996.D
Acq On : 08 May 2023 16:45
Operator : CG/JU
Sample : 02589-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREC5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

Quant Time: May 08 22:51:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 12:12:36 2023
Response via : Initial Calibration

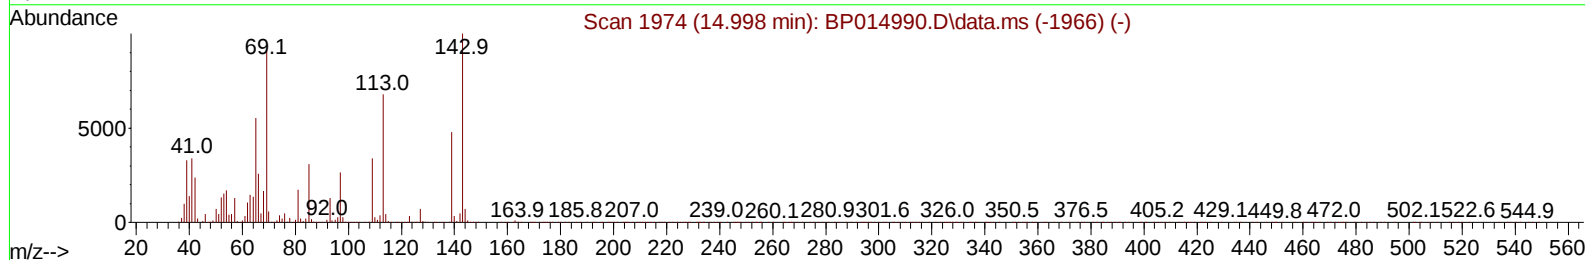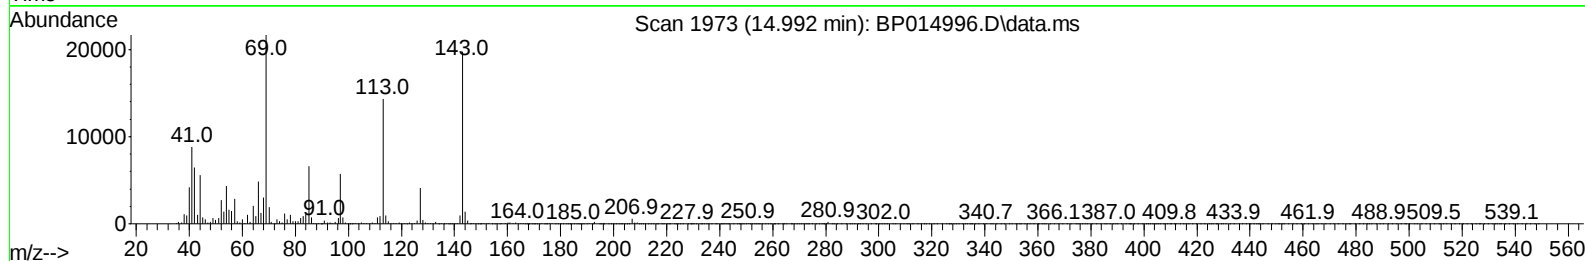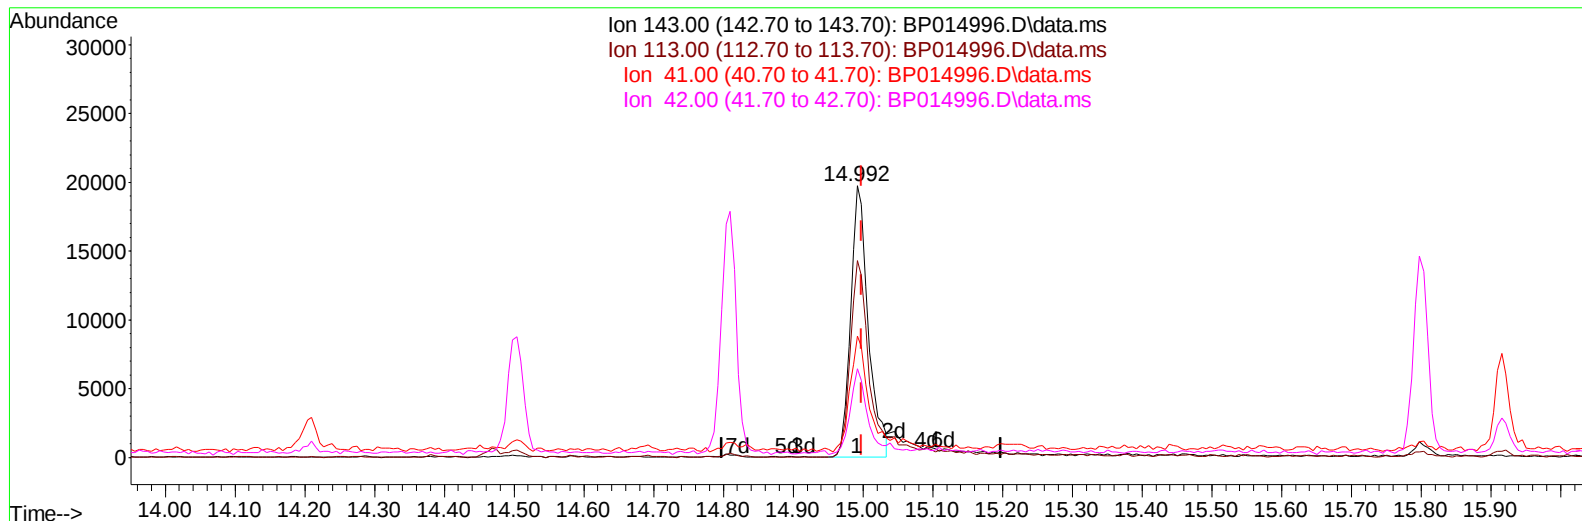

TIC: BP014996.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.992min (-0.006) 3.03 ng/u1****response 34664**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.30	72.60
41.00	38.10	44.76
42.00	25.20	32.58#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014996.D
Acq On : 08 May 2023 16:45
Operator : CG/JU
Sample : 02589-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREC5

Manual IntegrationsAPPROVED

Quant Time: May 08 22:51:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 12:12:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

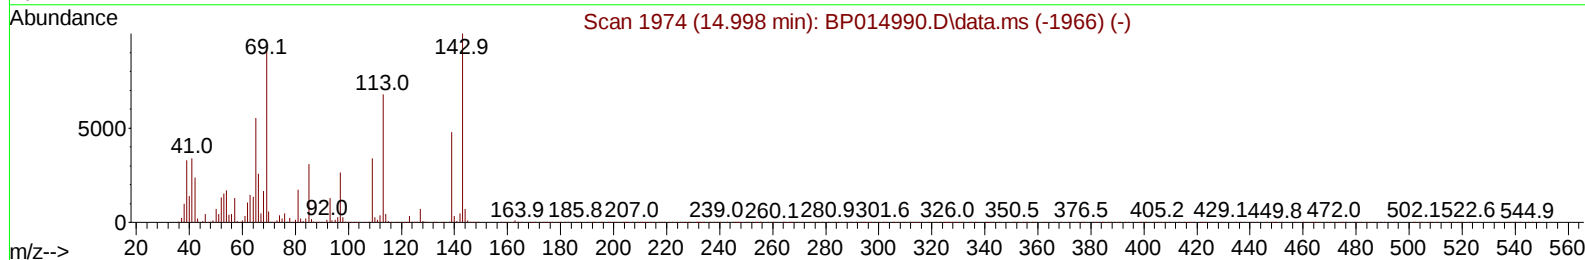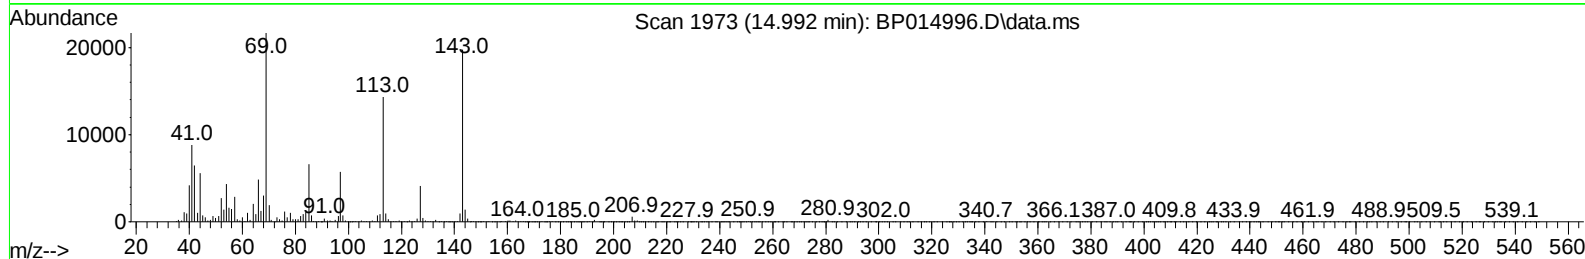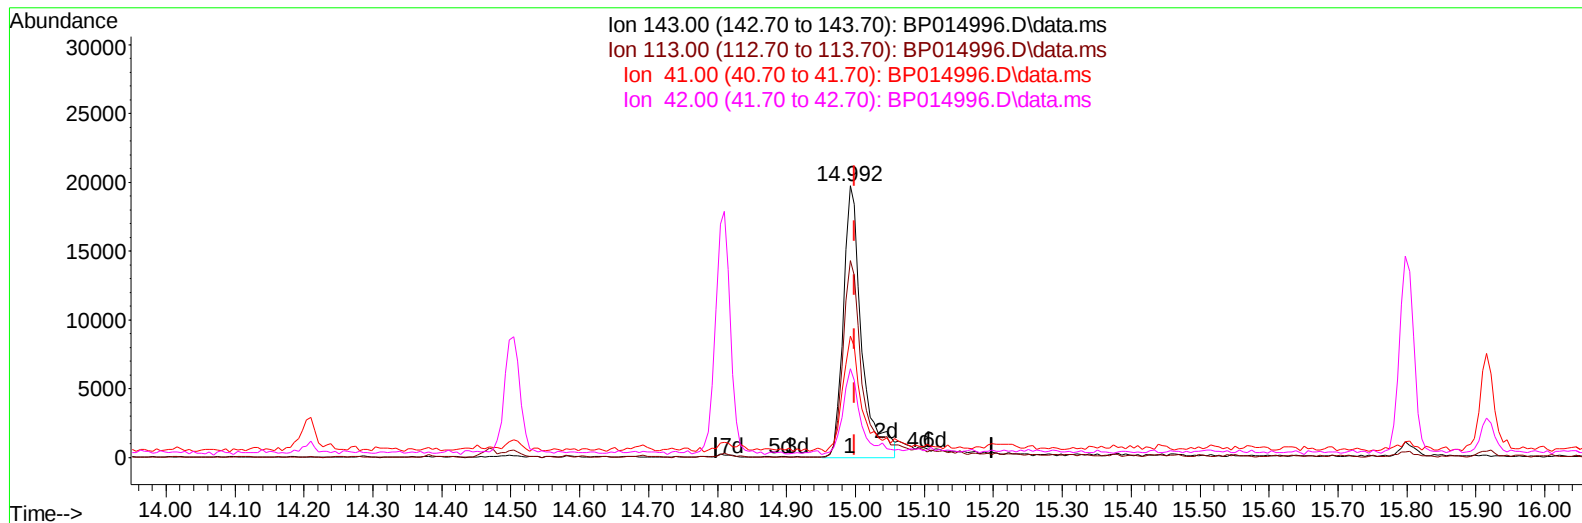

TIC: BP014996.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.992min (-0.006) 3.23 ng/ul m

response 36975

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	71.30	72.60
41.00	38.10	44.76
42.00	25.20	32.58#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
 Data File : BP014996.D
 Acq On : 08 May 2023 16:45
 Operator : CG/JU
 Sample : 02589-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREC5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/09/2023
 Supervised By :Jagrut Upadhyay 05/09/2023

Quant Time: May 08 23:18:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 12:12:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.163	152	308483	20.000	ng/ul	0.00
20) Naphthalene-d8	10.998	136	1420089	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.810	164	930383	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.568	188	1952593	20.000	ng/ul	0.00
79) Chrysene-d12	21.645	240	1416205	20.000	ng/ul	0.00
88) Perylene-d12	24.250	264	1182836	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.457	96	15190	1.831	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.310	99	273644	10.232	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.481	67	214384	12.969	ng/ul	0.00
11) 2-Chlorophenol-d4	7.687	132	251851	12.807	ng/ul	0.00
15) 4-Methylphenol-d8	8.869	113	246449	11.958	ng/ul	0.00
21) Nitrobenzene-d5	9.339	128	135022	13.369	ng/ul	0.00
24) 2-Nitrophenol-d4	10.069	143	148205	14.290	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.610	165	254569	12.501	ng/ul	0.00
31) 4-Chloroaniline-d4	11.133	131	287304	9.754	ng/ul	0.00
46) Dimethylphthalate-d6	14.210	166	1014972	15.414	ng/ul	0.00
49) Acenaphthylene-d8	14.504	160	1124916	14.244	ng/ul	0.00
54) 4-Nitrophenol-d4	14.992	143	36975m	3.228	ng/ul	0.00
60) Fluorene-d10	15.798	176	871511	15.384	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.916	200	102437	9.319	ng/ul	0.00
73) Anthracene-d10	17.662	188	1403562	15.998	ng/ul	0.00
81) Pyrene-d10	19.880	212	1587905	16.625	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.080	264	991279	17.200	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014996.D
Acq On : 08 May 2023 16:45
Operator : CG/JU
Sample : 02589-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREC5

Manual IntegrationsAPPROVED

Quant Time: May 08 23:18:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 12:12:36 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/09/2023
Supervised By :Jagrut Upadhyay 05/09/2023

