

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
 Data File : BP014991.D
 Acq On : 08 May 2023 12:36
 Operator : CG/JU
 Sample : PB152593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK593

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014991.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	8	12	27	rVB	82155	126699	1.98%	0.174%
2	3.899	84	87	105	rBV	920519	1437733	22.51%	1.970%
3	4.246	142	146	152	rVB	21843	33759	0.53%	0.046%
4	7.310	659	667	681	rBV	1153555	1846006	28.90%	2.529%
5	7.481	689	696	707	rVB	1019812	1571625	24.60%	2.153%
6	7.687	724	731	740	rBV	1195345	1889857	29.59%	2.589%
7	8.163	802	812	821	rBV	1152796	1841839	28.84%	2.523%
8	8.875	922	933	947	rBV	1465127	2420825	37.90%	3.316%
9	9.340	1004	1012	1022	rBV	1175458	1902944	29.79%	2.607%
10	9.446	1027	1030	1037	rVB9	5374	9169	0.14%	0.013%
11	10.069	1128	1136	1148	rBV	962723	1601382	25.07%	2.194%
12	10.610	1219	1228	1251	rBV	1410450	2465704	38.60%	3.378%
13	10.998	1284	1294	1307	rBV	1711593	2917884	45.68%	3.997%
14	11.134	1307	1317	1332	rBV	1422748	2454696	38.43%	3.363%
15	12.581	1552	1563	1573	rBV	25268	55380	0.87%	0.076%
16	13.787	1763	1768	1773	rBV3	4773	9030	0.14%	0.012%
17	14.210	1833	1840	1853	rBV	2753396	3757850	58.83%	5.148%
18	14.322	1857	1859	1867	rVB9	4032	6531	0.10%	0.009%
19	14.504	1883	1890	1906	rBV2	3165035	4726279	73.99%	6.475%
20	14.810	1935	1942	1954	rBV	2817355	4091287	64.05%	5.605%
21	14.992	1966	1973	1994	rBV	1084414	1753288	27.45%	2.402%
22	15.804	2103	2111	2124	rBV	3842375	5613866	87.89%	7.690%
23	15.916	2124	2130	2147	rVV	1227194	1758686	27.53%	2.409%
24	16.045	2147	2152	2156	rVB2	17968	31136	0.49%	0.043%
25	16.586	2240	2244	2248	rVB7	5488	7850	0.12%	0.011%
26	17.245	2350	2356	2361	rBV8	6335	12923	0.20%	0.018%
27	17.351	2370	2374	2380	rVB3	7354	12755	0.20%	0.017%
28	17.569	2404	2411	2420	rBV	3235382	4801483	75.17%	6.578%
29	17.663	2420	2427	2445	rVV2	4164238	6087802	95.31%	8.340%
30	19.463	2729	2733	2738	rVB3	51704	69851	1.09%	0.096%
31	19.527	2740	2744	2748	rBV2	46542	63210	0.99%	0.087%
32	19.786	2785	2788	2791	rBV3	21670	23303	0.36%	0.032%
33	19.886	2799	2805	2813	rBV	4617873	6387496	100.00%	8.750%
34	21.645	3099	3104	3115	rBV	2574418	3730591	58.40%	5.111%
35	24.080	3511	3518	3531	rVB2	2034270	4352895	68.15%	5.963%
36	24.251	3540	3547	3562	rVB2	1425834	3124535	48.92%	4.280%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014991.D
Acq On : 08 May 2023 12:36
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK593

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 72998149

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014991.D
Acq On : 08 May 2023 12:36
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

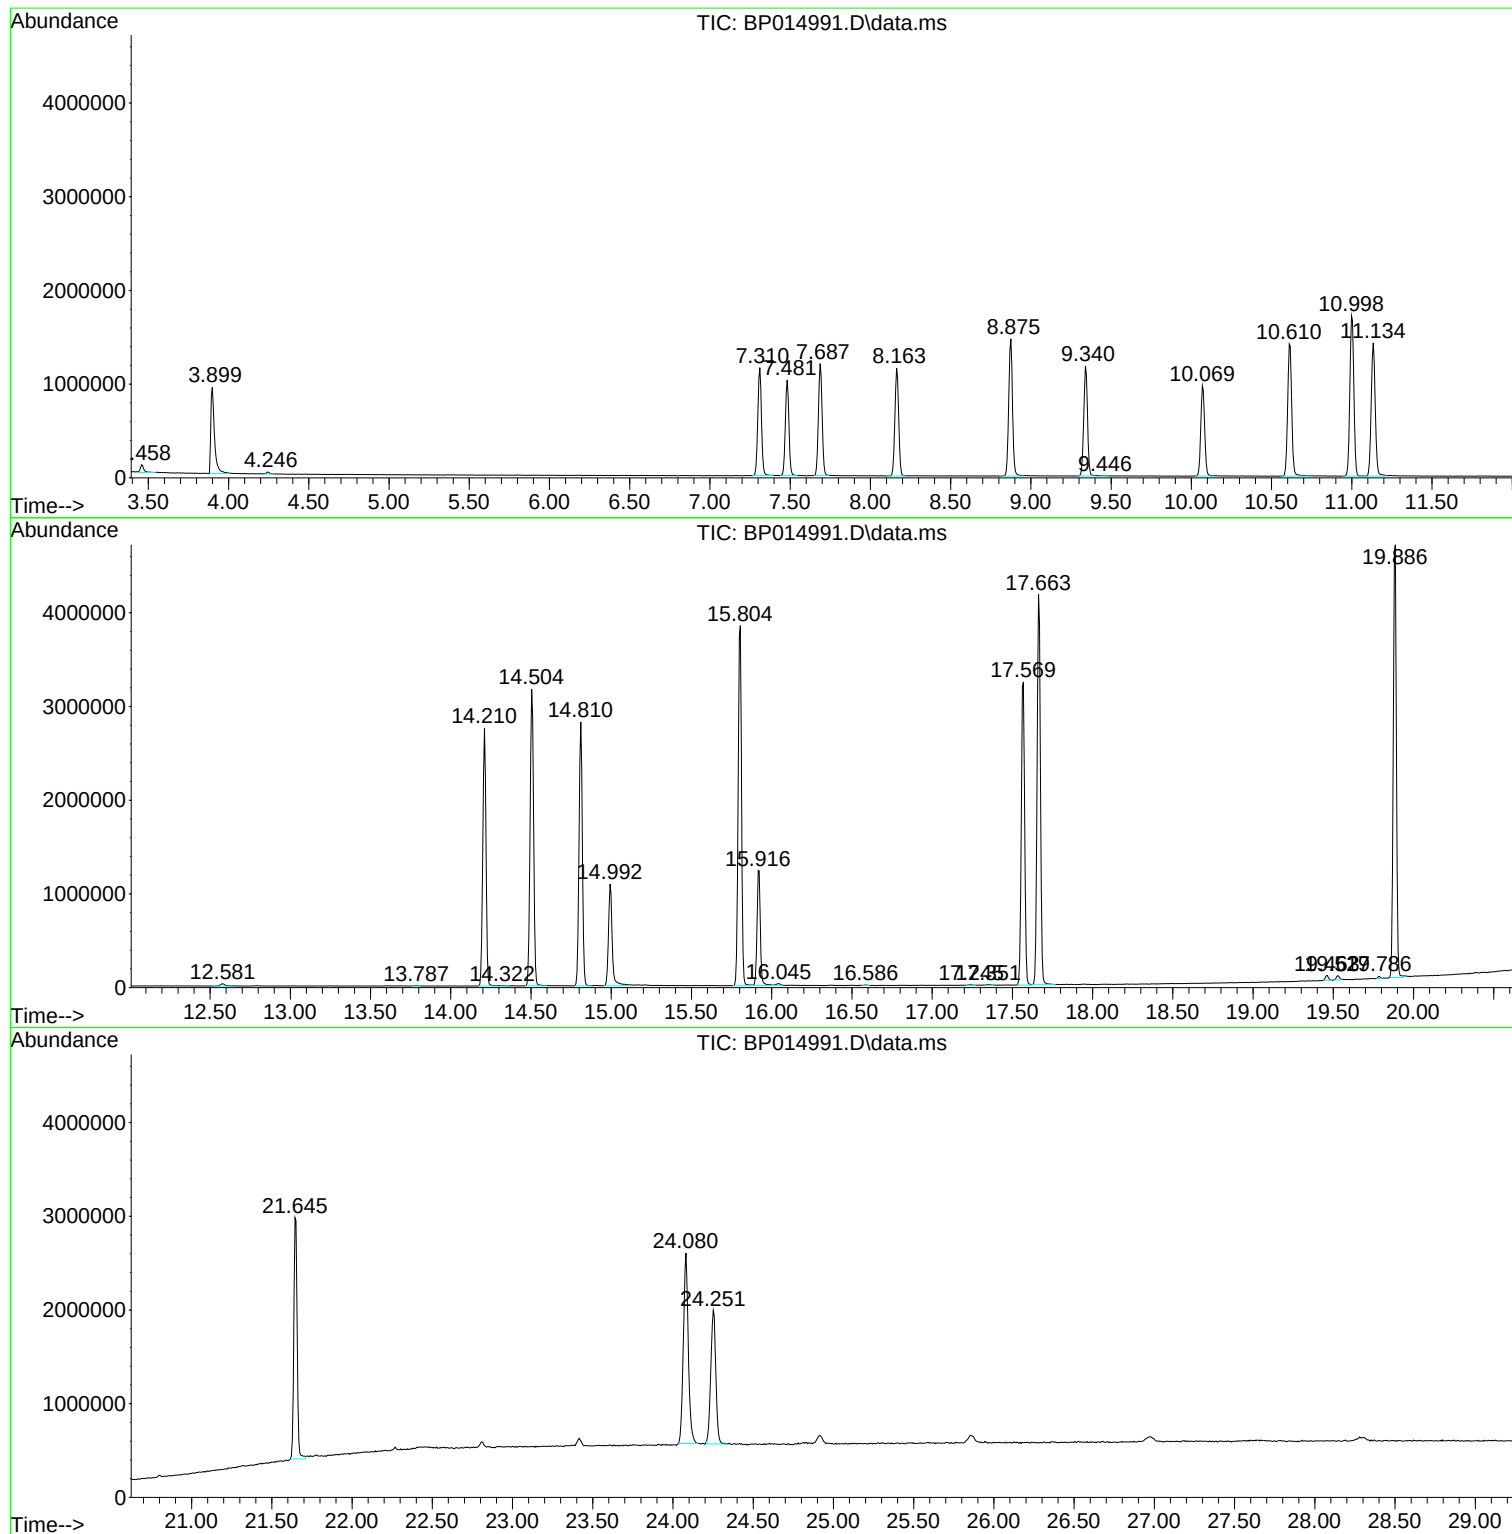

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014991.D
Acq On : 08 May 2023 12:36
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050823\
Data File : BP014991.D
Acq On : 08 May 2023 12:36
Operator : CG/JU
Sample : PB152593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK593

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc