
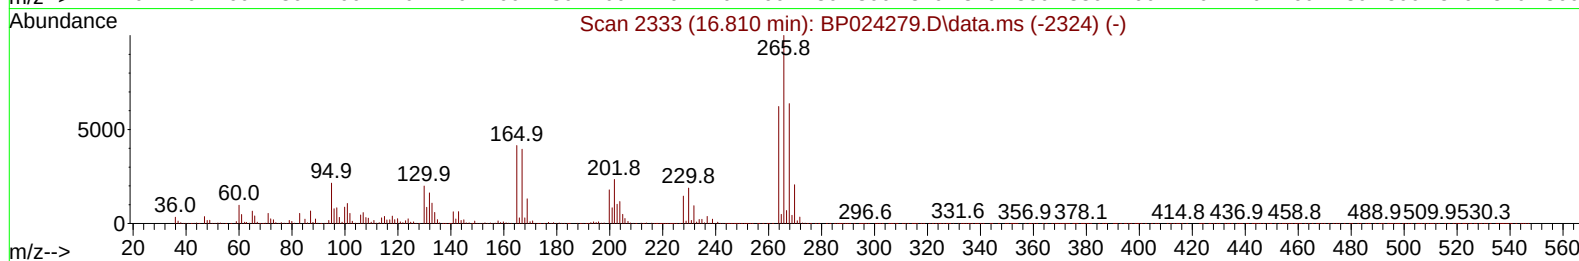
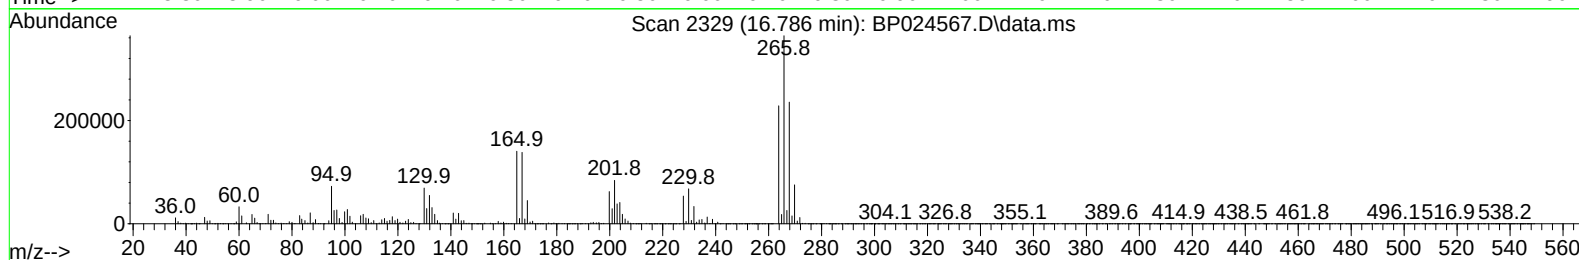


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050825\
Data File : BP024567.D
Acq On : 08 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 15:11:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

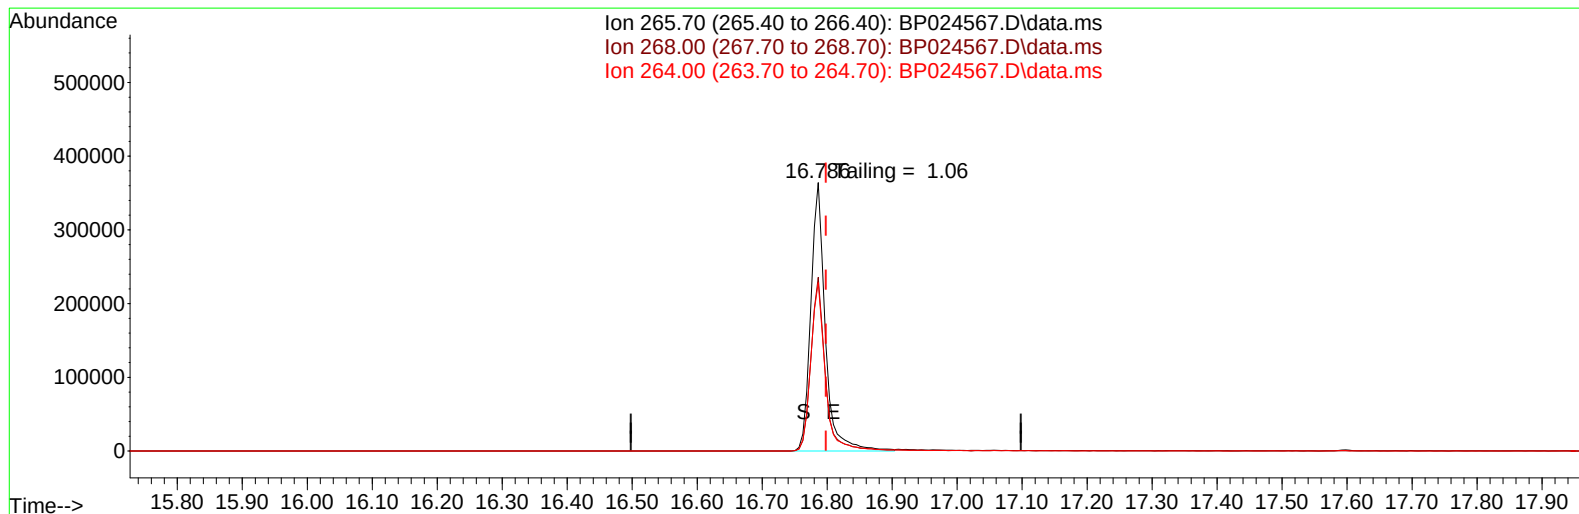

TIC: BP024567.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.012) 35045.60 ng

response 573194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.70
264.00	62.20	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050825\
Data File : BP024567.D
Acq On : 08 May 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 15:11:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

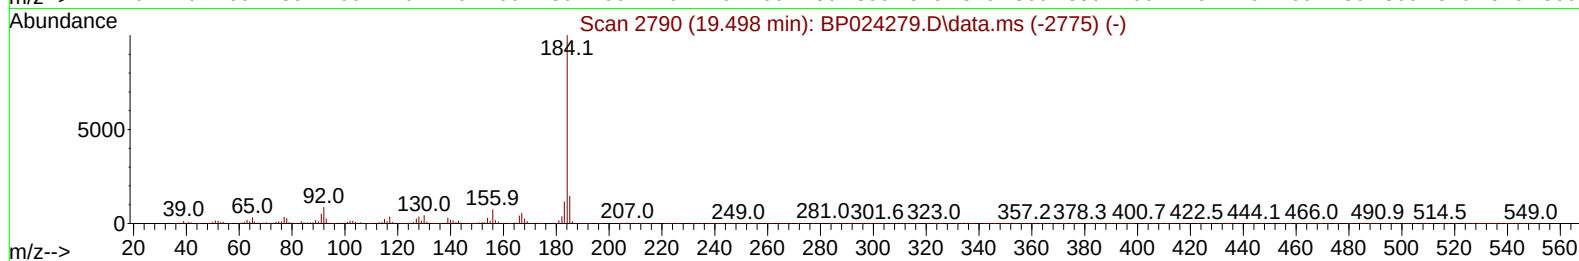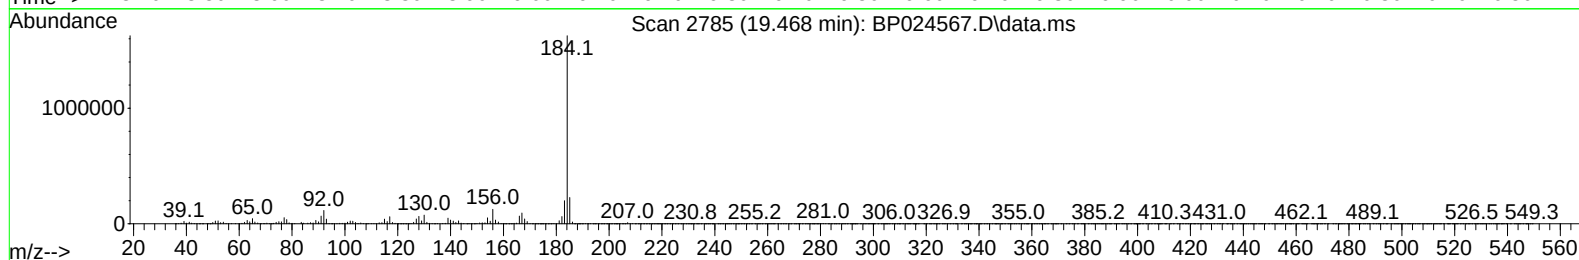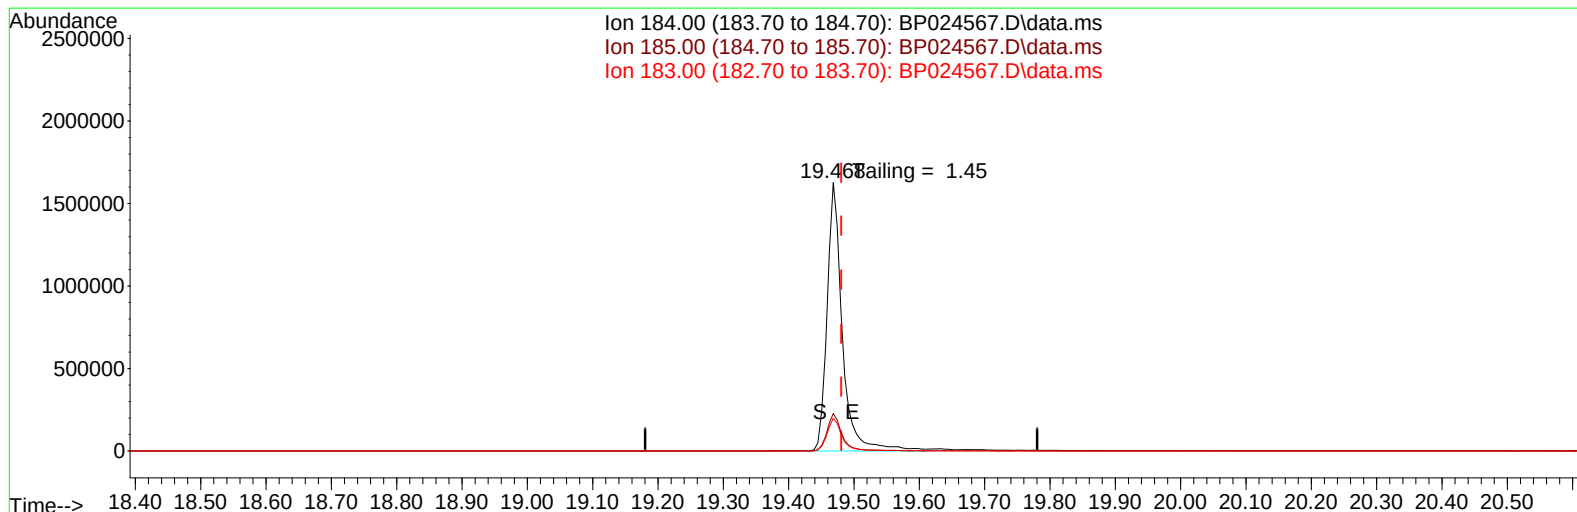

TIC: BP024567.D\data.ms

(77) Benzidine**19.468min (-0.012) 33720.75 ng****response 2634734**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.96
183.00	11.50	12.24
0.00	0.00	0.00