

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
 Data File : BP015029.D
 Acq On : 09 May 2023 21:27
 Operator : CG/JU
 Sample : 02694-23
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREK9

Quant Time: May 09 22:16:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 12:12:36 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.158	152	435153	20.000	ng/ul	0.00
20) Naphthalene-d8	10.993	136	1741266	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.804	164	1093599	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.557	188	2273560	20.000	ng/ul	-0.01
79) Chrysene-d12	21.639	240	1258842	20.000	ng/ul	0.00
88) Perylene-d12	24.233	264	1573271	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.458	96	33418	2.855	ng/uL	0.00
4) Pyridine-d5	3.905	84	113647	3.553	ng/ul	0.00
7) Phenol-d5	7.299	99	146508	3.883	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.475	67	372610	15.979	ng/ul	0.00
11) 2-Chlorophenol-d4	7.681	132	398328	14.359	ng/ul	0.00
15) 4-Methylphenol-d8	8.863	113	281898	9.696	ng/ul	-0.01
21) Nitrobenzene-d5	9.334	128	250342	20.215	ng/ul	0.00
24) 2-Nitrophenol-d4	10.063	143	255111	20.061	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.605	165	407871	16.335	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.128	131	296292	8.204	ng/ul	0.00
46) Dimethylphthalate-d6	14.204	166	1354109	17.495	ng/ul	0.00
49) Acenaphthylene-d8	14.493	160	1561034	16.817	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.993	143	34386	2.554	ng/ul	0.00
60) Fluorene-d10	15.792	176	1137886	17.088	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.910	200	121530	9.496	ng/ul	-0.01
73) Anthracene-d10	17.657	188	1709850	16.738	ng/ul	0.00
81) Pyrene-d10	19.875	212	1444155	17.010	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.063	264	1313600	17.136	ng/ul	-0.01
Target Compounds						
18) 4-Methylphenol	8.928	108	562816	17.238	ng/ul	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015029.D
Acq On : 09 May 2023 21:27
Operator : CG/JU
Sample : 02694-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREK9

Quant Time: May 09 22:16:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 12:12:36 2023
Response via : Initial Calibration

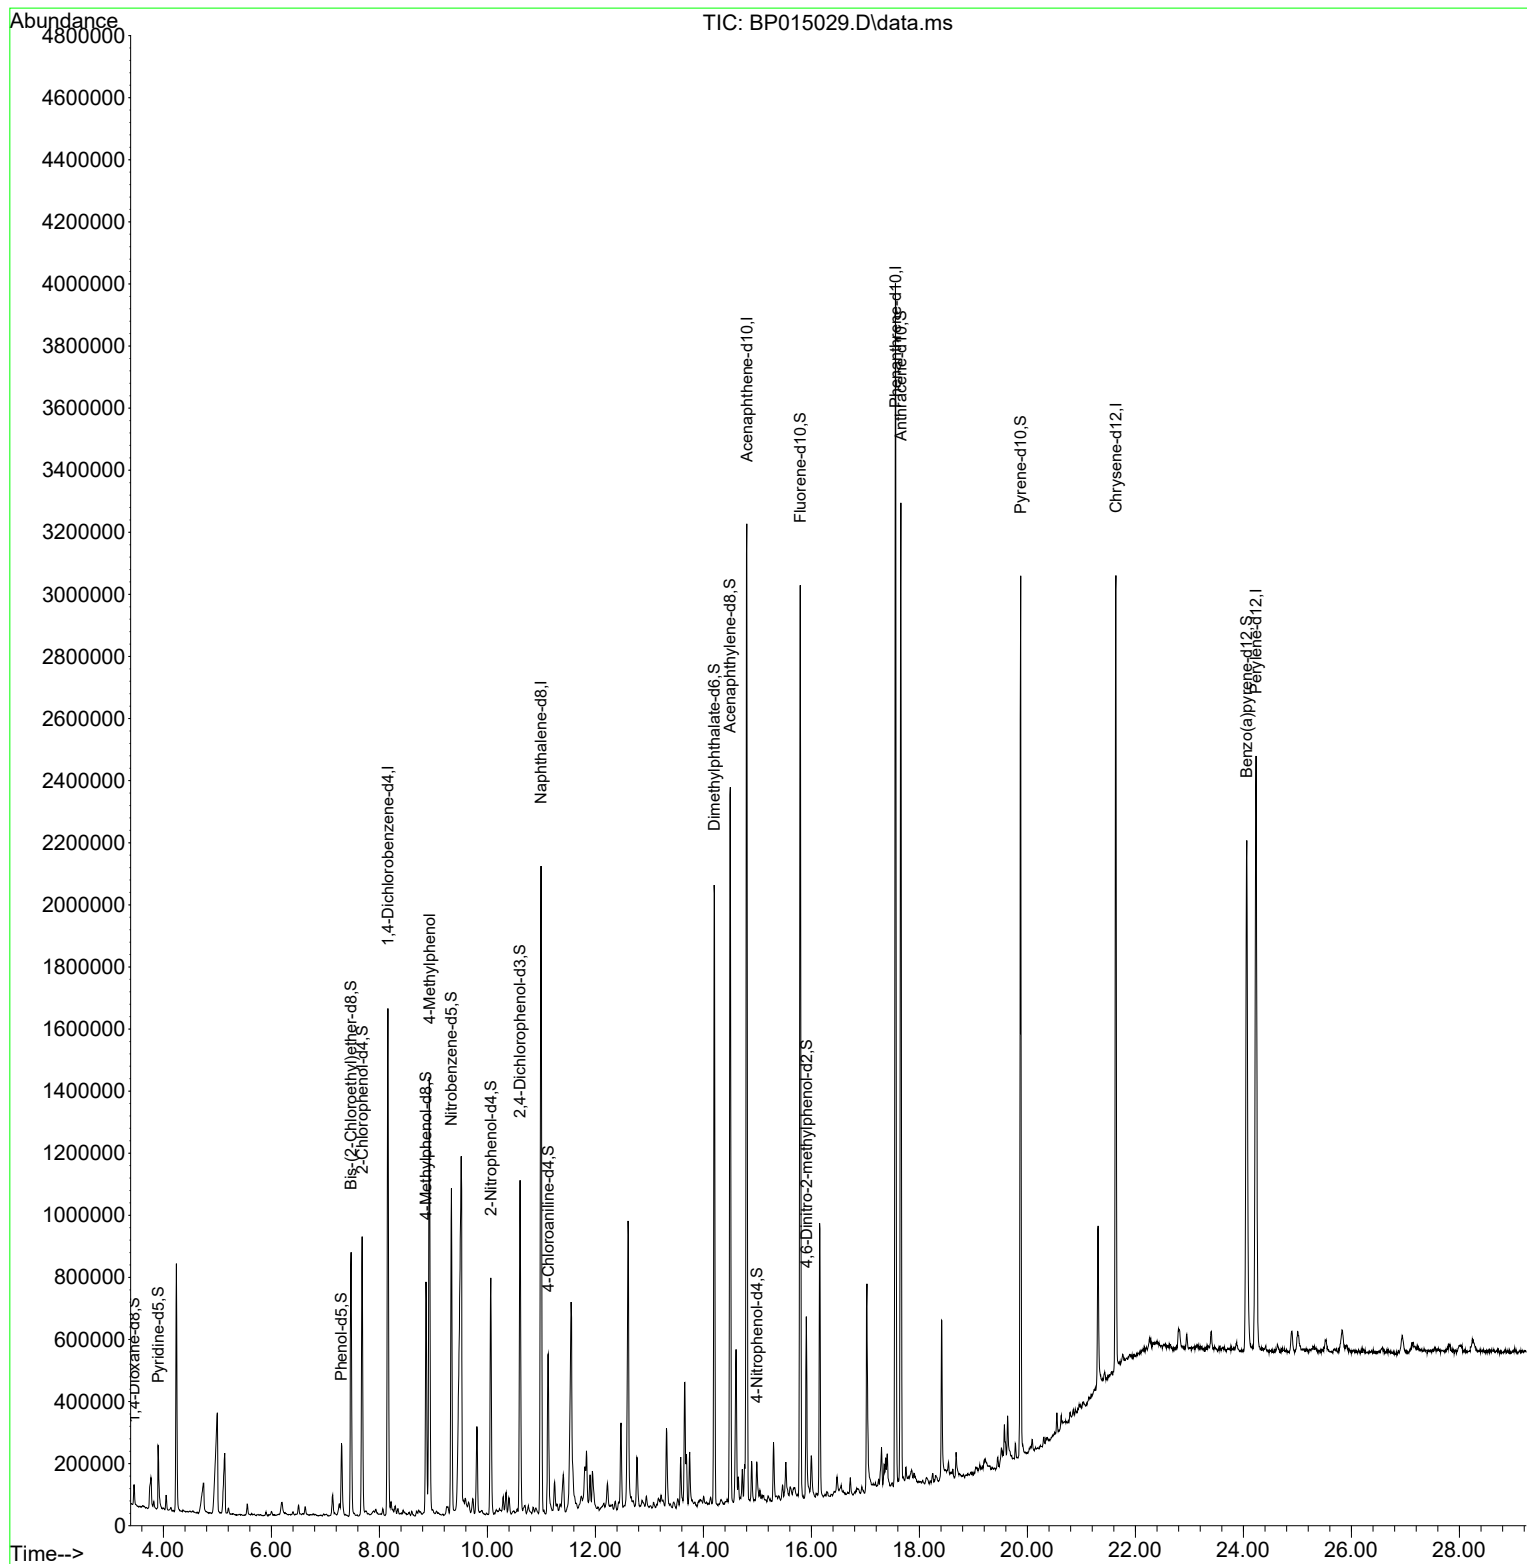

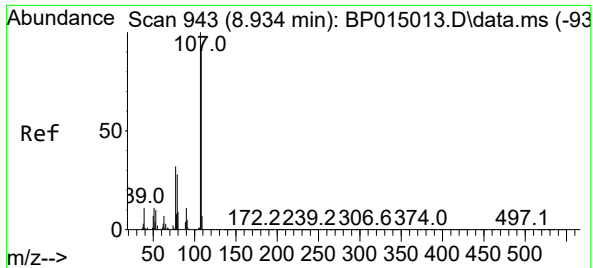

#18
 4-Methylphenol
 Concen: 17.238 ng/ul
 RT: 8.928 min Scan# 94
 Delta R.T. -0.012 min
 Lab File: BP015029.D
 Acq: 09 May 2023 21:27

Instrument :
 BNA_P
 ClientSampleId :
 JREK9

Tgt Ion:108 Resp: 562816
 Ion Ratio Lower Upper
 108 100
 107 120.9 87.2 130.8

