

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
 Data File : BP015014.D
 Acq On : 09 May 2023 10:23
 Operator : CG/JU
 Sample : PB152664BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	8	12	23	rVB	81026	124160	1.62%	0.162%
2	3.899	85	87	110	rBV	474756	767370	10.03%	1.002%
3	4.240	141	145	150	rBV	17968	24649	0.32%	0.032%
4	7.305	659	666	680	rBV	1233709	1981660	25.91%	2.587%
5	7.481	689	696	710	rBV	1071389	1657297	21.67%	2.164%
6	7.687	724	731	744	rBV	1257808	1996236	26.10%	2.606%
7	8.163	803	812	822	rBV	1083108	1716400	22.45%	2.241%
8	8.869	924	932	949	rBV	1438533	2424106	31.70%	3.165%
9	9.340	1004	1012	1026	rBV	1114635	1863701	24.37%	2.433%
10	10.069	1129	1136	1147	rBV	925413	1559420	20.39%	2.036%
11	10.610	1220	1228	1252	rBV	1423251	2487055	32.52%	3.247%
12	10.999	1286	1294	1304	rBV	1606706	2757941	36.07%	3.600%
13	11.134	1310	1317	1333	rBV	363268	662529	8.66%	0.865%
14	12.581	1555	1563	1573	rVB2	26067	45477	0.59%	0.059%
15	13.698	1747	1753	1761	rVV	33144	54391	0.71%	0.071%
16	13.787	1763	1768	1774	rBV8	4648	8848	0.12%	0.012%
17	14.210	1834	1840	1853	rBV	2614545	3732610	48.81%	4.873%
18	14.510	1882	1891	1906	rBV	3211243	4815162	62.97%	6.286%
19	14.816	1935	1943	1955	rBV	2669132	3992802	52.21%	5.212%
20	14.998	1967	1974	1995	rBV	1116783	1806997	23.63%	2.359%
21	15.216	2008	2011	2018	rVB8	7846	13347	0.17%	0.017%
22	15.804	2104	2111	2124	rBV	4457868	6310809	82.53%	8.238%
23	15.922	2124	2131	2143	rVV	1307953	1802847	23.58%	2.354%
24	16.045	2148	2152	2158	rVB2	21566	33014	0.43%	0.043%
25	17.357	2369	2375	2380	rBV3	8441	16615	0.22%	0.022%
26	17.575	2405	2412	2421	rBV	3563405	5145886	67.29%	6.718%
27	17.669	2422	2428	2446	rVB2	4829571	6886869	90.06%	8.991%
28	19.463	2730	2733	2740	rVB2	53918	71866	0.94%	0.094%
29	19.533	2741	2745	2749	rBV	52273	75324	0.99%	0.098%
30	19.792	2786	2789	2793	rBV5	22565	28366	0.37%	0.037%
31	19.892	2799	2806	2814	rBV	5553272	7647067	100.00%	9.983%
32	21.651	3100	3105	3119	rBV	3249612	4676321	61.15%	6.105%
33	24.092	3512	3520	3537	rVB2	2541626	5599228	73.22%	7.310%
34	24.263	3541	3549	3561	rVB2	1730109	3815138	49.89%	4.980%

Sum of corrected areas: 76601508




Instrument :
BNA_P
ClientSampleId :
SBLK664

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015014.D
Acq On : 09 May 2023 10:23
Operator : CG/JU
Sample : PB152664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

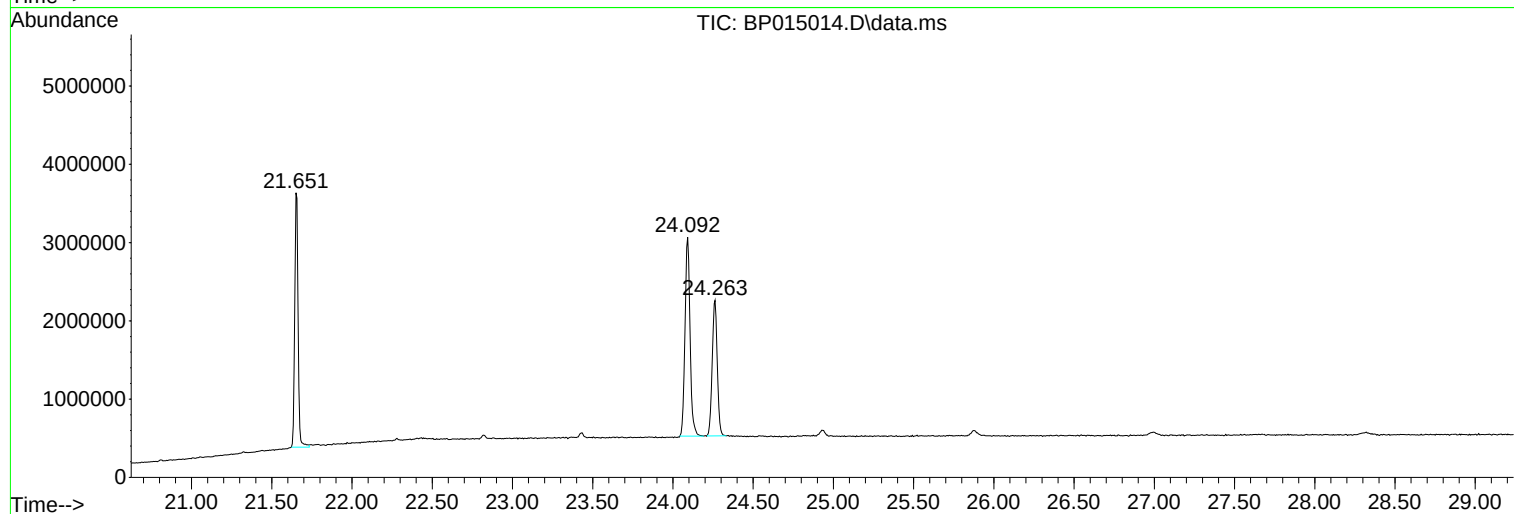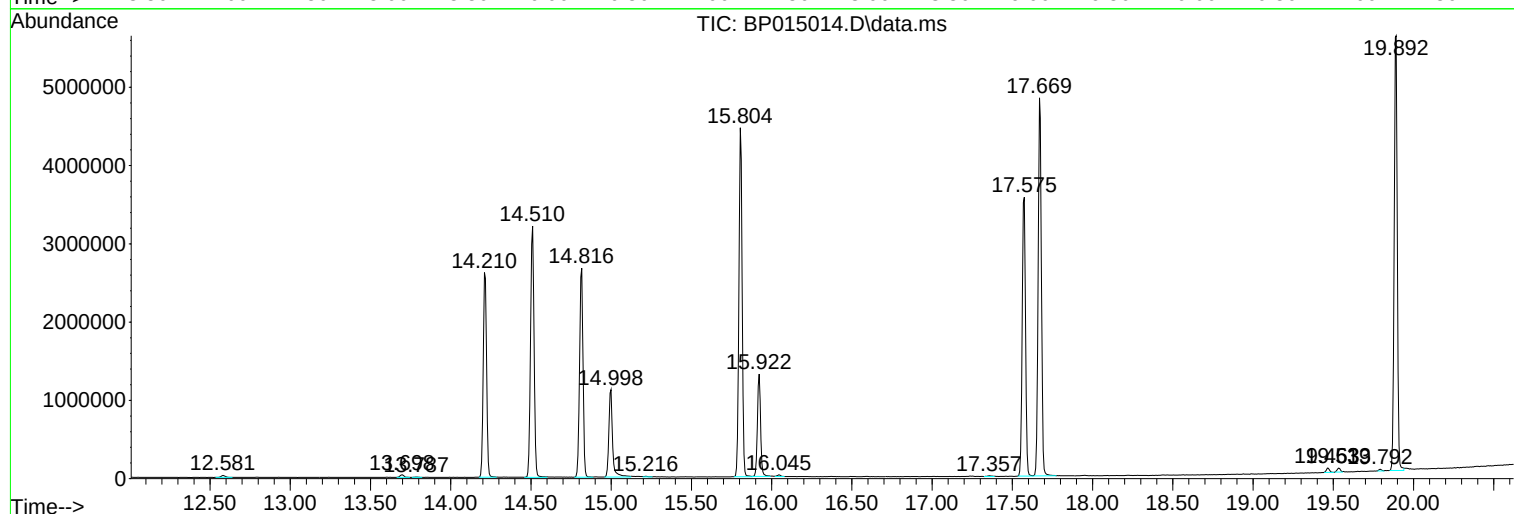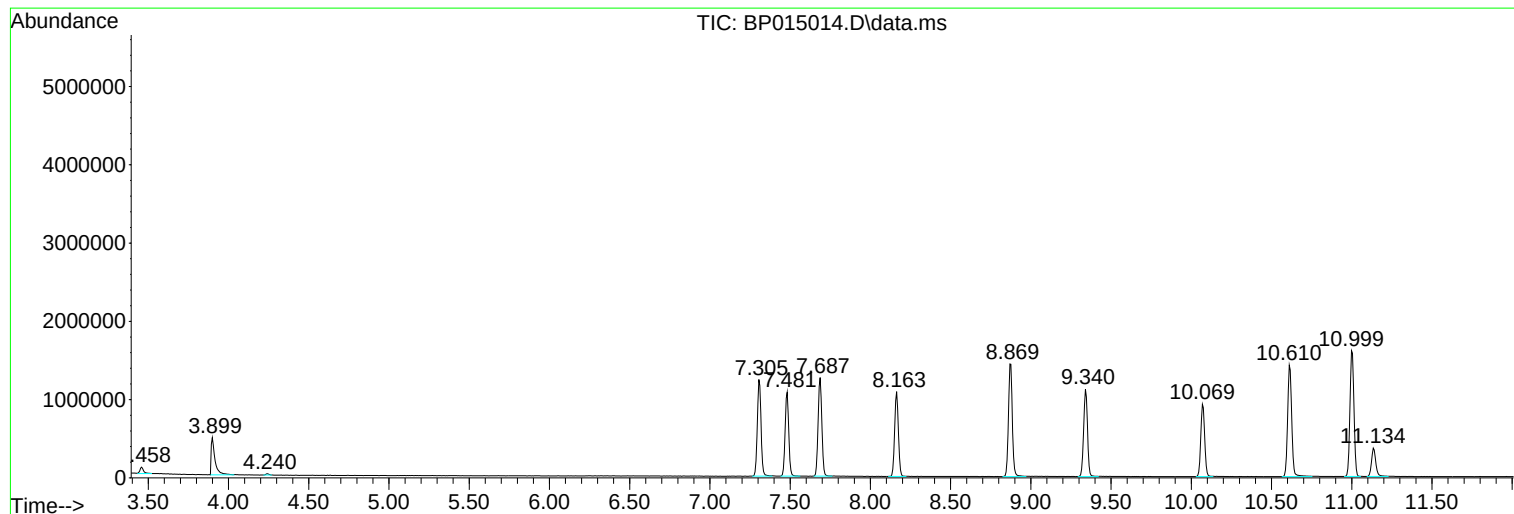

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015014.D
Acq On : 09 May 2023 10:23
Operator : CG/JU
Sample : PB152664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015014.D
Acq On : 09 May 2023 10:23
Operator : CG/JU
Sample : PB152664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK664

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc