

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
 Data File : BP015023.D
 Acq On : 09 May 2023 18:06
 Operator : CG/JU
 Sample : PB152682BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.458	7	12	18	rVB	71572	101423	1.47%	0.139%
2	3.893	83	86	101	rBV	424896	696771	10.08%	0.952%
3	4.240	141	145	149	rVB2	20705	28670	0.41%	0.039%
4	7.305	659	666	678	rBV	1094005	1799545	26.04%	2.458%
5	7.475	686	695	706	rBV	982107	1514506	21.92%	2.069%
6	7.681	722	730	739	rBV	1168241	1841139	26.64%	2.515%
7	8.158	803	811	820	rBV	1113201	1759343	25.46%	2.403%
8	8.869	924	932	946	rBV	1422674	2375045	34.37%	3.244%
9	9.334	1003	1011	1024	rBV	1129743	1842995	26.67%	2.517%
10	10.063	1126	1135	1146	rBV	932523	1574335	22.78%	2.150%
11	10.605	1219	1227	1242	rBV	1409171	2437650	35.28%	3.330%
12	10.993	1285	1293	1306	rBV	1730626	2898600	41.95%	3.959%
13	11.128	1308	1316	1332	rBV	760497	1372896	19.87%	1.875%
14	12.575	1555	1562	1569	rBV	23387	47209	0.68%	0.064%
15	13.687	1745	1751	1755	rBV7	5372	8975	0.13%	0.012%
16	13.775	1761	1766	1773	rBV5	4555	8739	0.13%	0.012%
17	14.204	1831	1839	1853	rBV	2722139	3704613	53.61%	5.060%
18	14.498	1881	1889	1904	rBV	3106148	4625509	66.94%	6.318%
19	14.804	1934	1941	1950	rBV	2809759	4124943	59.69%	5.634%
20	14.987	1964	1972	1989	rBV	1140652	1795476	25.98%	2.452%
21	15.210	2006	2010	2014	rVB7	5370	9534	0.14%	0.013%
22	15.798	2102	2110	2122	rBV	3840599	5606661	81.14%	7.658%
23	15.910	2123	2129	2145	rVV	1200994	1626356	23.54%	2.221%
24	16.040	2145	2151	2156	rVB3	17903	31997	0.46%	0.044%
25	16.487	2222	2227	2232	rBV9	4443	8018	0.12%	0.011%
26	16.581	2239	2243	2248	rBV6	4812	8230	0.12%	0.011%
27	17.234	2350	2354	2360	rVB8	6804	11016	0.16%	0.015%
28	17.345	2370	2373	2378	rVB2	7605	10599	0.15%	0.014%
29	17.563	2403	2410	2419	rBV	3439533	4967970	71.89%	6.786%
30	17.663	2420	2427	2440	rVV	4243142	6135261	88.79%	8.380%
31	18.204	2516	2519	2523	rBV6	4483	7867	0.11%	0.011%
32	19.457	2728	2732	2738	rBV2	62293	84611	1.22%	0.116%
33	19.522	2740	2743	2752	rVB	51862	79348	1.15%	0.108%
34	19.781	2785	2787	2791	rBV5	19491	20273	0.29%	0.028%
35	19.880	2798	2804	2814	rBV	5206177	6910090	100.00%	9.438%
36	21.645	3098	3104	3113	rBV	3225424	4485104	64.91%	6.126%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015023.D
Acq On : 09 May 2023 18:06
Operator : CG/JU
Sample : PB152682BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Title : SVOA CALIBRATION

37	24.074	3509	3517	3533	rVB2	2315025	5023842	72.70%	6.862%
38	24.245	3539	3546	3555	rVB2	1675997	3628296	52.51%	4.956%




Sum of corrected areas: 73213455

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015023.D
Acq On : 09 May 2023 18:06
Operator : CG/JU
Sample : PB152682BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

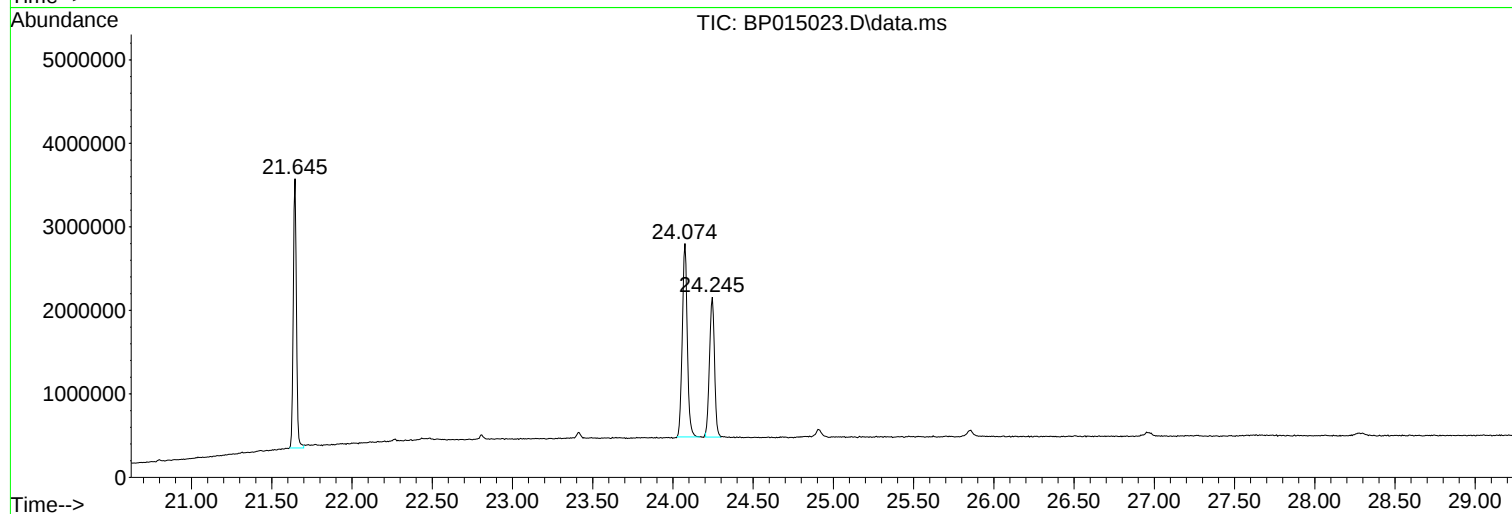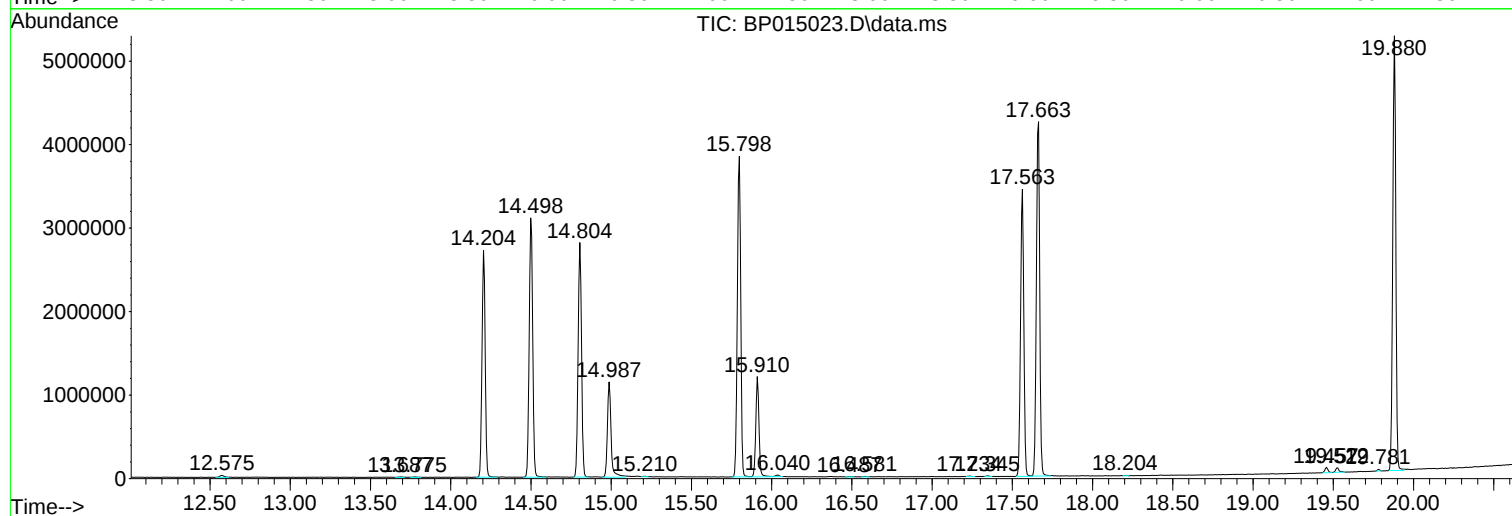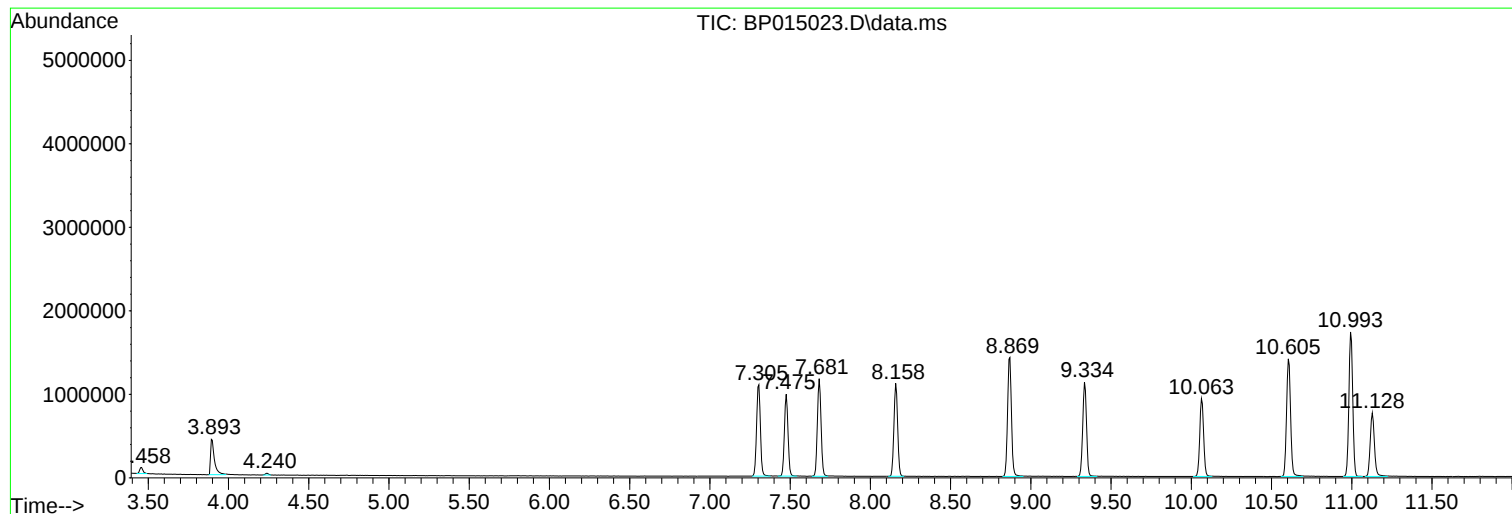

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015023.D
Acq On : 09 May 2023 18:06
Operator : CG/JU
Sample : PB152682BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050923\
Data File : BP015023.D
Acq On : 09 May 2023 18:06
Operator : CG/JU
Sample : PB152682BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------