


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050925\
Data File : BP024584.D
Acq On : 09 May 2025 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 09 12:07:46 2025

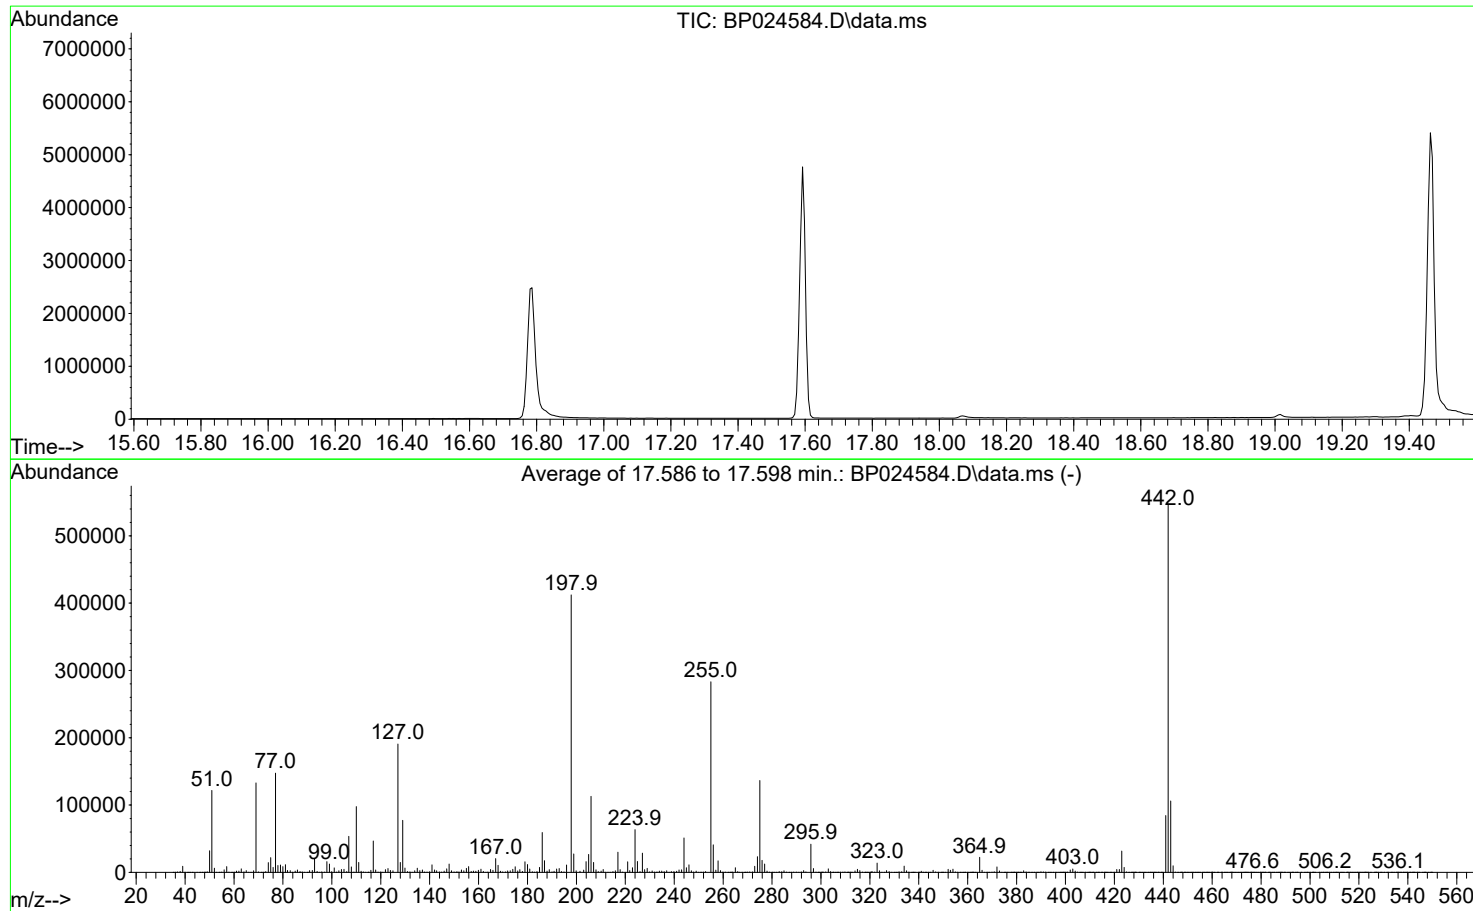

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	121657	PASS
68	69	0.00	2	1.9	2496	PASS
69	198	0.00	100	32.2	132894	PASS
70	69	0.00	2	0.5	656	PASS
127	198	10	80	46.3	190656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	412157	PASS
199	198	5	9	6.7	27483	PASS
275	198	10	60	33.1	136474	PASS
365	198	1	100	5.4	22291	PASS
441	198	0.01	100	20.5	84309	PASS
442	442	100	100	100.0	546560	PASS
443	442	15	24	19.4	106138	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/9/2025	BNA_P	<u>BP024584.D</u>
Compound Name	Response	Retention Time
DDT	1549241	20.745
DDD	31657	20.286
DDE	2730	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
34387	1583628	2.17

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050925\
Data File : BP024584.D
Acq On : 09 May 2025 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 09 11:27:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

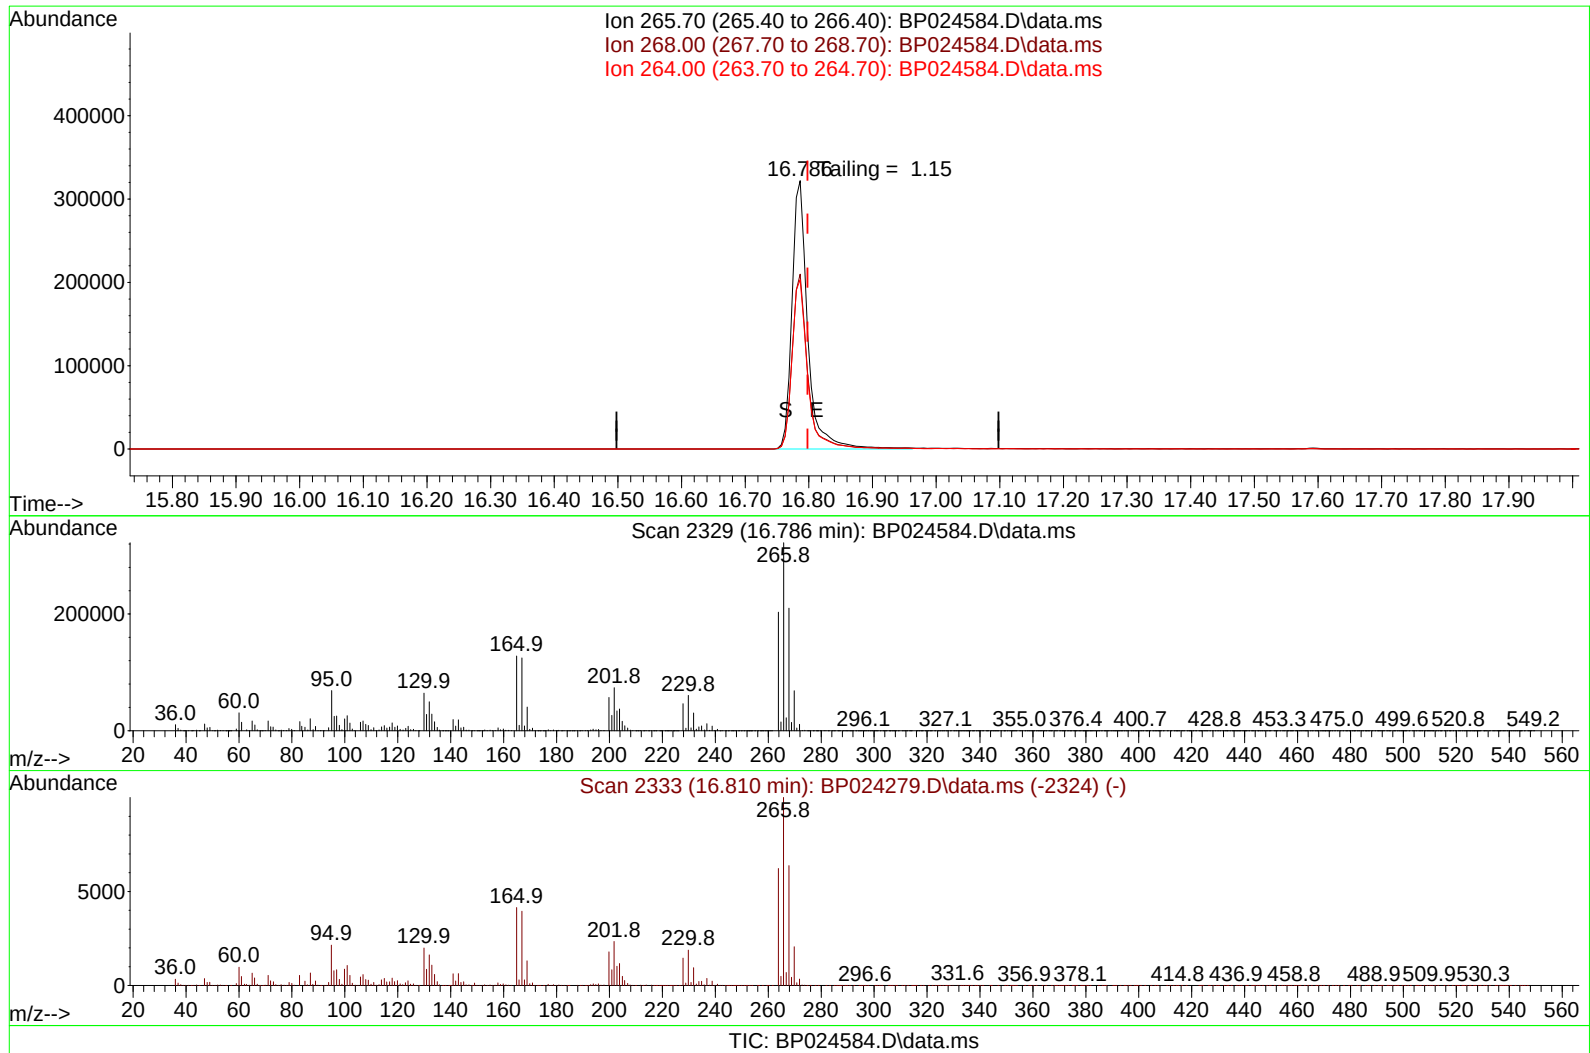

(70) Pentachlorophenol (C)

16.786min (-0.012) 40822.20 ng




response 557012

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.17
264.00	62.20	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP050925\
Data File : BP024584.D
Acq On : 09 May 2025 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 09 11:27:03 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP041425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 18 12:04:48 2025
Response via : Initial Calibration

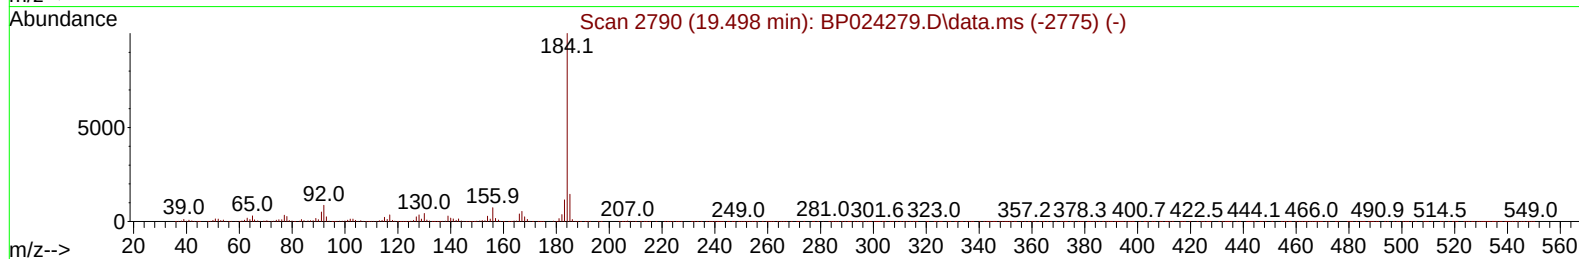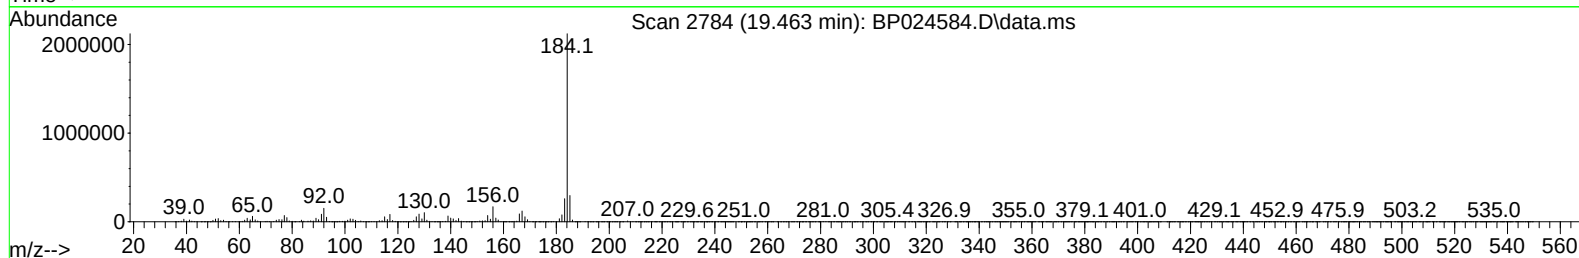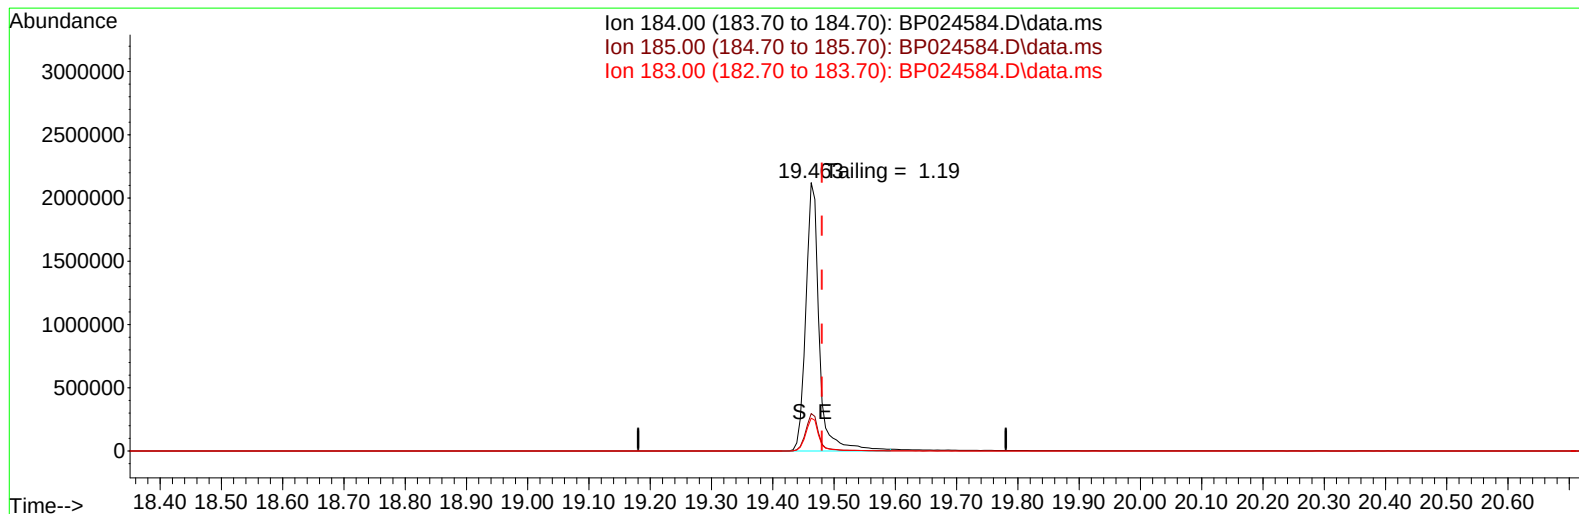

TIC: BP024584.D\data.ms

(77) Benzidine

19.463min (-0.018) 54705.75 ng

response 3284833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.94
183.00	11.50	12.24
0.00	0.00	0.00