
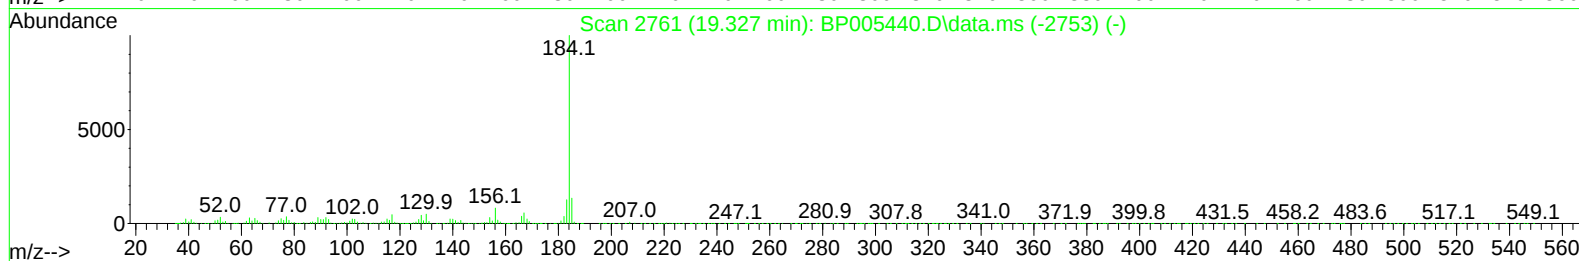
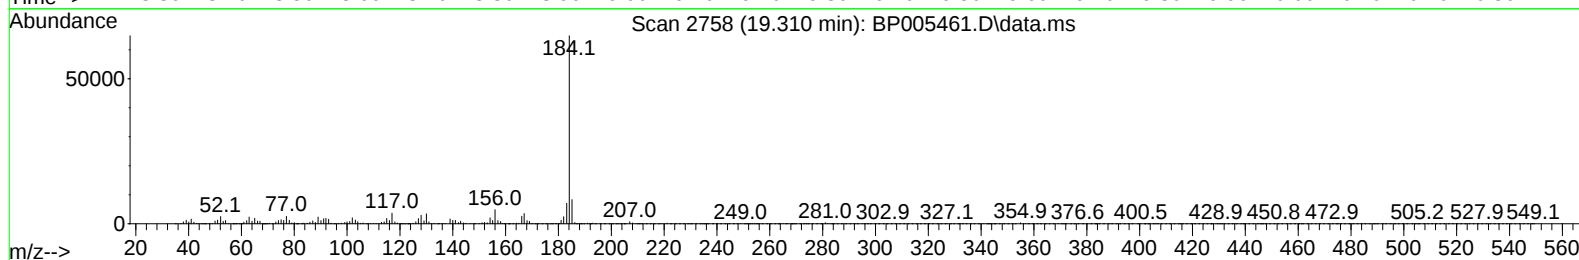


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
 Data File : BP005461.D
 Acq On : 10 May 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 11:00:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 07 12:37:06 2021
 Response via : Initial Calibration

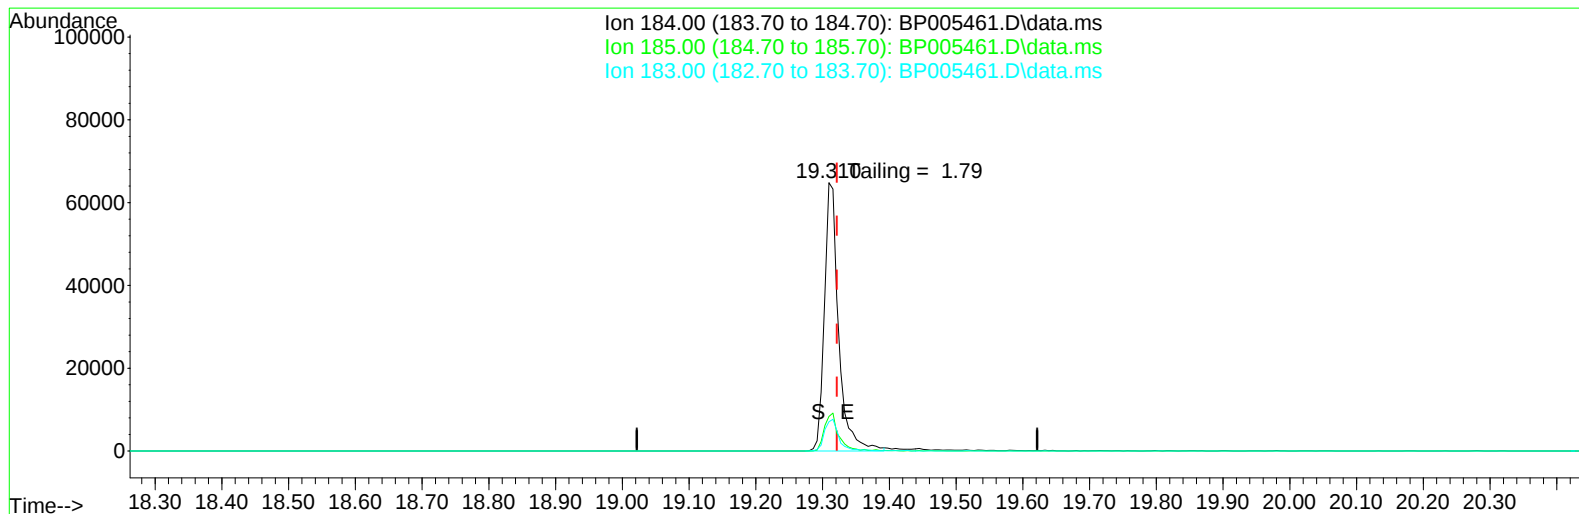




TIC: BP005461.D\data.ms

(77) Benzidine**19.310min (-0.012) 568889.99 ng****response 96863**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	12.89
183.00	12.30	10.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
Data File : BP005461.D
Acq On : 10 May 2021 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 11:00:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 12:37:06 2021
Response via : Initial Calibration

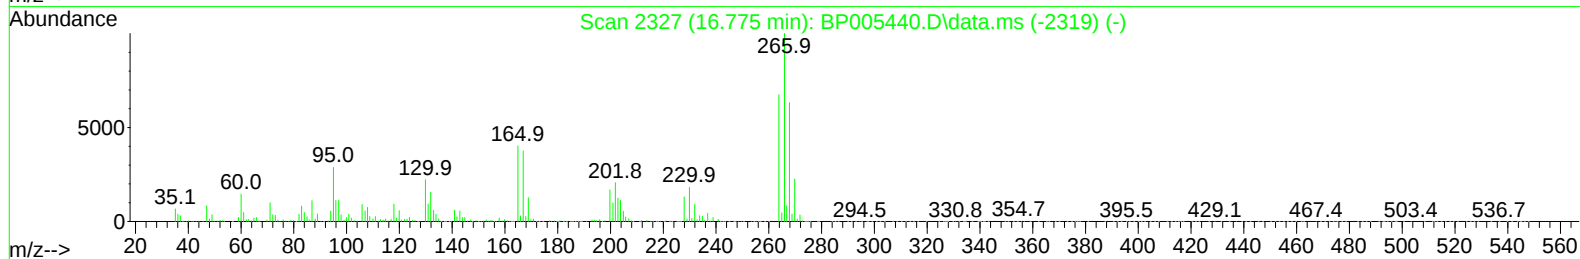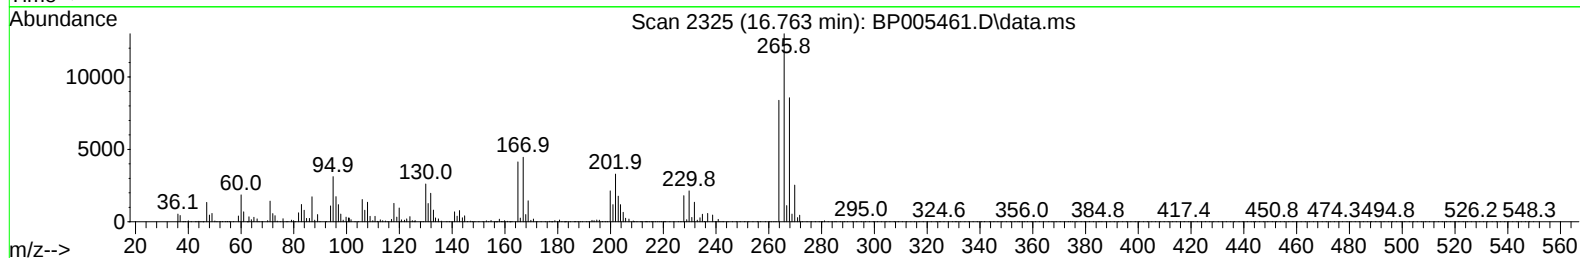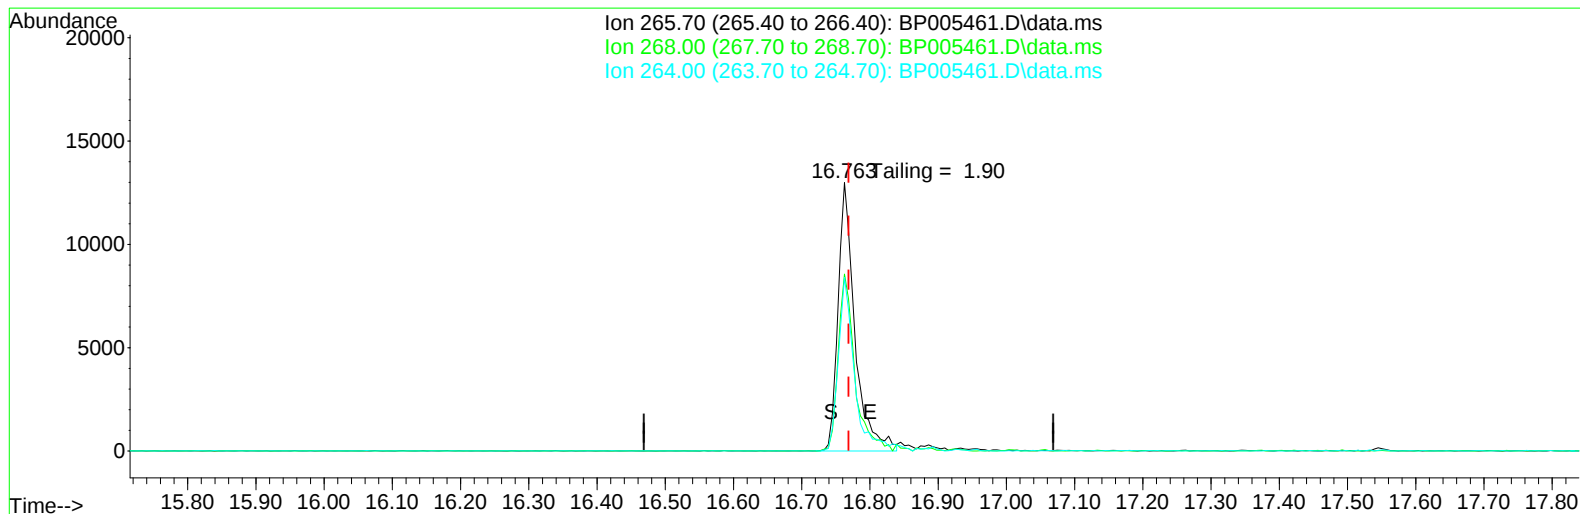

TIC: BP005461.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.006) 212280.63 ng

response 22297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.94
264.00	67.10	64.62
0.00	0.00	0.00