

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
 Data File : BP005468.D
 Acq On : 10 May 2021 14:54
 Operator : CG/JU
 Sample : M2330-01 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CFOS-SOIL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	15.134	2043	2048	2053	rBV2	681532	1066844	1.41%	0.250%
2	16.081	2205	2209	2220	rBV2	930775	2455569	3.25%	0.576%
3	16.392	2259	2262	2270	rVB	865333	1267335	1.68%	0.297%
4	16.504	2278	2281	2285	rVB	723007	885358	1.17%	0.208%
5	16.710	2312	2316	2323	rVB2	906974	1339319	1.77%	0.314%
6	17.022	2365	2369	2381	rVB	3709479	5183504	6.86%	1.215%
7	17.128	2382	2387	2392	rBV2	3057822	5277140	6.98%	1.237%
8	17.186	2393	2397	2404	rVB	2499882	3420935	4.52%	0.802%
9	17.292	2411	2415	2424	rBV	2619708	3691389	4.88%	0.865%
10	17.492	2444	2449	2453	rBV	4287727	5503074	7.28%	1.290%
11	17.798	2494	2501	2505	rBV	18327033	23550486	31.15%	5.522%
12	17.845	2505	2509	2510	rVV	3649451	4728785	6.25%	1.109%
13	17.863	2510	2512	2516	rVV	4392807	4996798	6.61%	1.172%
14	17.916	2517	2521	2527	rVB	5053559	6438275	8.52%	1.509%
15	18.022	2535	2539	2544	rBV	6102563	7510721	9.93%	1.761%
16	18.210	2566	2571	2576	rBV	13464270	18538012	24.52%	4.346%
17	18.404	2601	2604	2607	rBV2	888032	1092629	1.45%	0.256%
18	18.504	2612	2621	2624	rBV2	37820008	75607021	100.00%	17.727%
19	18.575	2630	2633	2641	rVB3	2277887	3655678	4.84%	0.857%
20	18.781	2664	2668	2670	rBV3	1932745	2944105	3.89%	0.690%
21	18.816	2671	2674	2678	rVB2	3184760	4456951	5.89%	1.045%
22	19.051	2710	2714	2717	rVB3	2641797	4030722	5.33%	0.945%
23	19.104	2718	2723	2726	rBV3	5392083	9917764	13.12%	2.325%
24	19.180	2733	2736	2740	rVV4	2248324	3320928	4.39%	0.779%
25	19.222	2740	2743	2746	rVB2	4313415	5340807	7.06%	1.252%
26	19.322	2755	2760	2763	rBV4	5587403	9560627	12.65%	2.242%
27	19.445	2777	2781	2784	rBV3	4890337	8535718	11.29%	2.001%
28	19.616	2806	2810	2812	rBV3	5186512	7490295	9.91%	1.756%
29	19.680	2818	2821	2825	rVB4	7262502	10327291	13.66%	2.421%
30	19.728	2825	2829	2831	rBV3	3896504	5079608	6.72%	1.191%
31	19.928	2859	2863	2866	rVB3	7226801	9223351	12.20%	2.162%
32	19.975	2867	2871	2873	rBV2	4744824	6704200	8.87%	1.572%
33	20.210	2908	2911	2914	rBV2	4991219	7164146	9.48%	1.680%
34	20.504	2957	2961	2966	rBV5	3993140	8401582	11.11%	1.970%
35	20.698	2990	2994	2996	rBV3	9511952	14113248	18.67%	3.309%
36	21.033	3048	3051	3058	rVB5	6531627	14025612	18.55%	3.288%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
 Data File : BP005468.D
 Acq On : 10 May 2021 14:54
 Operator : CG/JU
 Sample : M2330-01 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CFOS-SOIL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.098	3058	3062	3068	rBV5	10772441	24511880	32.42%	5.747%
38	21.145	3068	3070	3073	rVB2	7251797	7294466	9.65%	1.710%
39	21.192	3074	3078	3080	rBV	6088672	8144481	10.77%	1.910%
40	21.280	3090	3093	3094	rBV2	4707813	5177414	6.85%	1.214%
41	21.386	3107	3111	3119	rVB5	5998132	13527109	17.89%	3.172%
42	21.457	3119	3123	3126	rBV3	5643131	8471080	11.20%	1.986%
43	21.722	3163	3168	3173	rVB4	3199213	6683586	8.84%	1.567%
44	21.810	3180	3183	3192	rVB5	3110504	7271470	9.62%	1.705%
45	21.898	3193	3198	3202	rBV2	4680091	8037176	10.63%	1.884%
46	21.933	3202	3204	3208	rVB	2691276	2803701	3.71%	0.657%
47	21.980	3208	3212	3214	rBV	2387898	3621242	4.79%	0.849%
48	22.051	3222	3224	3227	rVV	1672038	1514040	2.00%	0.355%
49	22.086	3228	3230	3240	rVB3	2789296	5665893	7.49%	1.328%
50	22.180	3241	3246	3257	rVB3	2821427	6946021	9.19%	1.629%
51	22.374	3274	3279	3285	rBV3	2890722	4730351	6.26%	1.109%
52	22.616	3317	3320	3325	rVB	1130310	1436567	1.90%	0.337%
53	22.686	3328	3332	3342	rVB	1649050	2863518	3.79%	0.671%
54	23.039	3388	3392	3400	rVB4	431987	972286	1.29%	0.228%


Sum of corrected areas: 426518108

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
Data File : BP005468.D
Acq On : 10 May 2021 14:54
Operator : CG/JU
Sample : M2330-01 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CFOS-SOIL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

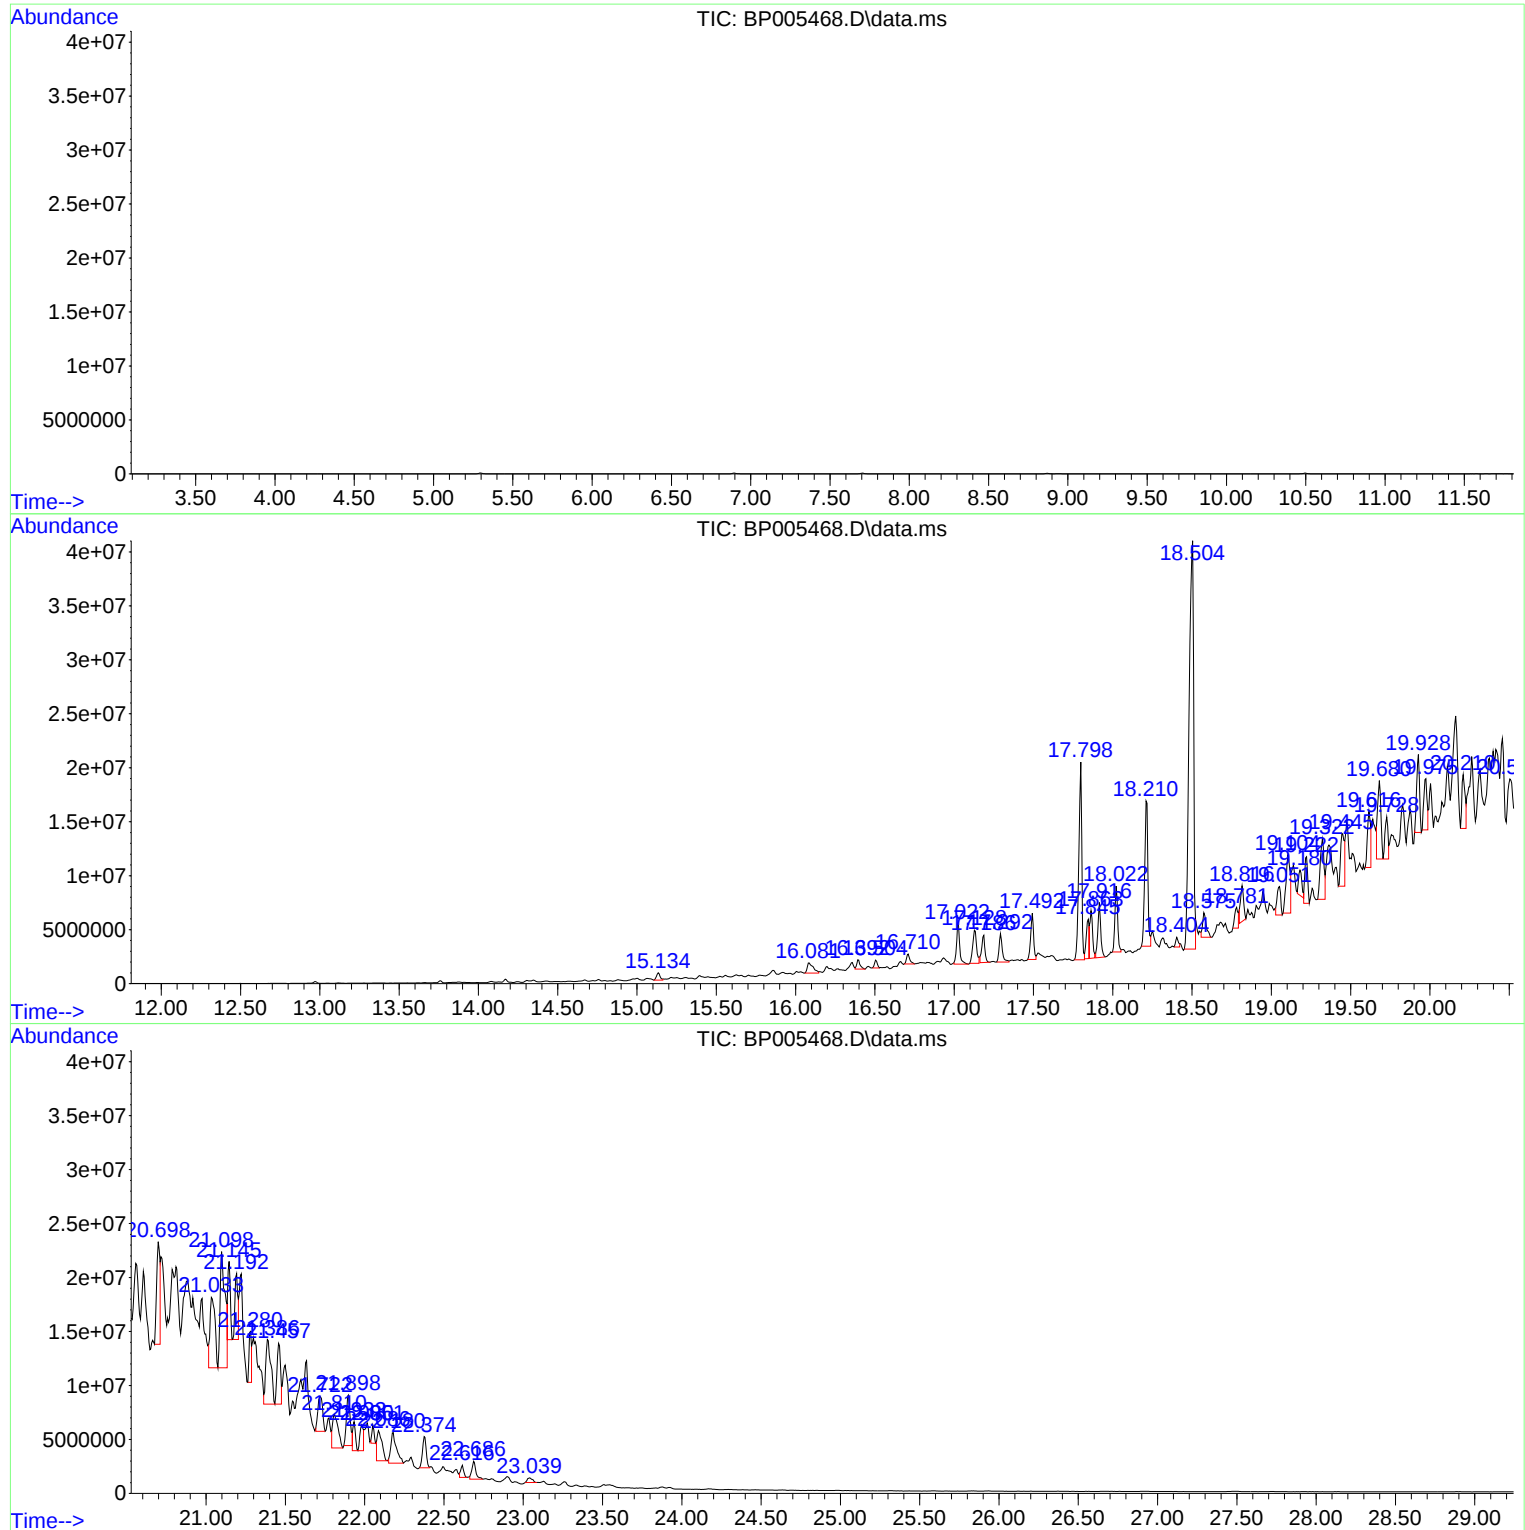

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
Data File : BP005468.D
Acq On : 10 May 2021 14:54
Operator : CG/JU
Sample : M2330-01 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CFOS-SOIL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
Data File : BP005468.D
Acq On : 10 May 2021 14:54
Operator : CG/JU
Sample : M2330-01 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CFOS-SOIL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc