
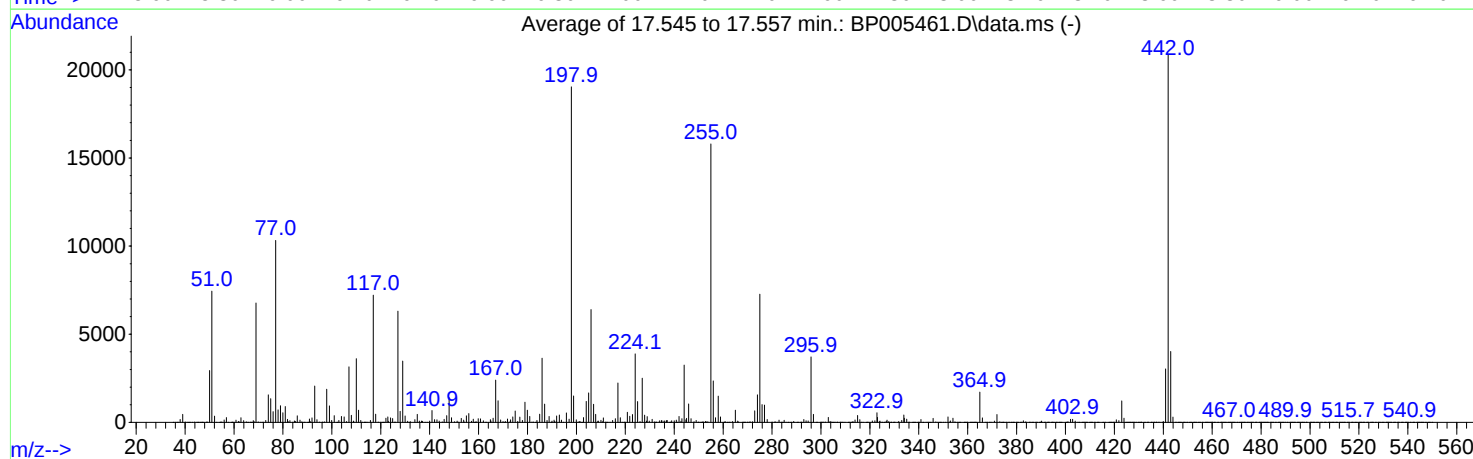


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
 Data File : BP005461.D
 Acq On : 10 May 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 11 11:20:59 2021

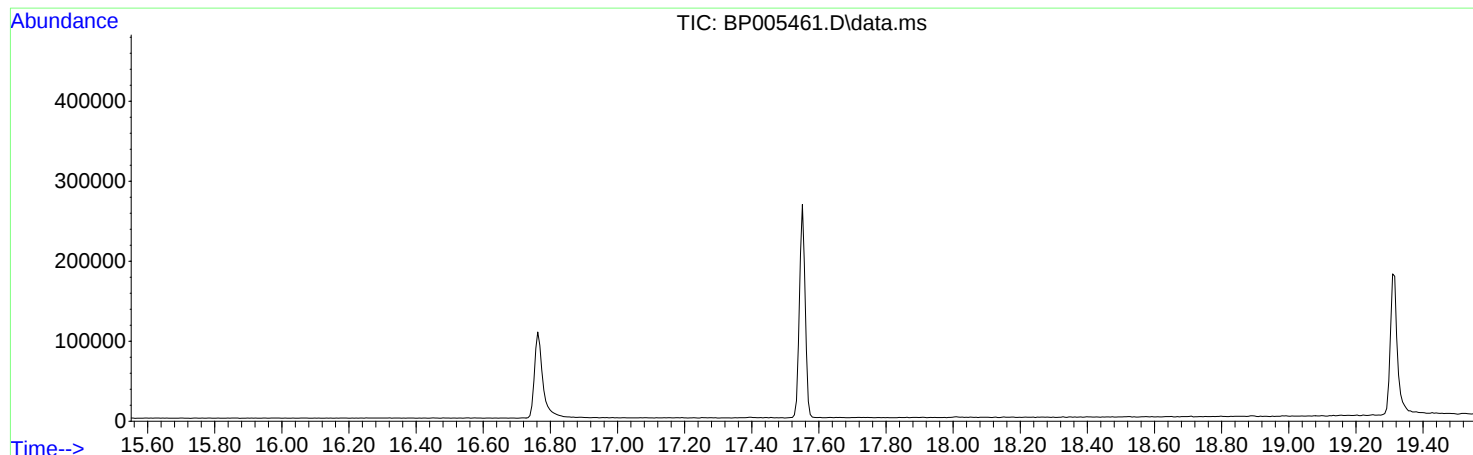




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	7443	PASS
68	69	0.00	2	1.5	101	PASS
69	198	0.00	100	35.6	6775	PASS
70	69	0.00	2	0.4	29	PASS
127	198	10	80	33.2	6313	PASS
197	198	0.00	2	1.0	183	PASS
198	198	100	100	100.0	19040	PASS
199	198	5	9	7.9	1499	PASS
275	198	10	60	38.2	7274	PASS
365	198	1	100	9.0	1713	PASS
441	198	0.01	100	15.9	3031	PASS
442	442	100	100	100.0	20870	PASS
443	442	15	24	19.3	4020	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
 Data File : BP005461.D
 Acq On : 10 May 2021 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 10 11:00:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 07 12:37:06 2021
 Response via : Initial Calibration

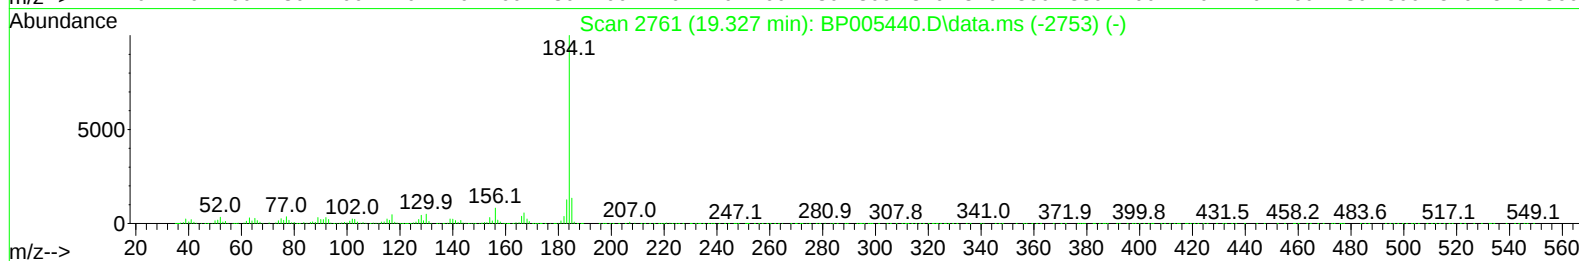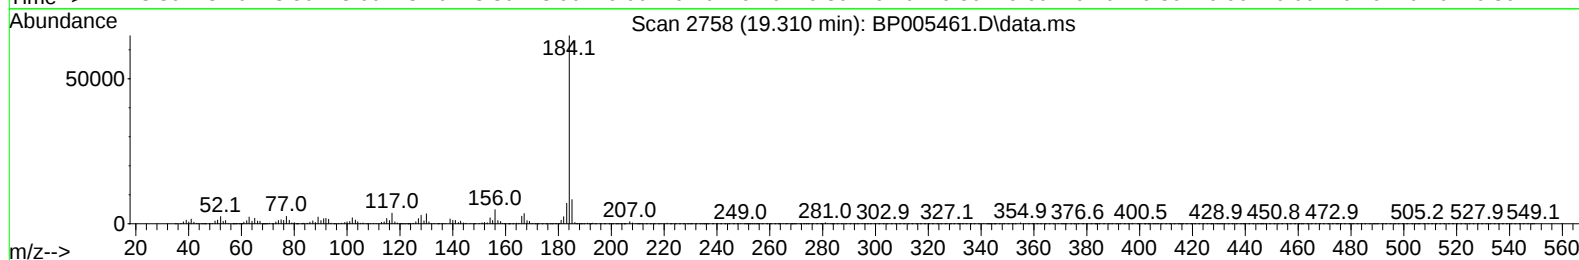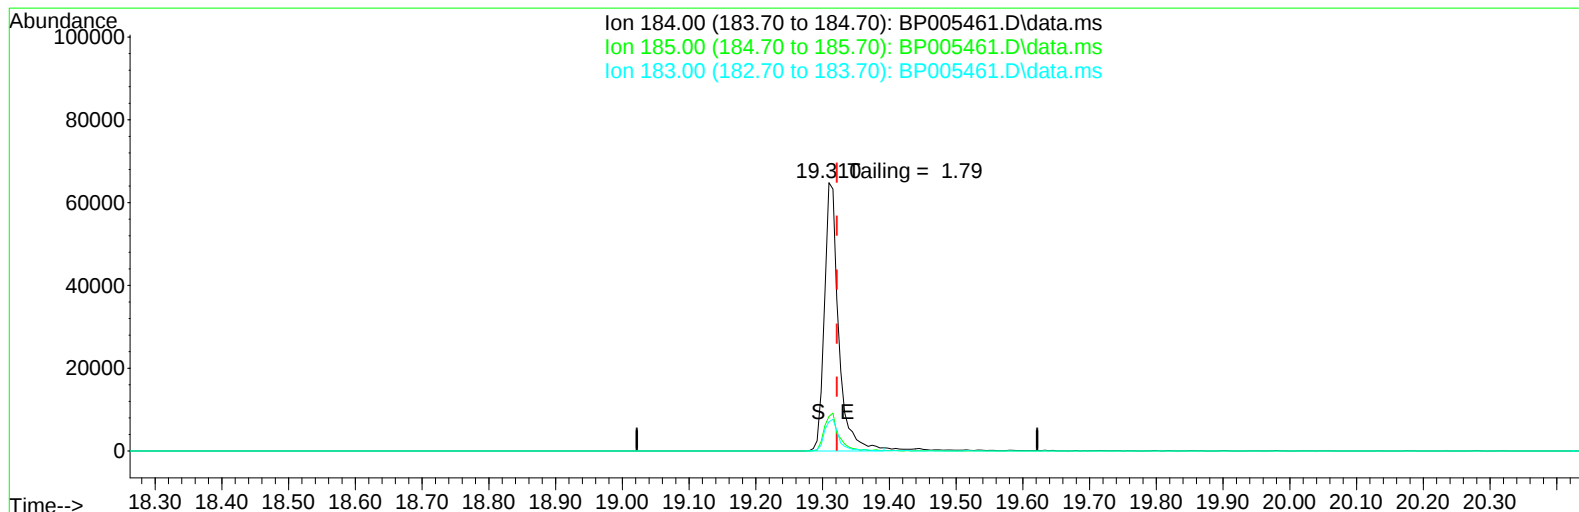

TIC: BP005461.D\data.ms

(77) Benzidine

19.310min (-0.012) 568889.99 ng




response 96863

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	12.89
183.00	12.30	10.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051021\
Data File : BP005461.D
Acq On : 10 May 2021 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 10 11:00:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 12:37:06 2021
Response via : Initial Calibration

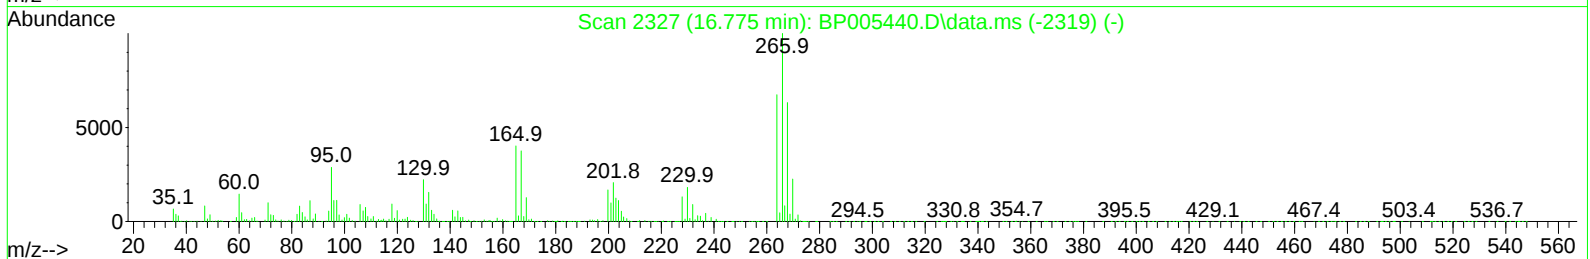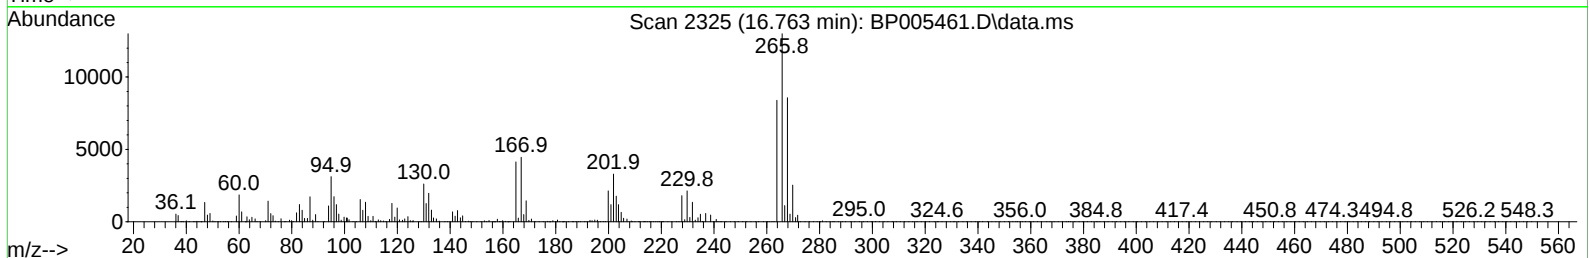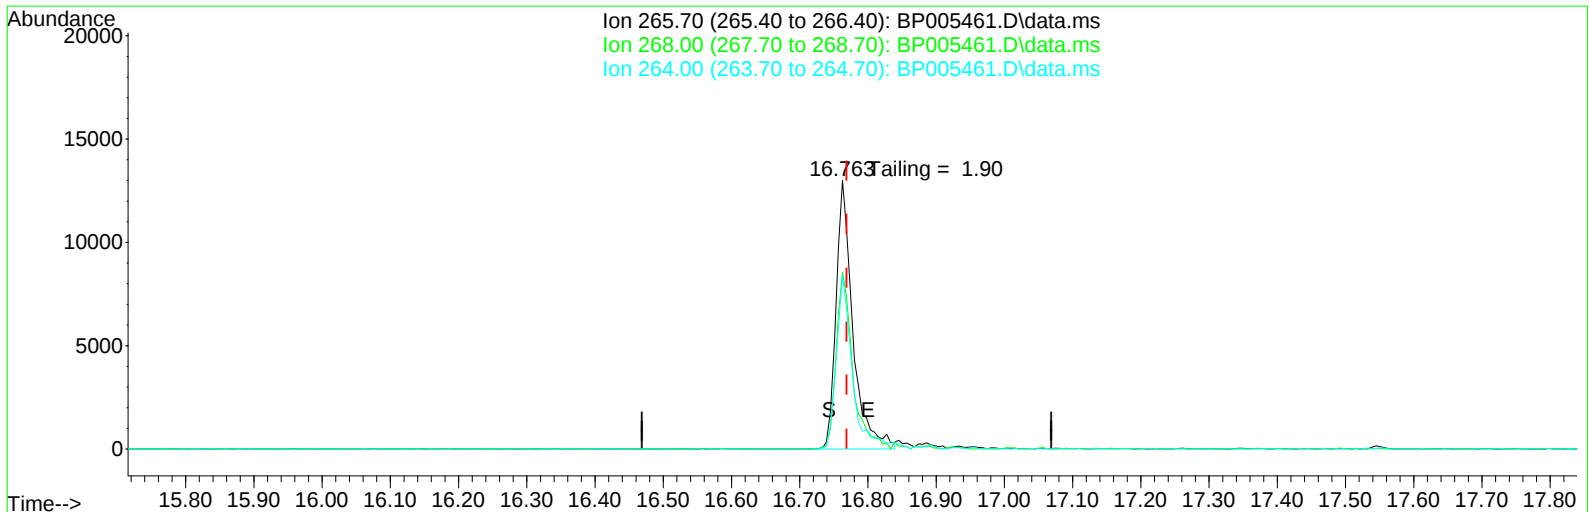

TIC: BP005461.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.006) 212280.63 ng

response 22297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	65.94
264.00	67.10	64.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2021	BNA_P	<u>BP005461.D</u>
Compound Name	Response	Retention Time
DDT	79710	20.5
DDD	626	20.08
DDE	239	19.57
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
865	80575	1.07