




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

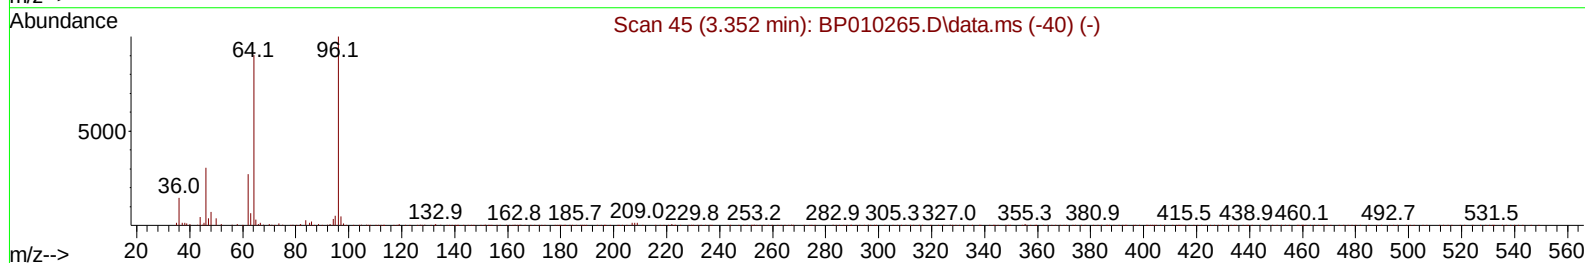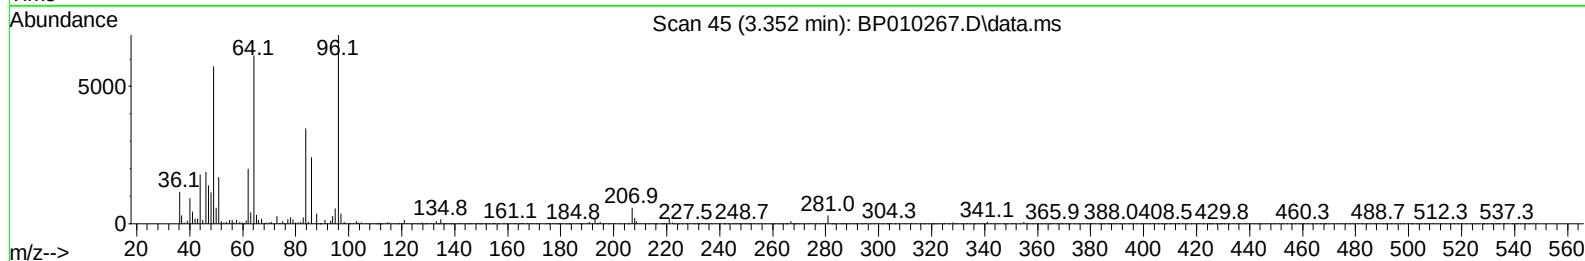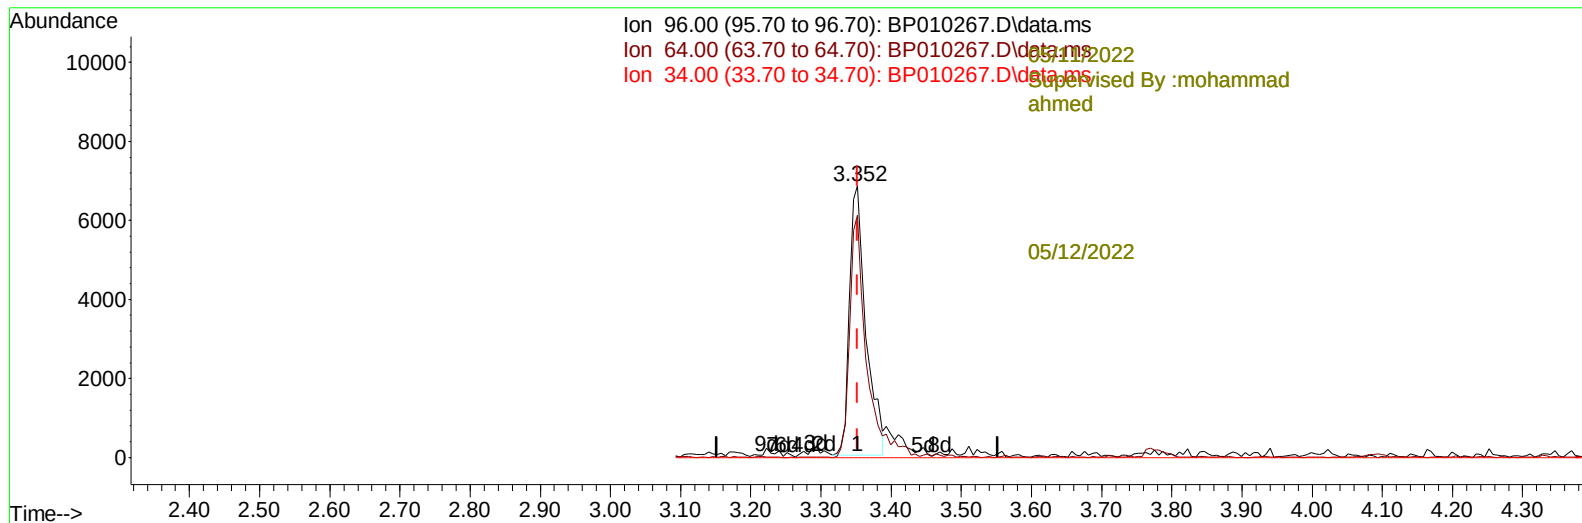

TIC: BP010267.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.26 ng/uL

response 11264

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	89.29#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

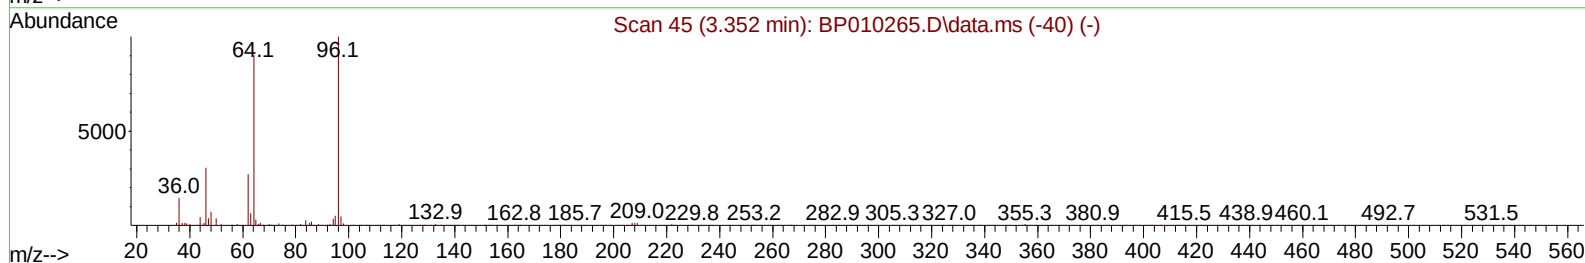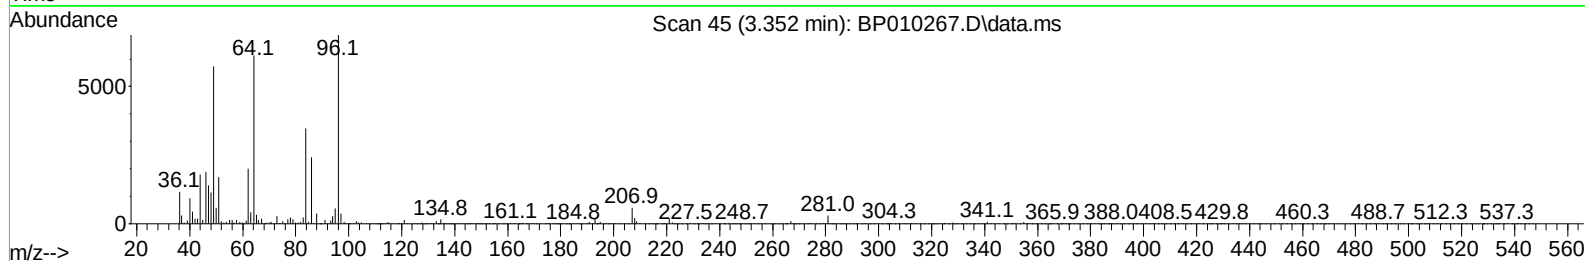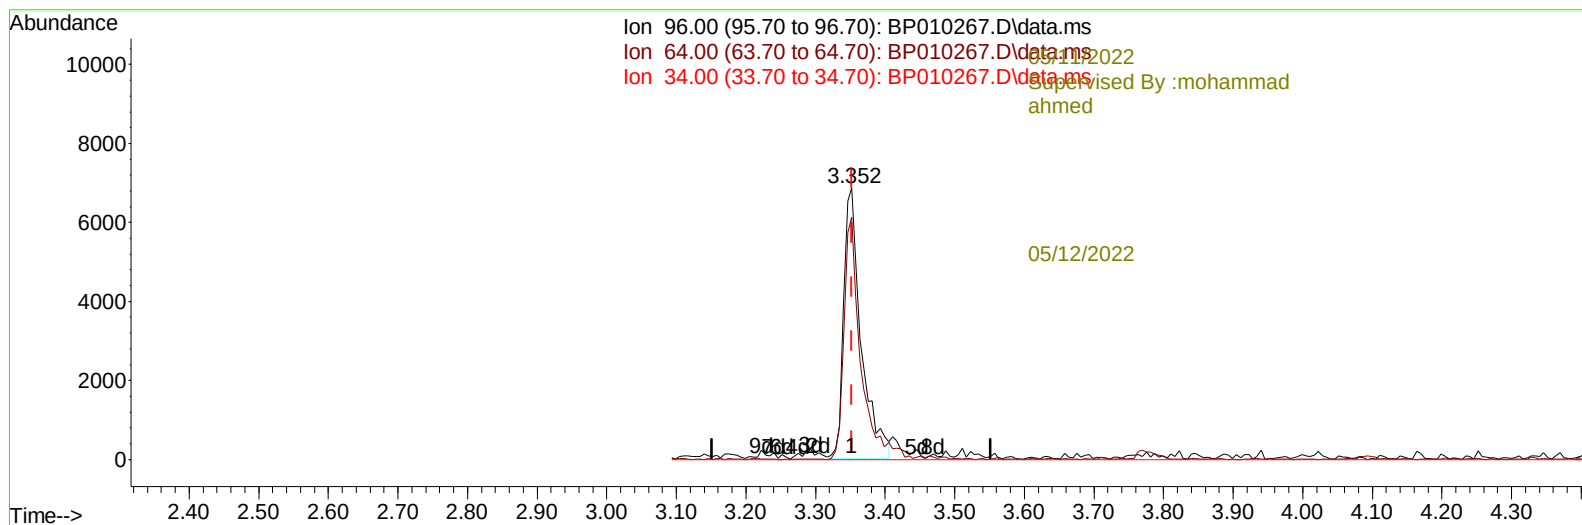

TIC: BP010267.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.60 ng/uL m

response 11985

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	89.29#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

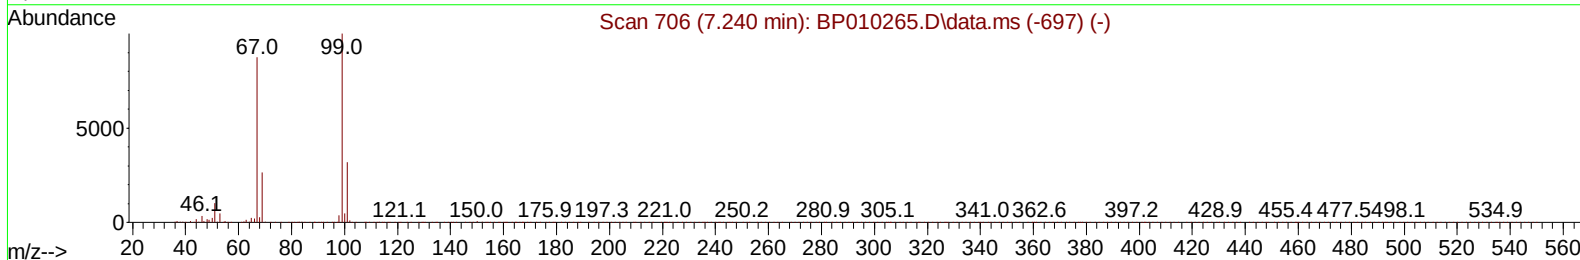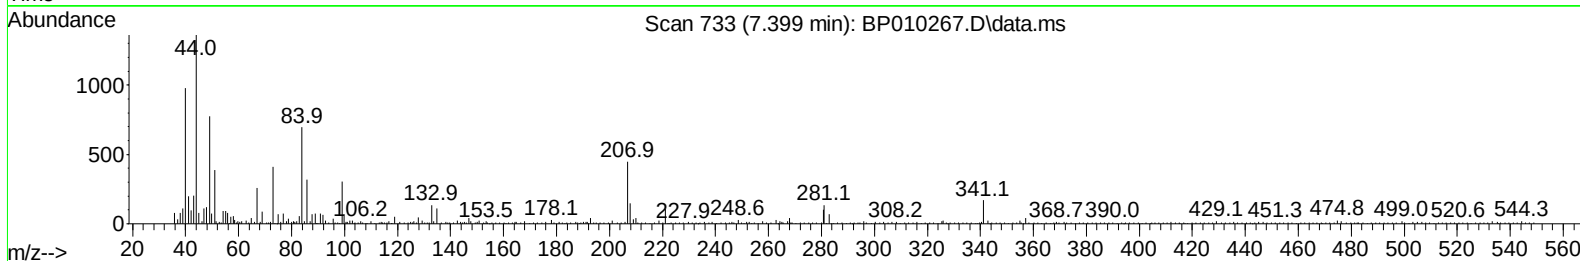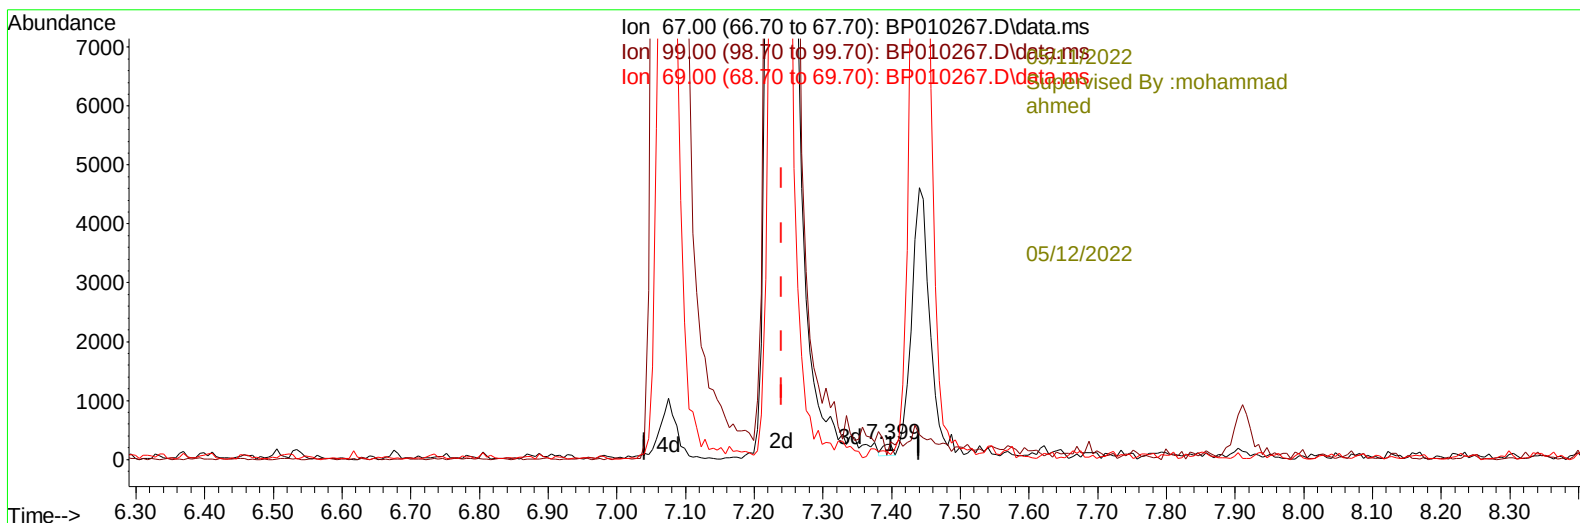

TIC: BP010267.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.399min (+ 0.159) 0.04 ng/uI

response 187

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	144.19
69.00	40.10	33.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

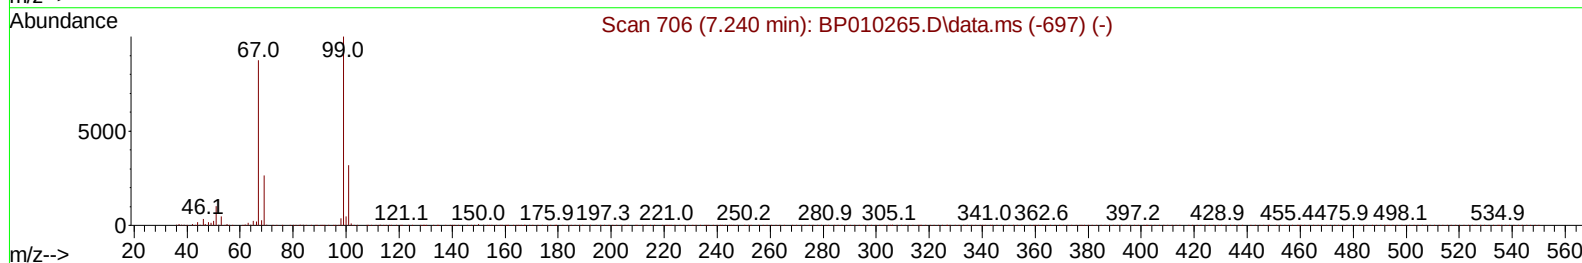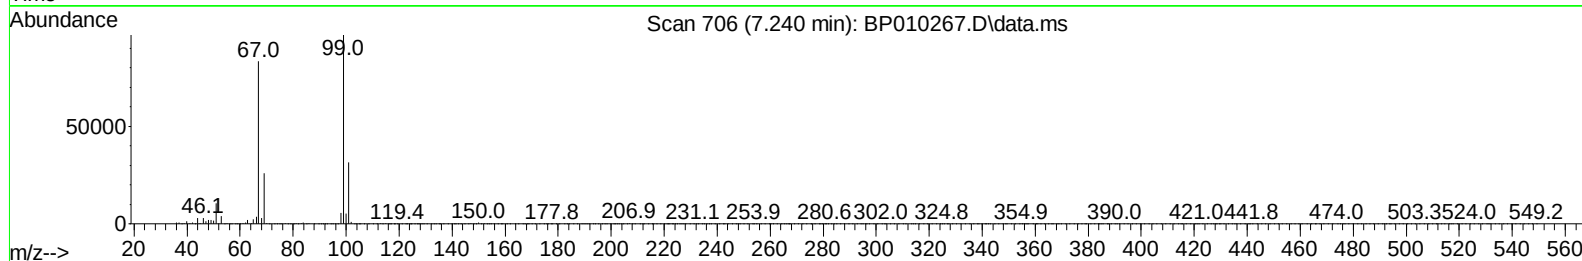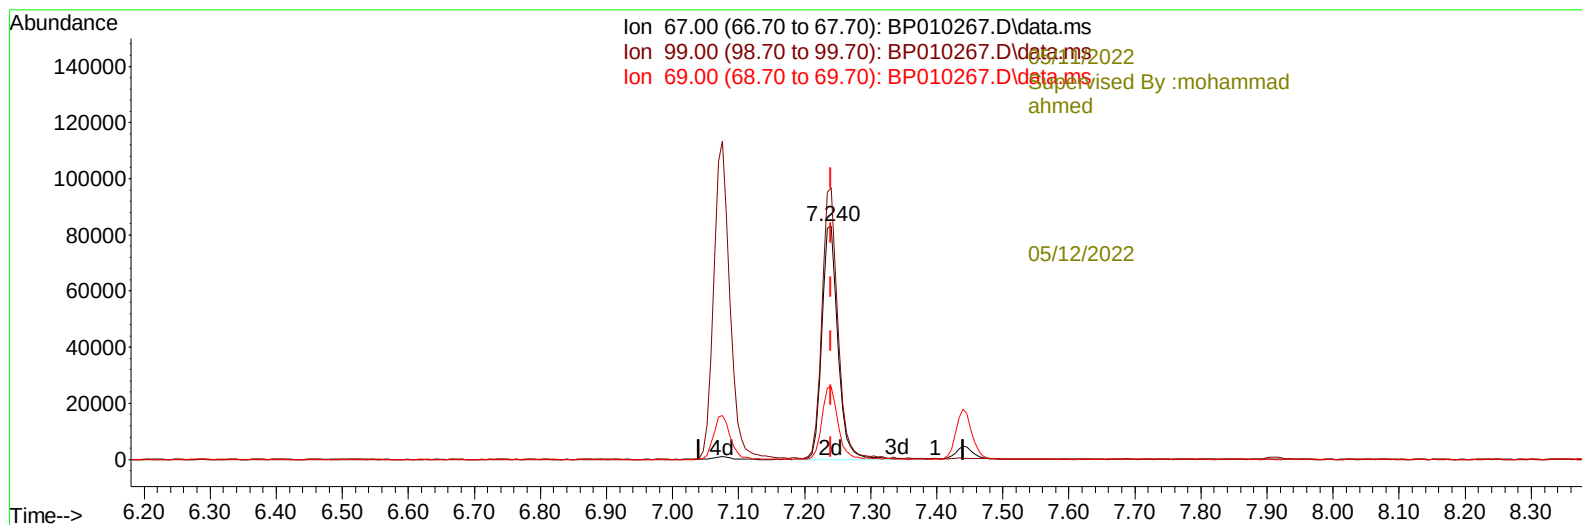

TIC: BP010267.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.240min (+ 0.000) 27.25 ng/ul m

response 142403

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	165.50	116.28#
69.00	40.10	31.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

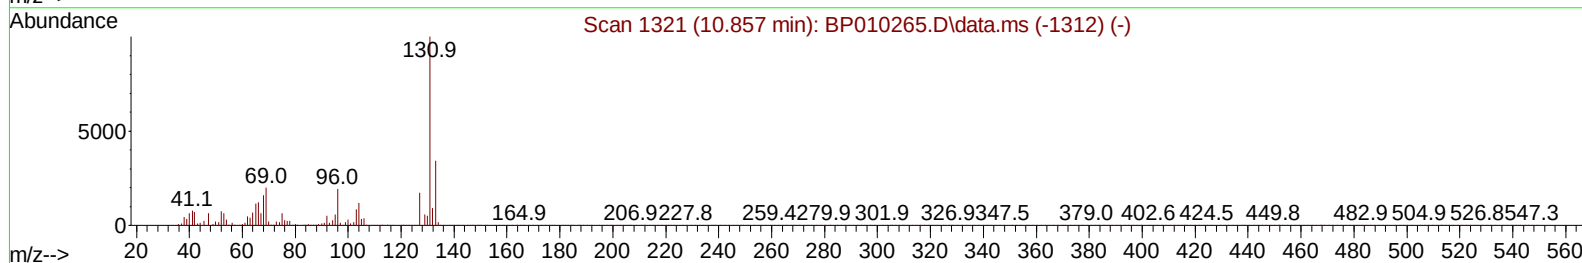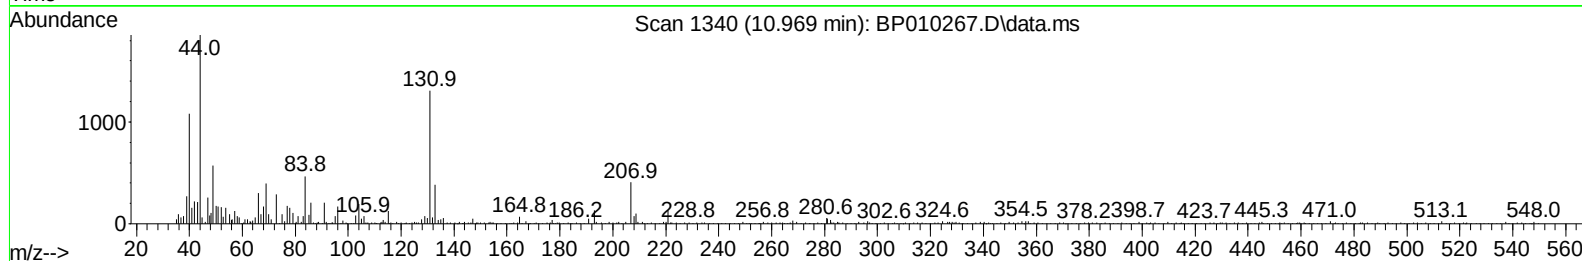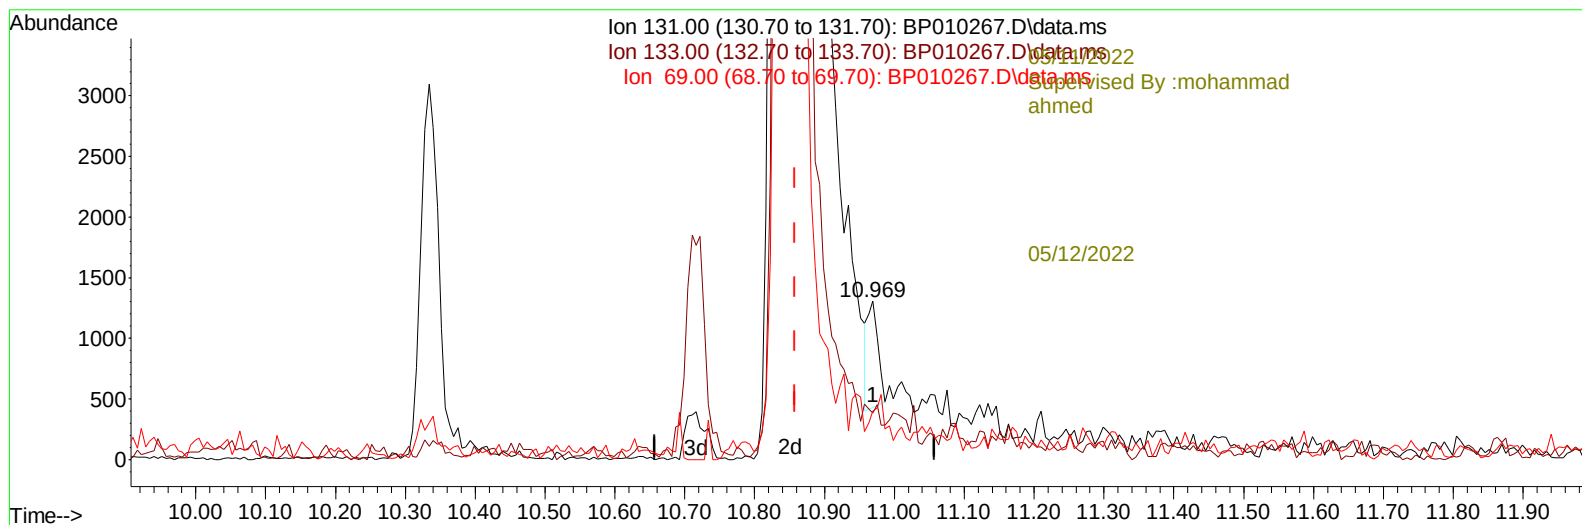

TIC: BP010267.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.969min (+ 0.112) 0.09 ng/ul

response 892

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	29.20
69.00	26.10	30.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

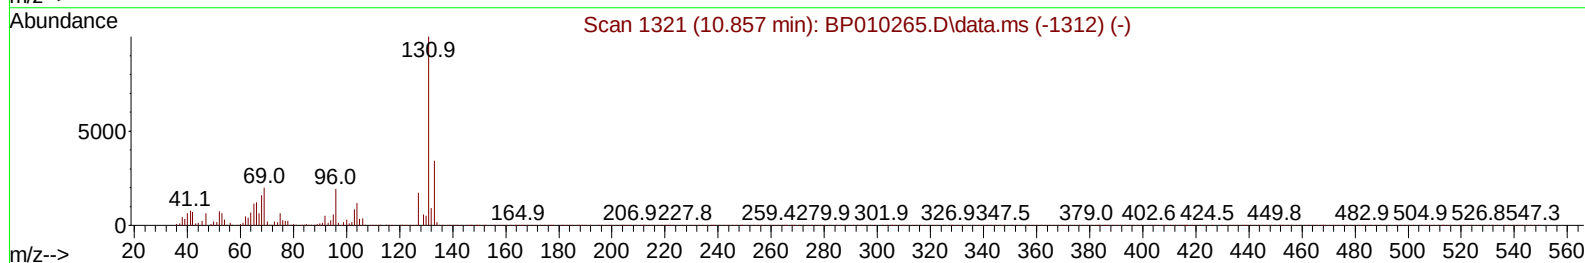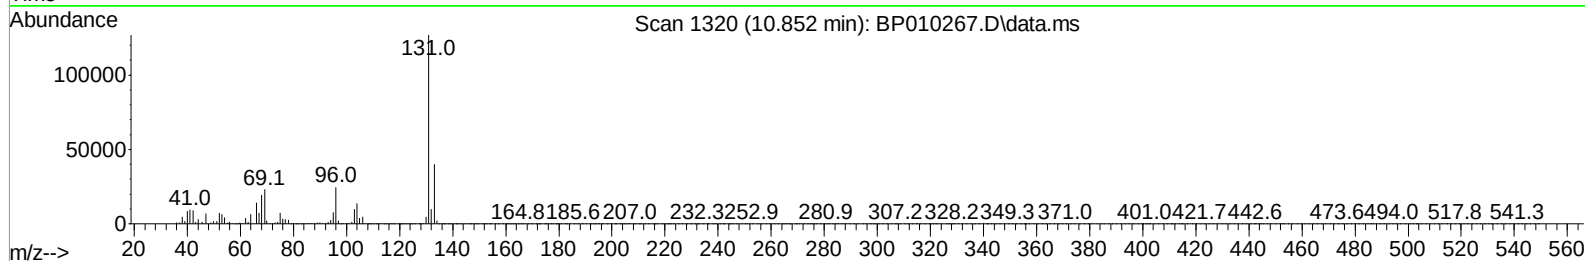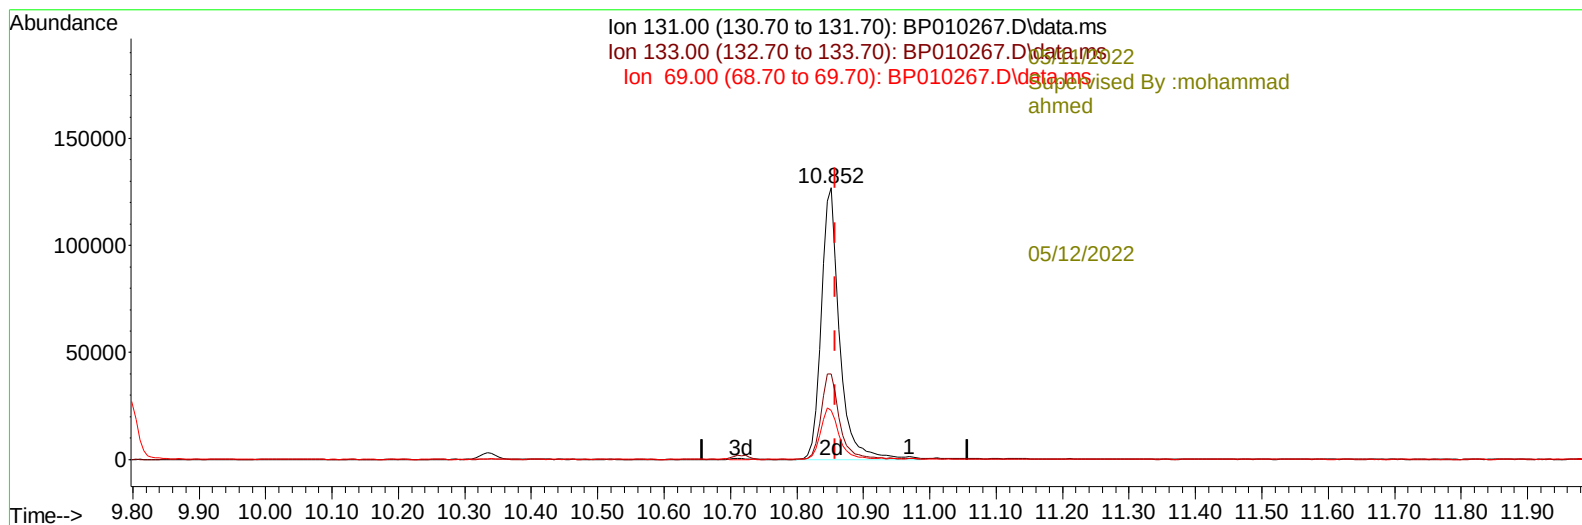

TIC: BP010267.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.852min (-0.006) 24.61 ng/ul m

response 244992

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	31.41
69.00	26.10	18.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
							-05/11/2022
							Supervised By :mohammad
							ahmed
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.911	152		90962	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136		405220	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.540	164		298184	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.292	188		697212	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.380	240		767982	20.000	ng/ul	# 0.00
88) Perylene-d12	23.816	264		813745	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.352	96		11985m	5.597	ng/uL	0.00
4) Pyridine-d5	3.770	84		157517	26.436	ng/ul	0.00
7) Phenol-d5	7.075	99		195741	23.169	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67		142403m	27.247	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132		162135	26.058	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113		166413	23.959	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128		86238	26.542	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143		91494	24.698	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165		155981	23.133	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131		244992m	24.612	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166		670732	28.235	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160		679152	23.979	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143		96651	21.211	ng/ul	0.00
60) Fluorene-d10	15.534	176		545342	27.196	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.657	200		99913	20.927	ng/ul	0.00
73) Anthracene-d10	17.392	188		913813	26.765	ng/ul	-0.01
81) Pyrene-d10	19.628	212		1156201	27.244	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.657	264		1249821	28.800	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010267.D
Acq On : 10 May 2022 16:17
Operator : CG/JU
Sample : PB144574BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

