




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

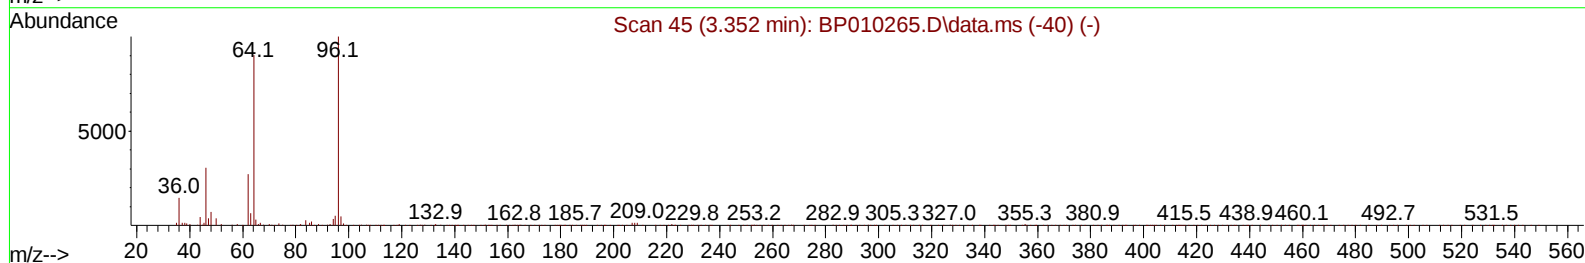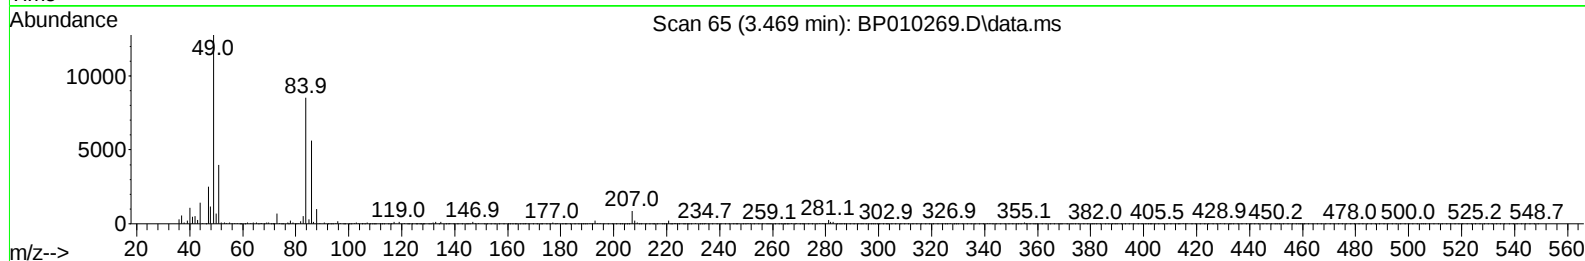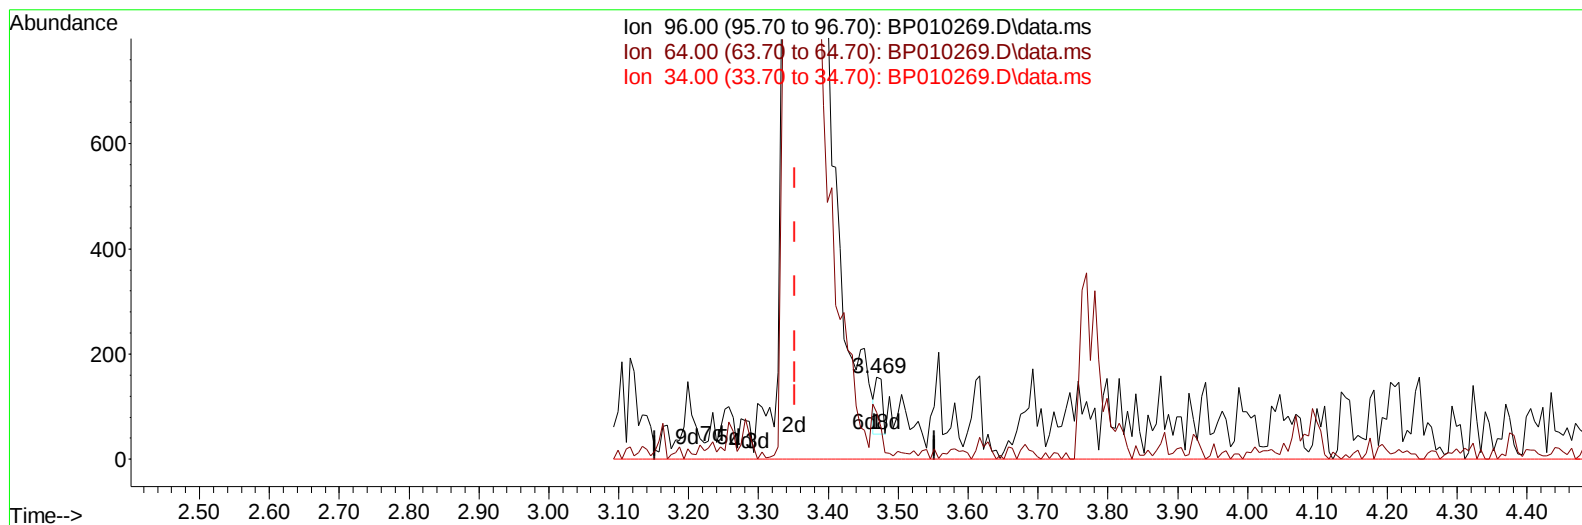

TIC: BP010269.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.469min (+ 0.117) 0.03 ng/uL

response 75

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	57.05
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

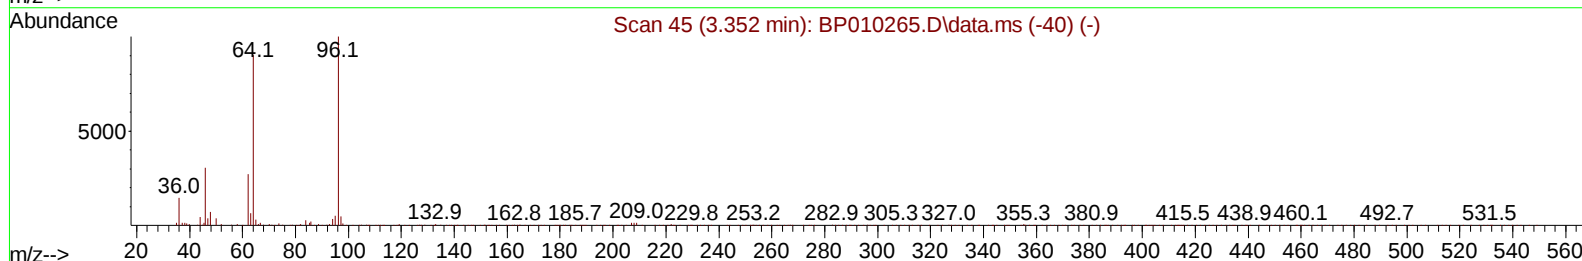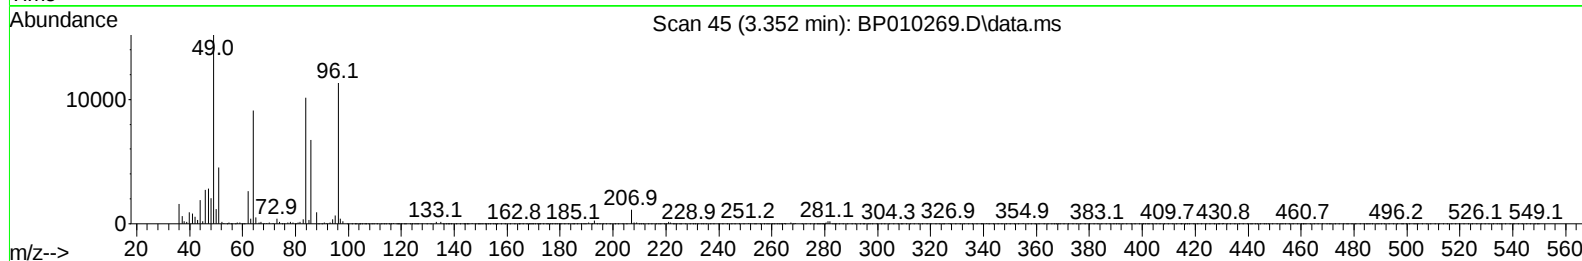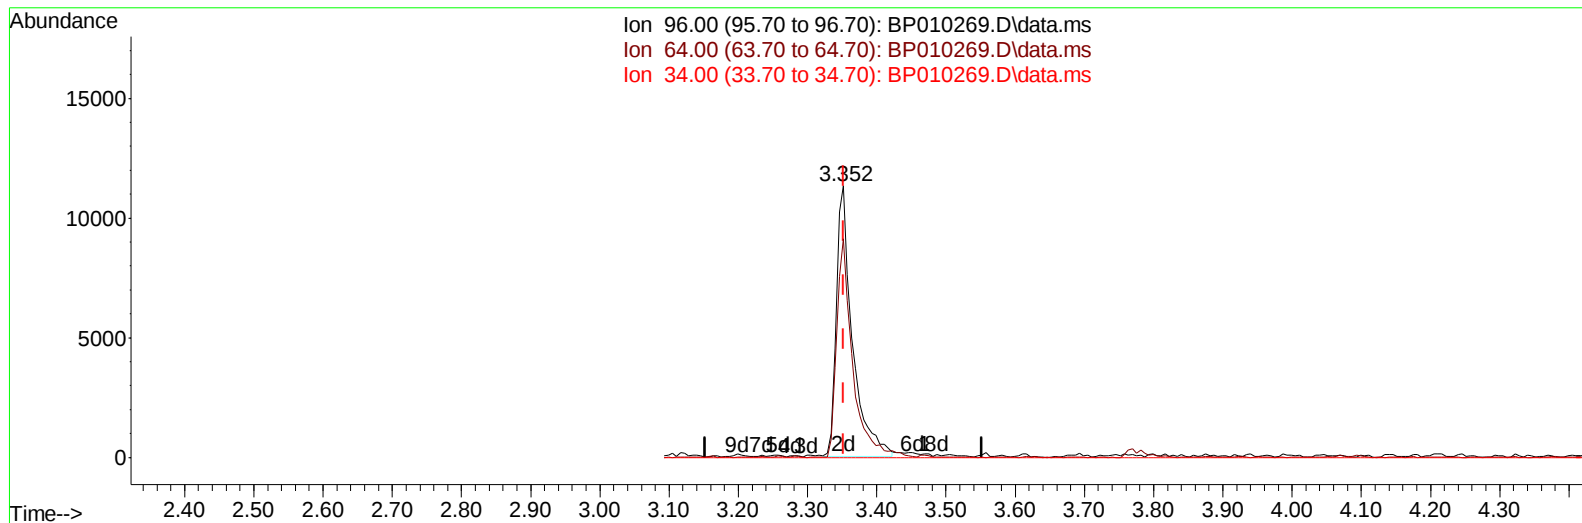

TIC: BP010269.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 6.67 ng/uL m

response 18168

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	80.46#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010269.D
Acq On : 10 May 2022 17:25
Operator : CG/JU
Sample : PB144591BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

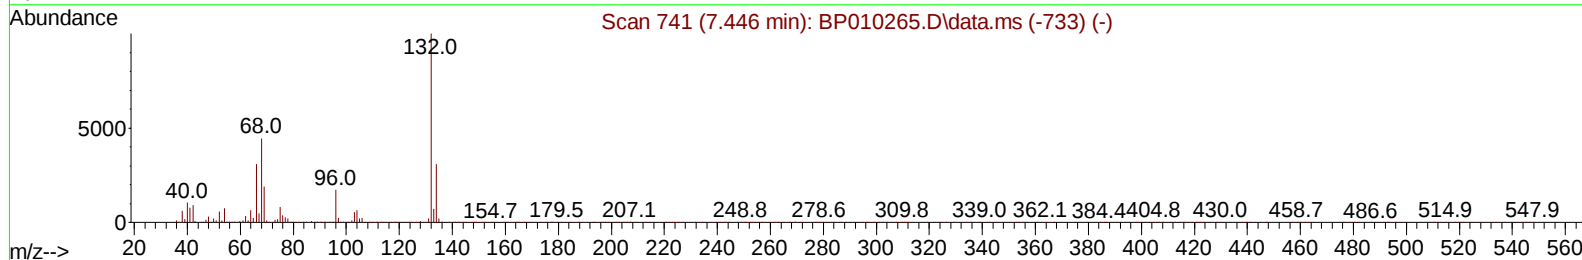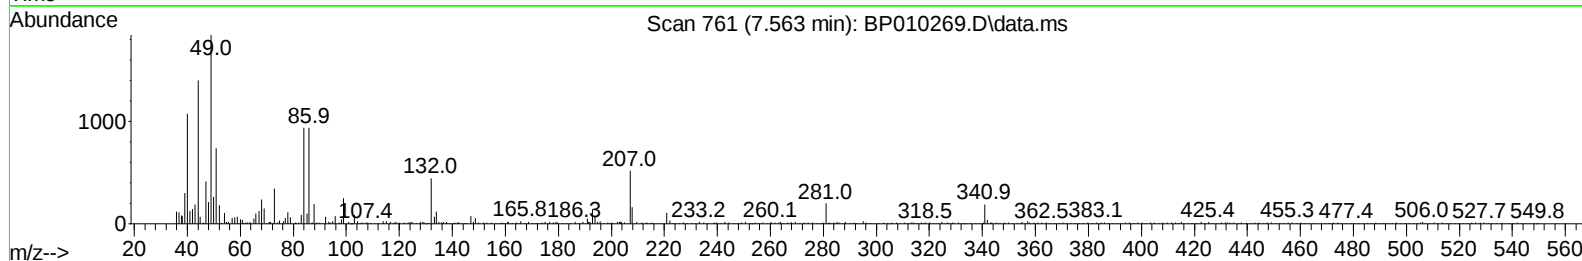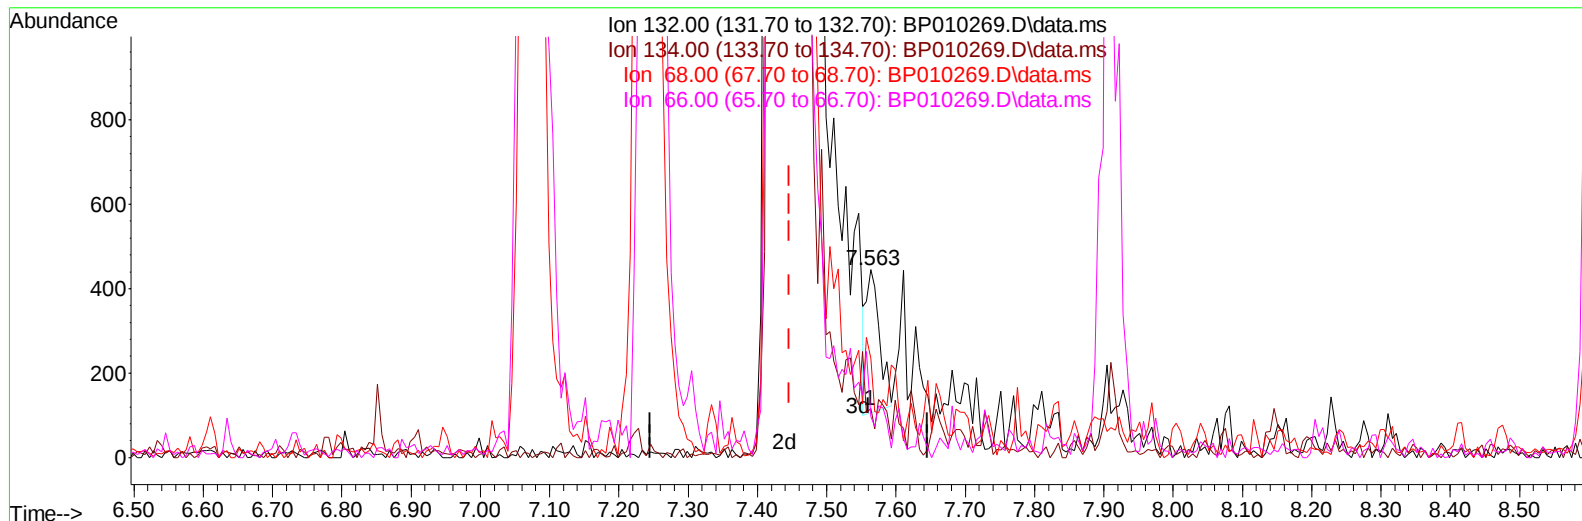

TIC: BP010269.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.563min (+ 0.118) 0.06 ng/u1

response 457

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	26.07
68.00	51.40	52.81
66.00	26.30	21.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

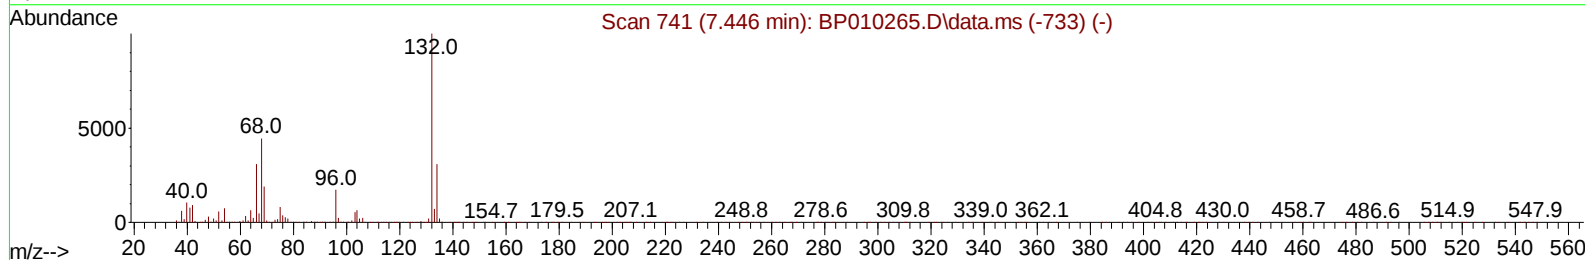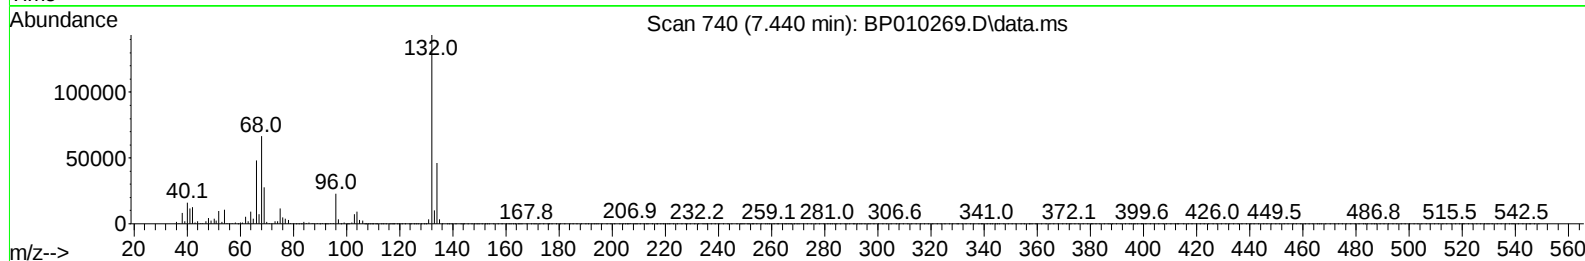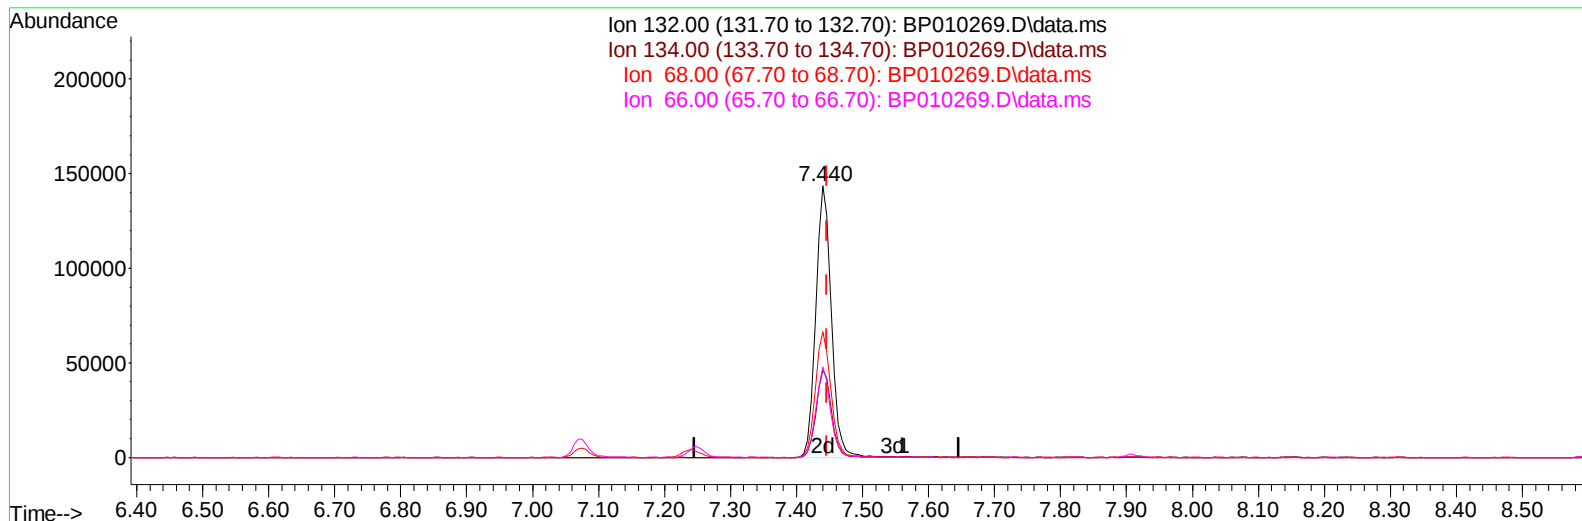

TIC: BP010269.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.440min (-0.006) 30.05 ng/ul m

response 237846

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	30.90	32.11
68.00	51.40	46.32
66.00	26.30	33.43#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

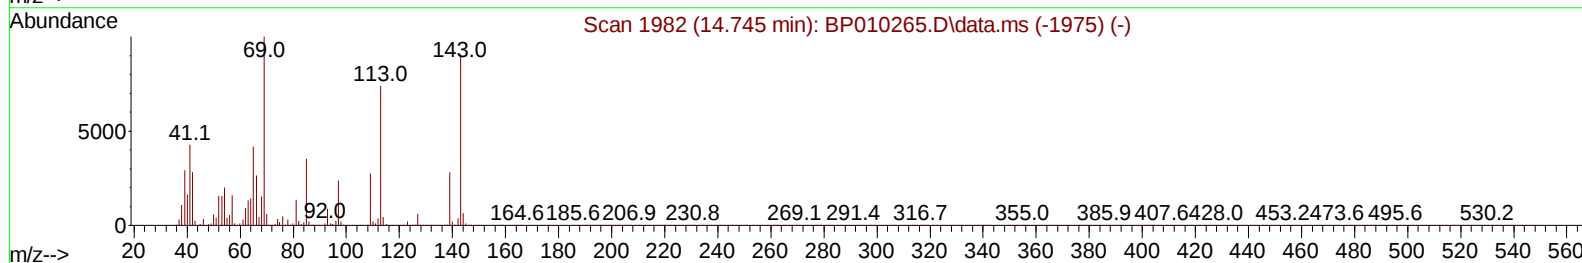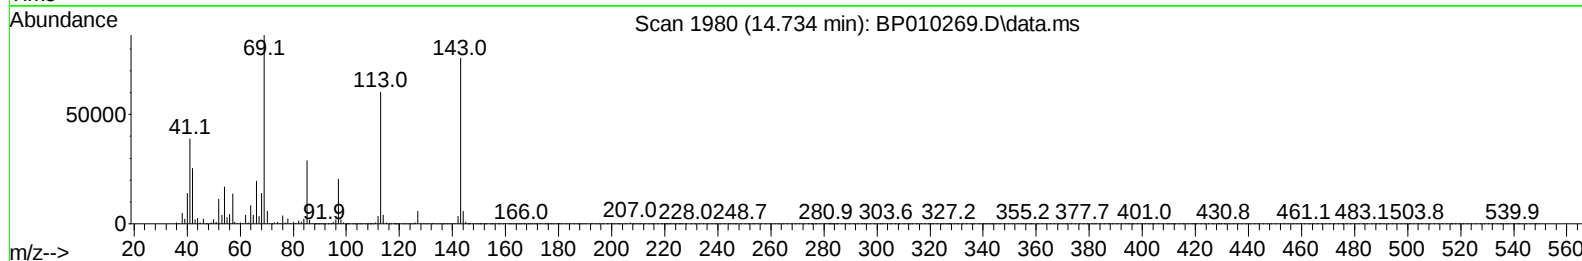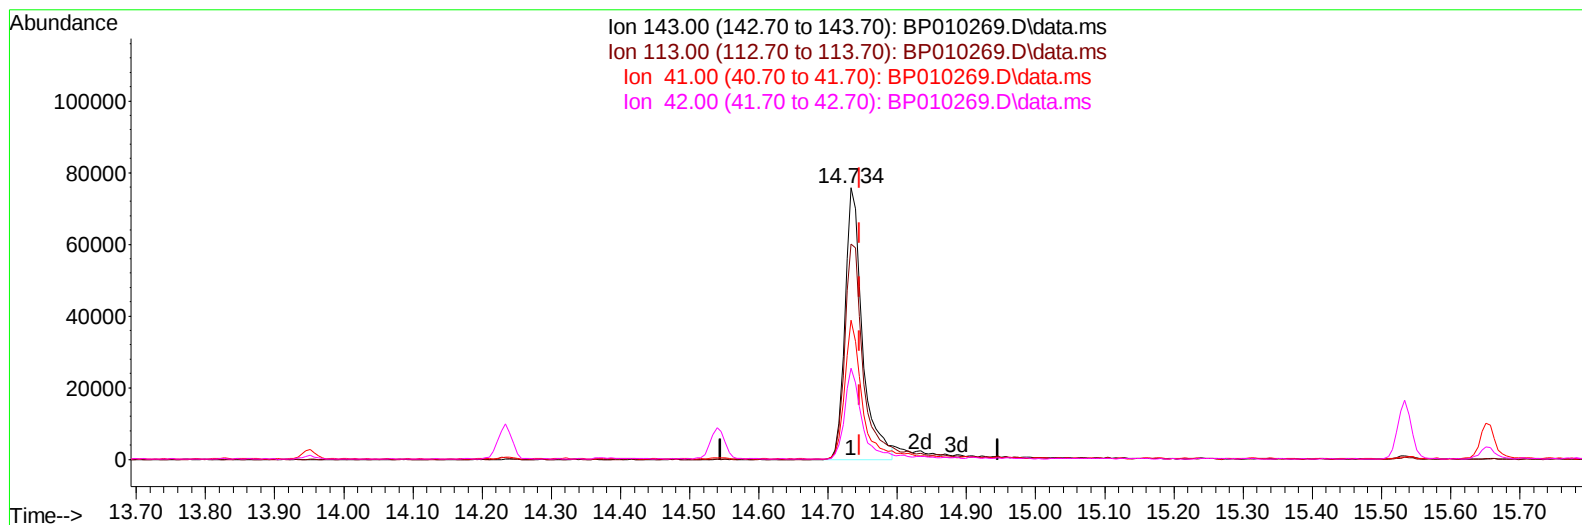

TIC: BP010269.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.012) 24.06 ng/u1

response 132103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.39#
41.00	23.20	51.19#
42.00	18.00	33.64#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

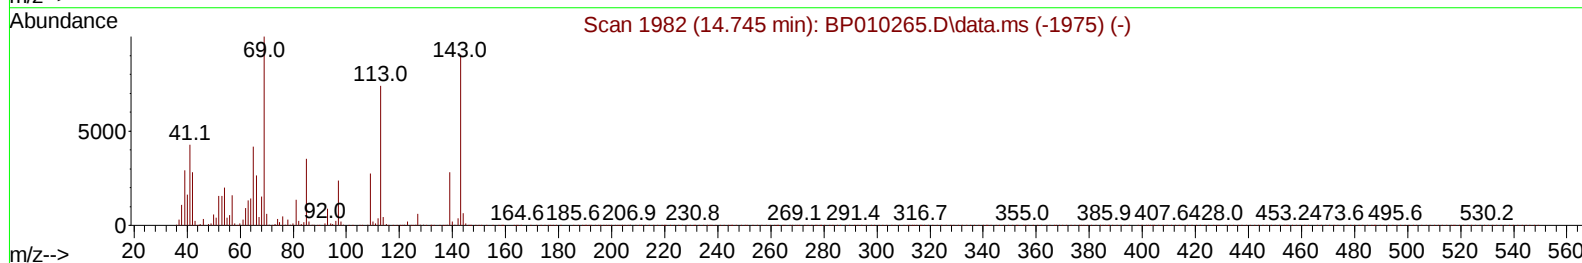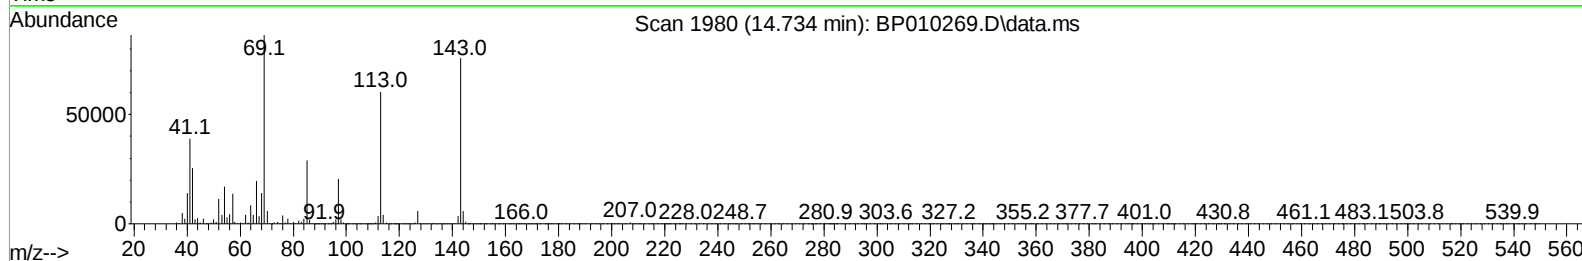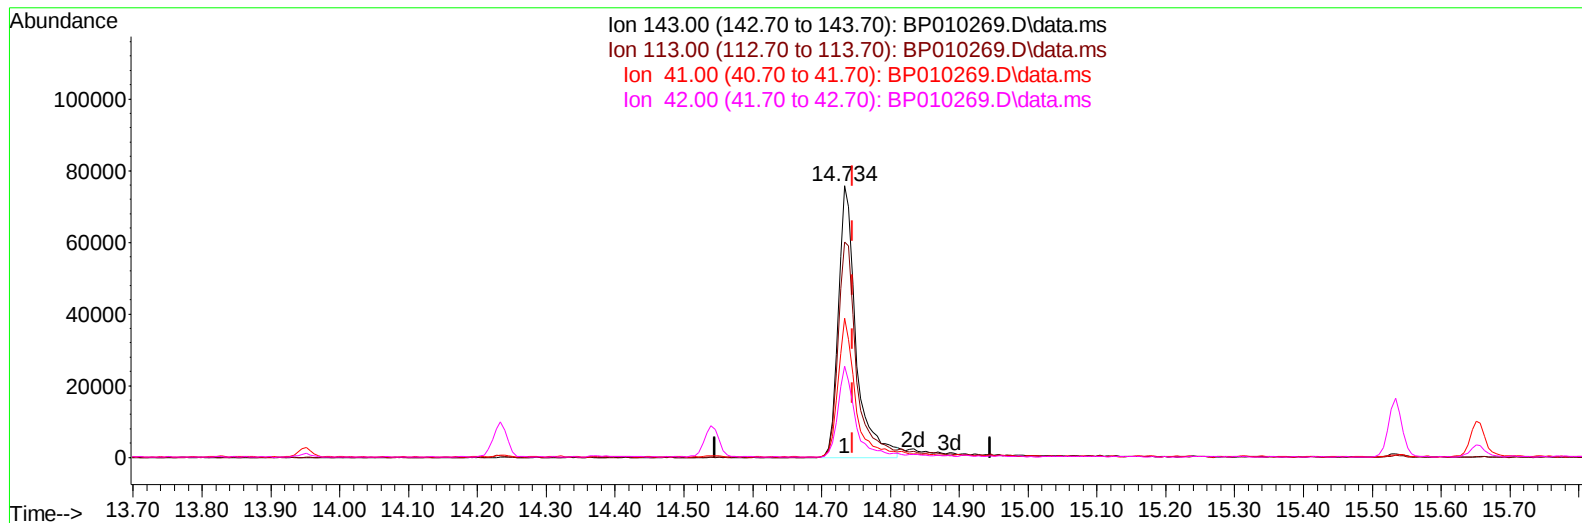

TIC: BP010269.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.012) 24.68 ng/ul m

response 135502

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	79.39#
41.00	23.20	51.19#
42.00	18.00	33.64#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010269.D
 Acq On : 10 May 2022 17:25
 Operator : CG/JU
 Sample : PB144591BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	115702	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	499152	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.539	164	359245	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.292	188	819693	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.374	240	847494	20.000	ng/ul	#-0.01
88) Perylene-d12	23.810	264	857497	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	18168m	6.671	ng/uL	0.00
4) Pyridine-d5	3.769	84	235015	31.009	ng/ul	0.00
7) Phenol-d5	7.075	99	289528	26.942	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	205637	30.933	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	237846m	30.053	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	245752	27.816	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	123953	30.971	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	137192	30.064	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	229334	27.612	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	350379	28.575	ng/ul	-0.01
46) Dimethylphthalate-d6	13.951	166	937822	32.768	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	987618	28.944	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	135502m	24.683	ng/ul	-0.01
60) Fluorene-d10	15.533	176	768775	31.822	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.651	200	147049	26.197	ng/ul	-0.01
73) Anthracene-d10	17.392	188	1266902	31.562	ng/ul	-0.01
81) Pyrene-d10	19.627	212	1567495	33.470	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.657	264	1516415	33.160	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010269.D
Acq On : 10 May 2022 17:25
Operator : CG/JU
Sample : PB144591BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:17:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

