




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

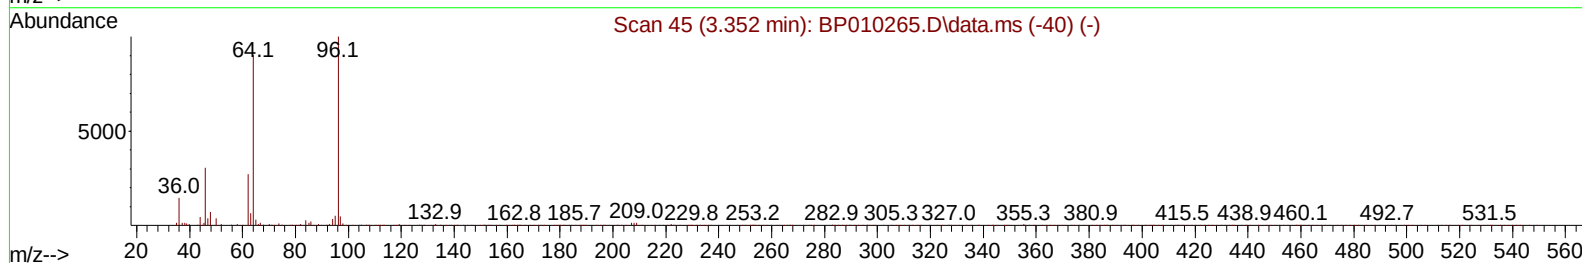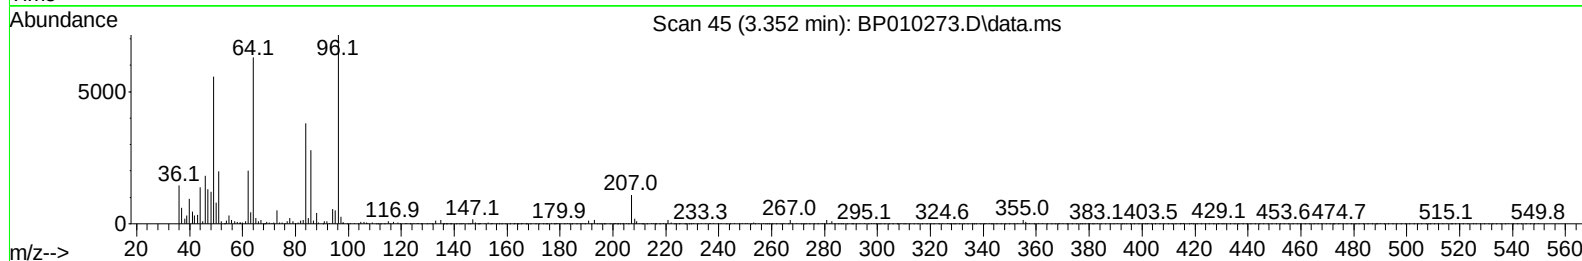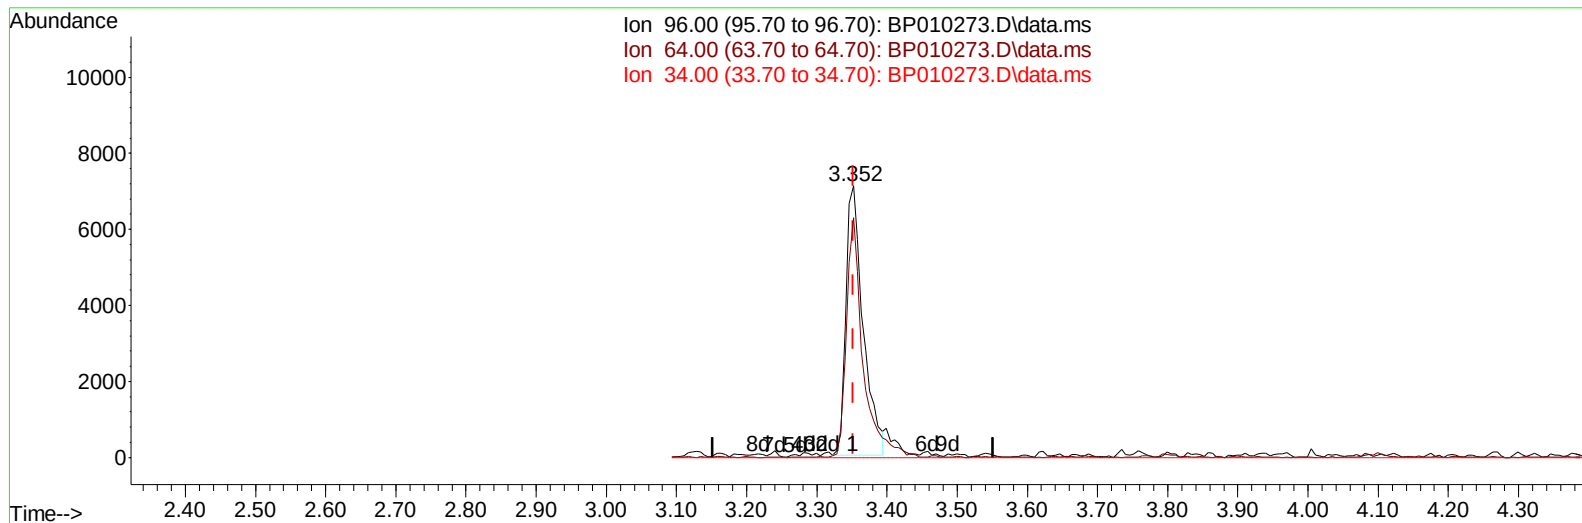

TIC: BP010273.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 4.30 ng/uL

response 12139

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	88.29#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

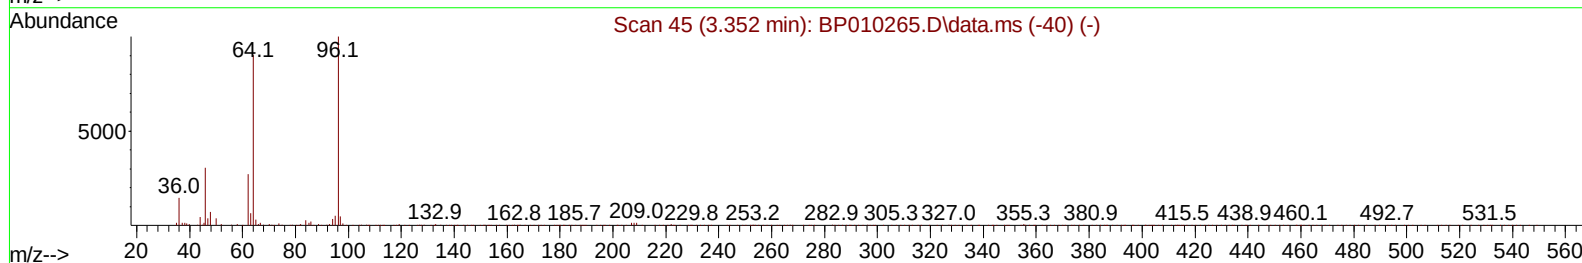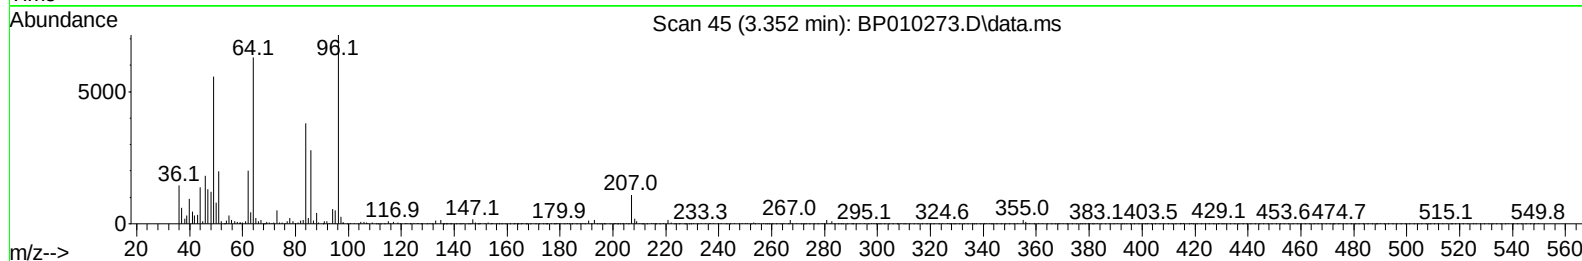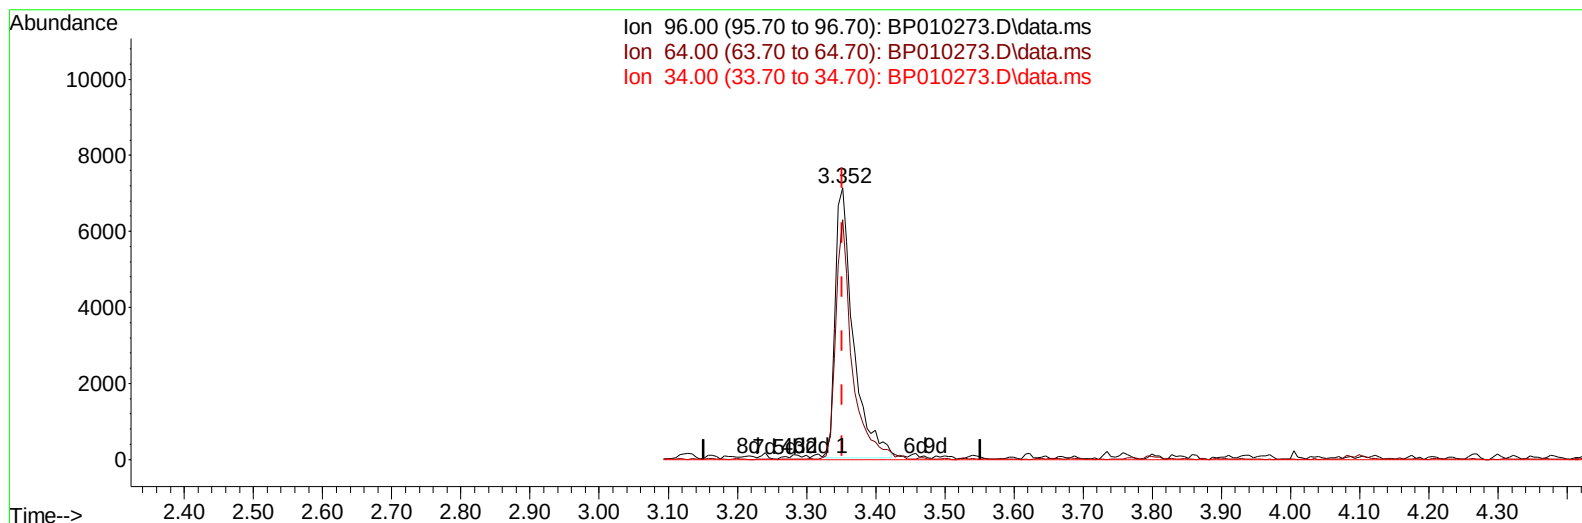

TIC: BP010273.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 4.56 ng/uL m

response 12887

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	88.29#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

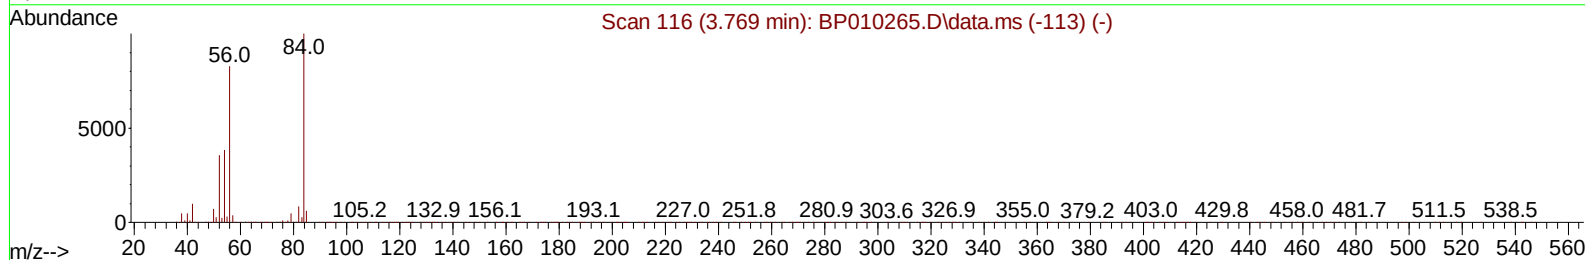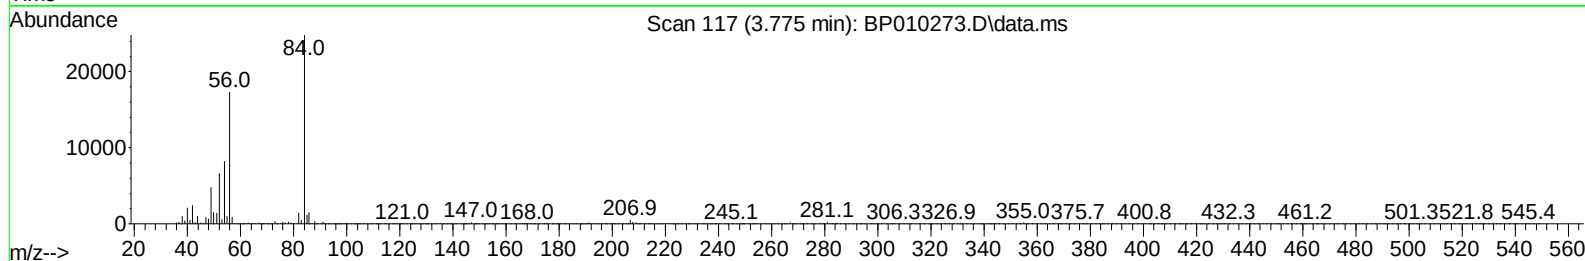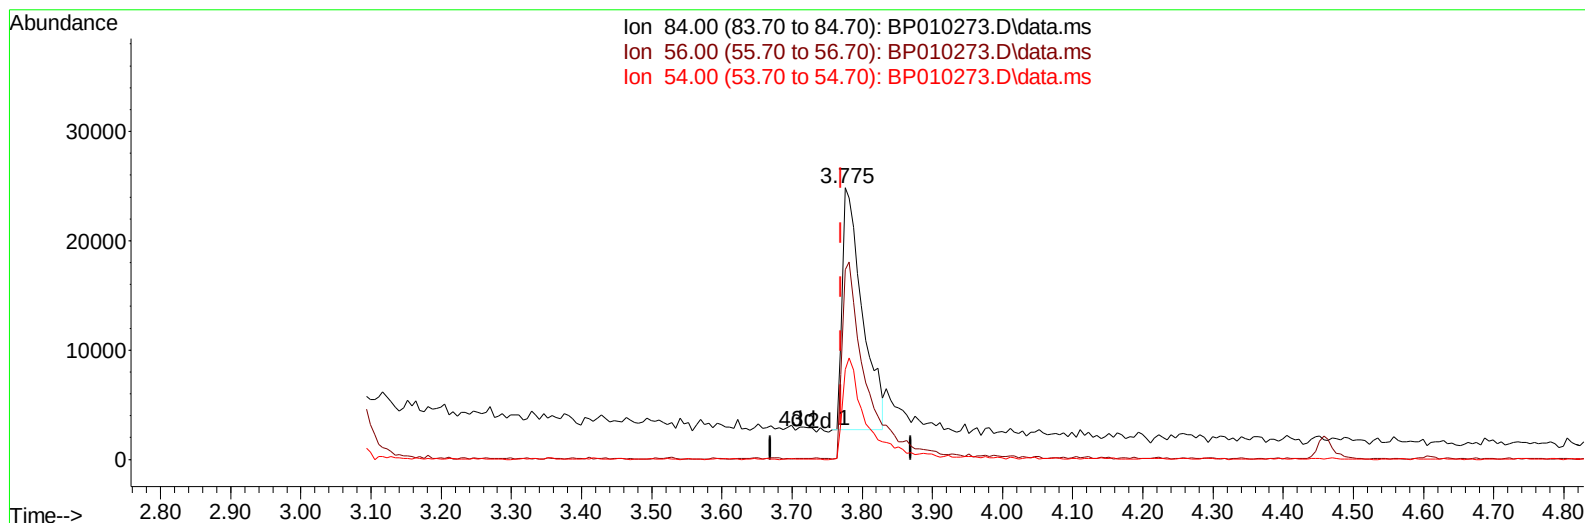

TIC: BP010273.D\data.ms

(4) Pyridine-d5 (S)

3.775min (+ 0.006) 5.57 ng/u1

response 43788

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	69.91#
54.00	24.80	33.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

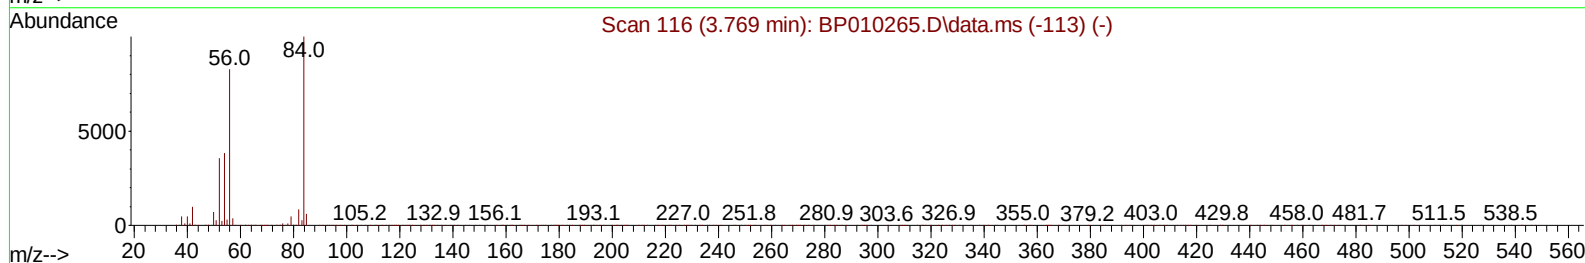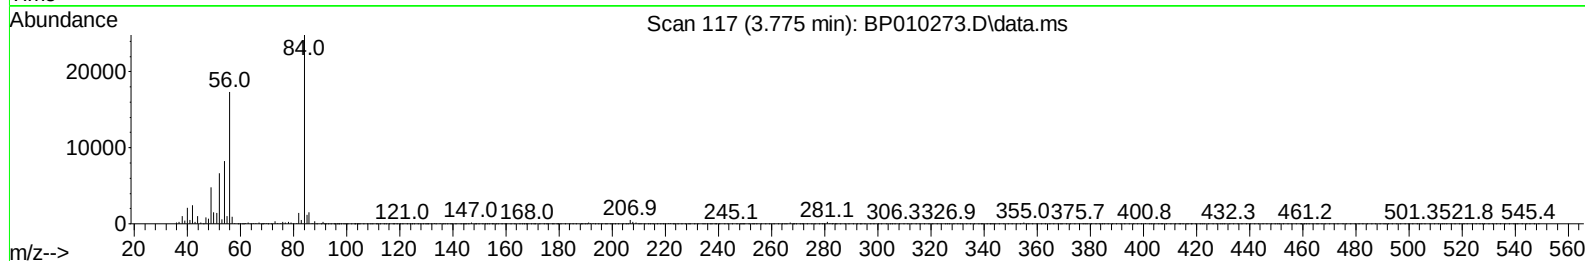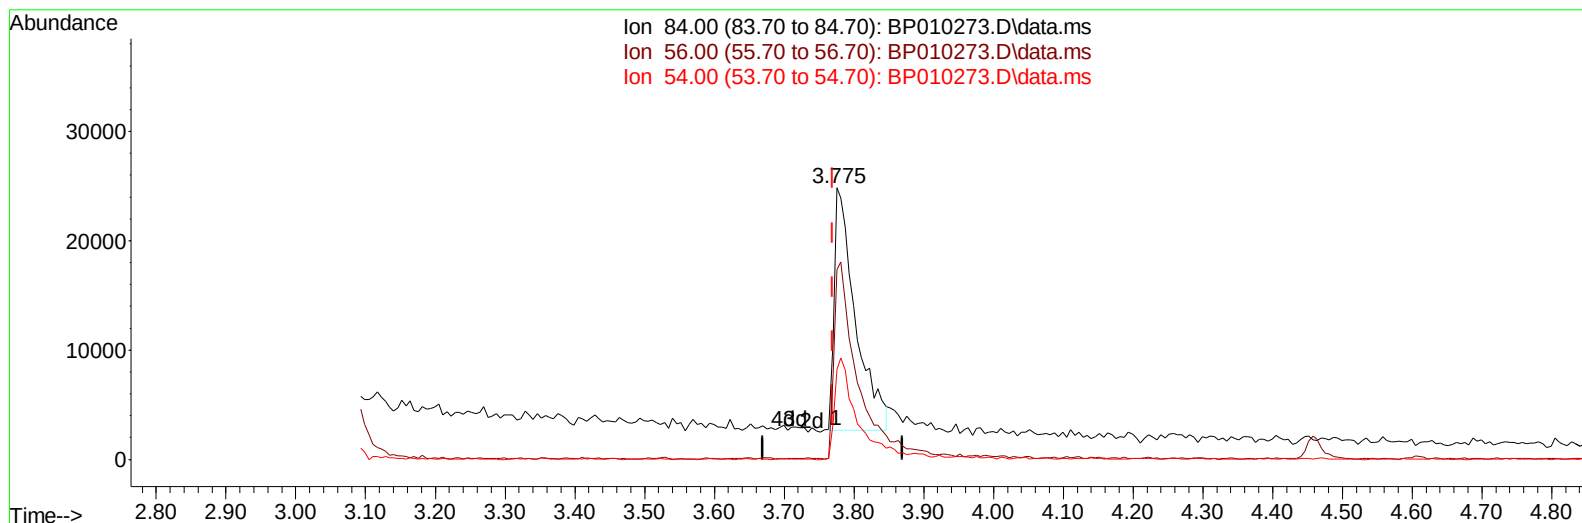

TIC: BP010273.D\data.ms

(4) Pyridine-d5 (S)

3.775min (+ 0.006) 5.98 ng/ul m

response 47009

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	30.50	69.91#
54.00	24.80	33.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

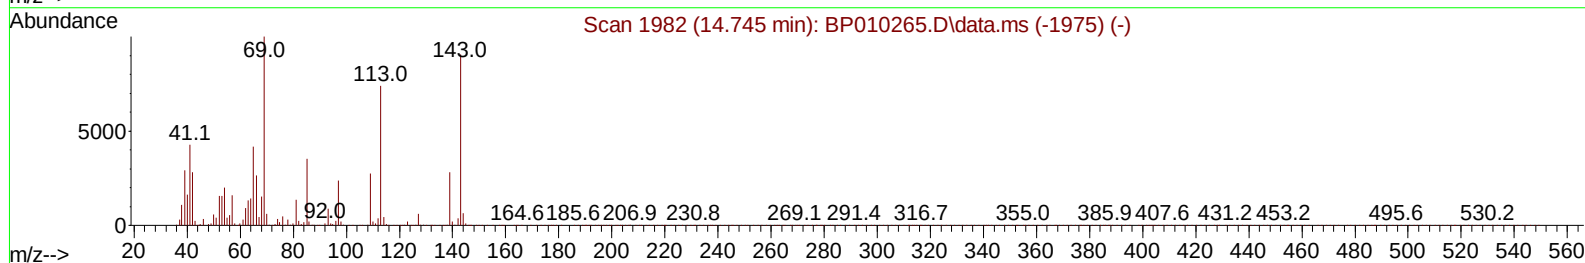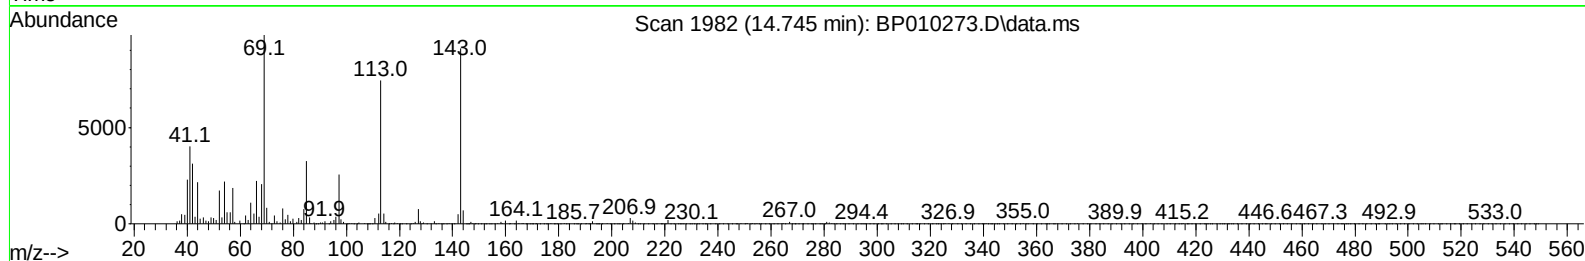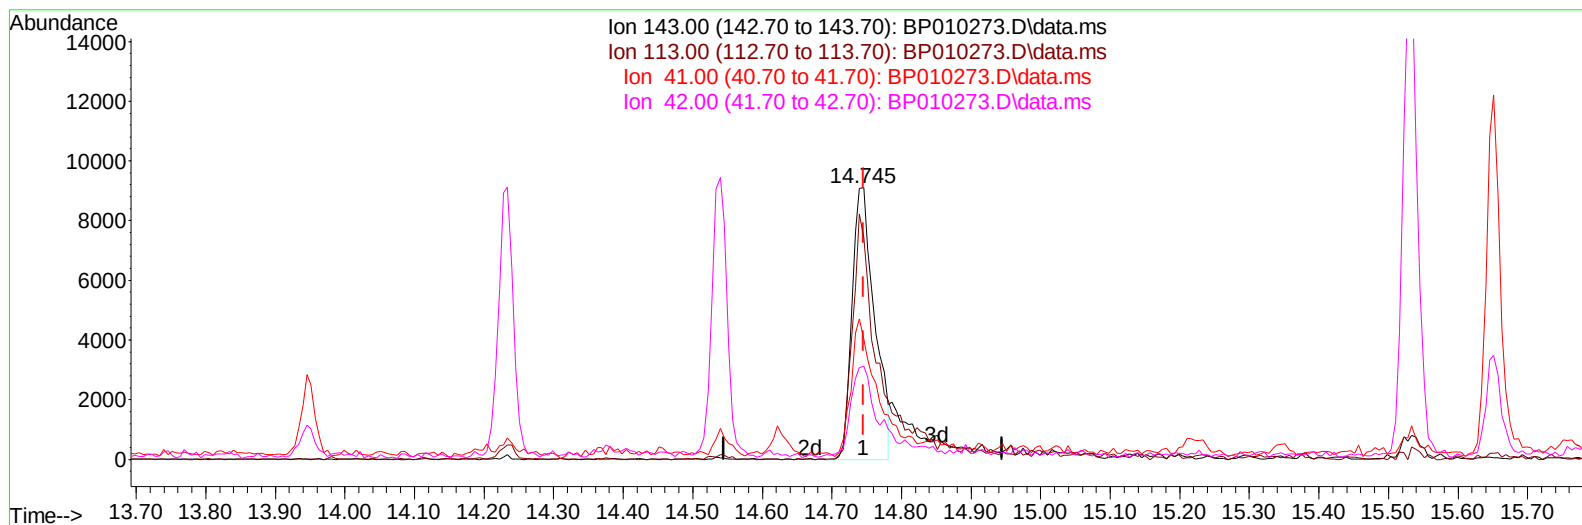

TIC: BP010273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.000) 3.50 ng/ul

response 20523

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.76#
41.00	23.20	44.12#
42.00	18.00	34.26#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

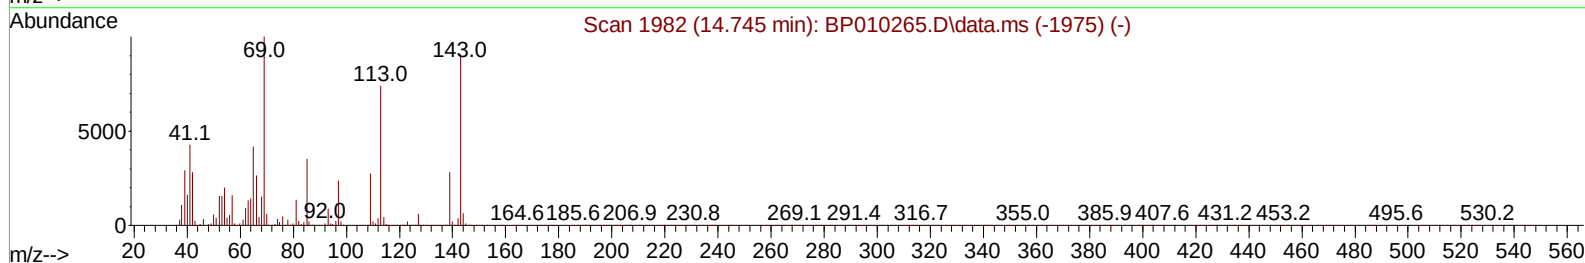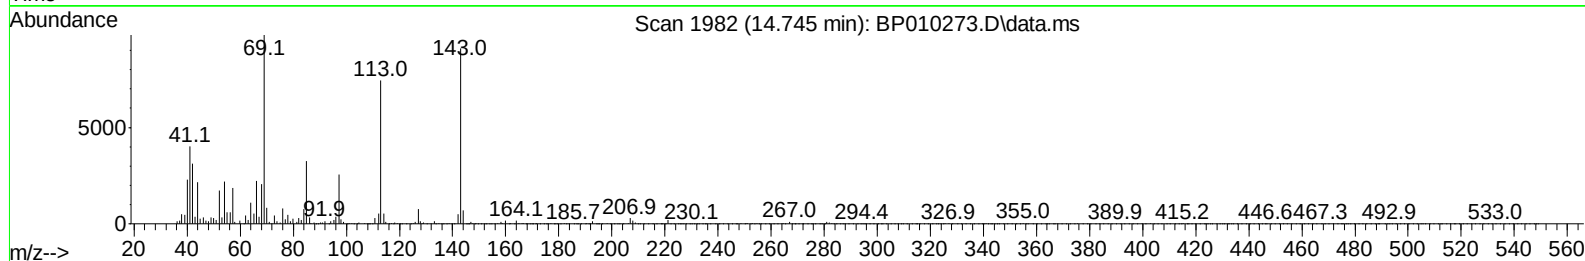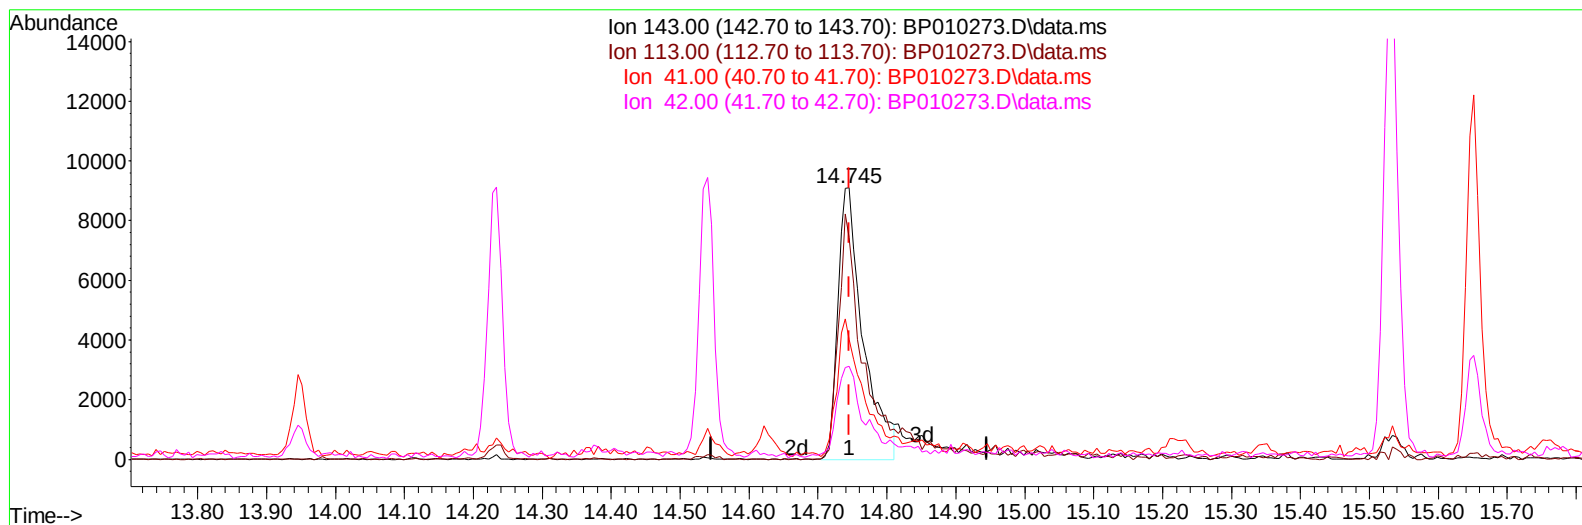

TIC: BP010273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.000) 3.93 ng/ul m

response 23057

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	81.76#
41.00	23.20	44.12#
42.00	18.00	34.26#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010273.D
 Acq On : 10 May 2022 19:40
 Operator : CG/JU
 Sample : N2678-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:18:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	120012	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.710	136	527379	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.540	164	384137	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.292	188	874551	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.375	240	893651	20.000	ng/ul	#-0.01
88) Perylene-d12	23.810	264	902344	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	12887m	4.562	ng/uL	0.00
4) Pyridine-d5	3.775	84	47009m	5.980	ng/ul	0.00
7) Phenol-d5	7.075	99	56066	5.030	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	188011	27.266	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	164286	20.013	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	111543	12.172	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	113776	26.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	118001	24.475	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	191665	21.841	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	198004	15.284	ng/ul	-0.01
46) Dimethylphthalate-d6	13.951	166	918104	30.001	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	958528	26.271	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	23057m	3.928	ng/ul	0.00
60) Fluorene-d10	15.534	176	799406	30.946	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.651	200	156299	26.098	ng/ul	-0.01
73) Anthracene-d10	17.392	188	1429309	33.374	ng/ul	-0.01
81) Pyrene-d10	19.622	212	1768866	35.819	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.657	264	1689732	35.113	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010273.D
Acq On : 10 May 2022 19:40
Operator : CG/JU
Sample : N2678-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:18:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

