




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

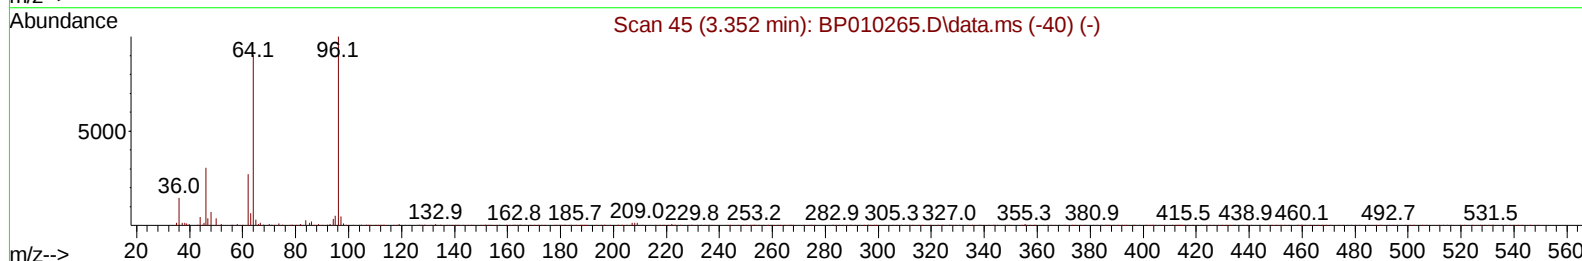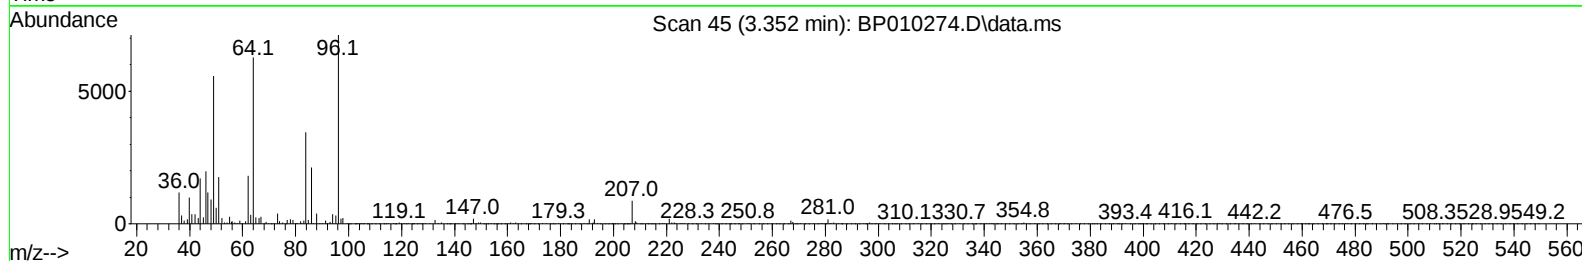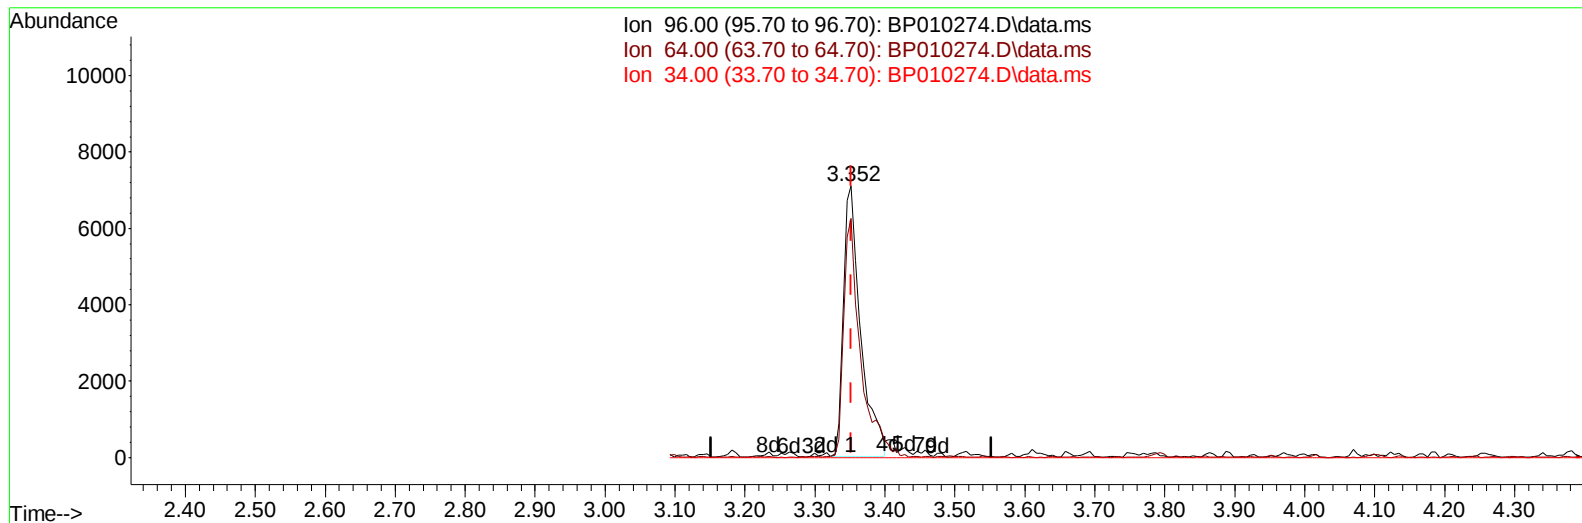

TIC: BP010274.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.12 ng/uL

response 12039

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	88.15#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

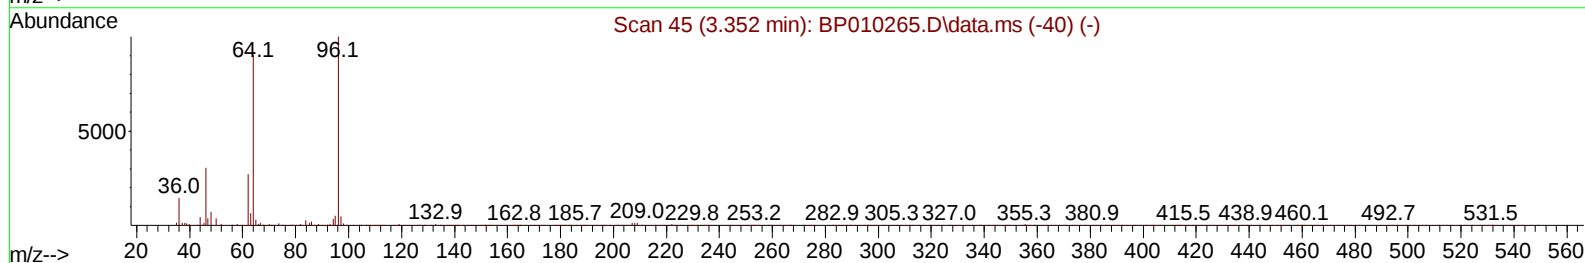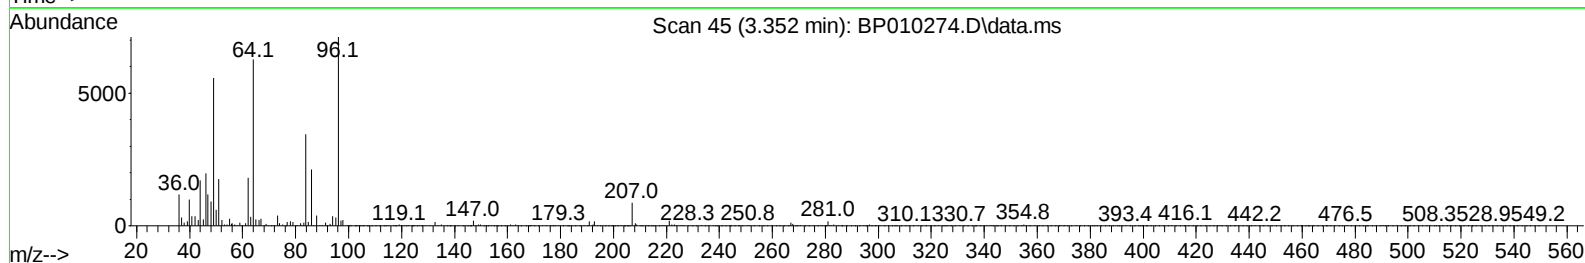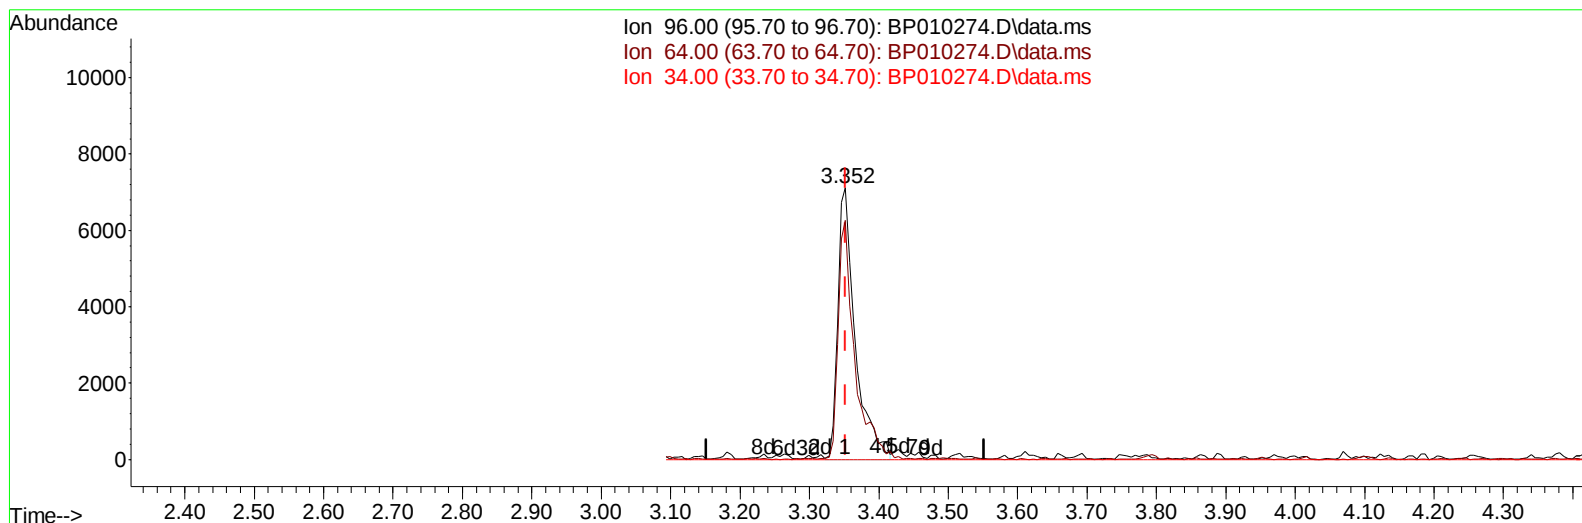

TIC: BP010274.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.32 ng/uL m

response 12509

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	88.15#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

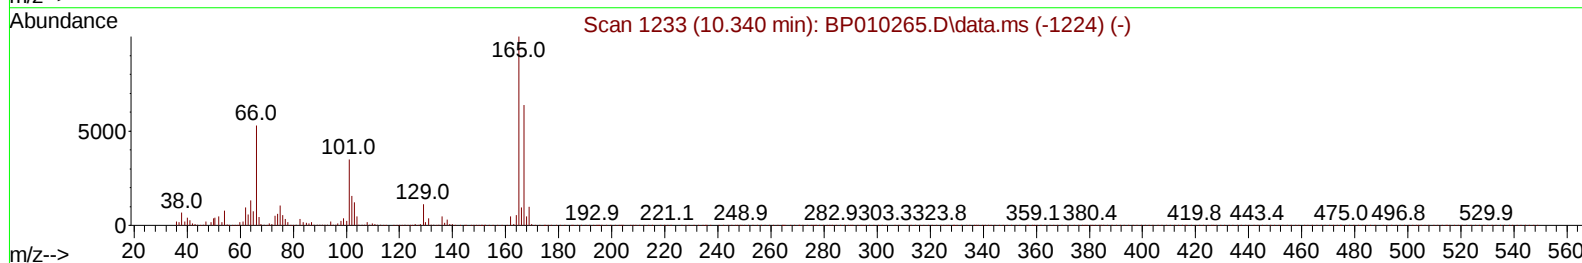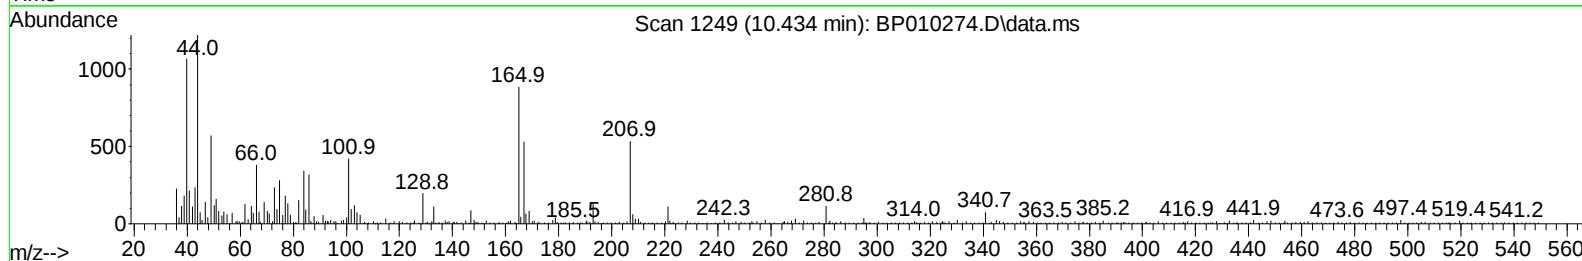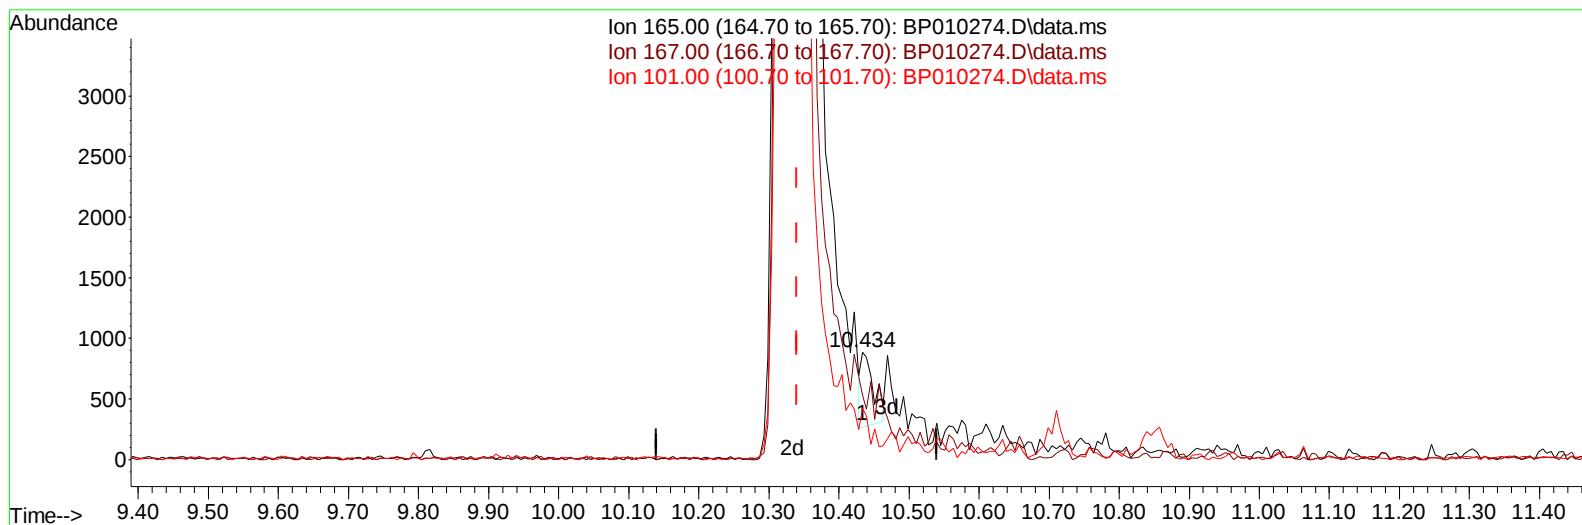

TIC: BP010274.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.434min (+ 0.094) 0.11 ng/u1

response 788

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	67.61
101.00	49.80	47.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

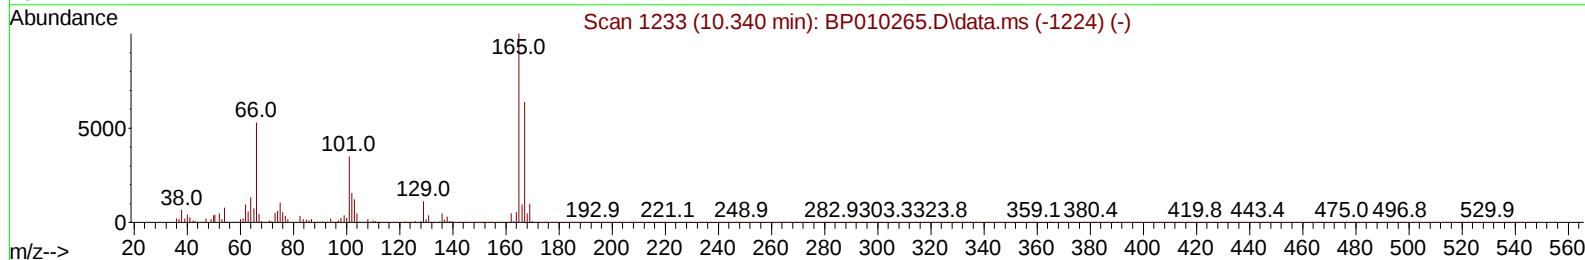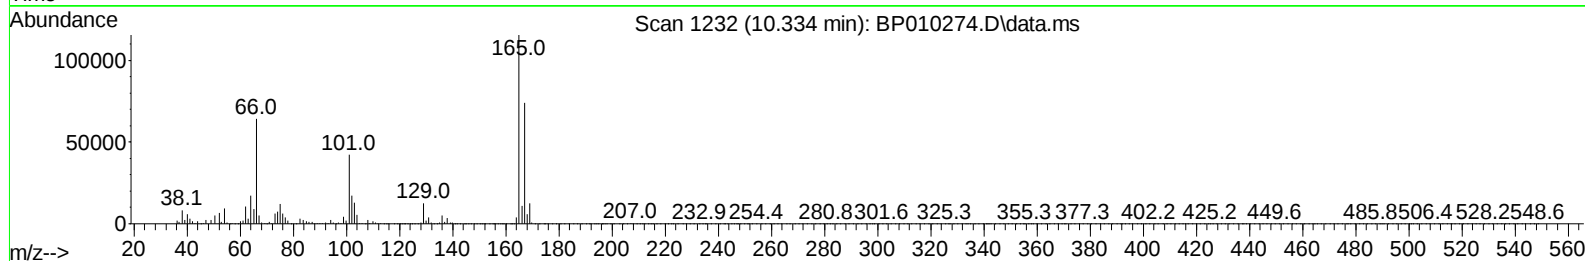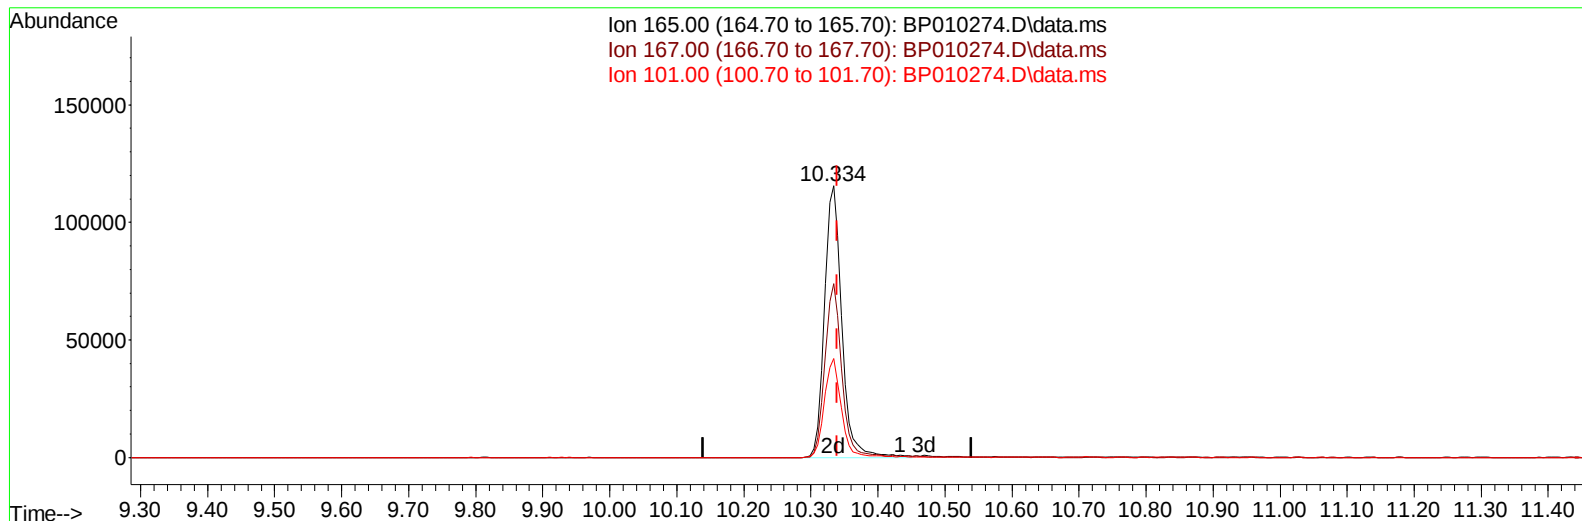

TIC: BP010274.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.334min (-0.006) 27.69 ng/ul m

response 207121

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	64.09
101.00	49.80	36.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010274.D
Acq On : 10 May 2022 20:13
Operator : CG/JU
Sample : N2678-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

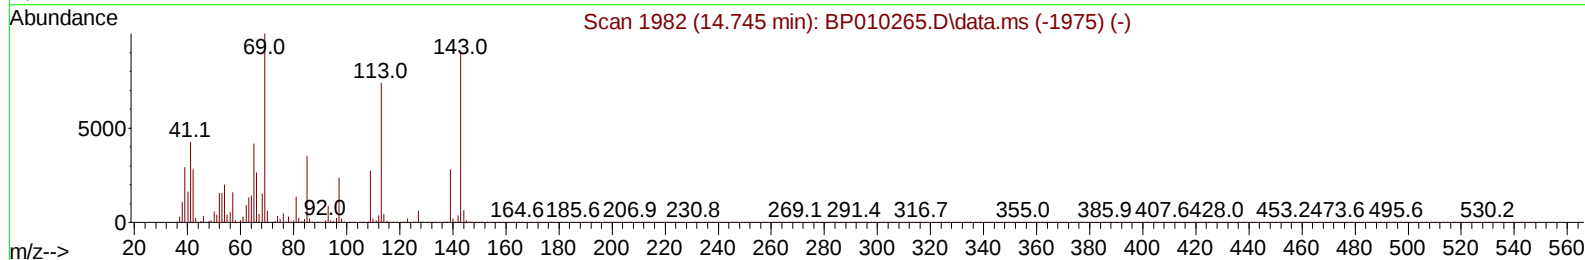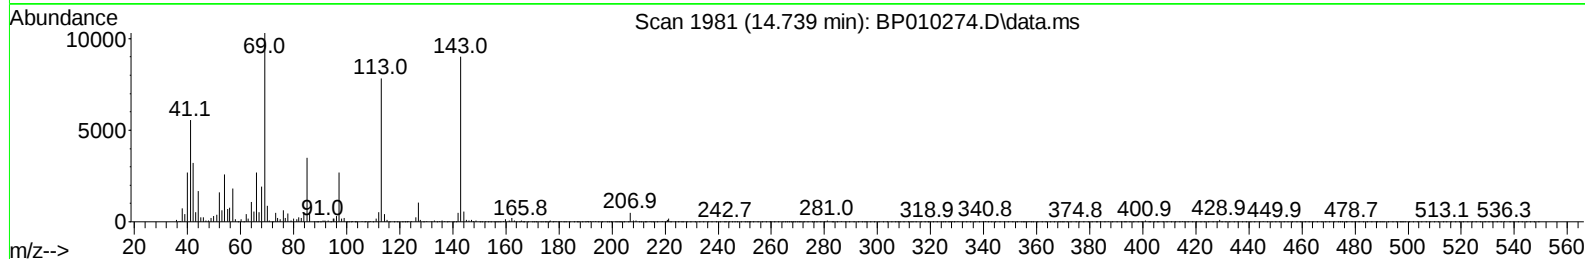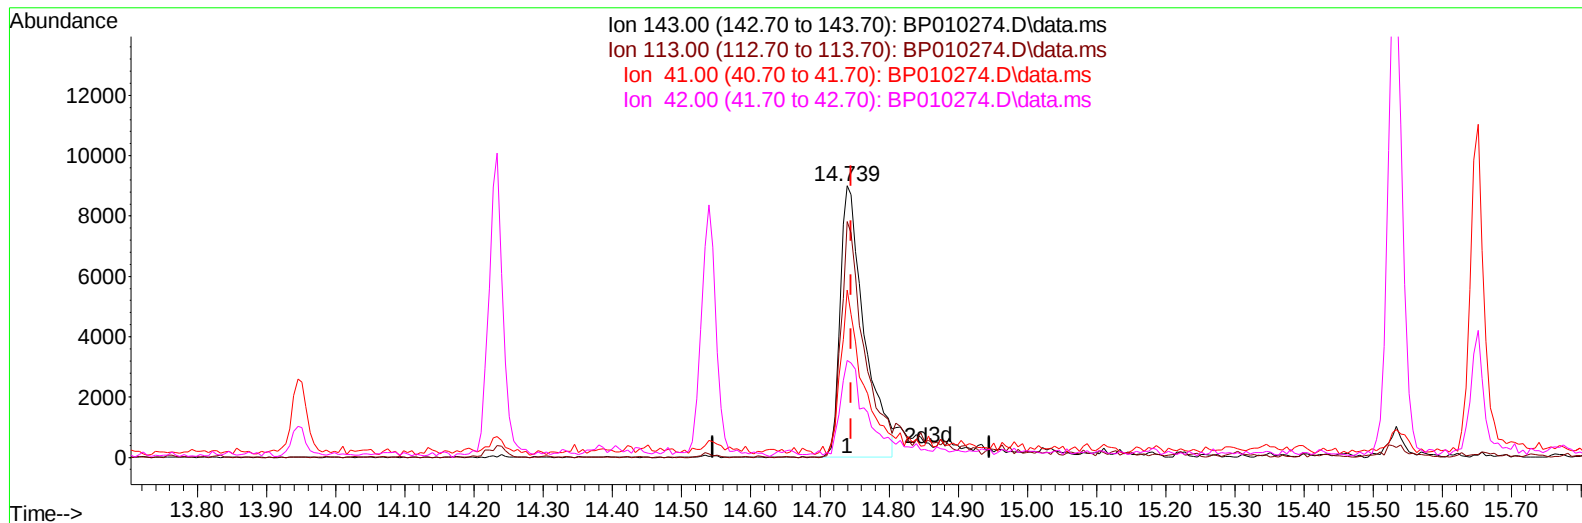

TIC: BP010274.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (-0.006) 4.32 ng/u1

response 21720

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	86.95#
41.00	23.20	61.59#
42.00	18.00	35.81#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

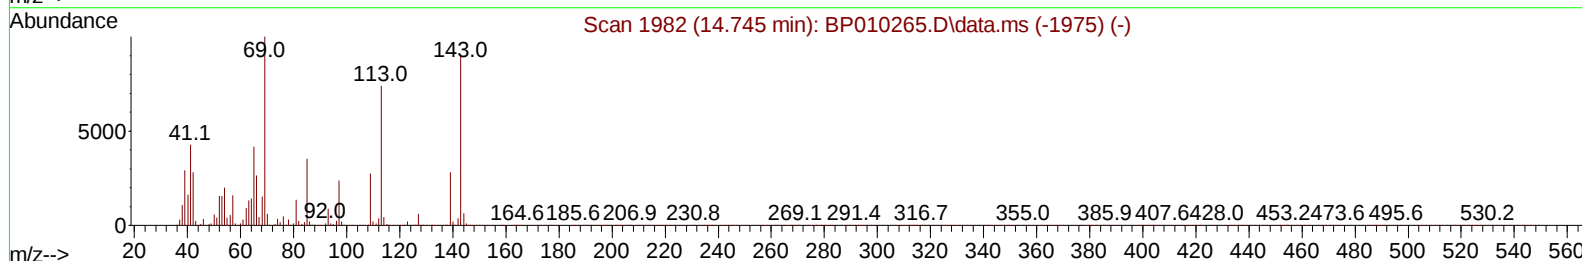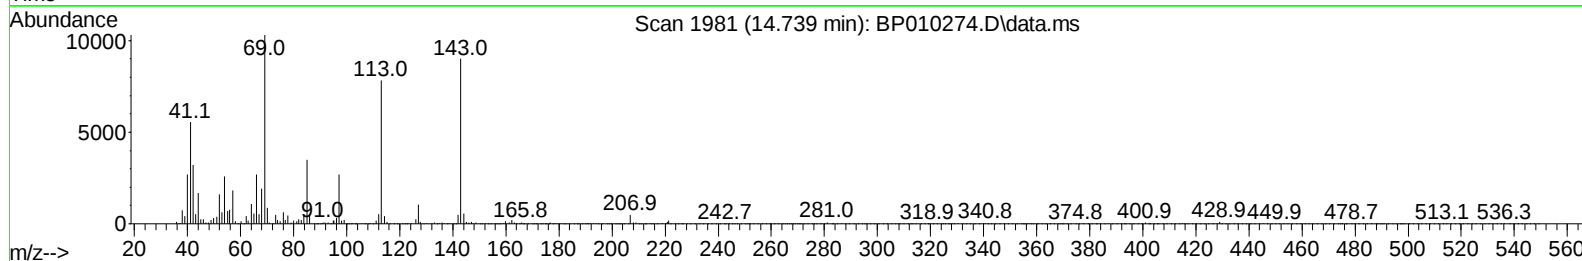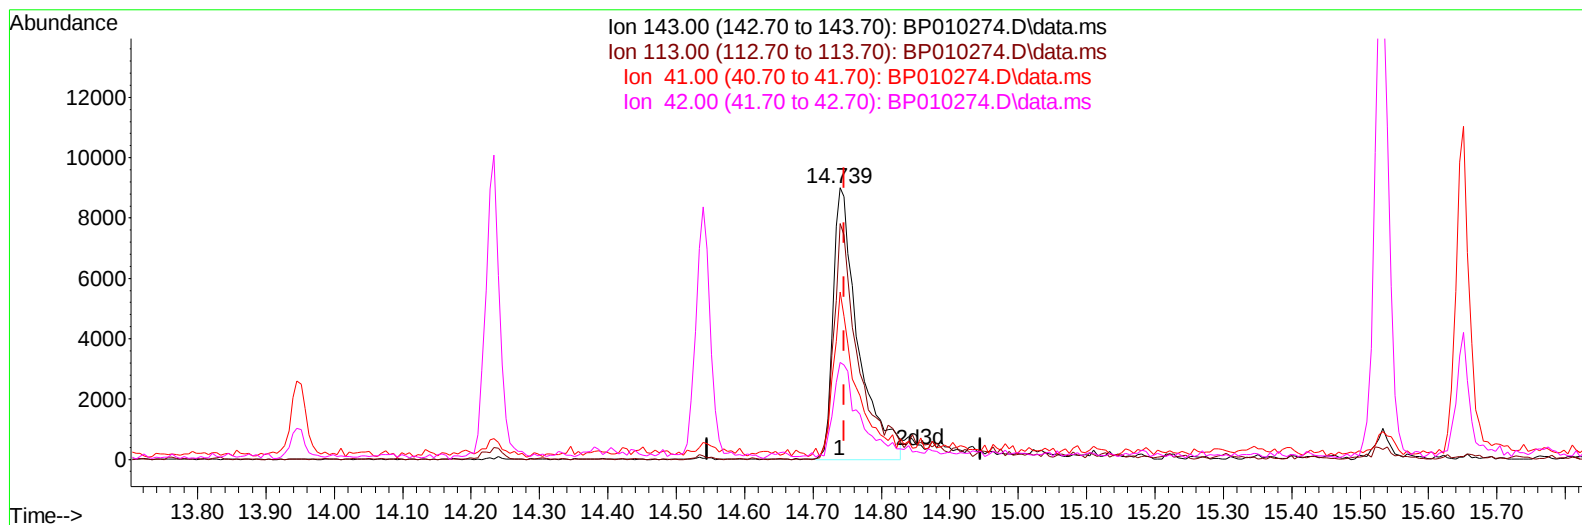

TIC: BP010274.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (-0.006) 4.58 ng/ul m

response 23026

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	86.95#
41.00	23.20	61.59#
42.00	18.00	35.81#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010274.D
 Acq On : 10 May 2022 20:13
 Operator : CG/JU
 Sample : N2678-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
 Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:19:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 10 15:59:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	99806	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	449501	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.539	164	328799	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.292	188	744075	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.374	240	786567	20.000	ng/ul	#-0.01
88) Perylene-d12	23.804	264	818593	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	12509m	5.324	ng/uL	0.00
4) Pyridine-d5	3.781	84	34132	5.221	ng/ul	0.01
7) Phenol-d5	7.075	99	54327	5.861	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	192636	33.592	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	170712	25.005	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	118050	15.490	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	116981	32.457	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	122557	29.824	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	207121m	27.692	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	195905	17.742	ng/ul	-0.01
46) Dimethylphthalate-d6	13.945	166	893814	34.122	ng/ul	-0.01
49) Acenaphthylene-d8	14.234	160	952686	30.505	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	23026m	4.583	ng/ul	0.00
60) Fluorene-d10	15.534	176	769073	34.782	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.651	200	147661	28.979	ng/ul	-0.01
73) Anthracene-d10	17.392	188	1309958	35.951	ng/ul	-0.01
81) Pyrene-d10	19.622	212	1641920	37.774	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.651	264	1659546	38.014	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010274.D
Acq On : 10 May 2022 20:13
Operator : CG/JU
Sample : N2678-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/11/2022
Supervised By :mohammad ahmed 05/12/2022

Quant Time: May 11 01:19:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 10 15:59:46 2022
Response via : Initial Calibration

