

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010267.D
 Acq On : 10 May 2022 16:17
 Operator : CG/JU
 Sample : PB144574BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK574

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	52	rBV	20073	29964	0.93%	0.098%
2	3.770	112	116	139	rBV	248121	532971	16.51%	1.750%
3	4.093	167	171	176	rVB2	7551	11930	0.37%	0.039%
4	5.205	358	360	366	rBV7	2110	4621	0.14%	0.015%
5	7.075	671	678	693	rBV	339418	598475	18.54%	1.965%
6	7.240	699	706	716	rBV	290176	493698	15.29%	1.621%
7	7.440	732	740	750	rBV	372698	620770	19.23%	2.038%
8	7.911	813	820	832	rBV	340652	570511	17.67%	1.873%
9	8.616	933	940	952	rBV	464273	786565	24.36%	2.582%
10	9.069	1010	1017	1028	rBV	381545	667211	20.66%	2.191%
11	9.793	1132	1140	1152	rBV	316484	545841	16.91%	1.792%
12	9.934	1162	1164	1170	rVB7	2011	3404	0.11%	0.011%
13	10.334	1224	1232	1251	rVV	420947	779630	24.15%	2.560%
14	10.710	1289	1296	1306	rBV	493415	867785	26.88%	2.849%
15	10.852	1312	1320	1339	rBV	428581	855419	26.49%	2.808%
16	12.310	1560	1568	1575	rBV7	7676	17261	0.53%	0.057%
17	13.951	1839	1847	1857	rBV	1064345	1490936	46.18%	4.895%
18	14.046	1862	1863	1868	rVB5	2540	3730	0.12%	0.012%
19	14.234	1885	1895	1906	rBV	1056558	1534734	47.53%	5.039%
20	14.381	1914	1920	1927	rBV10	6969	18519	0.57%	0.061%
21	14.540	1940	1947	1960	rBV	867323	1306570	40.47%	4.290%
22	14.740	1973	1981	2007	rBV	340669	739804	22.91%	2.429%
23	14.951	2015	2017	2020	rBV4	3250	3901	0.12%	0.013%
24	15.363	2083	2087	2089	rBV5	2469	3254	0.10%	0.011%
25	15.534	2109	2116	2129	rBV	1423598	2062198	63.87%	6.770%
26	15.657	2130	2137	2152	rVV	474206	770485	23.86%	2.530%
27	15.775	2153	2157	2164	rVB2	15891	27854	0.86%	0.091%
28	16.322	2246	2250	2255	rVB7	5718	8720	0.27%	0.029%
29	16.969	2357	2360	2365	rBV7	3503	5402	0.17%	0.018%
30	17.292	2409	2415	2426	rBV	1181048	1704845	52.80%	5.597%
31	17.392	2426	2432	2446	rVV2	1630575	2386714	73.92%	7.836%
32	17.969	2526	2530	2532	rVB4	5491	6529	0.20%	0.021%
33	18.186	2562	2567	2570	rBV6	9791	17087	0.53%	0.056%
34	19.204	2736	2740	2745	rBV4	22162	29212	0.90%	0.096%
35	19.275	2749	2752	2757	rVV2	17817	23136	0.72%	0.076%
36	19.628	2806	2812	2819	rBV	2125808	3023920	93.65%	9.928%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010267.D
Acq On : 10 May 2022 16:17
Operator : CG/JU
Sample : PB144574BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Title : SVOA CALIBRATION

37	19.839	2839	2848	2849	rBV2	106518	236315	7.32%	0.776%
38	19.980	2868	2872	2873	rBV2	79782	88758	2.75%	0.291%
39	21.375	3104	3109	3125	rBV	1459701	2182685	67.60%	7.166%
40	23.657	3490	3497	3505	rBV	1604102	3228825	100.00%	10.601%
41	23.816	3517	3524	3535	rVB2	1076239	2168856	67.17%	7.121%


Sum of corrected areas: 30459045

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010267.D
Acq On : 10 May 2022 16:17
Operator : CG/JU
Sample : PB144574BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

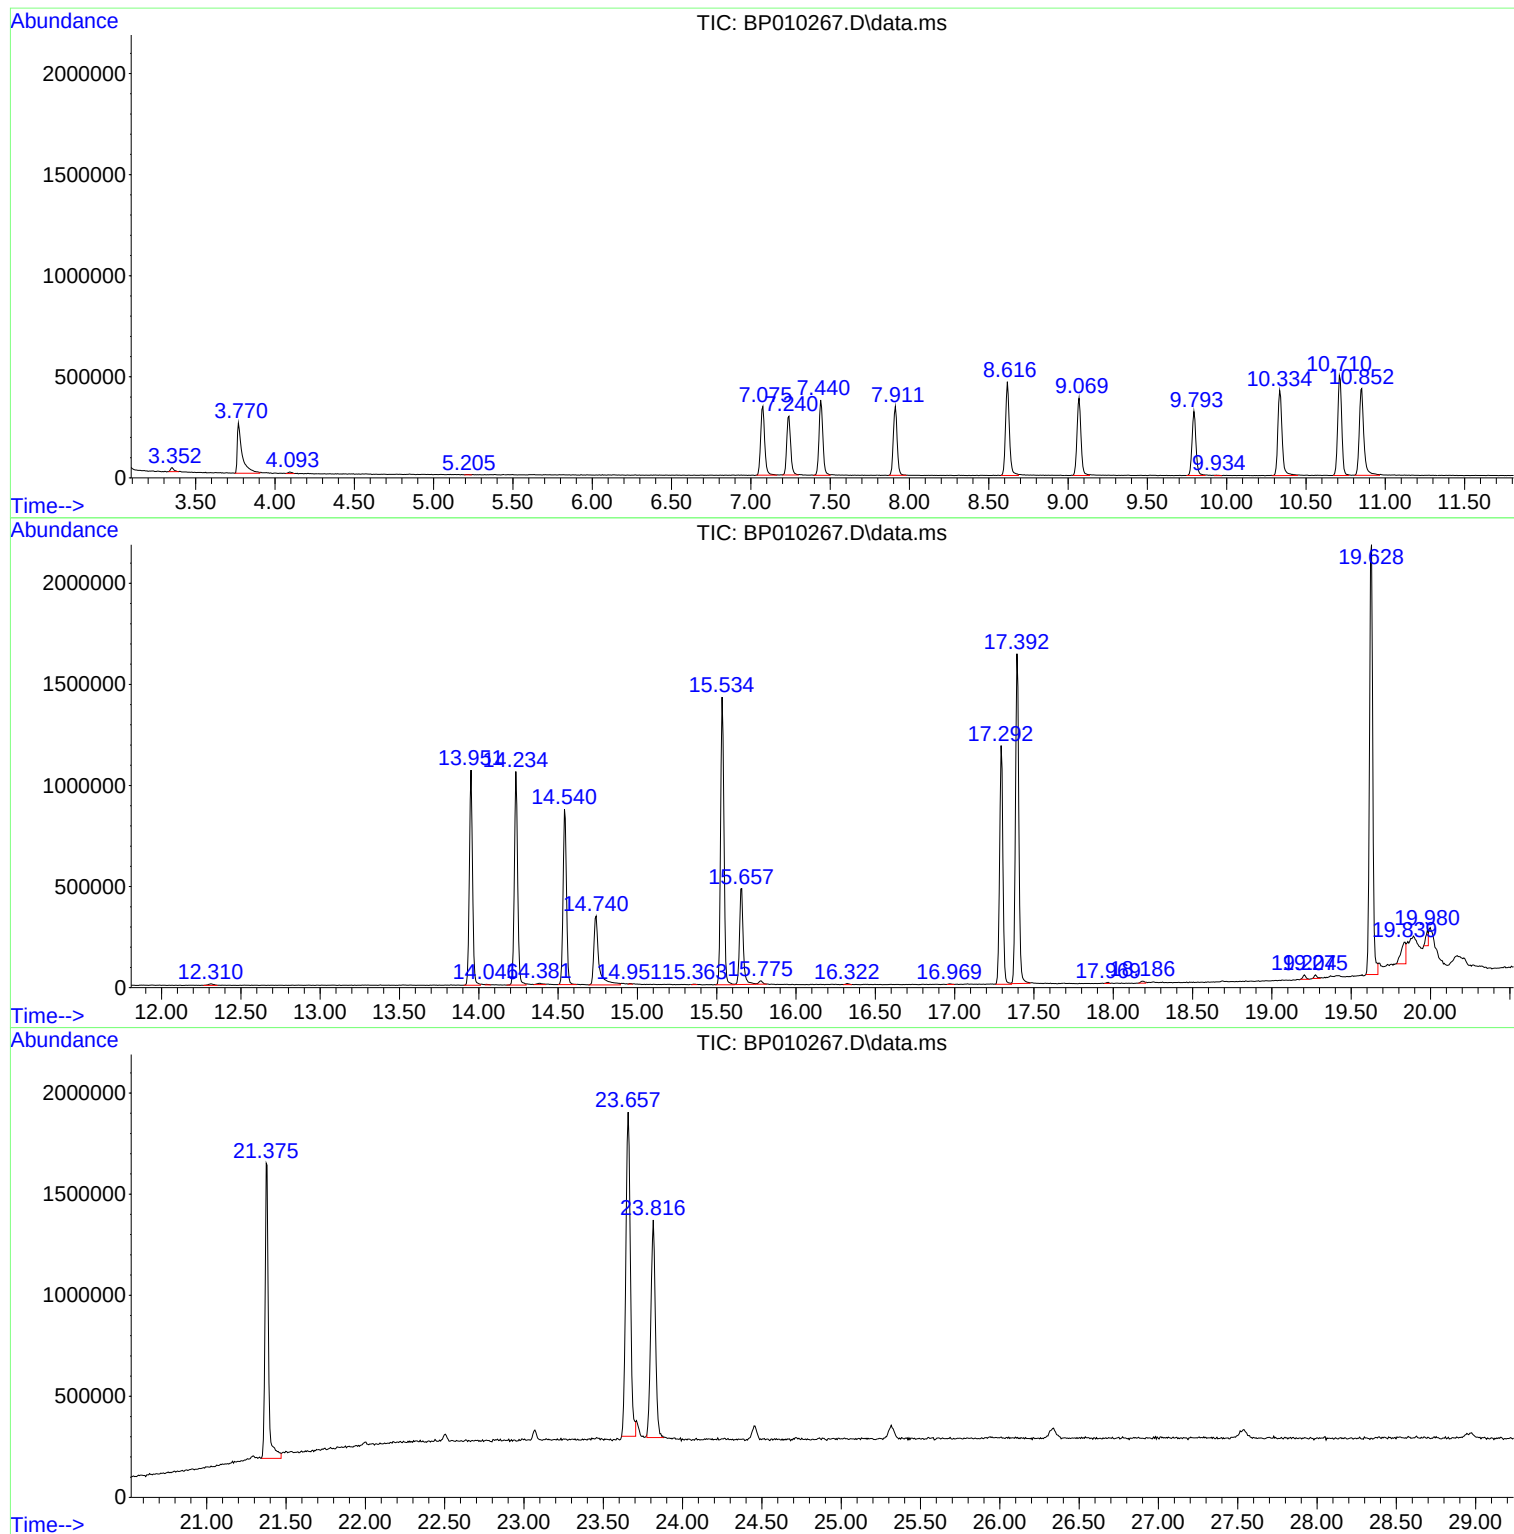

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010267.D
Acq On : 10 May 2022 16:17
Operator : CG/JU
Sample : PB144574BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 D:A-Friedooleanan-3-ol, (3.... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.839	2.17 ng/ul	236315	Chrysene-d12	21.380

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			D:A-Friedooleanan-3-ol, (3.alpha.)-	428	C30H52O	005085-72-3	96
2			N,N'-Dibenzylidene-3,3'-dichloro...	428	C26H18Cl2N2	010147-75-8	74
3			1-Zirconacyclopenta-2,4-diene, 2...	428	C26H26Zr	1000161-48-2	47
4			3,12-Diazatetrabenzof[a,cd,j,lm]p...	428	C32H16N2	095264-24-7	47
5			Naphthacene, 5,12-bis(phenylethy...	428	C34H20	018826-29-4	47

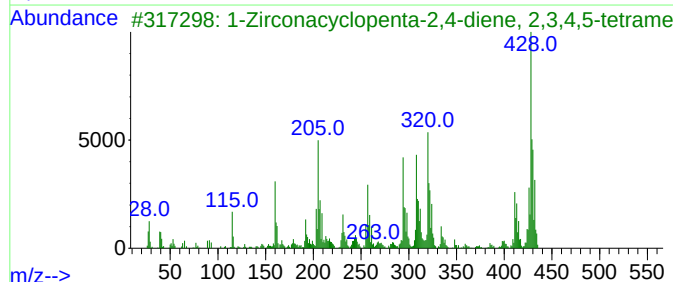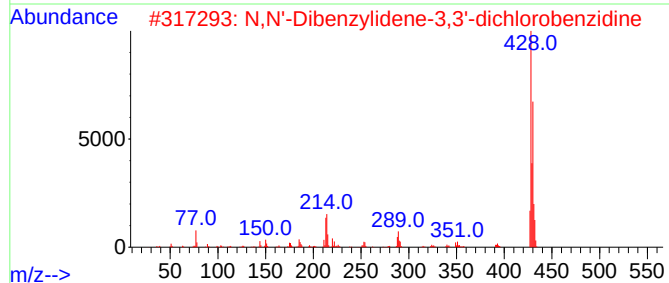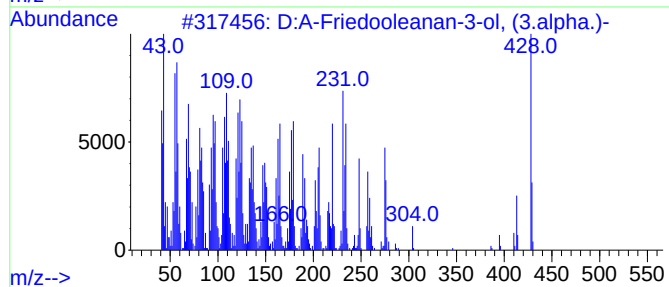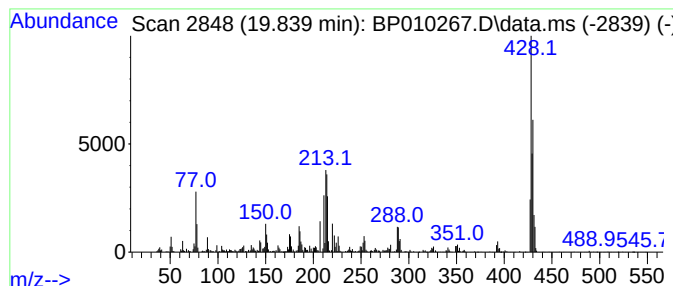

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010267.D
Acq On : 10 May 2022 16:17
Operator : CG/JU
Sample : PB144574BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK574

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
D:A-Friedoolean...	19.839	2.2	ng/u1	236315	5	21.380	2182690	20.0