

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010270.D
 Acq On : 10 May 2022 17:59
 Operator : CG/JU
 Sample : N2678-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	49	rBV	25301	33750	0.74%	0.090%
2	3.775	115	117	131	rBV	67471	151376	3.30%	0.403%
3	4.093	168	171	179	rVB4	7762	11592	0.25%	0.031%
4	5.016	322	328	332	rBV6	4592	9654	0.21%	0.026%
5	7.075	670	678	688	rBV	112336	207216	4.52%	0.551%
6	7.240	699	706	718	rBV	416828	712689	15.54%	1.897%
7	7.440	733	740	749	rBV	424236	701133	15.29%	1.866%
8	7.910	812	820	828	rBV	388950	640785	13.98%	1.705%
9	8.263	874	880	884	rBV8	3504	5524	0.12%	0.015%
10	8.616	931	940	954	rBV	349248	595545	12.99%	1.585%
11	8.840	974	978	982	rBV6	3873	5649	0.12%	0.015%
12	9.069	1008	1017	1030	rBV	570116	984608	21.48%	2.620%
13	9.310	1052	1058	1064	rVB	13398	24146	0.53%	0.064%
14	9.516	1089	1093	1098	rVB5	5971	9177	0.20%	0.024%
15	9.622	1106	1111	1118	rBV8	3734	6602	0.14%	0.018%
16	9.793	1133	1140	1148	rBV	454111	760399	16.59%	2.024%
17	10.334	1224	1232	1247	rBV	600970	1077530	23.50%	2.868%
18	10.510	1258	1262	1272	rBV5	11424	31196	0.68%	0.083%
19	10.710	1288	1296	1311	rVB	567402	959944	20.94%	2.555%
20	10.845	1311	1319	1332	rBV	340058	661041	14.42%	1.759%
21	11.375	1404	1409	1414	rVB8	5460	12041	0.26%	0.032%
22	11.493	1423	1429	1438	rBV6	6395	17419	0.38%	0.046%
23	11.569	1438	1442	1447	rVB5	4497	8999	0.20%	0.024%
24	11.851	1486	1490	1494	rBV5	6571	9172	0.20%	0.024%
25	12.298	1560	1566	1572	rBV3	11550	20079	0.44%	0.053%
26	13.151	1708	1711	1719	rVB9	4689	7791	0.17%	0.021%
27	13.951	1840	1847	1859	rBV	1535320	2172792	47.39%	5.783%
28	14.234	1884	1895	1907	rBV	1499856	2238048	48.82%	5.956%
29	14.375	1913	1919	1921	rBV7	6536	10328	0.23%	0.027%
30	14.416	1922	1926	1937	rVV	36129	63363	1.38%	0.169%
31	14.539	1941	1947	1957	rVV	960953	1415896	30.88%	3.768%
32	14.628	1960	1962	1969	rVB8	5822	8036	0.18%	0.021%
33	14.739	1975	1981	2001	rBV2	82824	215666	4.70%	0.574%
34	14.957	2012	2018	2032	rBV2	50151	86295	1.88%	0.230%
35	15.092	2039	2041	2044	rVB2	5606	5603	0.12%	0.015%
36	15.151	2047	2051	2055	rVB2	11398	12904	0.28%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
 Data File : BP010270.D
 Acq On : 10 May 2022 17:59
 Operator : CG/JU
 Sample : N2678-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0C1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	15.310	2074	2078	2081	rBV3	4084	4803	0.10%	0.013%
38	15.351	2081	2085	2090	rVV5	6543	11176	0.24%	0.030%
39	15.398	2090	2093	2096	rVV3	5449	5193	0.11%	0.014%
40	15.451	2099	2102	2109	rBV8	4983	9121	0.20%	0.024%
41	15.533	2109	2116	2130	rBV	2184047	3083242	67.25%	8.206%
42	15.651	2130	2136	2149	rVV	857243	1189632	25.95%	3.166%
43	15.775	2152	2157	2168	rVB5	25737	55209	1.20%	0.147%
44	15.969	2184	2190	2192	rBV7	5567	9739	0.21%	0.026%
45	16.110	2209	2214	2218	rBV7	3793	7512	0.16%	0.020%
46	16.251	2228	2238	2239	rBV9	5905	14803	0.32%	0.039%
47	16.322	2246	2250	2254	rVB6	8914	14021	0.31%	0.037%
48	16.433	2265	2269	2273	rBV7	4215	5975	0.13%	0.016%
49	16.969	2357	2360	2363	rBV5	3440	4797	0.10%	0.013%
50	17.063	2372	2376	2379	rBV6	3773	6875	0.15%	0.018%
51	17.292	2408	2415	2423	rBV	1244175	1803185	39.33%	4.799%
52	17.392	2425	2432	2453	rVB	2505229	3683277	80.34%	9.803%
53	17.622	2468	2471	2475	rVB3	6623	7031	0.15%	0.019%
54	17.680	2477	2481	2484	rBV6	3198	6423	0.14%	0.017%
55	17.963	2525	2529	2533	rVB7	13922	18961	0.41%	0.050%
56	18.175	2561	2565	2574	rBV	70429	117457	2.56%	0.313%
57	18.251	2575	2578	2582	rVB3	11007	16047	0.35%	0.043%
58	18.463	2611	2614	2618	rBV6	5656	8895	0.19%	0.024%
59	19.204	2736	2740	2743	rBV2	31056	40232	0.88%	0.107%
60	19.269	2747	2751	2755	rBV	29764	45773	1.00%	0.122%
61	19.410	2771	2775	2780	rBV4	40214	63379	1.38%	0.169%
62	19.621	2805	2811	2818	rBV	3186342	4505055	98.26%	11.990%
63	21.080	3056	3059	3064	rBV2	105561	140738	3.07%	0.375%
64	21.374	3104	3109	3125	rBV	1554742	2117570	46.19%	5.636%
65	23.657	3489	3497	3504	rBV2	2195663	4584695	100.00%	12.202%
66	23.810	3517	3523	3534	rVB2	1002151	2099941	45.80%	5.589%


Sum of corrected areas: 37574745

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010270.D
Acq On : 10 May 2022 17:59
Operator : CG/JU
Sample : N2678-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

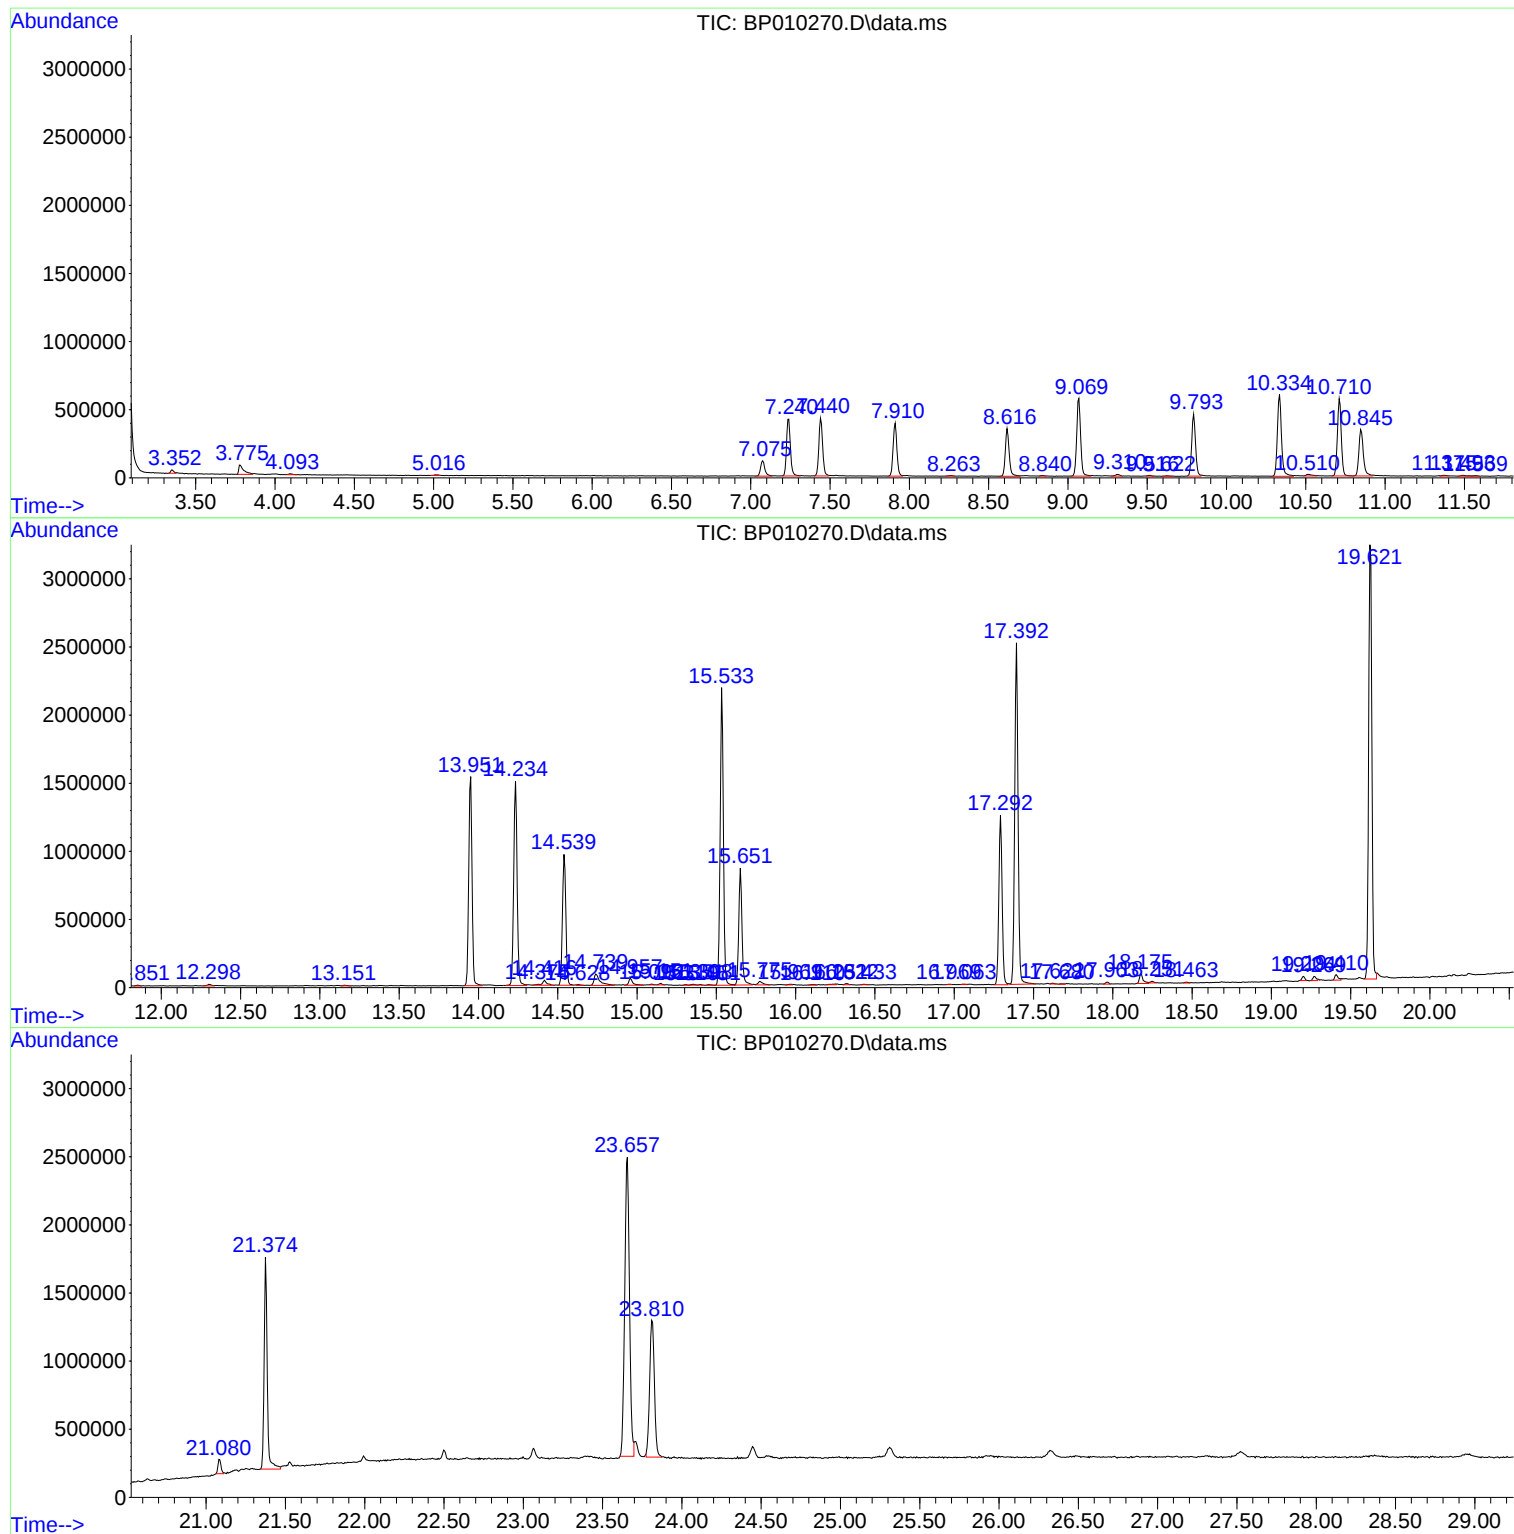

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010270.D
Acq On : 10 May 2022 17:59
Operator : CG/JU
Sample : N2678-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051022\
Data File : BP010270.D
Acq On : 10 May 2022 17:59
Operator : CG/JU
Sample : N2678-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0C1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc