

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051023\
 Data File : BP015048.D
 Acq On : 10 May 2023 18:17
 Operator : CG/JU
 Sample : 02591-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREB5

Quant Time: May 10 23:00:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 10 15:17:56 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.146	152	256334	20.000	ng/ul	0.00
20) Naphthalene-d8	10.981	136	1128289	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.787	164	695804	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.539	188	1379056	20.000	ng/ul	0.00
79) Chrysene-d12	21.621	240	822209	20.000	ng/ul	0.00
88) Perylene-d12	24.198	264	980967	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.452	96	15004	2.176	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.293	99	279897	12.595	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.463	67	173114	12.603	ng/ul	0.00
11) 2-Chlorophenol-d4	7.669	132	229400	14.038	ng/ul	0.00
15) 4-Methylphenol-d8	8.857	113	226733	13.239	ng/ul	0.00
21) Nitrobenzene-d5	9.322	128	111076	13.842	ng/ul	0.00
24) 2-Nitrophenol-d4	10.051	143	122719	14.893	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.593	165	232550	14.373	ng/ul	0.00
31) 4-Chloroaniline-d4	11.116	131	95127	4.065	ng/ul	0.00
46) Dimethylphthalate-d6	14.187	166	756241	15.357	ng/ul	0.00
49) Acenaphthylene-d8	14.481	160	858327	14.533	ng/ul	0.00
54) 4-Nitrophenol-d4	14.969	143	56935	6.646	ng/ul	0.00
60) Fluorene-d10	15.781	176	639380	15.091	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.892	200	71139	9.164	ng/ul	0.00
73) Anthracene-d10	17.639	188	891668	14.390	ng/ul	0.00
81) Pyrene-d10	19.857	212	869794	15.685	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.027	264	695830	14.558	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.981	105	54438	1.944	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.504	149	114427	4.202	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051023\
Data File : BP015048.D
Acq On : 10 May 2023 18:17
Operator : CG/JU
Sample : 02591-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREB5

Quant Time: May 10 23:00:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 10 15:17:56 2023
Response via : Initial Calibration




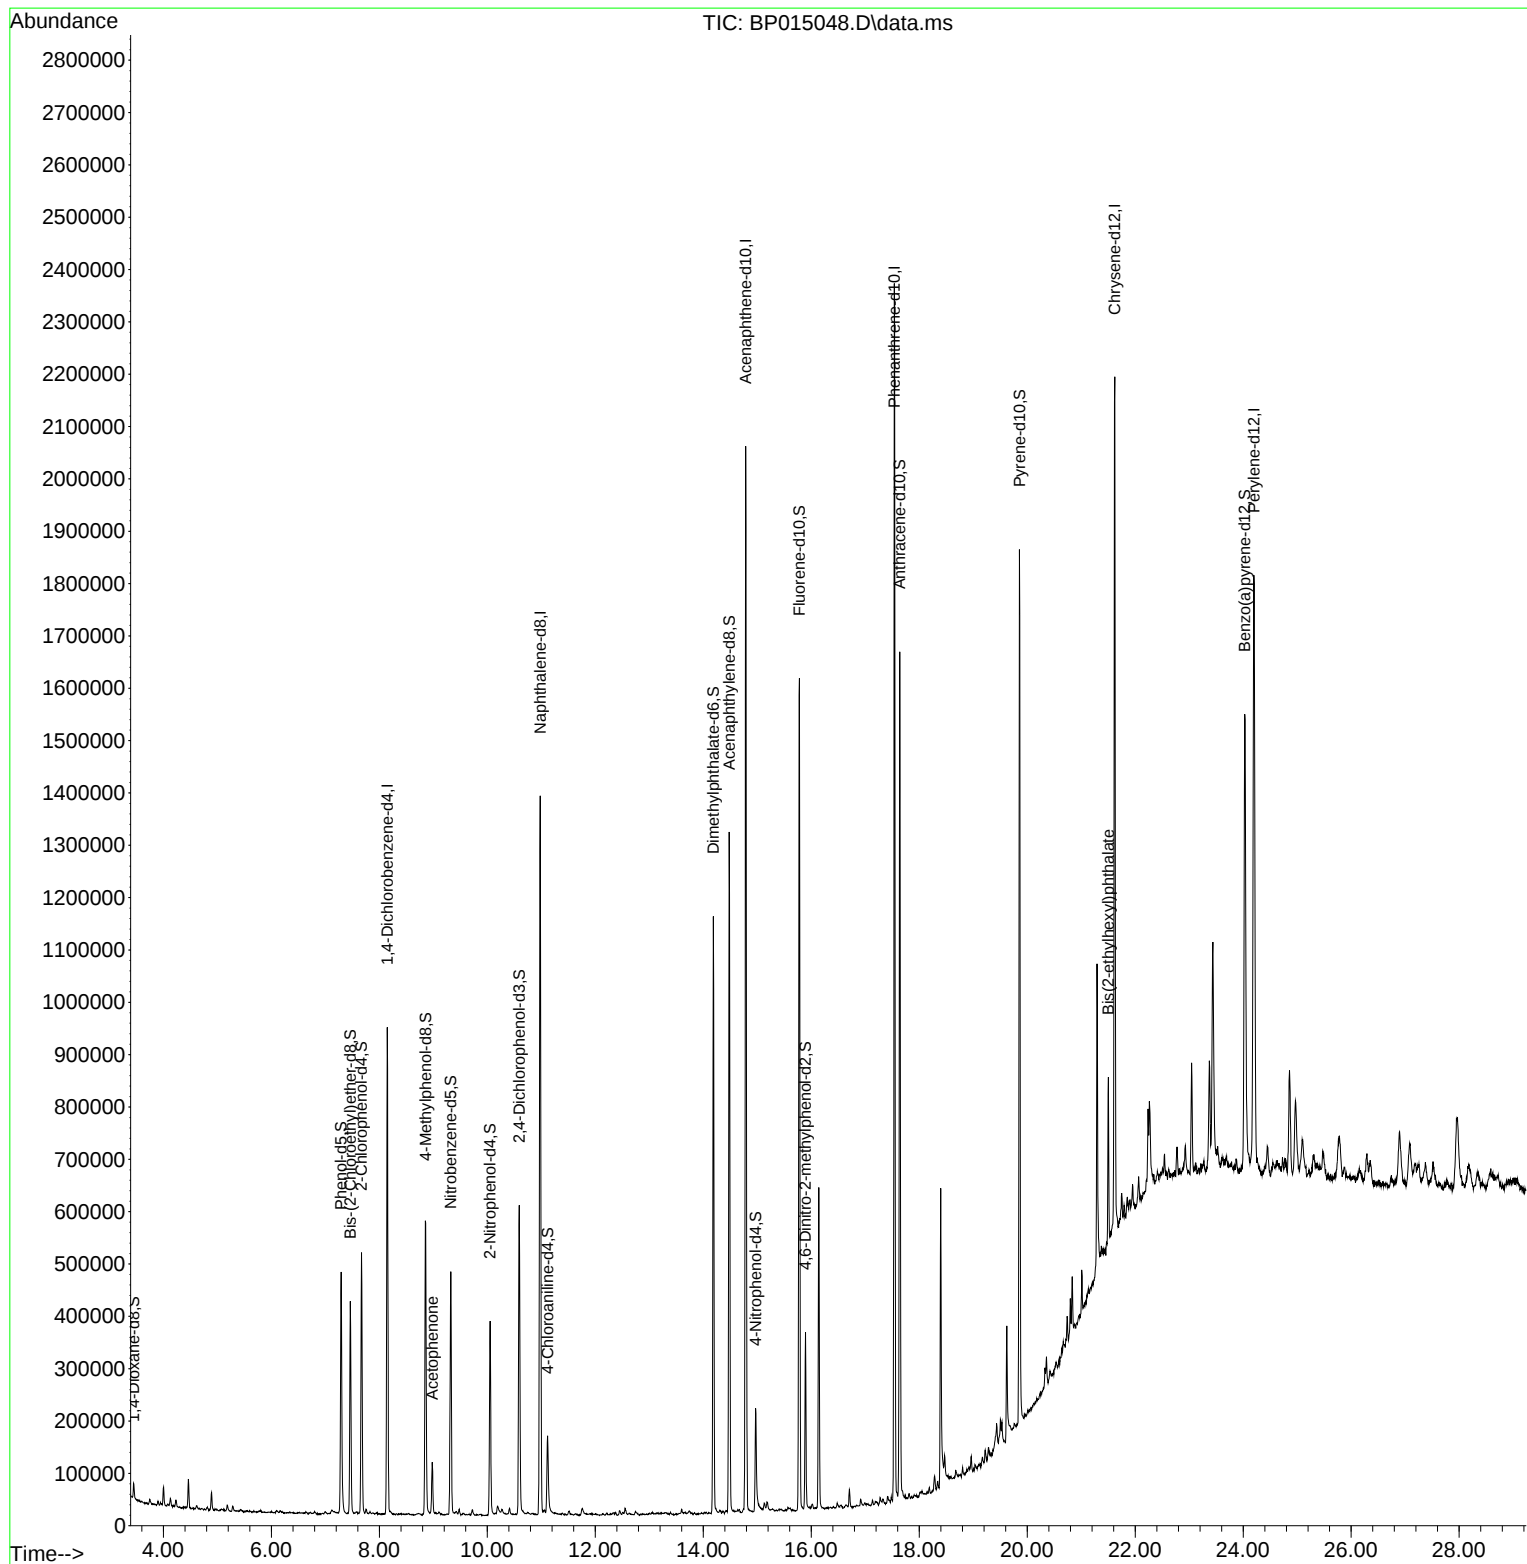


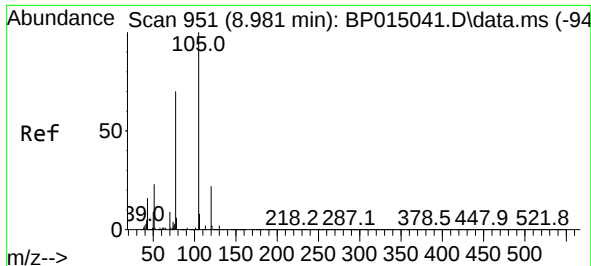

#16
Acetophenone
Concen: 1.944 ng/ul
RT: 8.981 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP015048.D
Acq: 10 May 2023 18:17

Instrument :
BNA_P
ClientSampleId :
JREB5

Tgt Ion:105 Resp: 54438
Ion Ratio Lower Upper
105 100
77 73.1 61.2 91.8
51 23.6 19.4 29.2

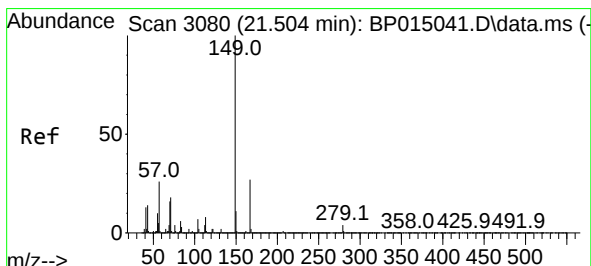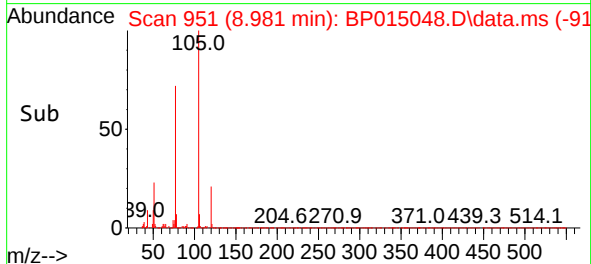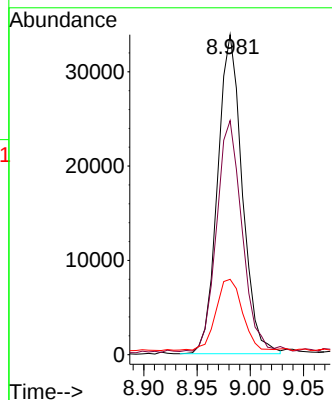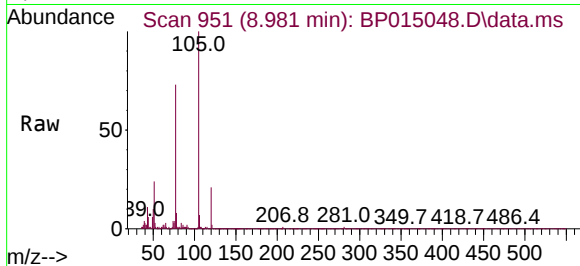

#86
Bis(2-ethylhexyl)phthalate
Concen: 4.202 ng/ul
RT: 21.504 min Scan# 3080
Delta R.T. 0.000 min
Lab File: BP015048.D
Acq: 10 May 2023 18:17

Tgt Ion:149 Resp: 114427
Ion Ratio Lower Upper
149 100
167 29.0 22.0 33.0
279 4.9 2.9 4.3#

