




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020284.D
Acq On : 10 May 2024 09:38
Operator : MA/JU
Sample : PB160761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK761

Manual IntegrationsAPPROVED

Quant Time: May 10 11:04:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

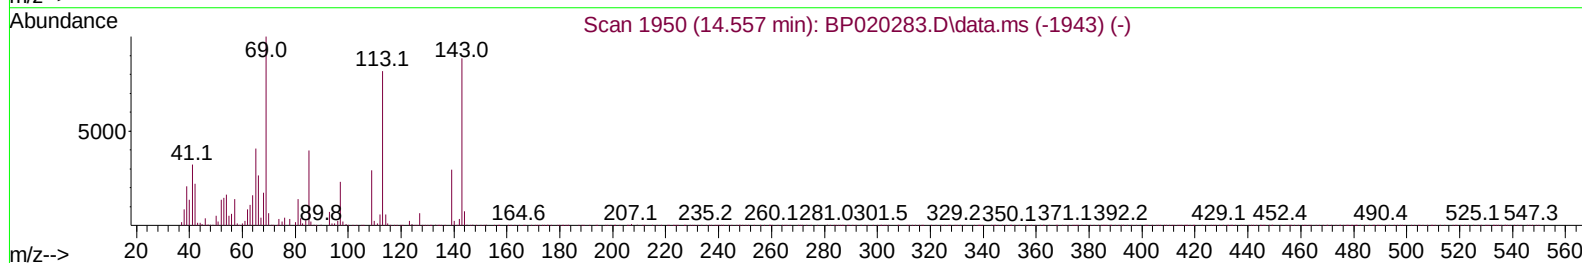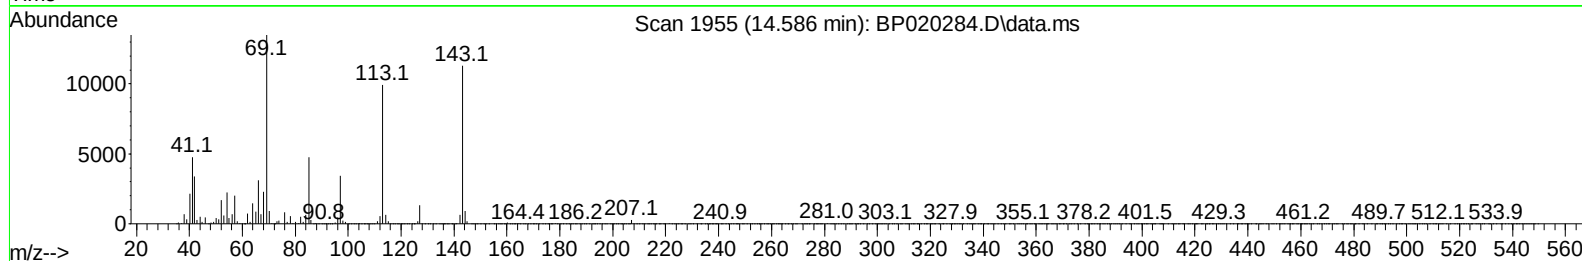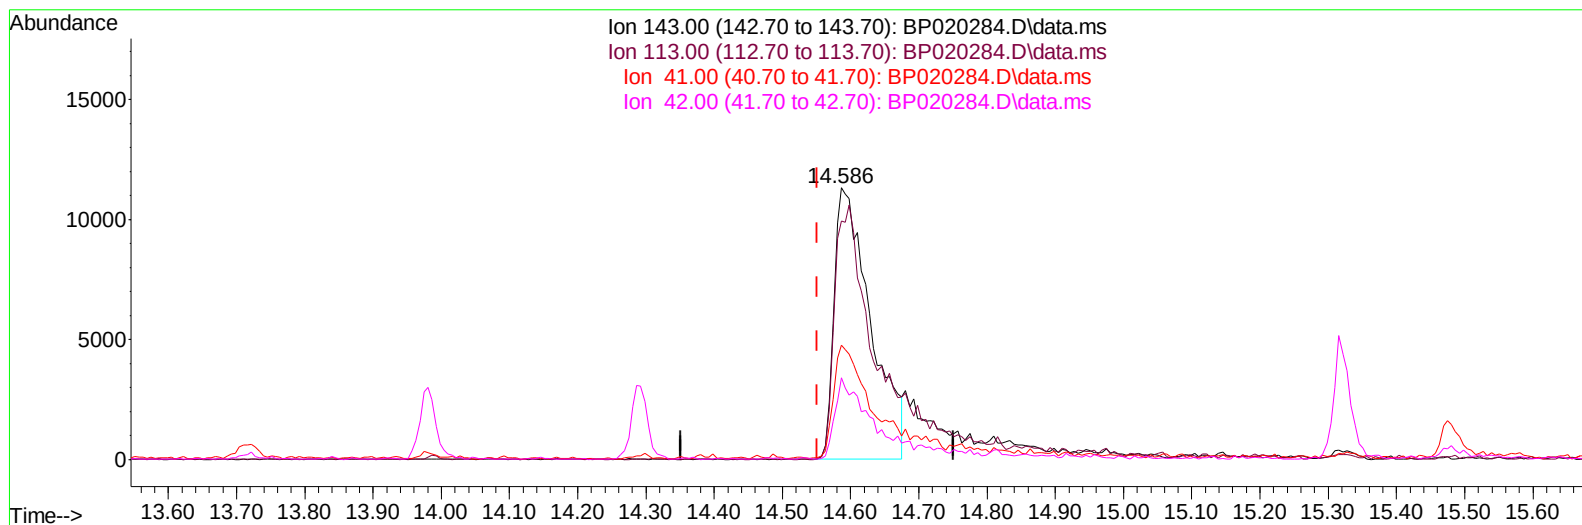

TIC: BP020284.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.035) 24.07 ng/ul

response 42079

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	87.88
41.00	50.30	42.10
42.00	32.50	30.01




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020284.D
Acq On : 10 May 2024 09:38
Operator : MA/JU
Sample : PB160761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK761

Manual IntegrationsAPPROVED

Quant Time: May 10 11:04:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

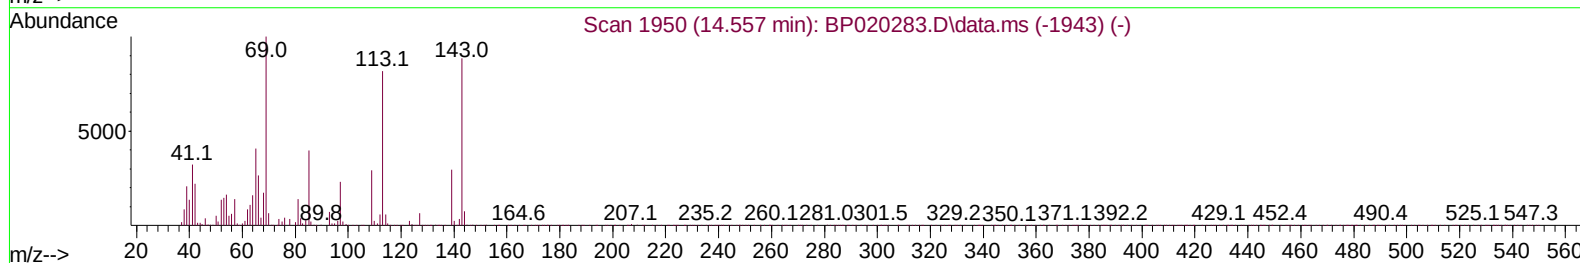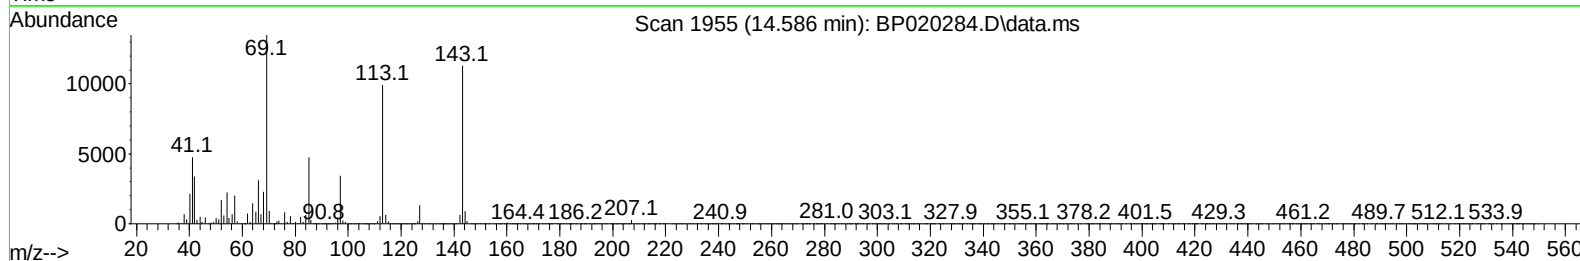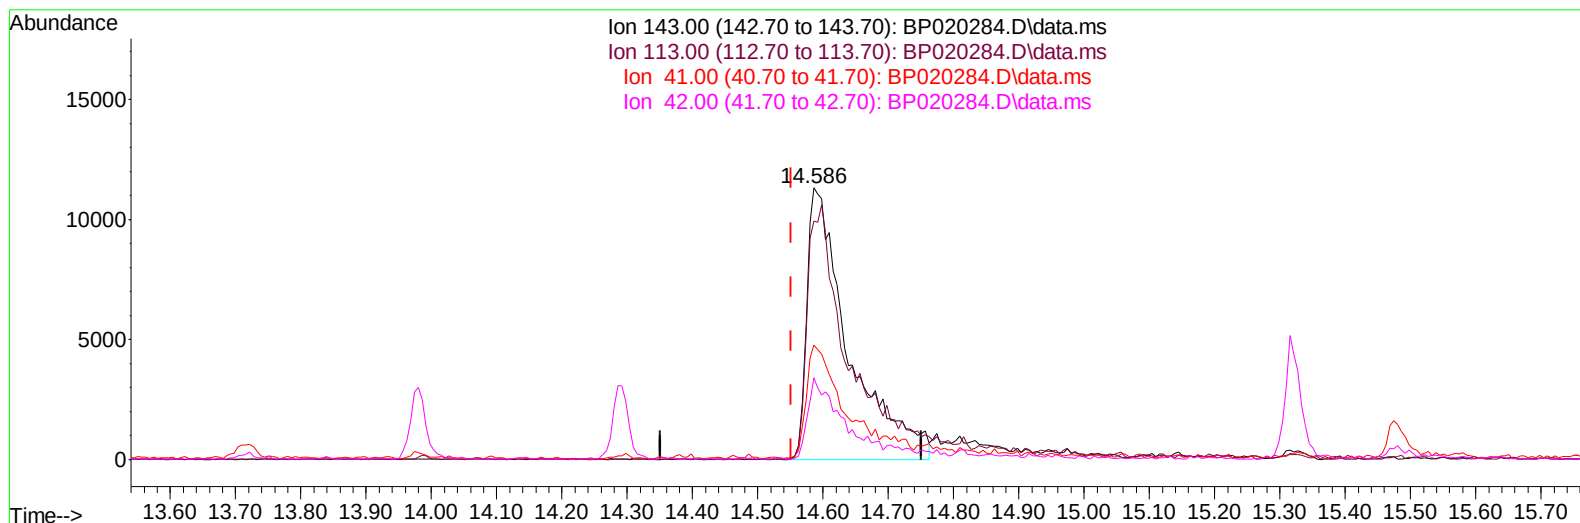

TIC: BP020284.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.035) 28.85 ng/ul m

response 50449

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	87.88
41.00	50.30	42.10
42.00	32.50	30.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020284.D
 Acq On : 10 May 2024 09:38
 Operator : MA/JU
 Sample : PB160761BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK761

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

Quant Time: May 10 11:05:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	57345	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	228881	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.292	164	155788	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	368211	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240	395412	20.000	ng/ul	0.00
88) Perylene-d12	25.003	264	453276	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.216	96	7802	5.746	ng/uL	0.00
4) Pyridine-d5	3.616	84	97551	24.726	ng/ul	0.00
7) Phenol-d5	6.810	99	127512	25.892	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	76226	25.480	ng/ul	0.00
11) 2-Chlorophenol-d4	7.151	132	105408	29.941	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	105335	26.456	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	49149	28.676	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	55971	28.517	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.034	165	94590	26.410	ng/ul	0.01
31) 4-Chloroaniline-d4	10.557	131	143108	28.548	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	359890	31.634	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	380231	30.256	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	50449m	28.853	ng/ul	0.04
60) Fluorene-d10	15.322	176	308647	32.527	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	40669	17.405	ng/ul	0.00
73) Anthracene-d10	17.239	188	530487	33.303	ng/ul	0.00
81) Pyrene-d10	19.639	212	680388	29.436	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.780	264	719278	32.819	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020284.D
Acq On : 10 May 2024 09:38
Operator : MA/JU
Sample : PB160761BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK761

Manual IntegrationsAPPROVED

Quant Time: May 10 11:05:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

