




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020303.D
 Acq On : 10 May 2024 23:45
 Operator : MA/JU
 Sample : P2370-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43P9

Manual IntegrationsAPPROVED

Quant Time: May 11 00:28:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

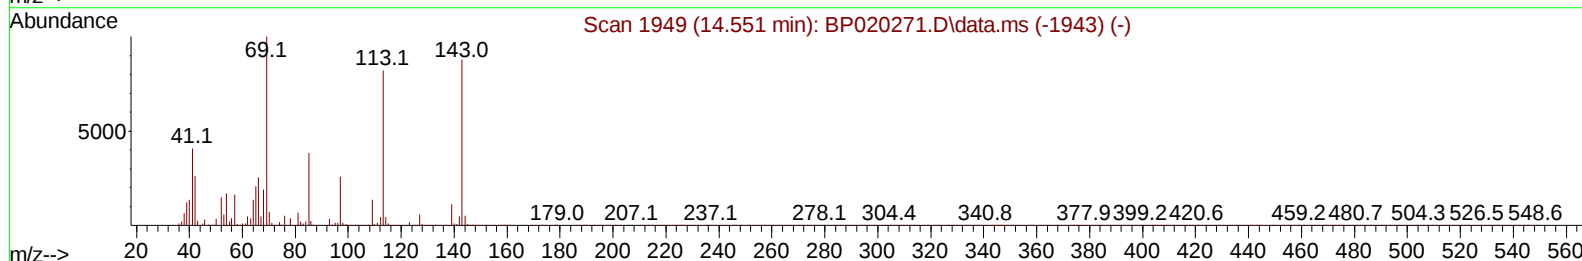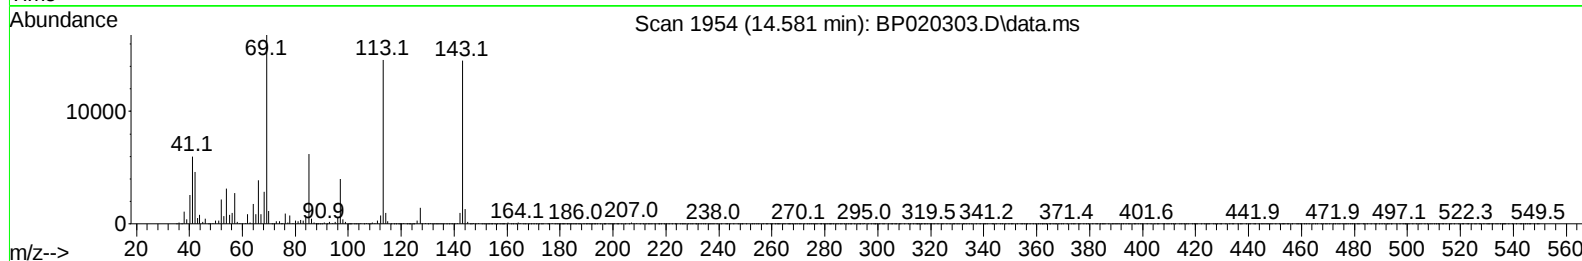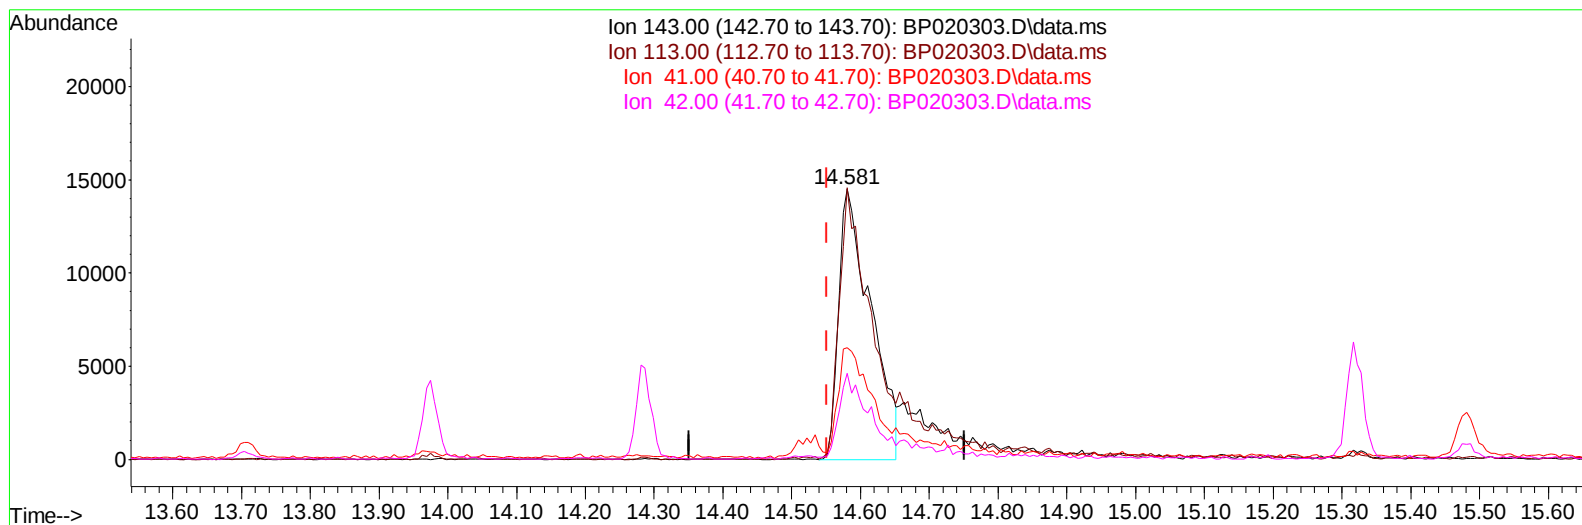

TIC: BP020303.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.029) 19.51 ng/u1

response 46978

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	100.39
41.00	50.30	41.31
42.00	32.50	31.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020303.D
Acq On : 10 May 2024 23:45
Operator : MA/JU
Sample : P2370-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43P9

Manual IntegrationsAPPROVED

Quant Time: May 11 00:28:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

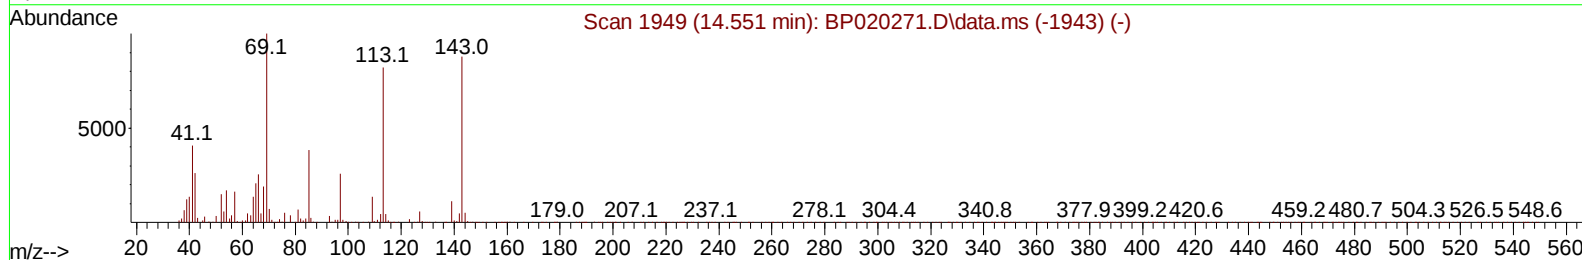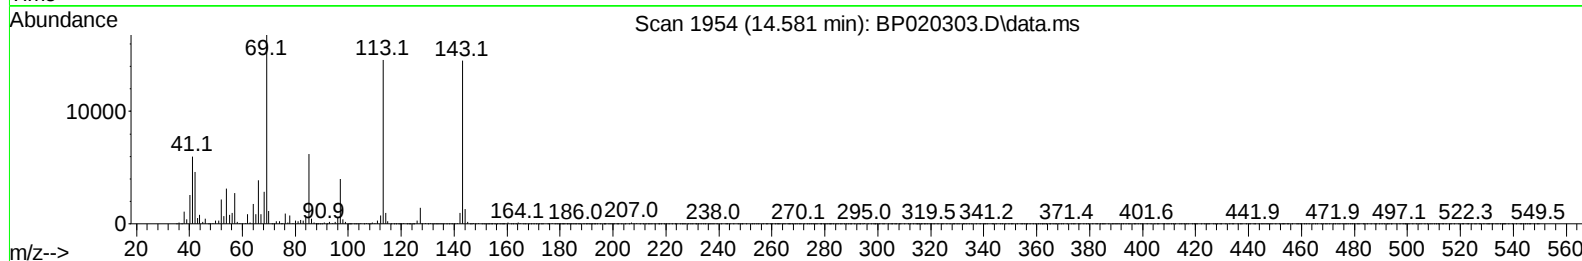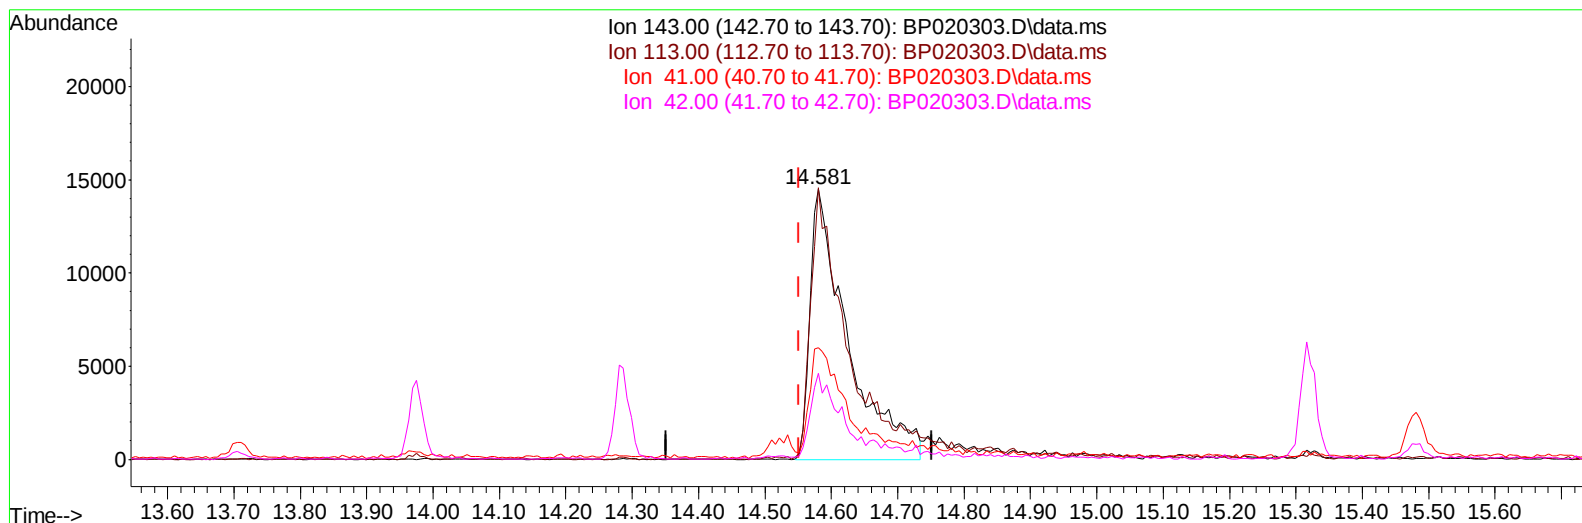

TIC: BP020303.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.029) 23.75 ng/ul m

response 57180

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	100.39
41.00	50.30	41.31
42.00	32.50	31.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020303.D
 Acq On : 10 May 2024 23:45
 Operator : MA/JU
 Sample : P2370-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43P9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

Quant Time: May 11 00:29:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.616	152		76213	20.000	ng/ul	0.00
20) Naphthalene-d8	10.381	136		310622	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.287	164		214488	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.134	188		477491	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240		461267	20.000	ng/ul	0.00
88) Perylene-d12	25.010	264		503826	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.217	96		8075	4.475	ng/uL	0.00
4) Pyridine-d5	3.622	84		103414	19.722	ng/ul	0.00
7) Phenol-d5	6.805	99		158297	24.186	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67		95494	24.018	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132		125037	26.723	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113		125583	23.733	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128		62350	26.805	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143		70836	26.593	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165		127244	26.178	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131		166950	24.540	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166		450310	28.749	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160		493487	28.521	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143		57180m	23.753	ng/ul	0.03
60) Fluorene-d10	15.322	176		387593	29.668	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200		57872	19.100	ng/ul	0.00
73) Anthracene-d10	17.233	188		611747	29.615	ng/ul	-0.01
81) Pyrene-d10	19.633	212		752687	27.915	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.768	264		739013	30.336	ng/ul	0.00
Target Compounds							
						Qvalue	
71) Pentachlorophenol	16.781	266		26286	7.260	ng/ul	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020303.D
Acq On : 10 May 2024 23:45
Operator : MA/JU
Sample : P2370-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43P9

Manual IntegrationsAPPROVED

Quant Time: May 11 00:29:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

