




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020315.D
Acq On : 11 May 2024 09:15
Operator : MA/JU
Sample : P2374-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0Y33

Manual IntegrationsAPPROVED

Quant Time: May 12 23:09:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

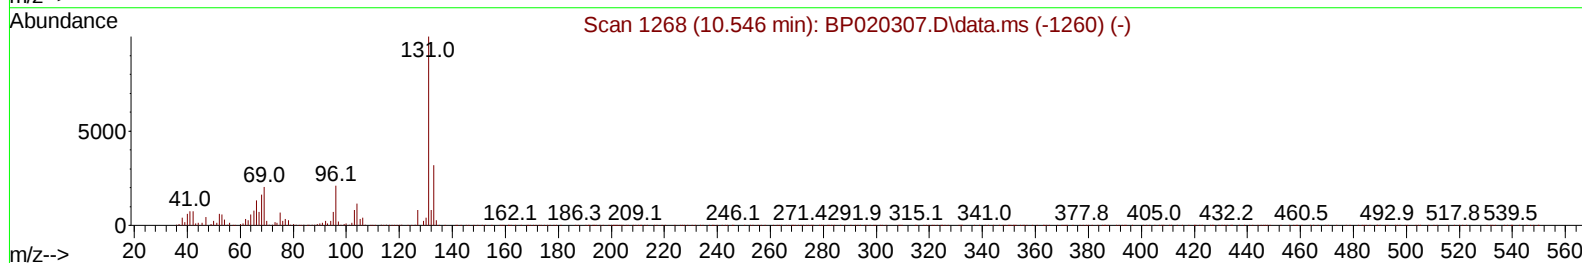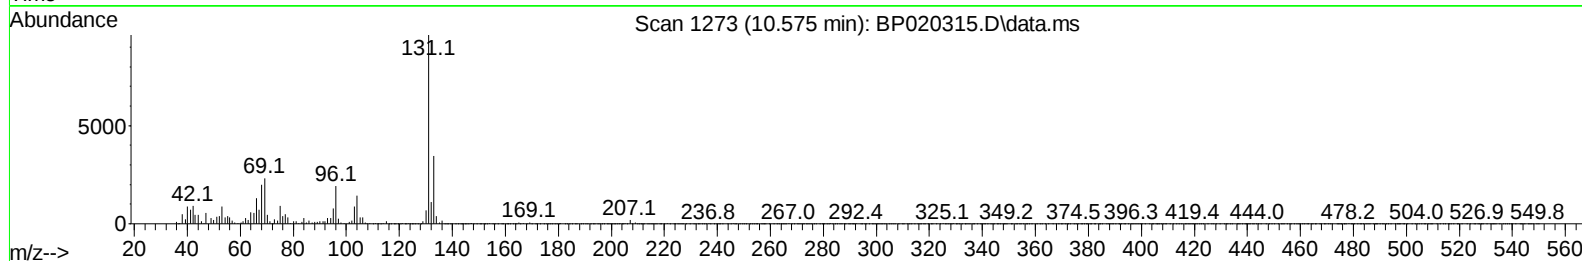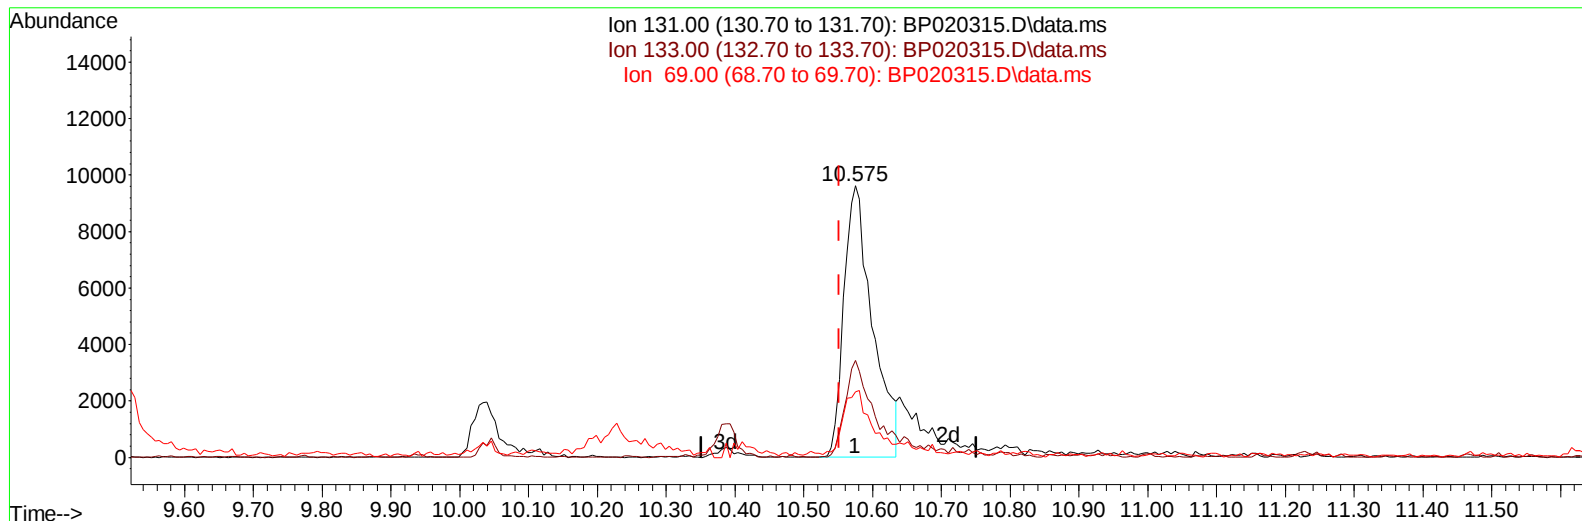

TIC: BP020315.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.575min (+ 0.023) 4.40 ng/u1

response 27987

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.40	35.84
69.00	20.50	24.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020315.D
Acq On : 11 May 2024 09:15
Operator : MA/JU
Sample : P2374-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0Y33

Manual IntegrationsAPPROVED

Quant Time: May 12 23:09:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

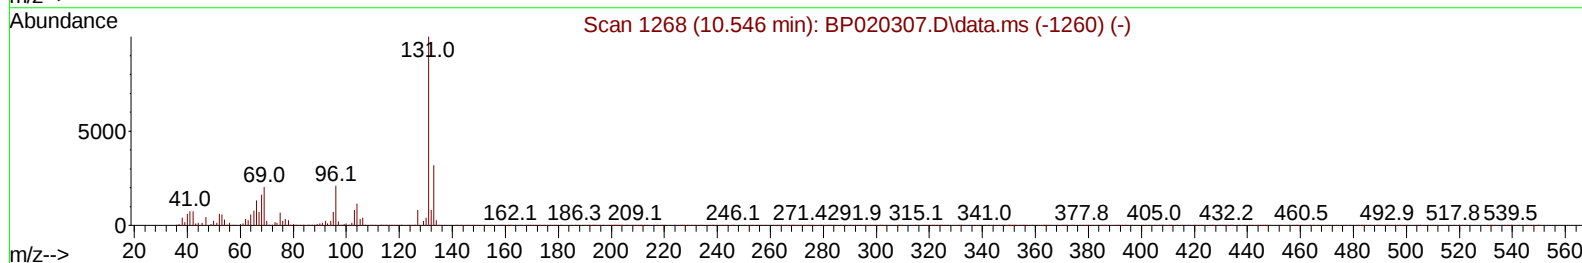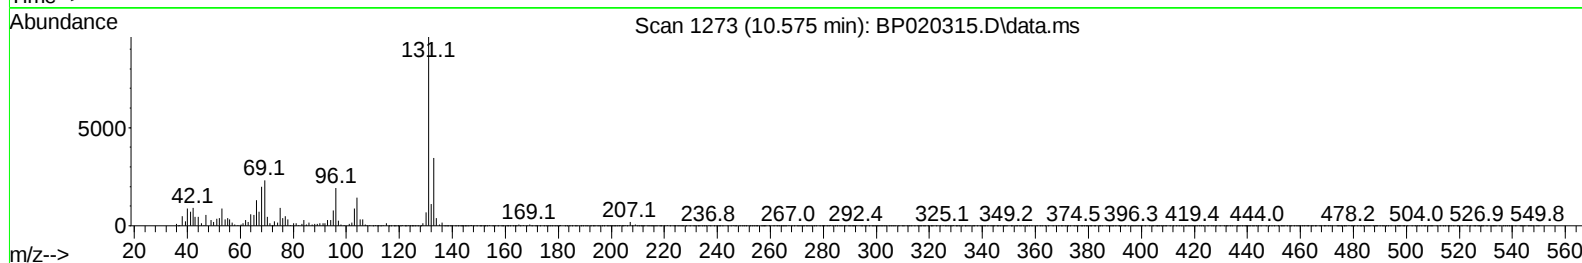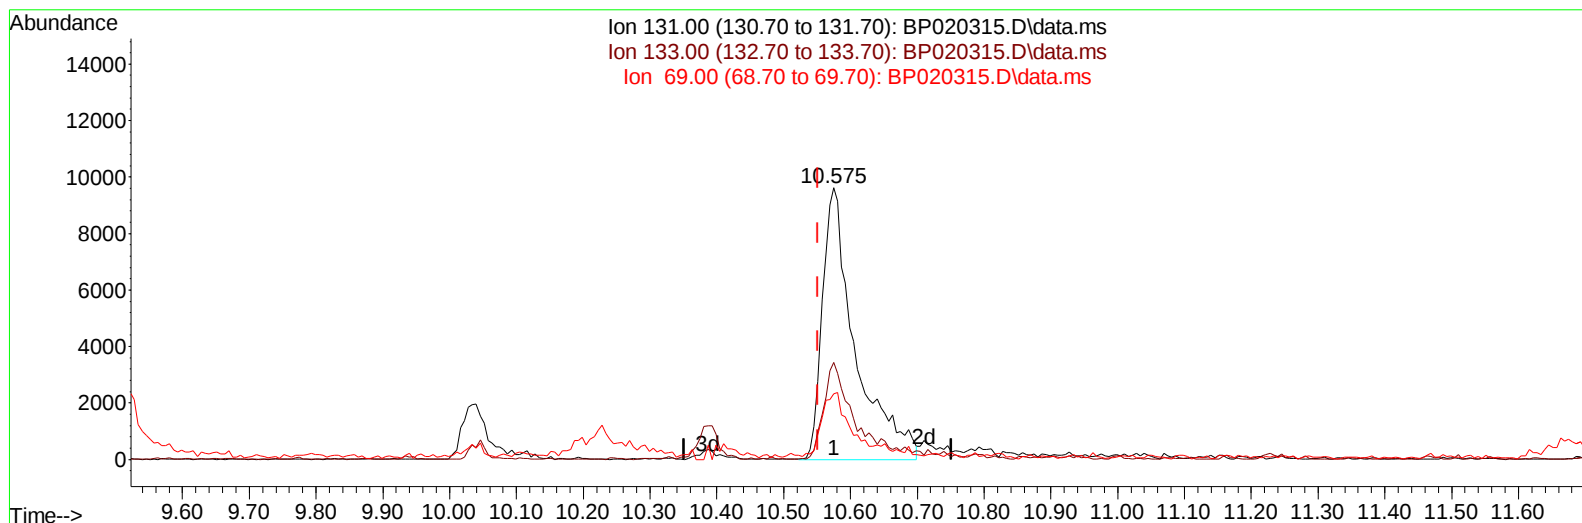

TIC: BP020315.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.575min (+ 0.023) 5.15 ng/ul m

response 32810

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.40	35.84
69.00	20.50	24.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020315.D
 Acq On : 11 May 2024 09:15
 Operator : MA/JU
 Sample : P2374-03 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0Y33

Manual IntegrationsAPPROVED

Quant Time: May 12 23:09:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

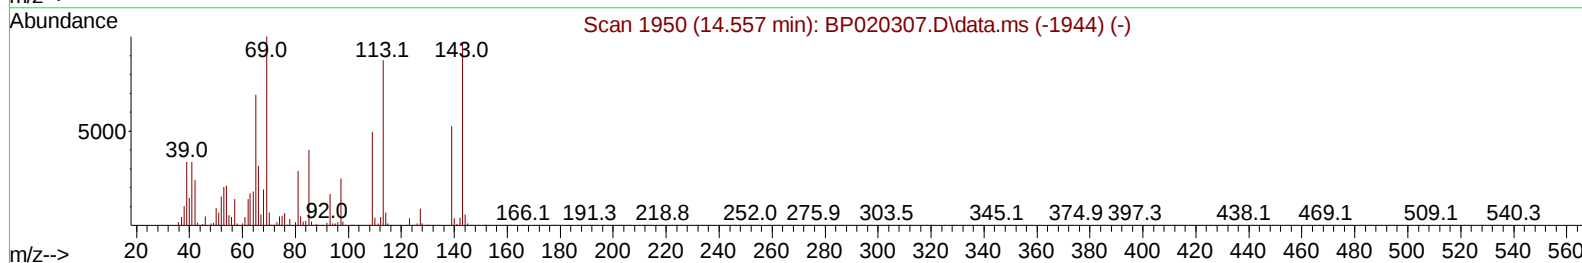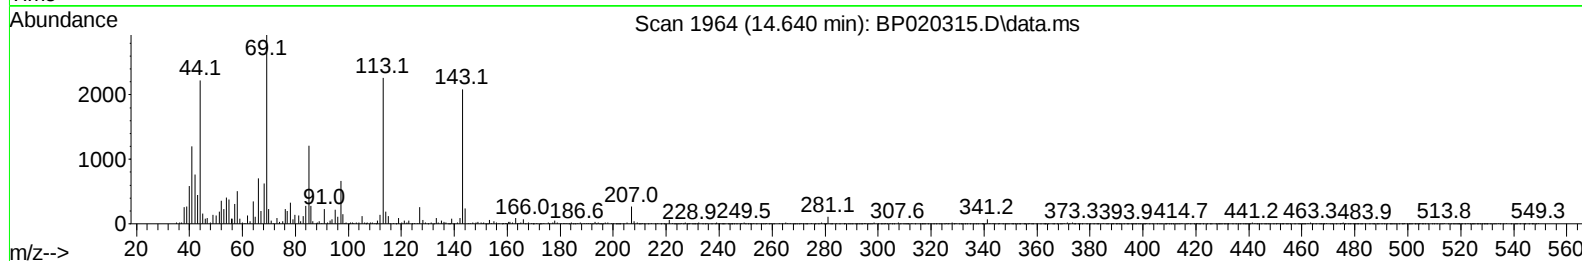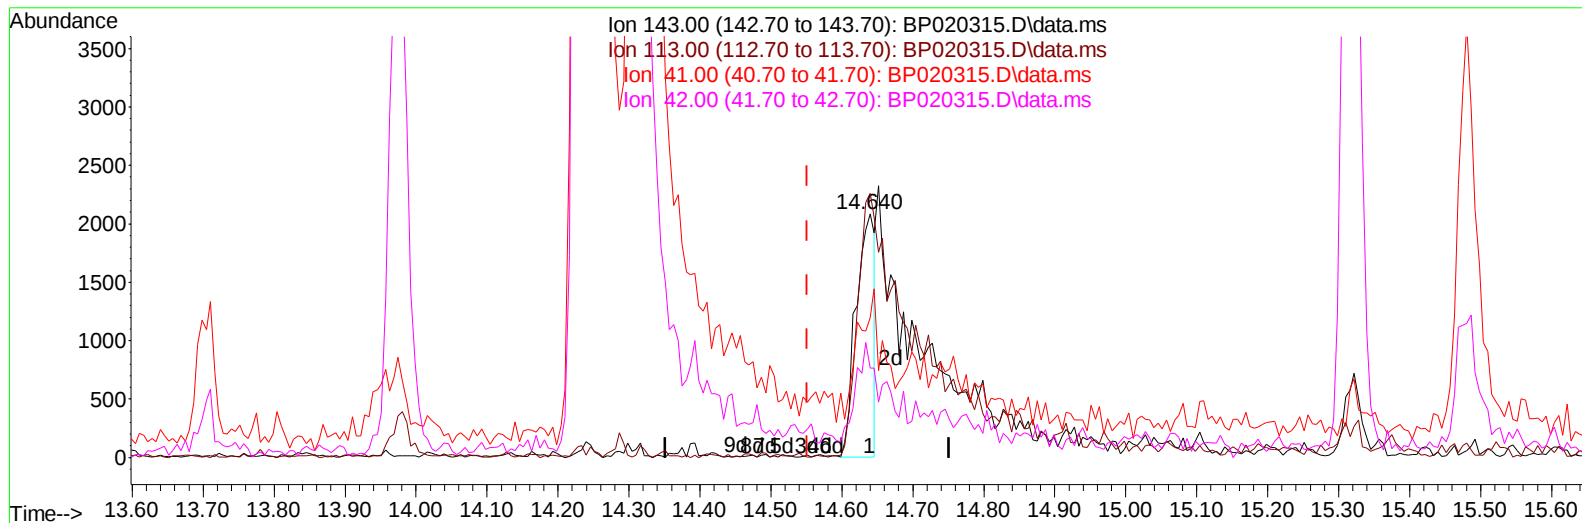

TIC: BP020315.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.640min (+ 0.088) 1.62 ng/u1

response 3793

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	108.59
41.00	50.30	57.39
42.00	32.50	36.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020315.D
Acq On : 11 May 2024 09:15
Operator : MA/JU
Sample : P2374-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0Y33

Manual IntegrationsAPPROVED

Quant Time: May 12 23:09:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

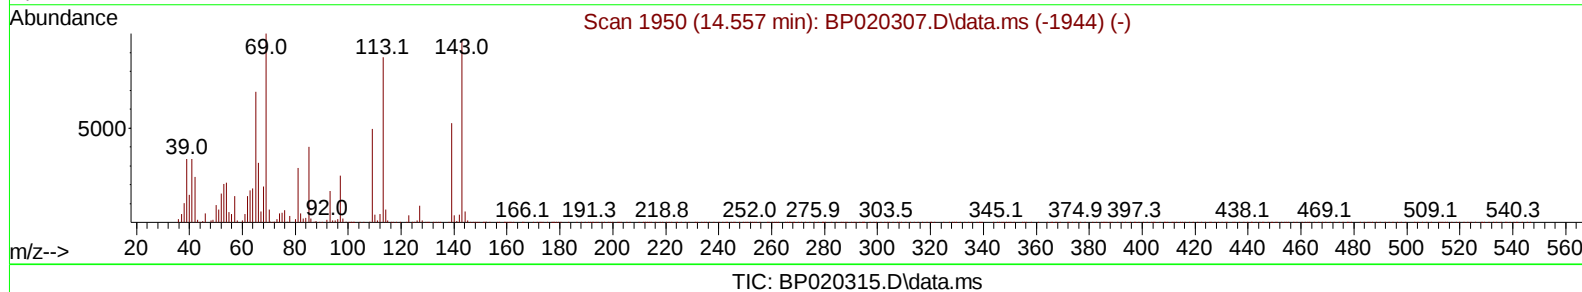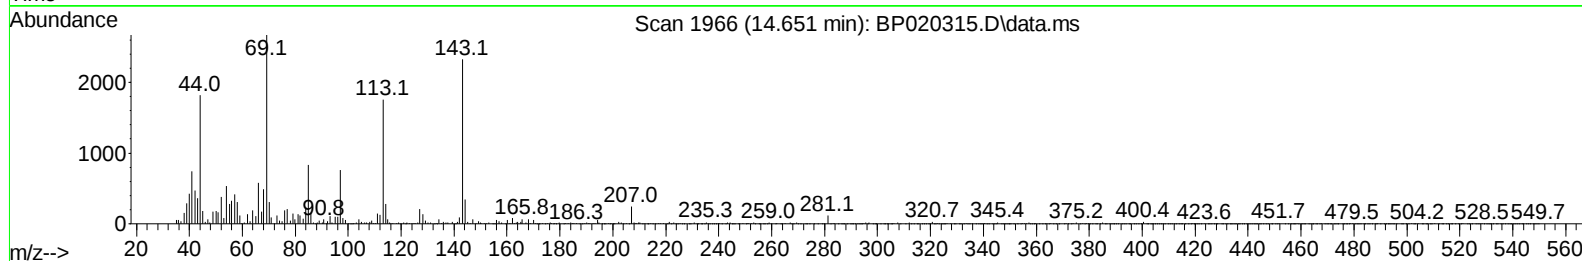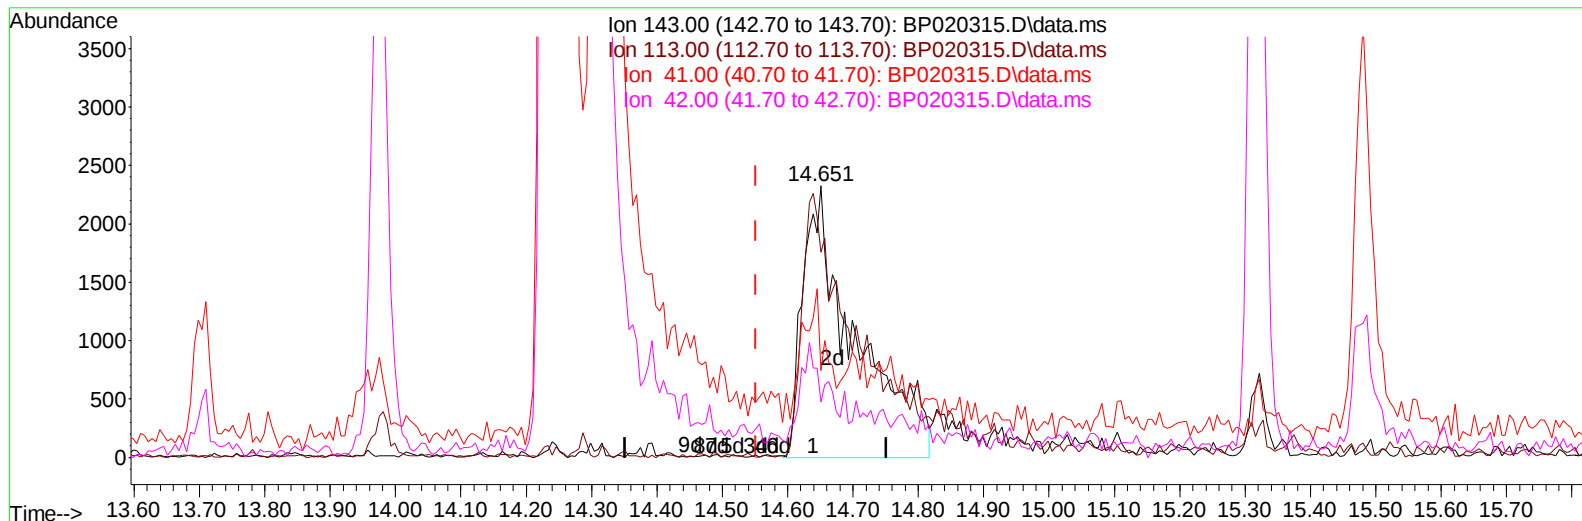

(54) 4-Nitrophenol-d4 (S)

14.651min (+ 0.100) 5.51 ng/ul m

response 12906

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	75.65#
41.00	50.30	31.88#
42.00	32.50	20.40#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020315.D
 Acq On : 11 May 2024 09:15
 Operator : MA/JU
 Sample : P2374-03 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0Y33

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

Quant Time: May 12 23:24:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	71804	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	290641	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.292	164	208620	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	486273	20.000	ng/ul	-0.01
79) Chrysene-d12	21.633	240	489121	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	530971	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	3449	2.029	ng/uL	0.00
4) Pyridine-d5	3.628	84	45982	9.308	ng/ul	0.01
7) Phenol-d5	6.822	99	38043	6.169	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.969	67	112344	29.991	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132	116398	26.405	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	78310	15.708	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	75838	34.846	ng/ul	0.00
24) 2-Nitrophenol-d4	9.487	143	81330	32.632	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	146940	32.308	ng/ul	0.00
31) 4-Chloroaniline-d4	10.575	131	32810m	5.154	ng/ul	0.02
46) Dimethylphthalate-d6	13.704	166	559670	36.736	ng/ul	0.00
49) Acenaphthylene-d8	13.975	160	595659	35.394	ng/ul	0.00
54) 4-Nitrophenol-d4	14.651	143	12906m	5.512	ng/ul	0.10
60) Fluorene-d10	15.322	176	481561	37.897	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	80289	26.019	ng/ul	0.00
73) Anthracene-d10	17.239	188	816725	38.824	ng/ul	0.00
81) Pyrene-d10	19.633	212	991861	34.691	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.762	264	981853	38.244	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020315.D
Acq On : 11 May 2024 09:15
Operator : MA/JU
Sample : P2374-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0Y33

Manual IntegrationsAPPROVED

Quant Time: May 12 23:24:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

