




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020341.D
Acq On : 12 May 2024 05:35
Operator : MA/JU
Sample : P2371-20
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43T2

Manual IntegrationsAPPROVED

Quant Time: May 13 00:28:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 13 00:21:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

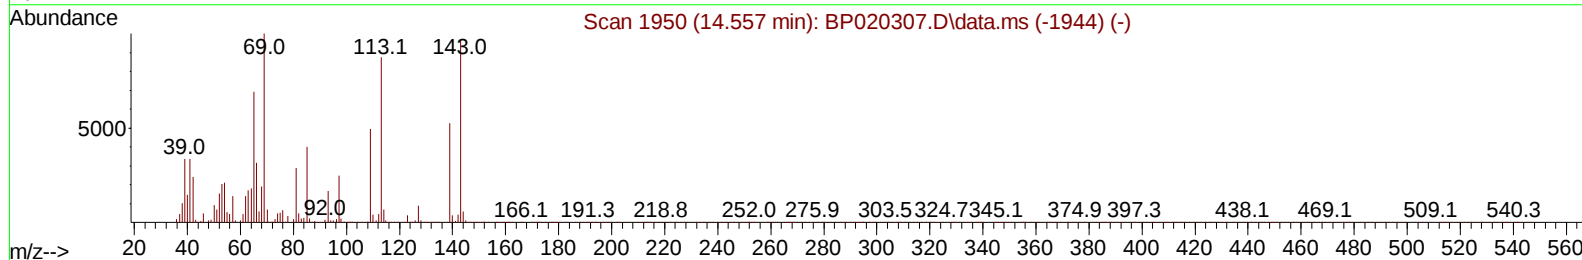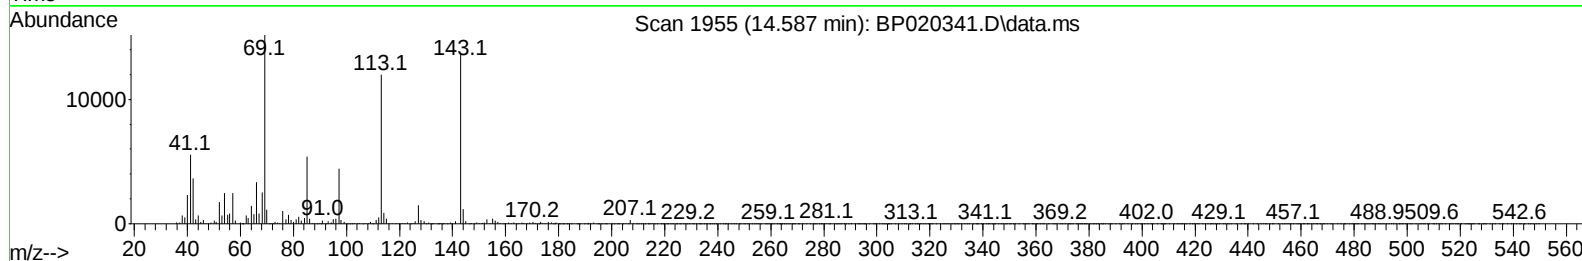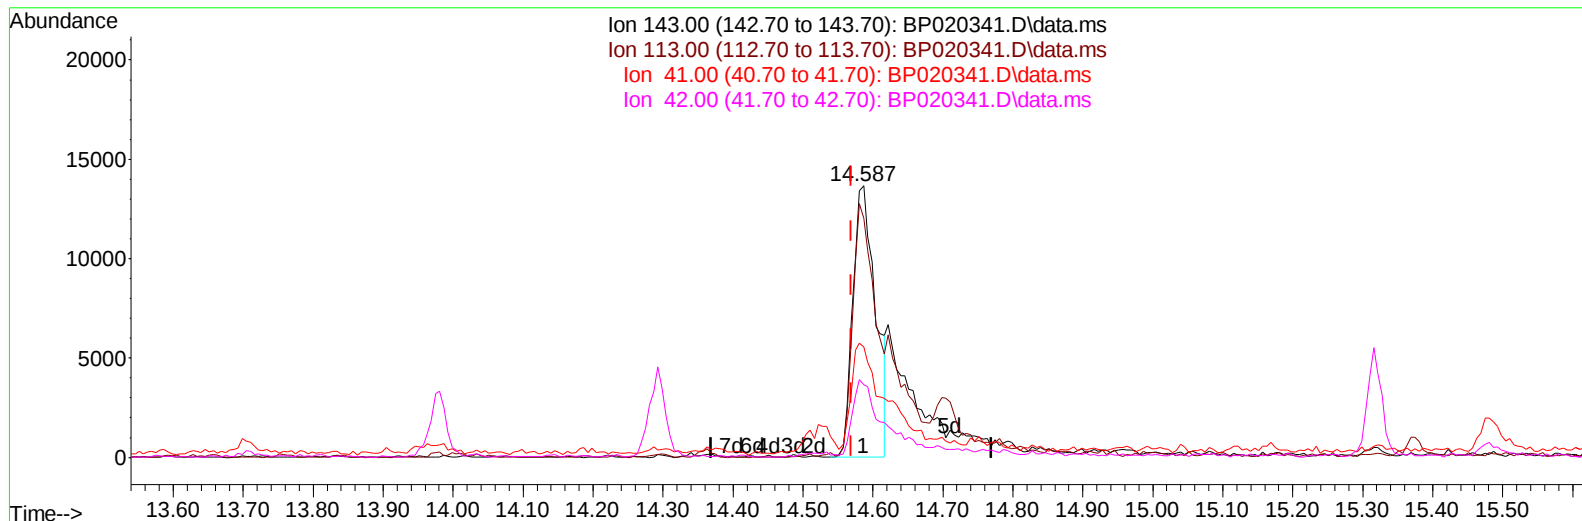

TIC: BP020341.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.018) 12.54 ng/u1

response 30609

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	87.95
41.00	50.30	40.71
42.00	32.50	26.84




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020341.D
 Acq On : 12 May 2024 05:35
 Operator : MA/JU
 Sample : P2371-20
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T2

Manual IntegrationsAPPROVED

Quant Time: May 13 00:28:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 13 00:21:03 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

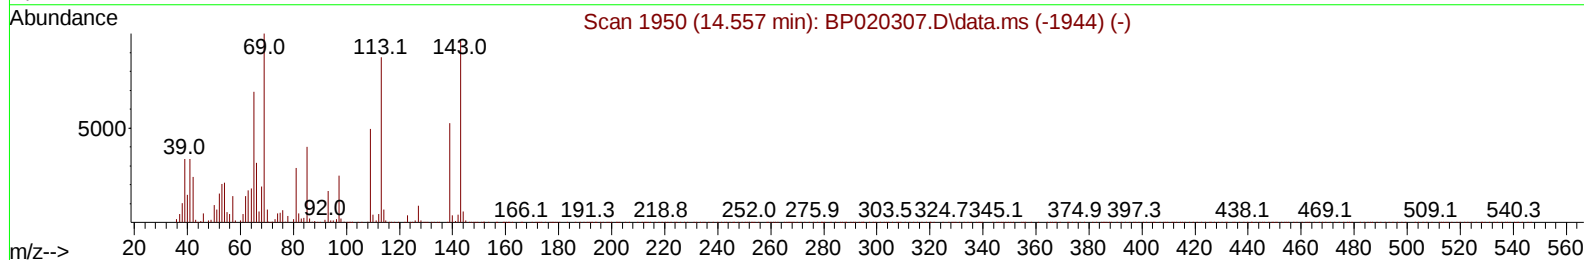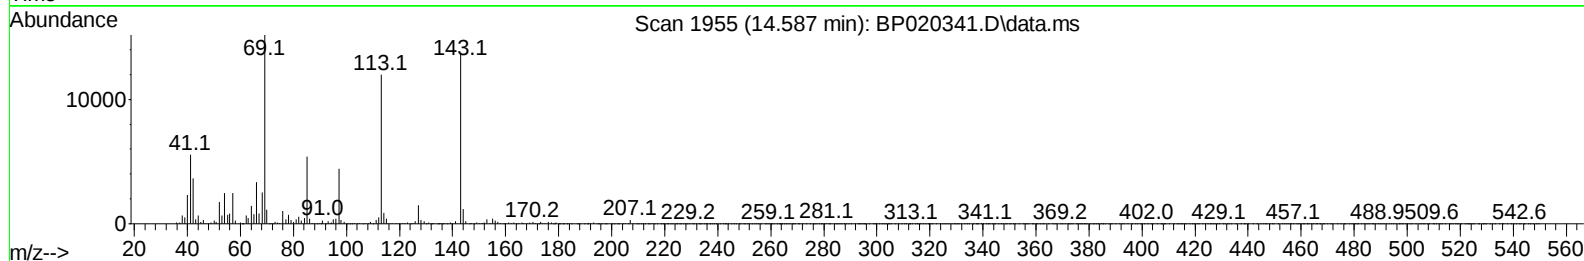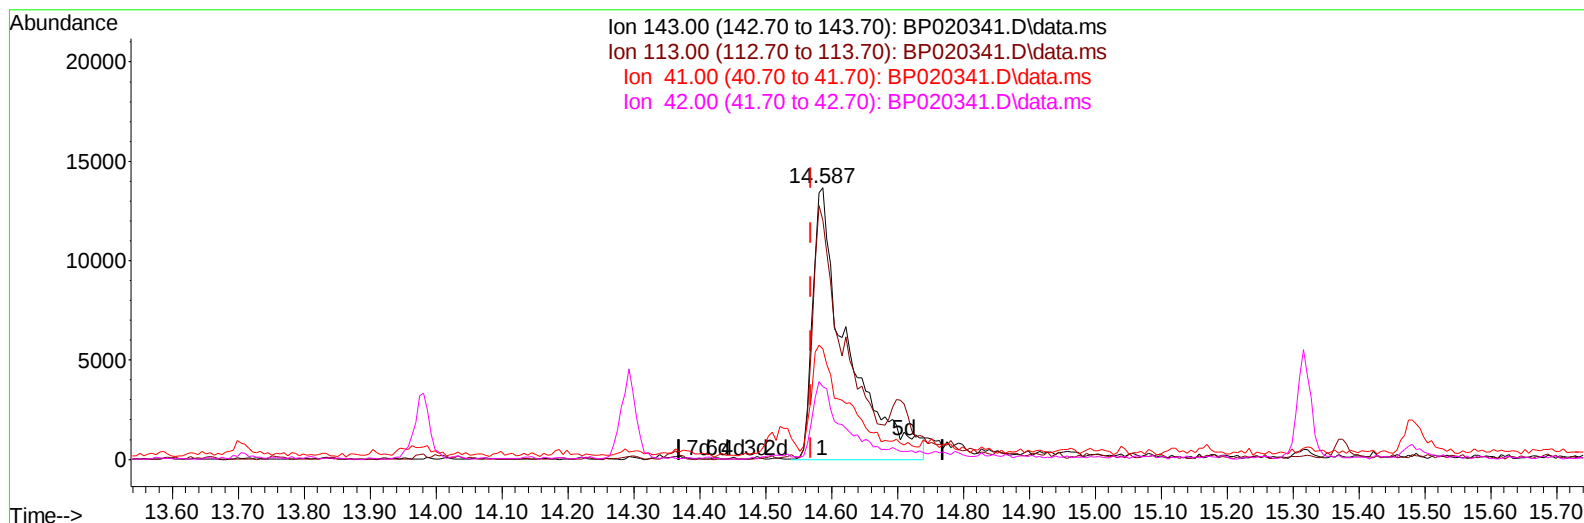

TIC: BP020341.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.587min (+ 0.018) 20.39 ng/ul m

response 49788

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	87.95
41.00	50.30	40.71
42.00	32.50	26.84

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020341.D
 Acq On : 12 May 2024 05:35
 Operator : MA/JU
 Sample : P2371-20
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/13/2024
 Supervised By :mohammad ahmed 05/14/2024

Quant Time: May 13 01:31:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon May 13 00:21:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	78356	20.000	ng/ul	0.00
20) Naphthalene-d8	10.381	136	316426	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.293	164	217541	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	496467	20.000	ng/ul	0.00
79) Chrysene-d12	21.616	240	497978	20.000	ng/ul	0.00
88) Perylene-d12	24.980	264	571720	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	5982	3.224	ng/uL	0.00
4) Pyridine-d5	3.623	84	44773	8.305	ng/ul	0.00
7) Phenol-d5	6.811	99	126217	18.757	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.969	67	69754	17.064	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132	101635	21.128	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	101122	18.587	ng/ul	0.00
21) Nitrobenzene-d5	8.775	128	49227	20.775	ng/ul	0.00
24) 2-Nitrophenol-d4	9.487	143	57538	21.205	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	96370	19.462	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	103851	14.985	ng/ul	0.01
46) Dimethylphthalate-d6	13.704	166	342139	21.537	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	388042	22.112	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	49788m	20.392	ng/ul	0.02
60) Fluorene-d10	15.316	176	310618	23.442	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	44449	14.109	ng/ul	0.00
73) Anthracene-d10	17.234	188	524931	24.441	ng/ul	0.00
81) Pyrene-d10	19.633	212	663099	22.780	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.745	264	686370	24.829	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020341.D
Acq On : 12 May 2024 05:35
Operator : MA/JU
Sample : P2371-20
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43T2

Manual IntegrationsAPPROVED

Quant Time: May 13 01:31:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 13 00:21:03 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/13/2024
Supervised By :mohammad ahmed 05/14/2024

