

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020285.D
 Acq On : 10 May 2024 10:21
 Operator : MA/JU
 Sample : P2370-23
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y6

Quant Time: May 10 13:12:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 08 22:57:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	70232	20.000	ng/ul	0.00
20) Naphthalene-d8	10.387	136	273060	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.292	164	181182	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.133	188	397203	20.000	ng/ul	0.00
79) Chrysene-d12	21.639	240	427528	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	495534	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	5599	3.367	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.810	99	118142	19.588	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	65677	17.925	ng/ul	0.00
11) 2-Chlorophenol-d4	7.157	132	94227	21.854	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	93204	19.114	ng/ul	0.02
21) Nitrobenzene-d5	8.781	128	44449	21.738	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	50786	21.689	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165	110989	25.975	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	109196	18.259	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	358334	27.083	ng/ul	0.00
49) Acenaphthylene-d8	13.981	160	349299	23.899	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	71147	34.987	ng/ul	0.00
60) Fluorene-d10	15.316	176	312534	28.320	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	59461	23.591	ng/ul	0.00
73) Anthracene-d10	17.233	188	584488	34.015	ng/ul	-0.01
81) Pyrene-d10	19.639	212	747195	29.898	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.768	264	825432	34.451	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.775	266	830181	275.624	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020285.D
Acq On : 10 May 2024 10:21
Operator : MA/JU
Sample : P2370-23
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y6

Quant Time: May 10 13:12:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 08 22:57:55 2024
Response via : Initial Calibration

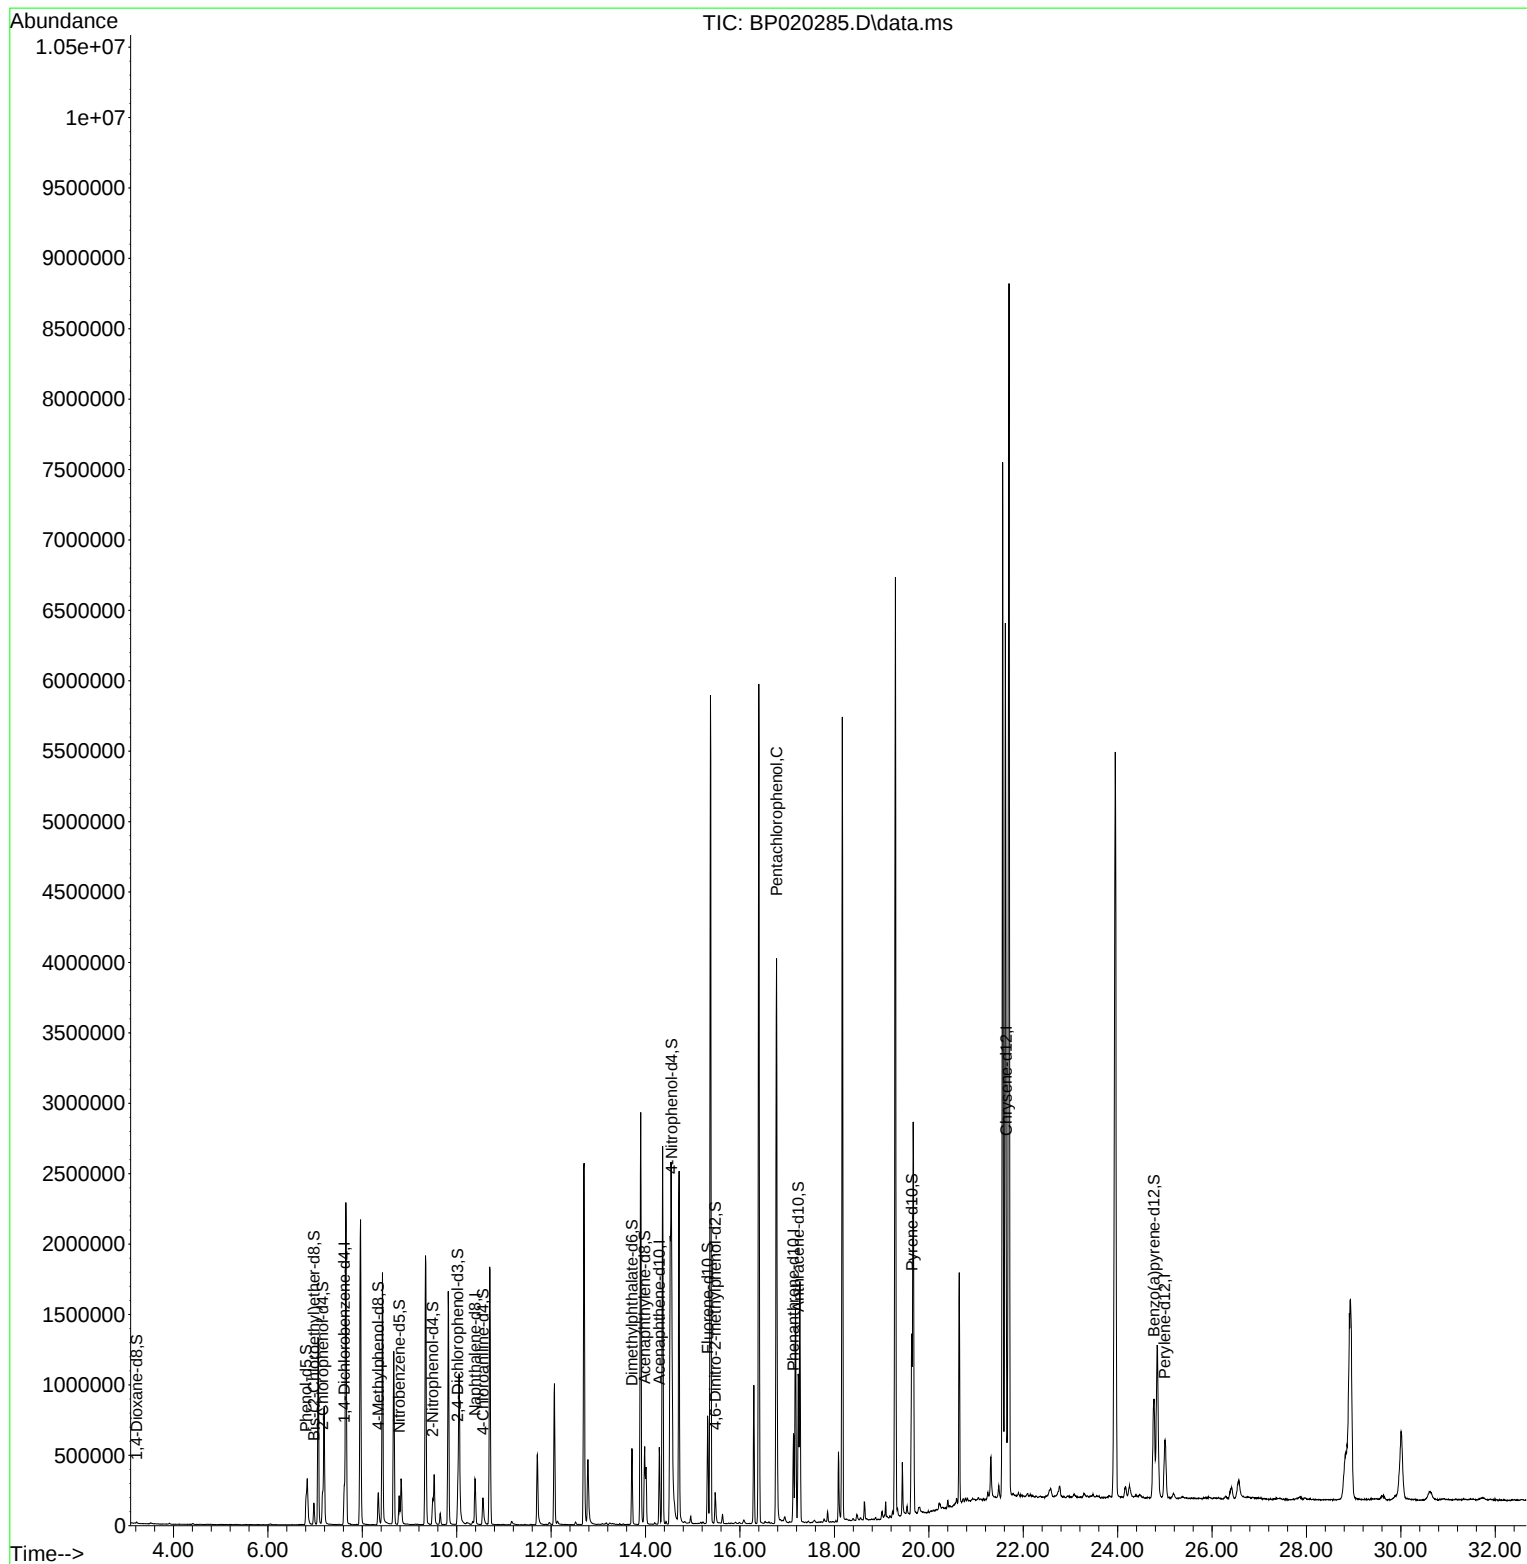

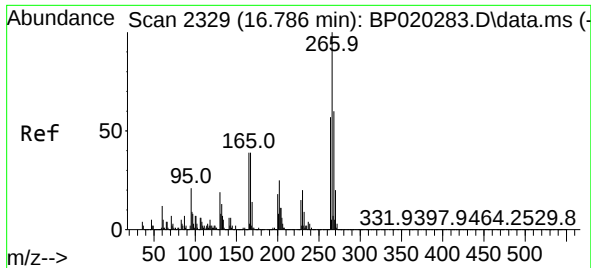

#71
 Pentachlorophenol
 Concen: 275.624 ng/ul
 RT: 16.775 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP020285.D
 Acq: 10 May 2024 10:21

Instrument :
 BNA_P
 ClientSampleId :
 A43Y6

Tgt Ion:266 Resp: 830181
 Ion Ratio Lower Upper
 266 100
 264 63.2 49.8 74.6
 268 62.9 50.4 75.6

