

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
 Data File : BP020335.D
 Acq On : 12 May 2024 01:11
 Operator : MA/JU
 Sample : PB160762BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	31	rVB	21485	34359	1.25%	0.127%
2	3.617	86	90	112	rBV	235099	474594	17.22%	1.752%
3	3.911	135	140	146	rVB	7644	14046	0.51%	0.052%
4	6.805	624	632	654	rBV	282132	638733	23.18%	2.357%
5	6.963	654	659	682	rVV	247220	462467	16.78%	1.707%
6	7.152	684	691	711	rVB	334966	639346	23.20%	2.360%
7	7.610	762	769	783	rBV	333438	600830	21.80%	2.217%
8	8.322	882	890	912	rBV	365803	793273	28.78%	2.928%
9	8.781	960	968	982	rBV	317105	634021	23.01%	2.340%
10	9.487	1080	1088	1109	rBV	304883	578310	20.98%	2.134%
11	10.034	1173	1181	1205	rBV	293026	816093	29.61%	3.012%
12	10.387	1232	1241	1252	rBV	488041	857024	31.10%	3.163%
13	10.551	1261	1269	1295	rBV	321650	876212	31.79%	3.234%
14	12.028	1516	1520	1530	rBV5	4767	10496	0.38%	0.039%
15	13.710	1798	1806	1828	rBV	798438	1343263	48.74%	4.958%
16	13.975	1844	1851	1868	rBV	890980	1460925	53.01%	5.392%
17	14.287	1897	1904	1920	rBV	761936	1206760	43.79%	4.454%
18	14.575	1946	1953	1964	rBV2	157129	470002	17.05%	1.735%
19	15.310	2069	2078	2098	rBV	1140353	1895105	68.76%	6.994%
20	15.475	2100	2106	2120	rBV	291993	563439	20.44%	2.079%
21	16.798	2327	2331	2334	rBV6	2659	3359	0.12%	0.012%
22	16.910	2346	2350	2354	rBV7	2254	4145	0.15%	0.015%
23	17.133	2380	2388	2398	rBV	1032337	1543209	56.00%	5.695%
24	17.228	2398	2404	2420	rVV	1407292	2188142	79.40%	8.076%
25	17.816	2499	2504	2507	rBV7	1804	3389	0.12%	0.013%
26	18.092	2548	2551	2557	rVV8	6050	11045	0.40%	0.041%
27	19.175	2731	2735	2740	rBV2	21116	30641	1.11%	0.113%
28	19.251	2745	2748	2753	rVV2	12919	18447	0.67%	0.068%
29	19.627	2806	2812	2824	rBV	1537485	2599517	94.32%	9.594%
30	21.616	3143	3150	3164	rBV	979683	1802612	65.41%	6.653%
31	24.739	3671	3681	3700	rBV	961995	2755970	100.00%	10.171%
32	24.974	3712	3721	3735	rVB	610348	1765671	64.07%	6.516%




Sum of corrected areas: 27095445

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020335.D
Acq On : 12 May 2024 01:11
Operator : MA/JU
Sample : PB160762BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

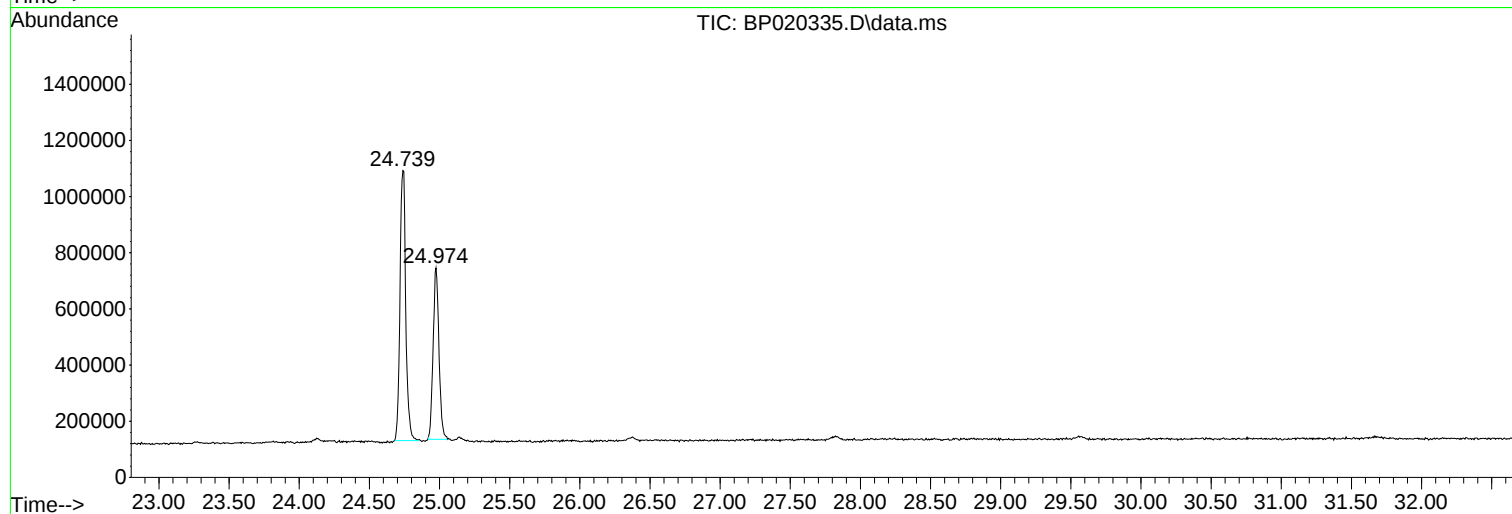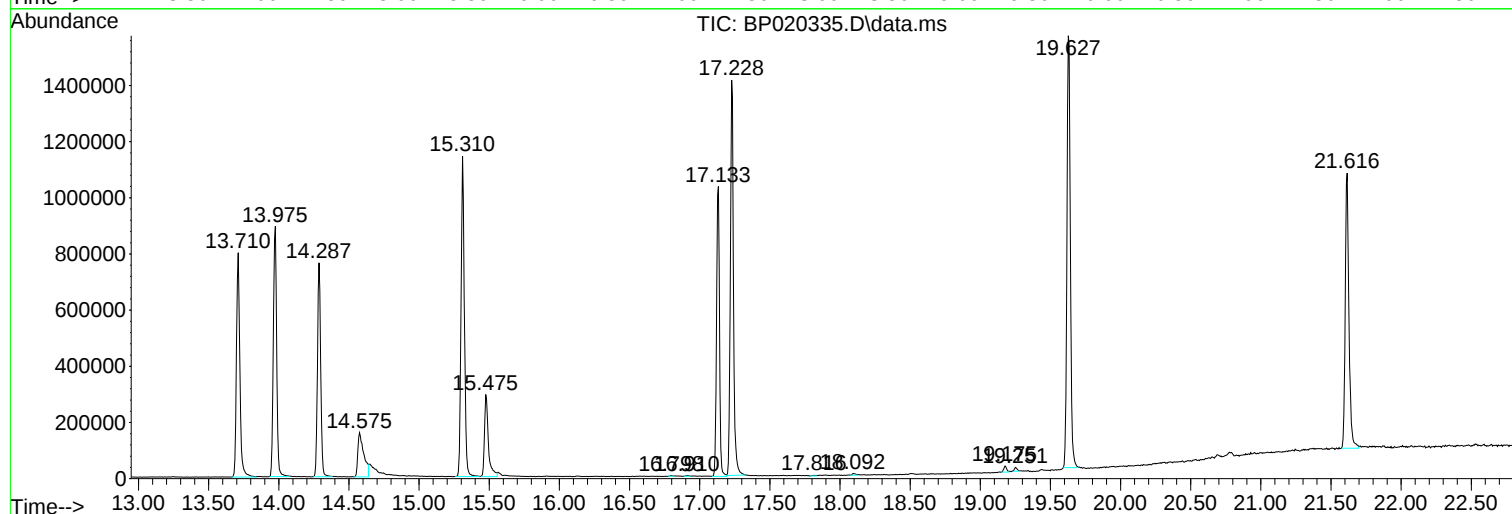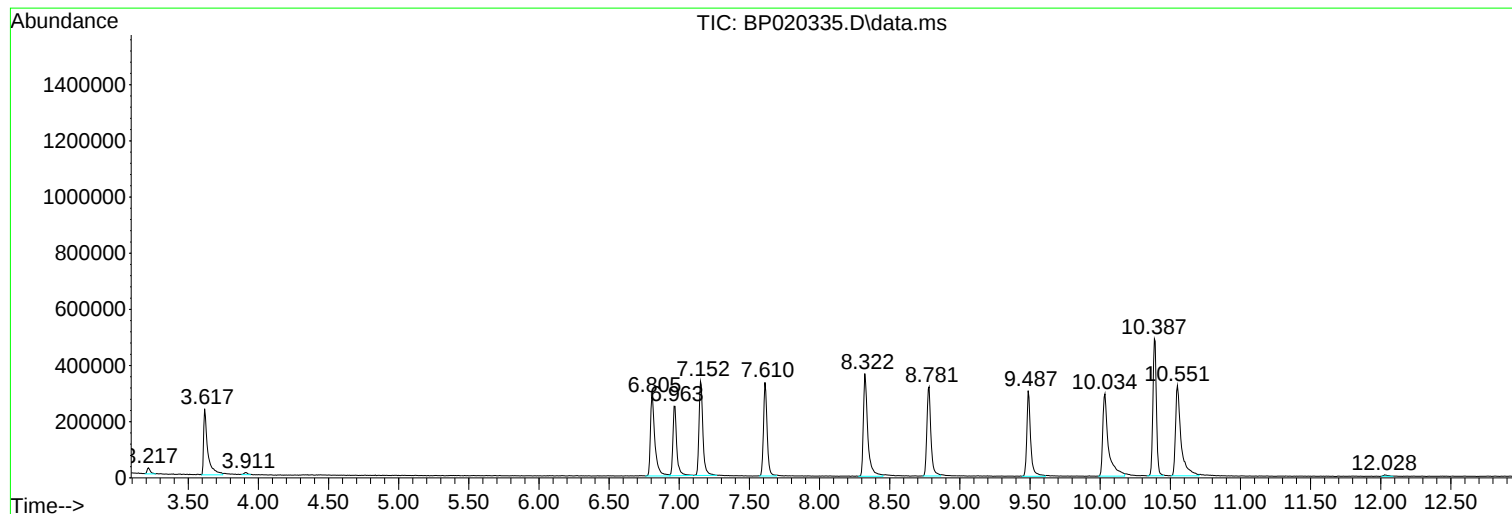

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020335.D
Acq On : 12 May 2024 01:11
Operator : MA/JU
Sample : PB160762BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051024\
Data File : BP020335.D
Acq On : 12 May 2024 01:11
Operator : MA/JU
Sample : PB160762BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------