
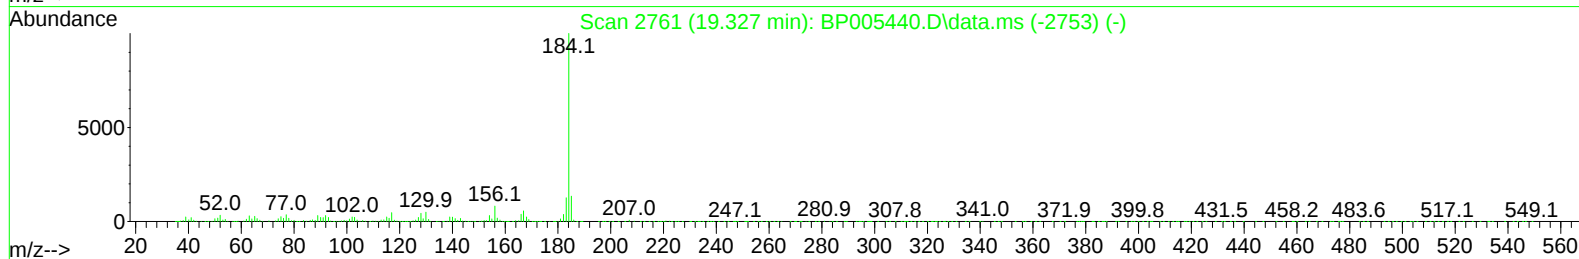
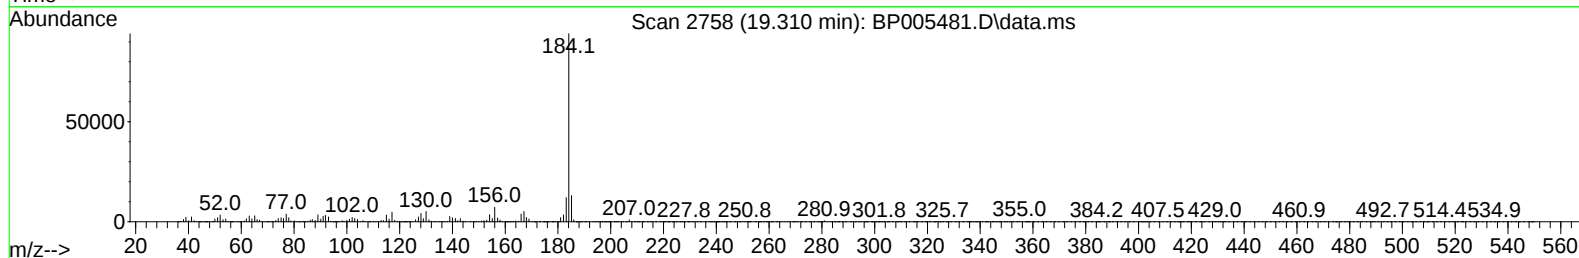


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005481.D
Acq On : 11 May 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 11:13:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 12:37:06 2021
Response via : Initial Calibration

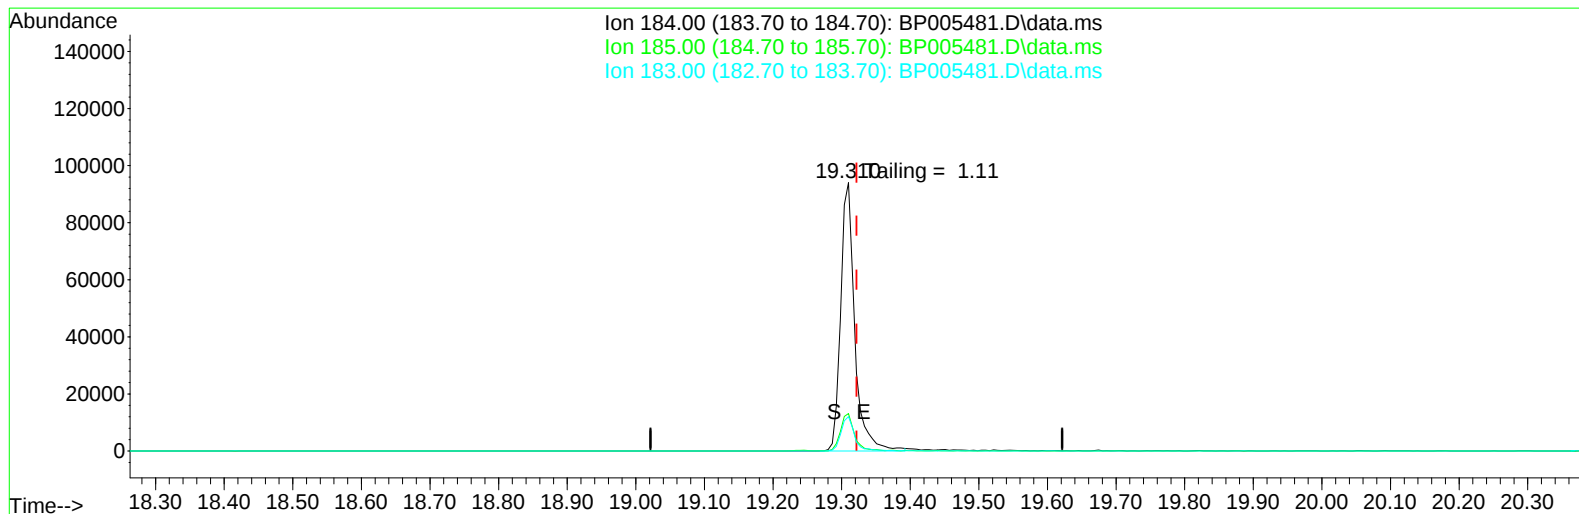

TIC: BP005481.D\data.ms

(77) Benzidine




19.310min (-0.012) 147496.63 ng

response 132418

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.95
183.00	12.30	12.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005481.D
Acq On : 11 May 2021 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 11:13:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 12:37:06 2021
Response via : Initial Calibration

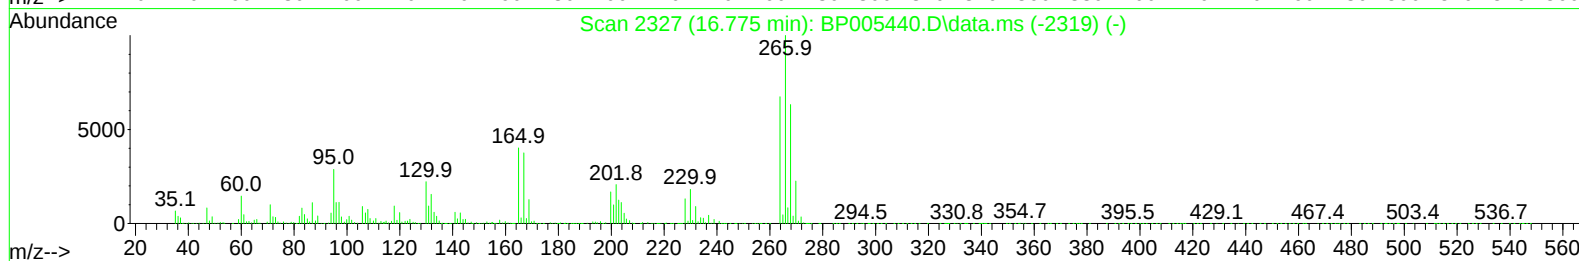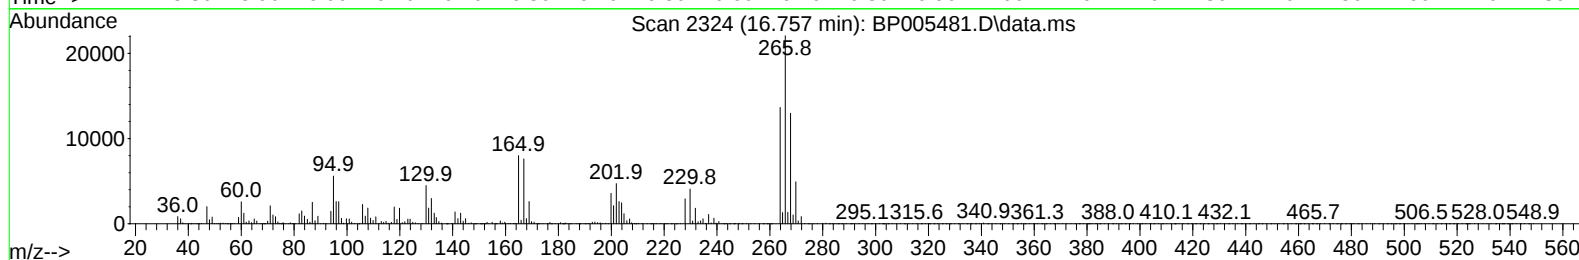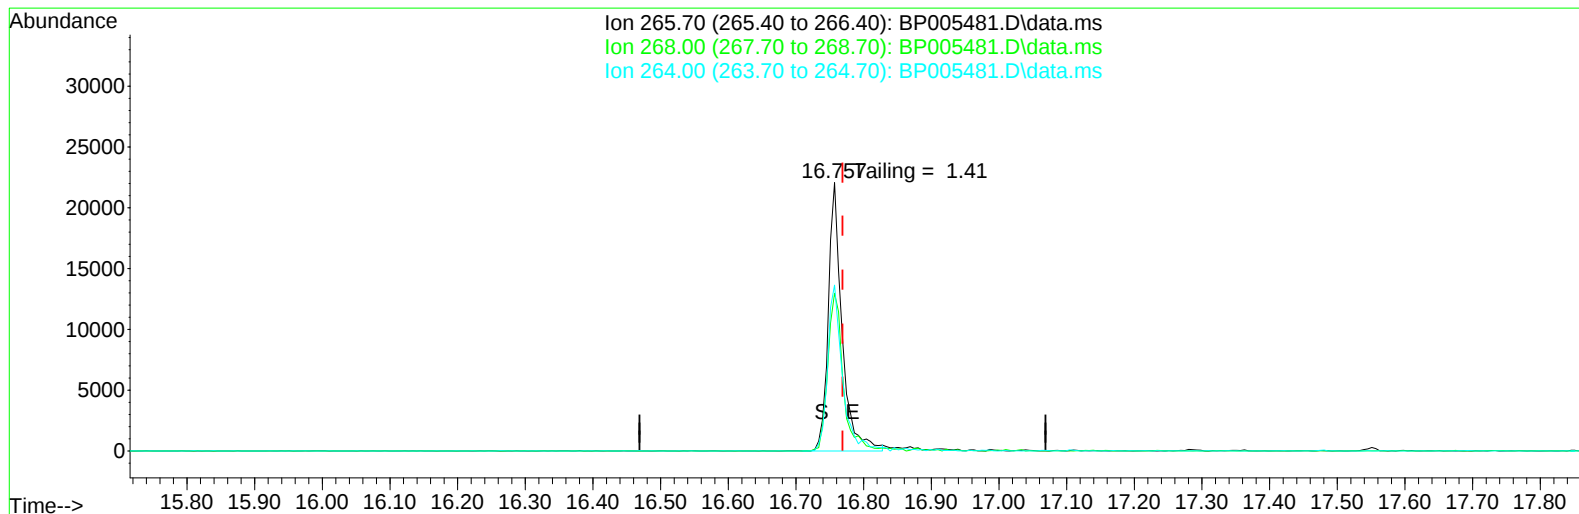

TIC: BP005481.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.012) 502512.69 ng

response 31669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	58.78
264.00	67.10	61.83
0.00	0.00	0.00