

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005485.D
 Acq On : 11 May 2021 12:17
 Operator : CG/JU
 Sample : PB136243BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136243BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	368	374	385	rBV	255968	372600	38.36%	10.474%
2	6.893	641	647	663	rBV	197481	311432	32.06%	8.754%
3	7.699	777	784	790	rBV2	46239	73135	7.53%	2.056%
4	8.863	975	982	997	rBV	119982	203027	20.90%	5.707%
5	10.487	1250	1258	1271	rVB	40943	72879	7.50%	2.049%
6	12.969	1671	1680	1690	rBV	326425	467300	48.11%	13.136%
7	14.345	1907	1914	1922	rBV2	57294	89641	9.23%	2.520%
8	15.839	2162	2168	2185	rBV	334979	473564	48.75%	13.312%
9	17.098	2376	2382	2391	rBV	79278	113586	11.69%	3.193%
10	19.669	2813	2819	2829	rBV	815682	971315	100.00%	27.303%
11	20.980	3039	3042	3048	rBV4	9402	15343	1.58%	0.431%
12	21.192	3073	3078	3083	rBV	137239	170115	17.51%	4.782%
13	23.498	3465	3470	3481	rVB	114142	223575	23.02%	6.285%




Sum of corrected areas: 3557512

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005485.D
Acq On : 11 May 2021 12:17
Operator : CG/JU
Sample : PB136243BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

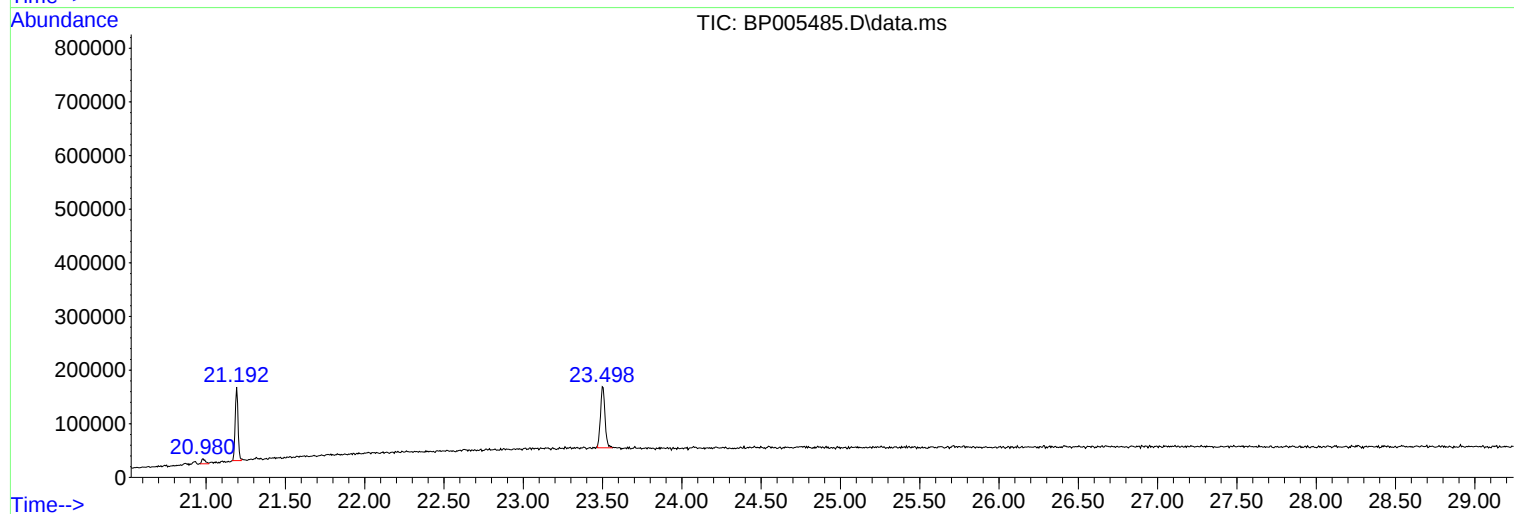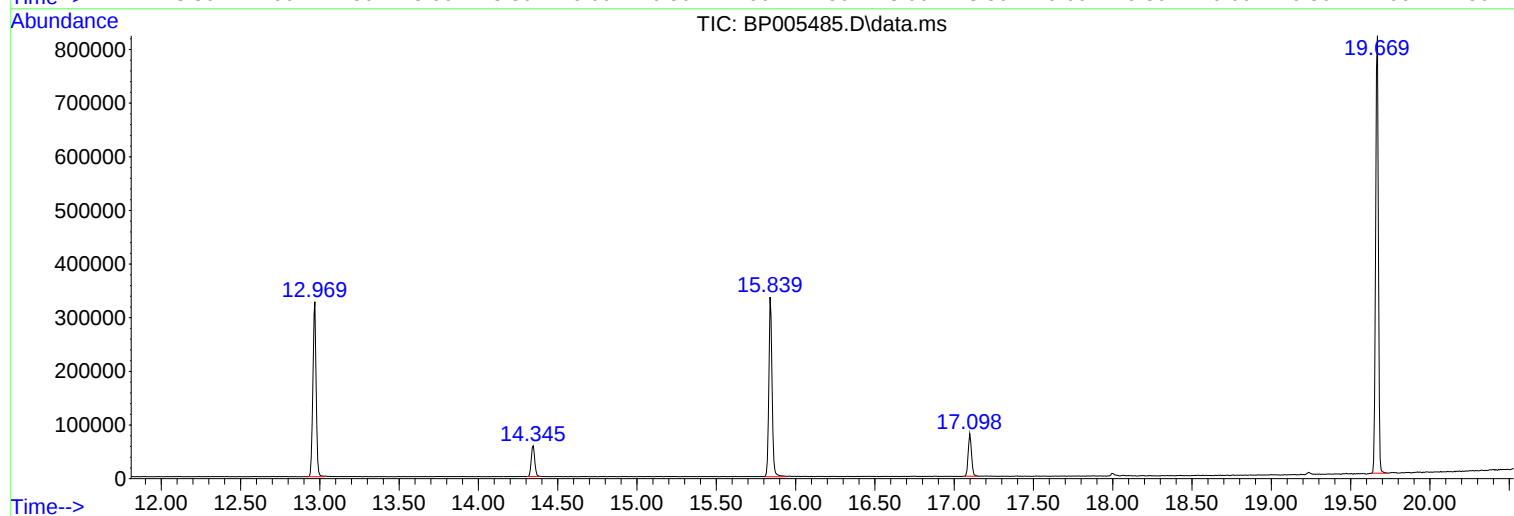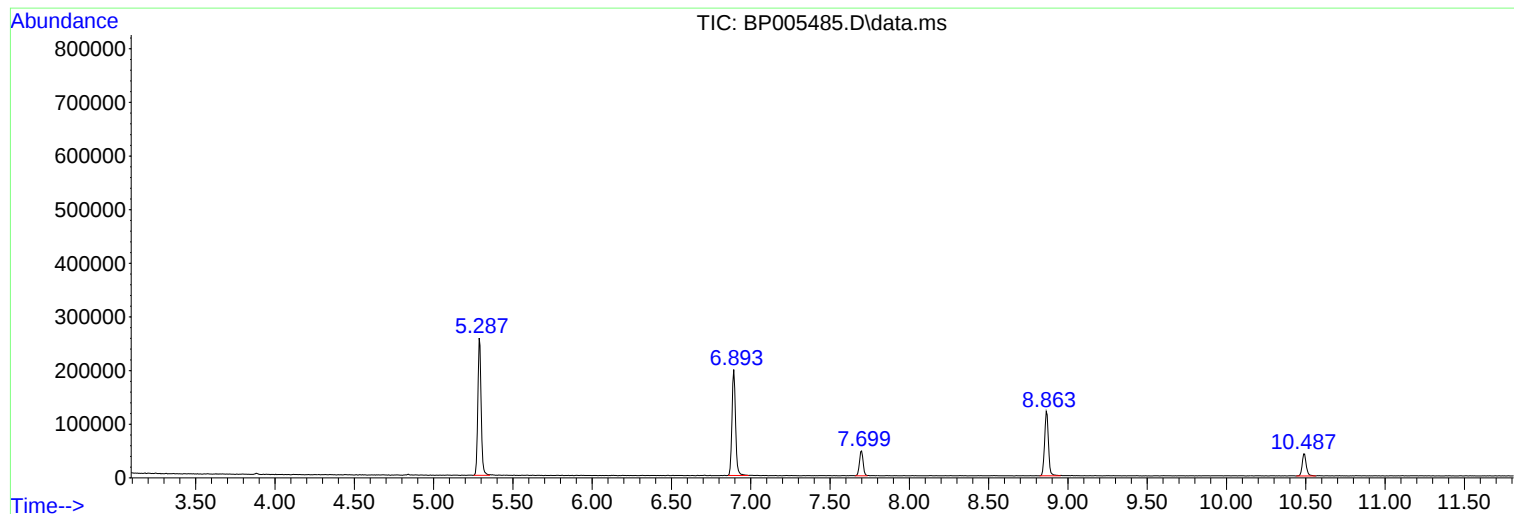

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005485.D
Acq On : 11 May 2021 12:17
Operator : CG/JU
Sample : PB136243BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005485.D
Acq On : 11 May 2021 12:17
Operator : CG/JU
Sample : PB136243BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136243BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------