

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005492.D
 Acq On : 11 May 2021 16:51
 Operator : CG/JU
 Sample : M2277-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FK-BPM-01-A3-A3A-B3-B3A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	368	374	389	rBV	303022	430707	34.82%	9.877%
2	6.893	640	647	661	rBV	231887	374098	30.24%	8.579%
3	7.693	776	783	792	rBV2	52633	79108	6.40%	1.814%
4	8.863	973	982	993	rBV	143943	237372	19.19%	5.444%
5	10.487	1251	1258	1267	rBV	45371	77014	6.23%	1.766%
6	12.963	1671	1679	1691	rBV	391902	540437	43.69%	12.394%
7	13.816	1818	1824	1834	rBV2	8771	15119	1.22%	0.347%
8	14.340	1907	1913	1923	rVB	66847	98808	7.99%	2.266%
9	15.840	2161	2168	2185	rBV	403374	586380	47.40%	13.447%
10	17.092	2375	2381	2392	rBV	91463	135174	10.93%	3.100%
11	17.992	2530	2534	2540	rBV4	14223	20115	1.63%	0.461%
12	19.663	2813	2818	2825	rBV	1162827	1236994	100.00%	28.368%
13	20.904	3024	3029	3034	rBV6	25975	40128	3.24%	0.920%
14	21.186	3072	3077	3083	rBV2	178173	220686	17.84%	5.061%
15	23.492	3463	3469	3478	rVB2	141418	268431	21.70%	6.156%




Sum of corrected areas: 4360571

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005492.D
Acq On : 11 May 2021 16:51
Operator : CG/JU
Sample : M2277-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

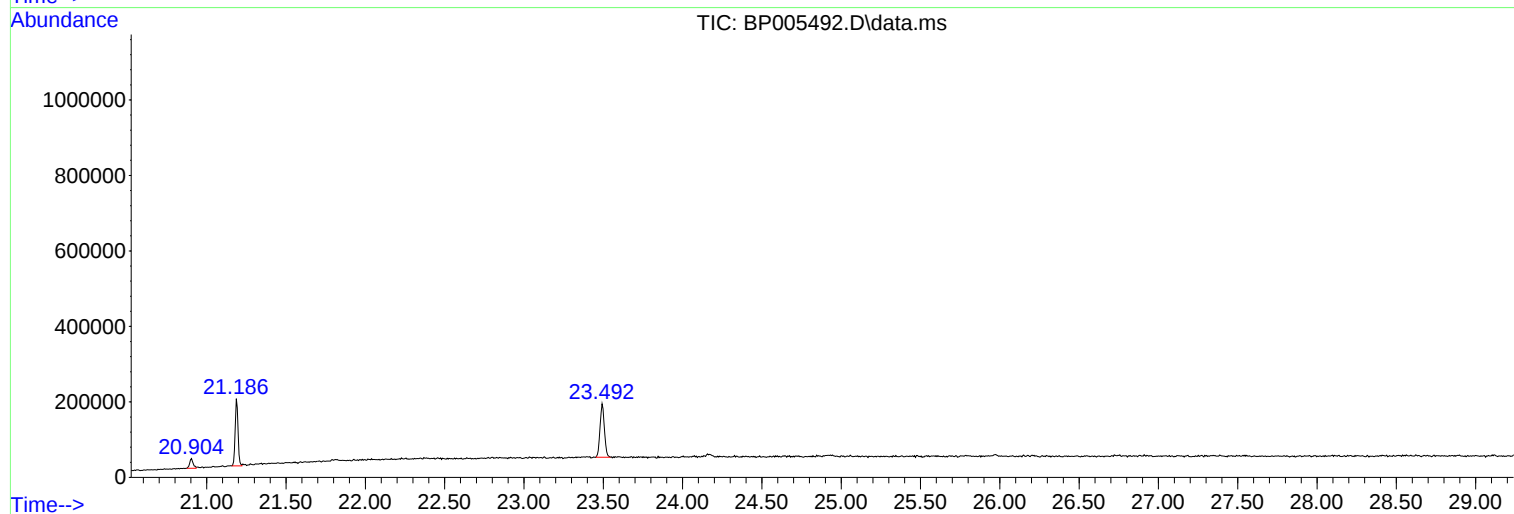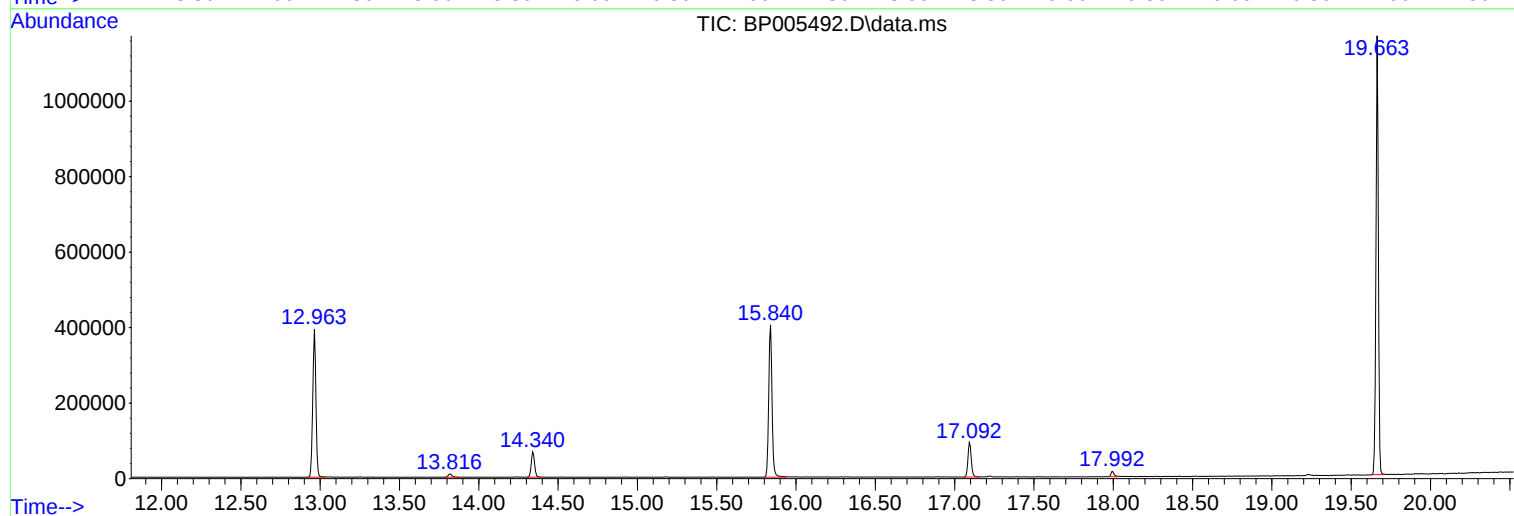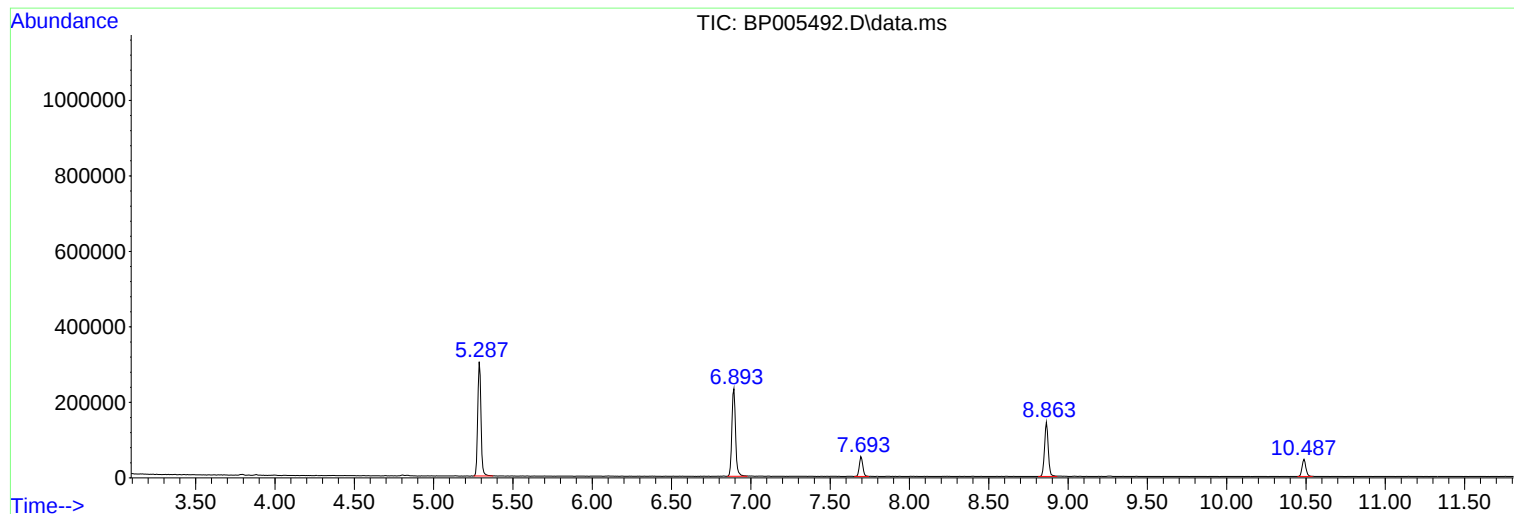

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005492.D
Acq On : 11 May 2021 16:51
Operator : CG/JU
Sample : M2277-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005492.D
Acq On : 11 May 2021 16:51
Operator : CG/JU
Sample : M2277-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-BPM-01-A3-A3A-B3-B3A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------