

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005495.D
 Acq On : 11 May 2021 18:33
 Operator : CG/JU
 Sample : M2322-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WC-20210505

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	369	374	384	rBV2	115024	182018	11.98%	1.990%
2	6.893	640	647	658	rBV	49181	89143	5.87%	0.975%
3	7.693	777	783	791	rBV2	42857	64916	4.27%	0.710%
4	8.528	916	925	931	rVB5	7627	17857	1.18%	0.195%
5	8.805	966	972	976	rBV2	42750	68951	4.54%	0.754%
6	8.863	976	982	990	rVB	131511	213759	14.07%	2.337%
7	10.487	1249	1258	1266	rBV	43165	72591	4.78%	0.794%
8	11.857	1483	1491	1497	rVB3	9210	16800	1.11%	0.184%
9	12.710	1625	1636	1640	rBV2	39813	79226	5.21%	0.866%
10	12.746	1640	1642	1647	rVB3	14810	20045	1.32%	0.219%
11	12.875	1653	1664	1671	rBV4	22326	46621	3.07%	0.510%
12	12.963	1671	1679	1688	rVB	415458	563940	37.12%	6.166%
13	13.193	1714	1718	1727	rVB2	11752	20047	1.32%	0.219%
14	13.510	1766	1772	1777	rBV2	10864	16603	1.09%	0.182%
15	13.722	1794	1808	1813	rBV2	268674	639461	42.09%	6.991%
16	13.857	1826	1831	1832	rBV3	21440	34220	2.25%	0.374%
17	13.934	1840	1844	1850	rVB2	42495	62876	4.14%	0.687%
18	14.187	1884	1887	1892	rVB	21663	27782	1.83%	0.304%
19	14.340	1908	1913	1919	rBV	83734	118457	7.80%	1.295%
20	14.457	1929	1933	1938	rBV3	23245	39013	2.57%	0.427%
21	14.510	1938	1942	1944	rVV3	27631	39561	2.60%	0.433%
22	14.540	1944	1947	1952	rVB	36001	55710	3.67%	0.609%
23	14.640	1959	1964	1968	rBV2	35221	67876	4.47%	0.742%
24	14.693	1968	1973	1977	rVV	98968	170267	11.21%	1.862%
25	14.740	1977	1981	1987	rVB2	63401	97449	6.41%	1.065%
26	14.875	2001	2004	2008	rVB3	12945	15682	1.03%	0.171%
27	15.175	2050	2055	2060	rBV	137876	177464	11.68%	1.940%
28	15.240	2060	2066	2069	rVV3	27679	49734	3.27%	0.544%
29	15.275	2069	2072	2076	rVV2	25446	35120	2.31%	0.384%
30	15.340	2078	2083	2085	rVV	43571	60654	3.99%	0.663%
31	15.375	2085	2089	2102	rVB	86253	129840	8.55%	1.420%
32	15.510	2105	2112	2116	rBV7	14399	34298	2.26%	0.375%
33	15.569	2116	2122	2125	rVV5	25387	47144	3.10%	0.515%
34	15.610	2125	2129	2131	rVV	23783	38024	2.50%	0.416%
35	15.634	2131	2133	2137	rVB2	26964	31975	2.10%	0.350%
36	15.722	2143	2148	2151	rBV6	14360	24651	1.62%	0.270%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005495.D
 Acq On : 11 May 2021 18:33
 Operator : CG/JU
 Sample : M2322-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 WC-20210505

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.840	2159	2168	2178	rBV2	567827	934257	61.49%	10.214%
38	15.910	2178	2180	2183	rVV2	22955	28274	1.86%	0.309%
39	15.957	2184	2188	2194	rVB3	36169	50361	3.31%	0.551%
40	16.087	2206	2210	2216	rVB5	18785	26522	1.75%	0.290%
41	16.145	2216	2220	2224	rBV3	24215	33459	2.20%	0.366%
42	16.187	2224	2227	2231	rVV6	20882	31624	2.08%	0.346%
43	16.257	2232	2239	2246	rVB7	31678	75680	4.98%	0.827%
44	16.481	2271	2277	2287	rBV	201357	278094	18.30%	3.040%
45	16.651	2300	2306	2310	rBV5	58209	106026	6.98%	1.159%
46	16.704	2310	2315	2320	rVV3	53347	103808	6.83%	1.135%
47	16.751	2320	2323	2329	rVB2	64432	91181	6.00%	0.997%
48	16.916	2347	2351	2353	rBV4	17359	25983	1.71%	0.284%
49	16.957	2354	2358	2363	rVV2	76197	110878	7.30%	1.212%
50	17.028	2368	2370	2375	rVB5	14691	18176	1.20%	0.199%
51	17.092	2376	2381	2385	rBV	133282	194684	12.81%	2.129%
52	17.175	2390	2395	2402	rVV3	45087	104913	6.90%	1.147%
53	17.257	2404	2409	2415	rVB	151361	215200	14.16%	2.353%
54	17.381	2426	2430	2434	rVB5	22987	32810	2.16%	0.359%
55	17.463	2441	2444	2447	rBV	23523	24112	1.59%	0.264%
56	17.651	2472	2476	2483	rBV6	26726	70166	4.62%	0.767%
57	17.716	2483	2487	2490	rVV	78383	126911	8.35%	1.388%
58	17.745	2490	2492	2501	rVV	69459	103876	6.84%	1.136%
59	17.828	2504	2506	2509	rVB3	21382	19385	1.28%	0.212%
60	17.916	2516	2521	2527	rBV2	54306	99665	6.56%	1.090%
61	18.004	2533	2536	2543	rVB4	51075	69311	4.56%	0.758%
62	18.063	2543	2546	2550	rVB3	18715	23514	1.55%	0.257%
63	18.992	2702	2704	2709	rBV4	19043	20366	1.34%	0.223%
64	19.234	2742	2745	2749	rBV4	39796	49439	3.25%	0.541%
65	19.522	2789	2794	2801	rVB5	87920	142143	9.36%	1.554%
66	19.598	2805	2807	2810	rVV2	47003	43680	2.87%	0.478%
67	19.663	2813	2818	2826	rVB	1249984	1519424	100.00%	16.612%
68	19.733	2828	2830	2833	rBV4	17398	21936	1.44%	0.240%
69	19.763	2833	2835	2842	rVB5	25739	38126	2.51%	0.417%
70	19.939	2863	2865	2868	rVB4	26320	22496	1.48%	0.246%
71	20.010	2874	2877	2879	rBV2	59447	75176	4.95%	0.822%
72	20.033	2879	2881	2886	rVB	111353	112107	7.38%	1.226%
73	20.116	2893	2895	2900	rVB2	41997	46561	3.06%	0.509%
74	21.186	3073	3077	3085	rVB	223226	288815	19.01%	3.158%
75	23.492	3464	3469	3477	rVB2	150294	297519	19.58%	3.253%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005495.D
Acq On : 11 May 2021 18:33
Operator : CG/JU
Sample : M2322-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-20210505

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION



Sum of corrected areas: 9146433

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005495.D
Acq On : 11 May 2021 18:33
Operator : CG/JU
Sample : M2322-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

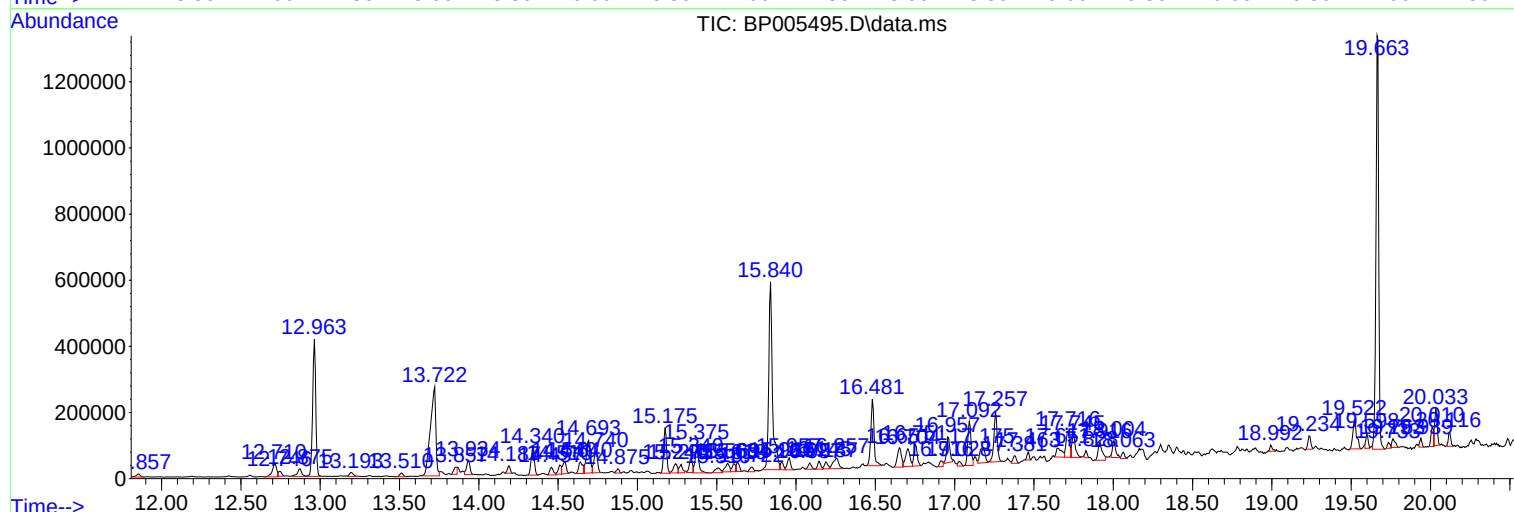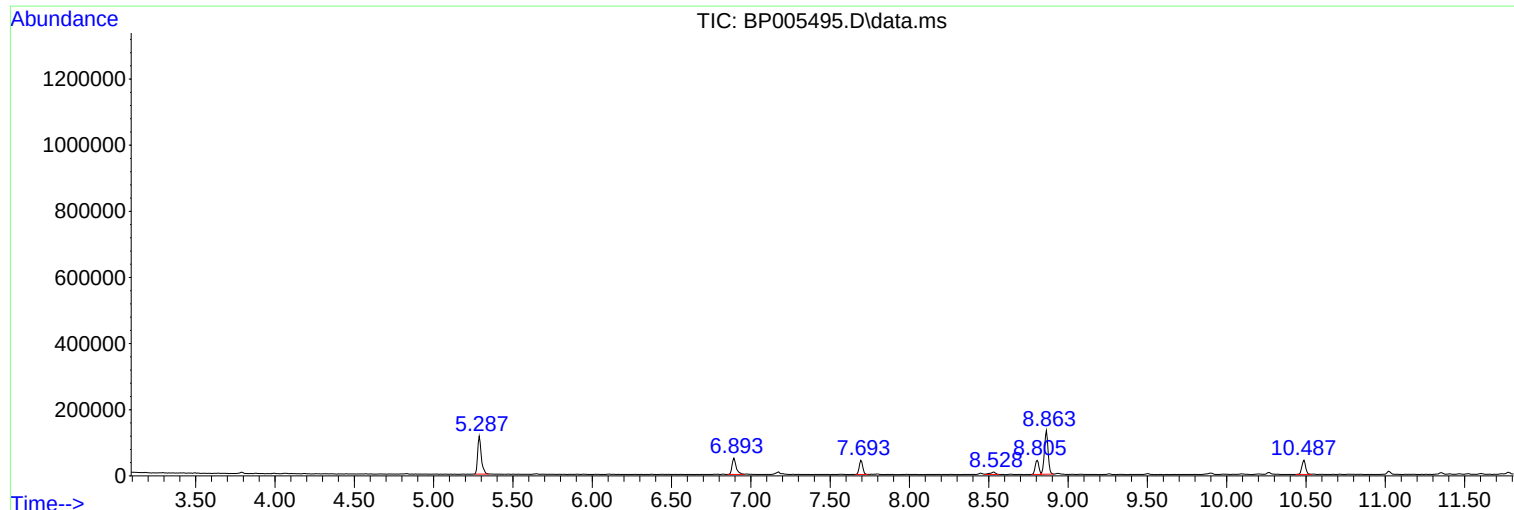

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005495.D
Acq On : 11 May 2021 18:33
Operator : CG/JU
Sample : M2322-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005495.D
Acq On : 11 May 2021 18:33
Operator : CG/JU
Sample : M2322-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
WC-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc