

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005497.D
 Acq On : 11 May 2021 19:40
 Operator : CG/JU
 Sample : M2280-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FK-PS-01-072

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.287	368	374	384	rBV	159572	230172	32.08%	5.545%
2	6.887	640	646	659	rBV	120519	201297	28.05%	4.849%
3	7.693	775	783	798	rVB	43248	65087	9.07%	1.568%
4	8.863	974	982	995	rBV	73780	130619	18.20%	3.147%
5	10.487	1249	1258	1264	rBV	39257	64579	9.00%	1.556%
6	12.963	1670	1679	1687	rBV	198719	284089	39.59%	6.844%
7	13.816	1819	1824	1829	rBV2	8412	13288	1.85%	0.320%
8	14.340	1907	1913	1921	rBV2	56411	84492	11.78%	2.035%
9	15.839	2159	2168	2178	rBV	214038	324406	45.21%	7.815%
10	17.092	2375	2381	2385	rBV	89313	122849	17.12%	2.960%
11	17.134	2385	2388	2394	rVB	19636	28263	3.94%	0.681%
12	17.992	2525	2534	2542	rBV8	16512	34628	4.83%	0.834%
13	18.675	2647	2650	2657	rVB9	4454	7836	1.09%	0.189%
14	19.110	2720	2724	2728	rBV2	30126	37579	5.24%	0.905%
15	19.157	2728	2732	2738	rVB2	17840	23826	3.32%	0.574%
16	19.463	2776	2784	2787	rBV3	23759	47687	6.65%	1.149%
17	19.663	2812	2818	2826	rBV	667663	717549	100.00%	17.286%
18	19.963	2865	2869	2875	rVB4	16286	19987	2.79%	0.482%
19	20.286	2921	2924	2928	rVB6	16867	18935	2.64%	0.456%
20	20.445	2947	2951	2957	rVB2	34177	36791	5.13%	0.886%
21	20.898	3025	3028	3036	rVB	86259	108250	15.09%	2.608%
22	21.186	3071	3077	3081	rBV	213402	291435	40.62%	7.021%
23	21.327	3098	3101	3104	rVB	62196	56837	7.92%	1.369%
24	21.769	3172	3176	3179	rBV	66401	85927	11.98%	2.070%
25	22.245	3253	3257	3262	rVB2	60101	78020	10.87%	1.880%
26	22.774	3343	3347	3353	rBV3	81443	120204	16.75%	2.896%
27	23.374	3444	3449	3458	rVB6	49375	109364	15.24%	2.635%
28	23.486	3463	3468	3477	rVB2	148549	290342	40.46%	6.995%
29	24.057	3561	3565	3571	rVB3	48582	92800	12.93%	2.236%
30	24.551	3644	3649	3661	rVB3	59602	149259	20.80%	3.596%
31	26.733	4013	4020	4030	rVB6	91929	274571	38.27%	6.615%




Sum of corrected areas: 4150968

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005497.D
Acq On : 11 May 2021 19:40
Operator : CG/JU
Sample : M2280-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-PS-01-072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

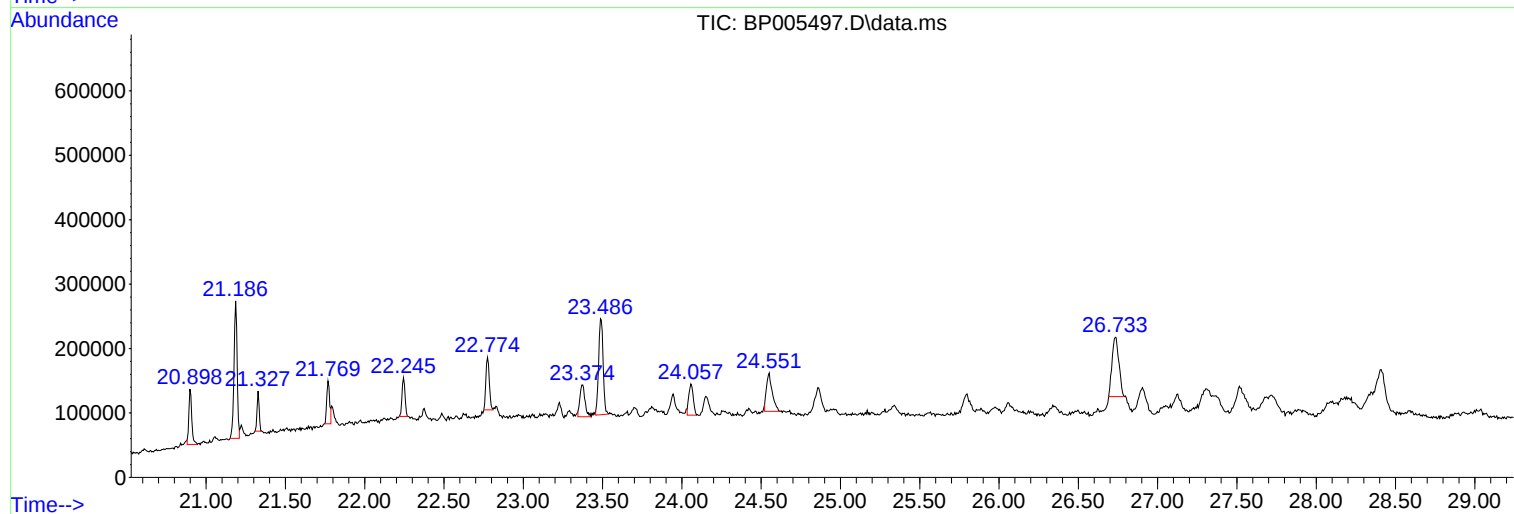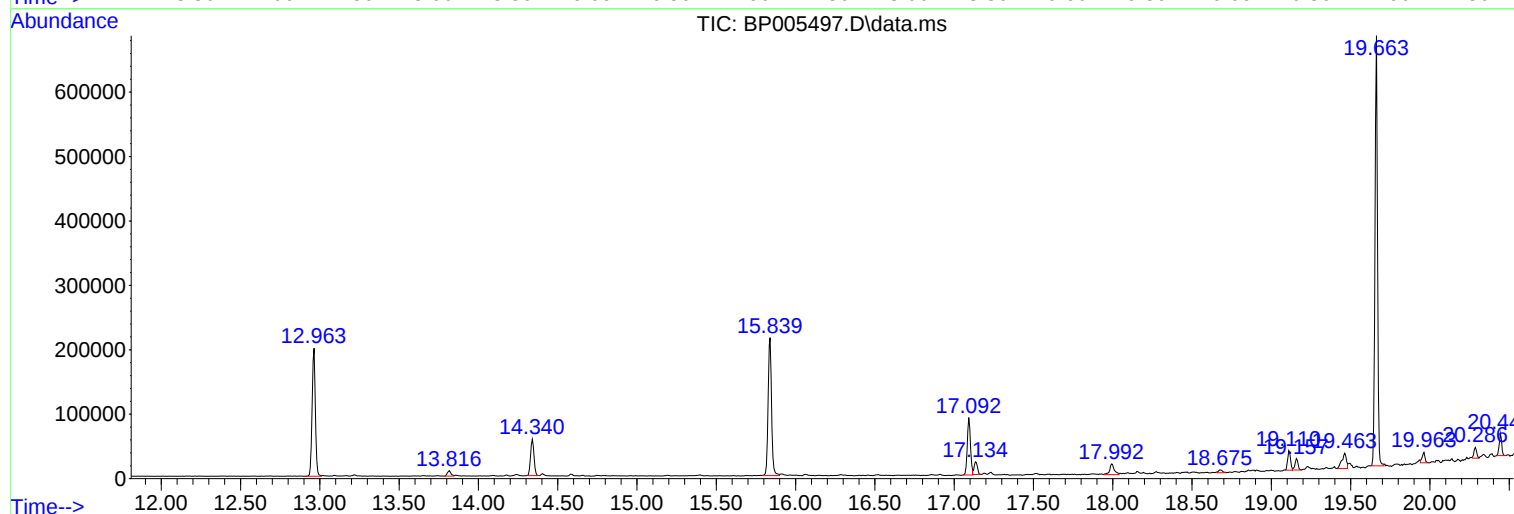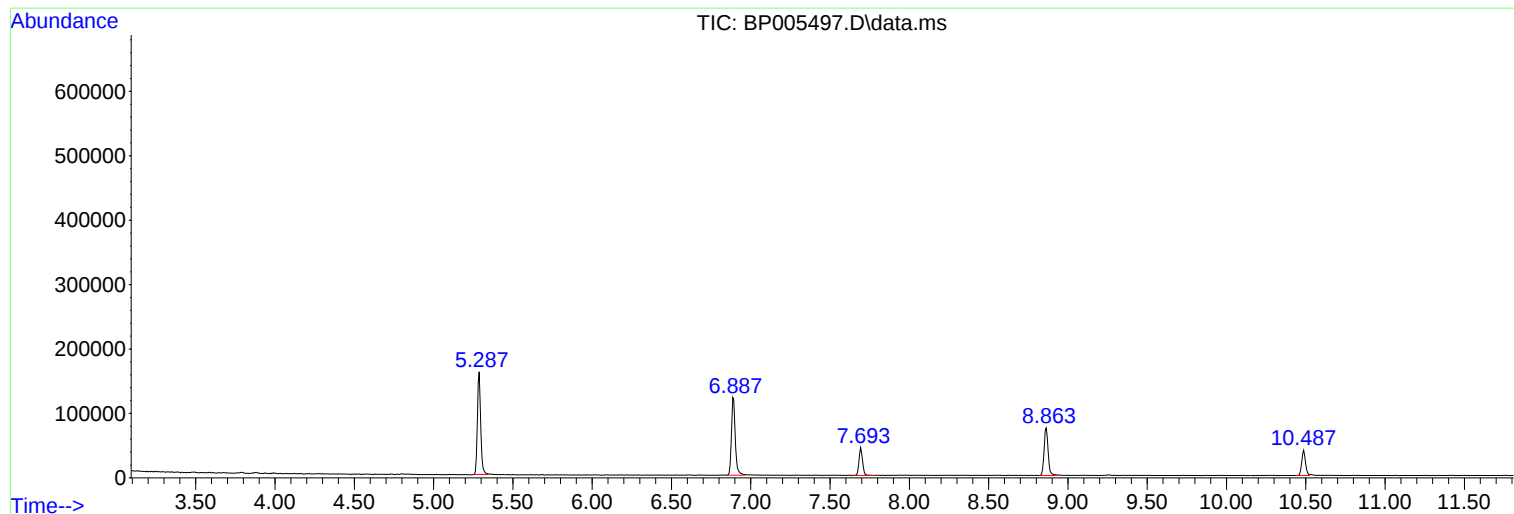

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005497.D
Acq On : 11 May 2021 19:40
Operator : CG/JU
Sample : M2280-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-PS-01-072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
Data File : BP005497.D
Acq On : 11 May 2021 19:40
Operator : CG/JU
Sample : M2280-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FK-PS-01-072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
