
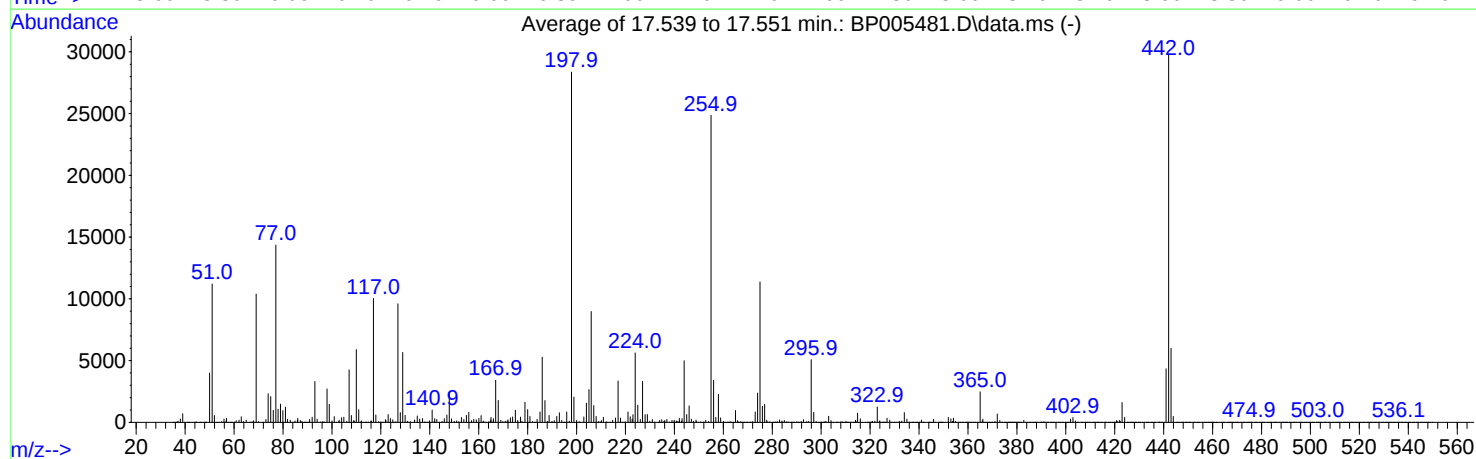


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005481.D
 Acq On : 11 May 2021 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 11 11:20:59 2021

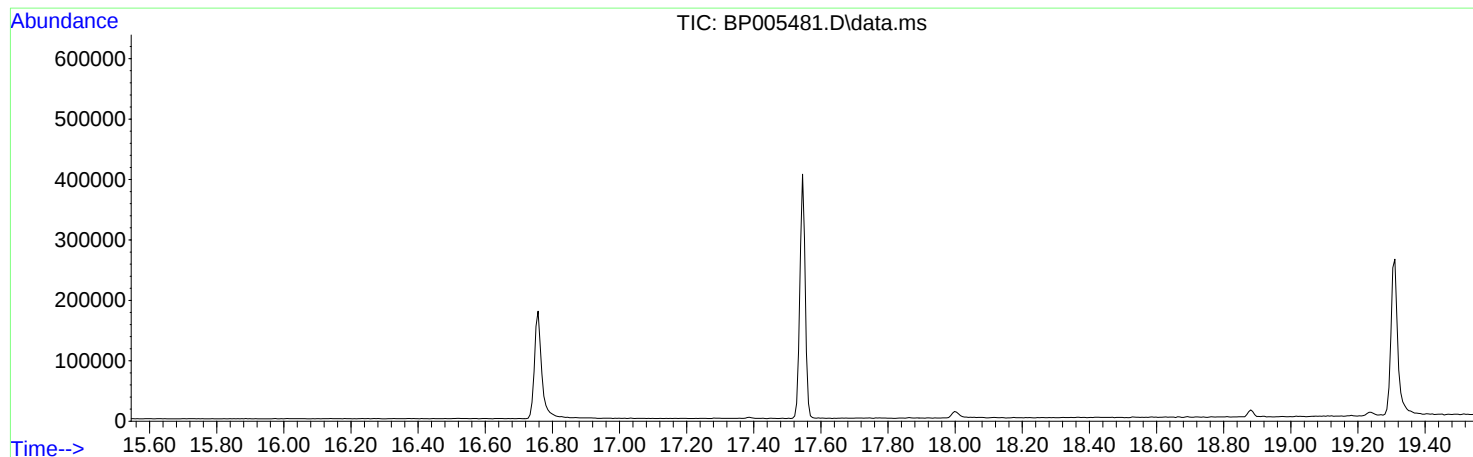




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	11202	PASS
68	69	0.00	2	1.3	131	PASS
69	198	0.00	100	36.6	10388	PASS
70	69	0.00	2	0.6	59	PASS
127	198	10	80	33.9	9607	PASS
197	198	0.00	2	0.4	101	PASS
198	198	100	100	100.0	28366	PASS
199	198	5	9	7.2	2043	PASS
275	198	10	60	40.1	11381	PASS
365	198	1	100	8.7	2476	PASS
441	198	0.01	100	15.3	4341	PASS
442	442	100	100	100.0	29786	PASS
443	442	15	24	20.1	6000	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005481.D
 Acq On : 11 May 2021 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 11 11:13:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 07 12:37:06 2021
 Response via : Initial Calibration

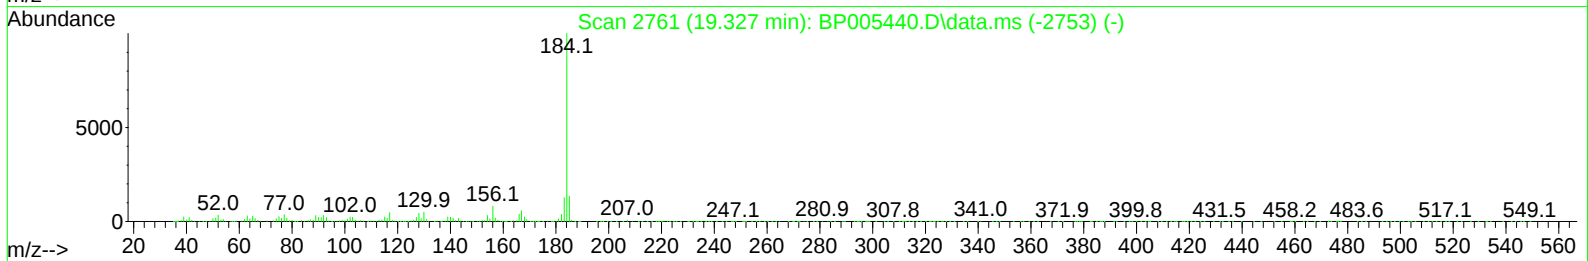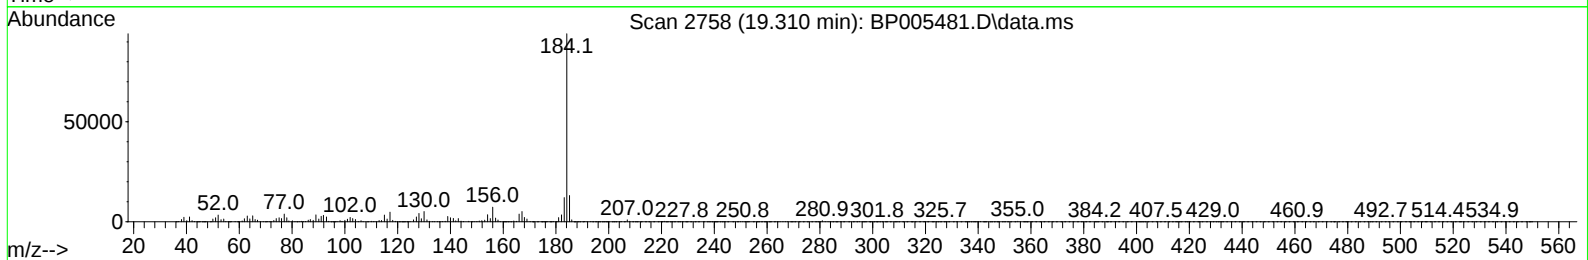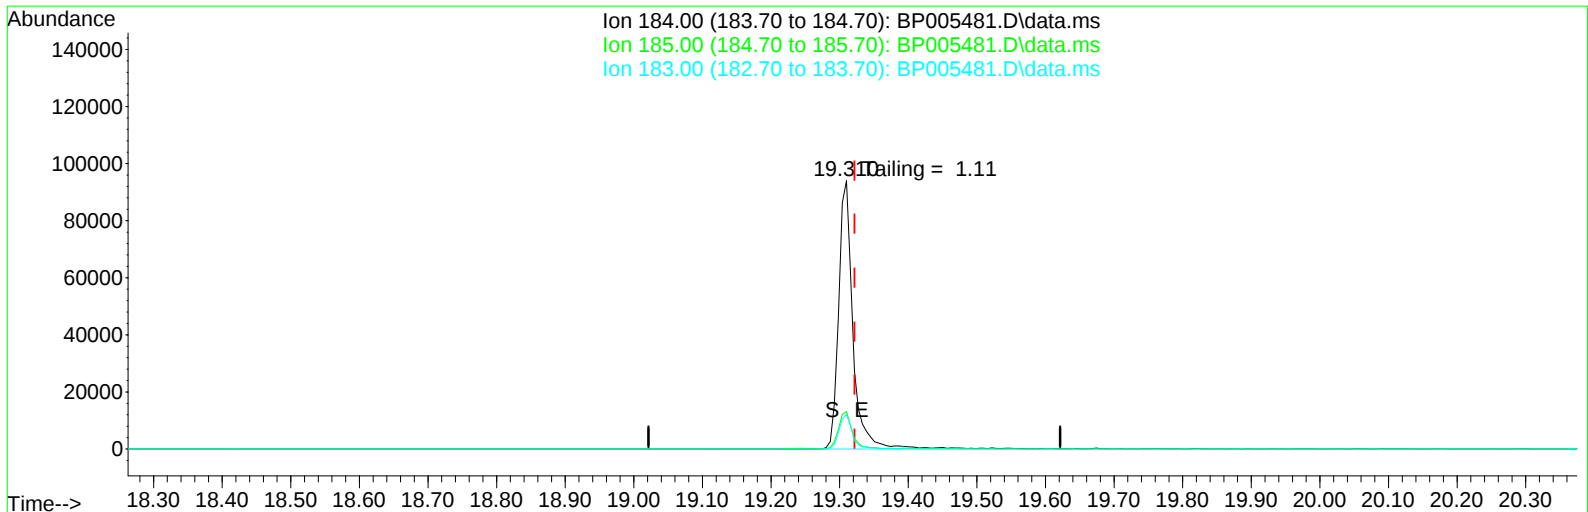

TIC: BP005481.D\data.ms

(77) Benzidine

19.310min (-0.012) 147496.63 ng




response 132418

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.95
183.00	12.30	12.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051121\
 Data File : BP005481.D
 Acq On : 11 May 2021 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 11 11:13:52 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 07 12:37:06 2021
 Response via : Initial Calibration

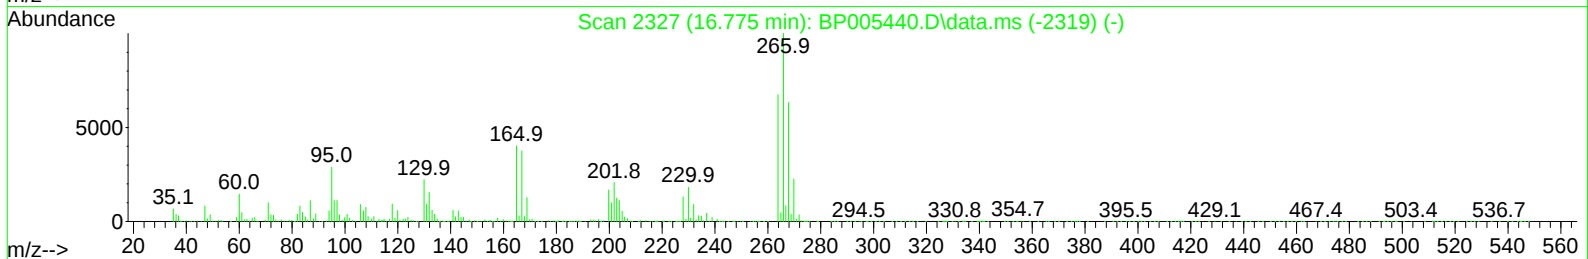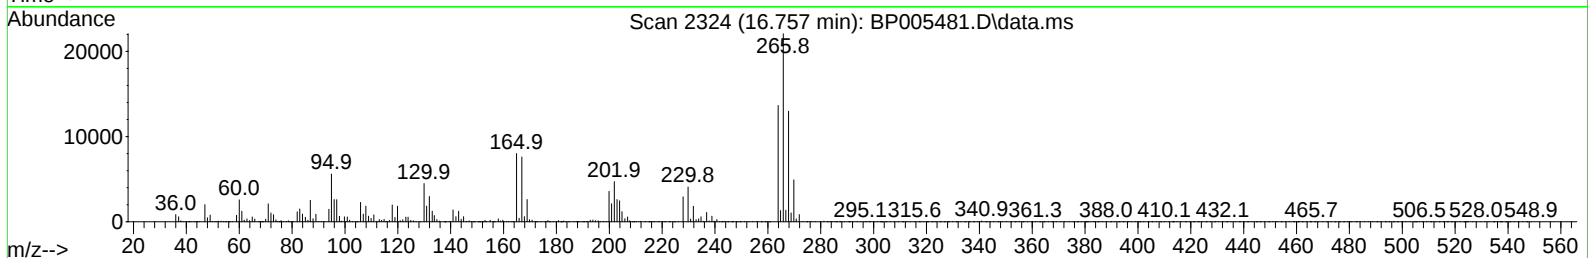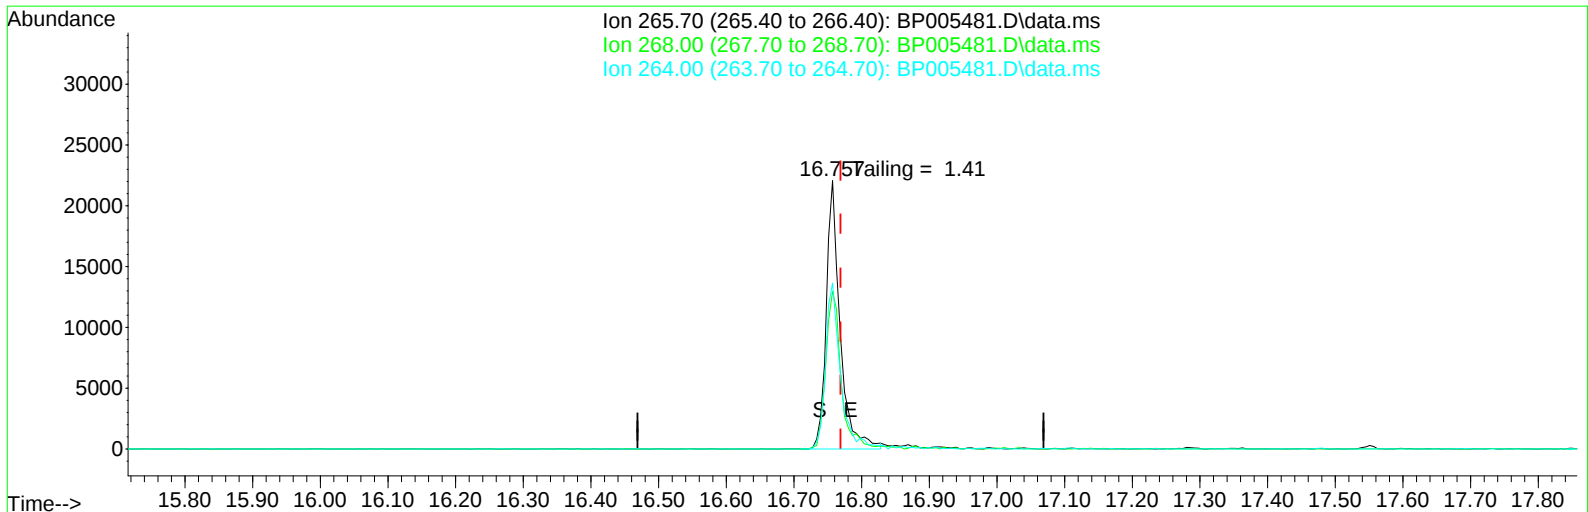

TIC: BP005481.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.012) 502512.69 ng

response 31669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	58.78
264.00	67.10	61.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2021	BNA_P	BP005481.D
Compound Name	Response	Retention Time
DDT	115392	20.49
DDD	1033	20.07
DDE	323	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1356	116748	1.16