




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010287.D
 Acq On : 11 May 2022 13:43
 Operator : CG/JU
 Sample : N2632-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B2

Manual IntegrationsAPPROVED

Quant Time: May 12 01:12:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

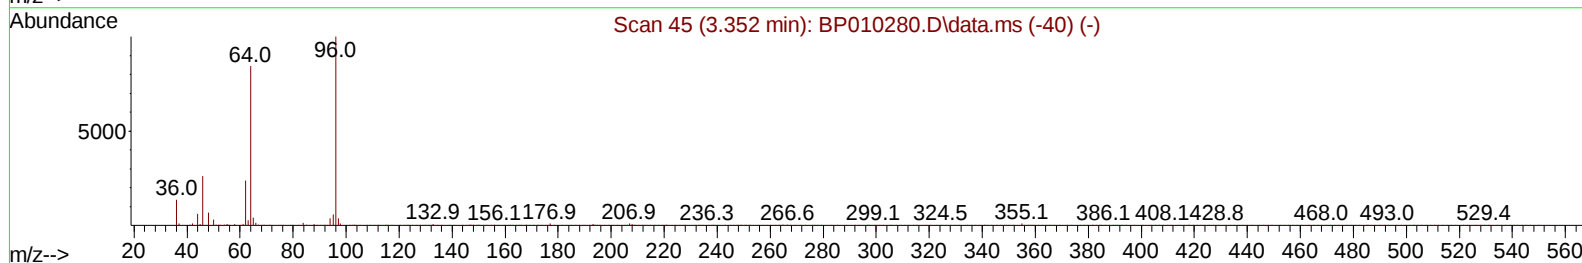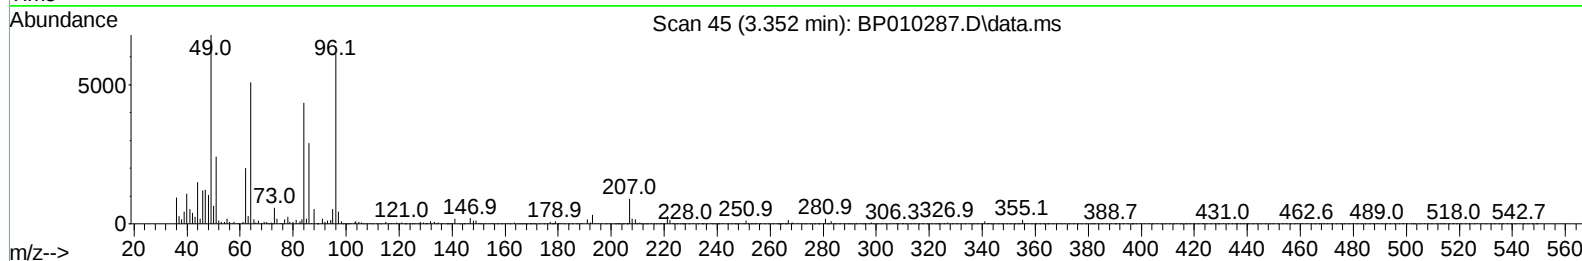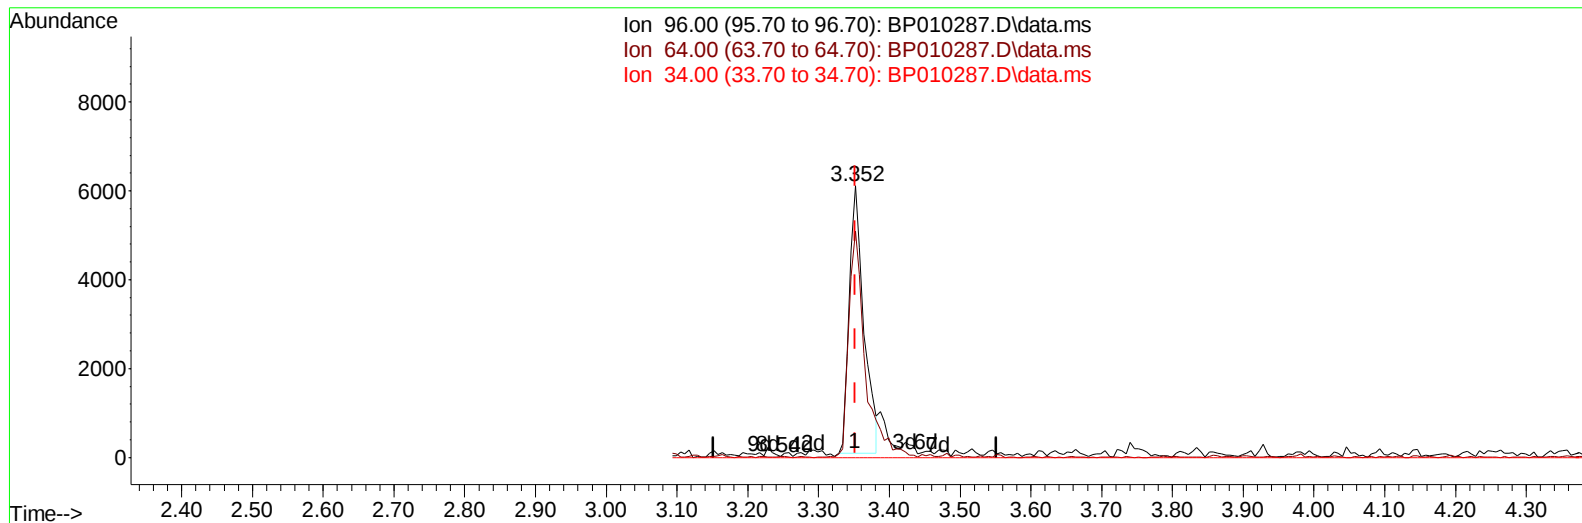

TIC: BP010287.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 2.62 ng/uL

response 8633

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.24#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010287.D
 Acq On : 11 May 2022 13:43
 Operator : CG/JU
 Sample : N2632-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B2

Manual IntegrationsAPPROVED

Quant Time: May 12 01:12:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

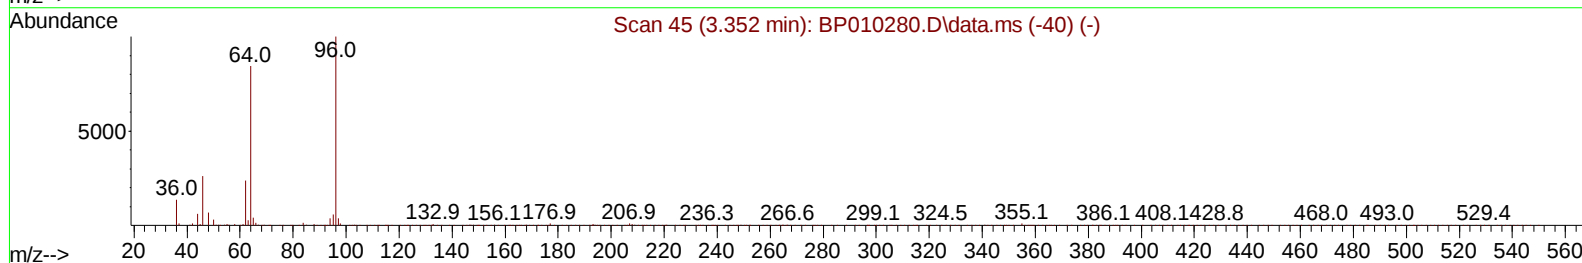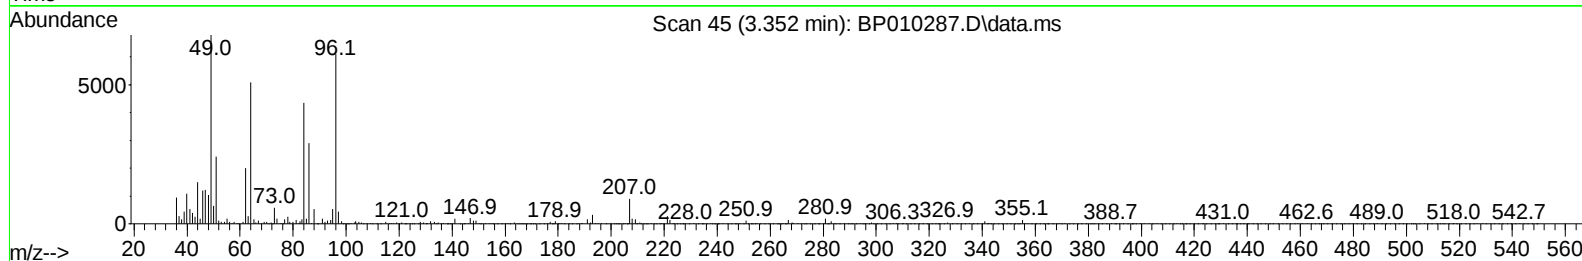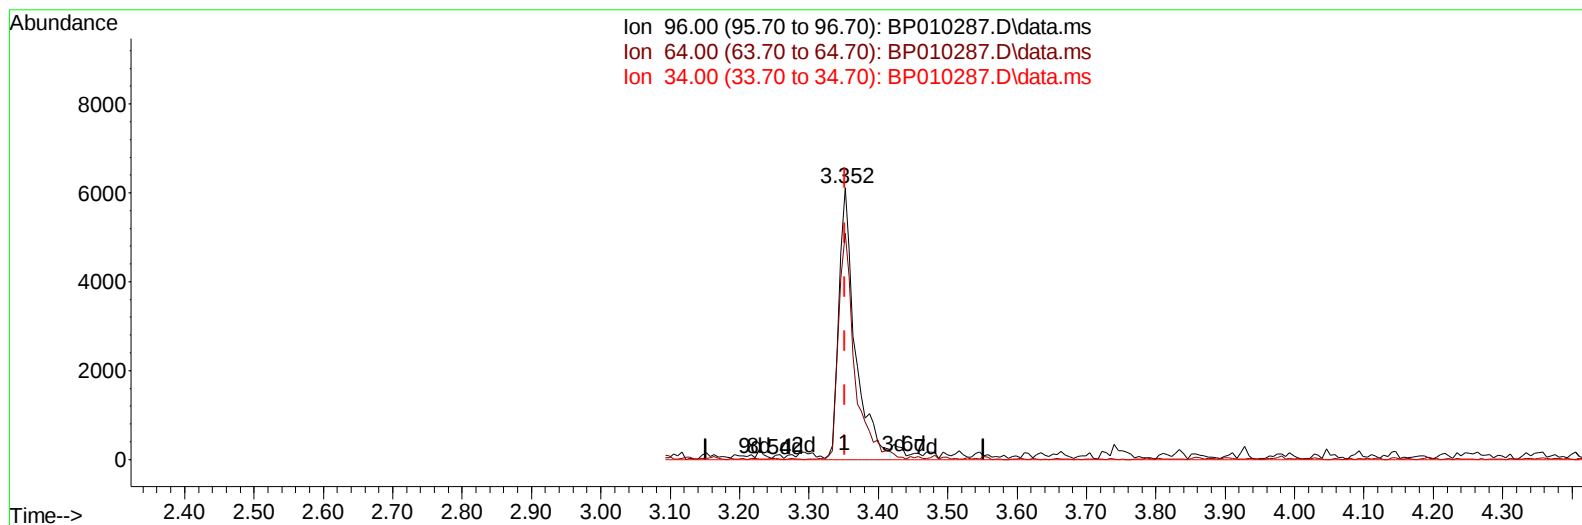

TIC: BP010287.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 3.05 ng/uL m

response 10046

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.24#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010287.D
Acq On : 11 May 2022 13:43
Operator : CG/JU
Sample : N2632-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B2

Manual IntegrationsAPPROVED

Quant Time: May 12 01:12:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

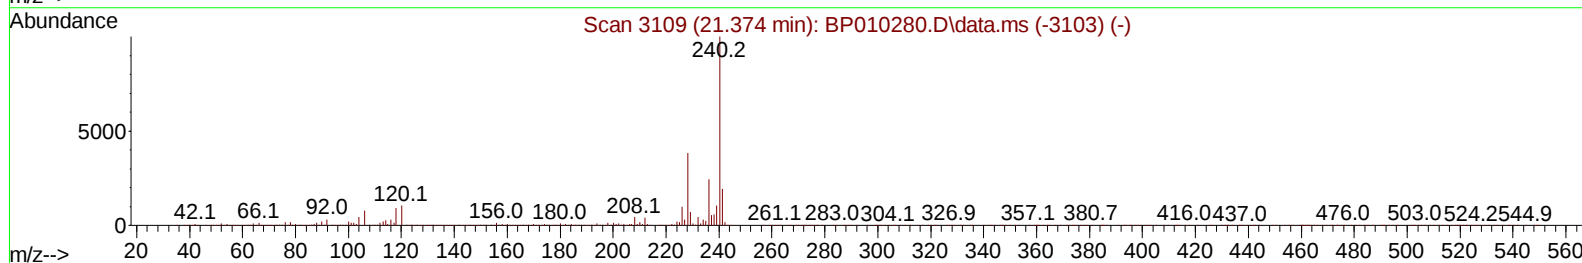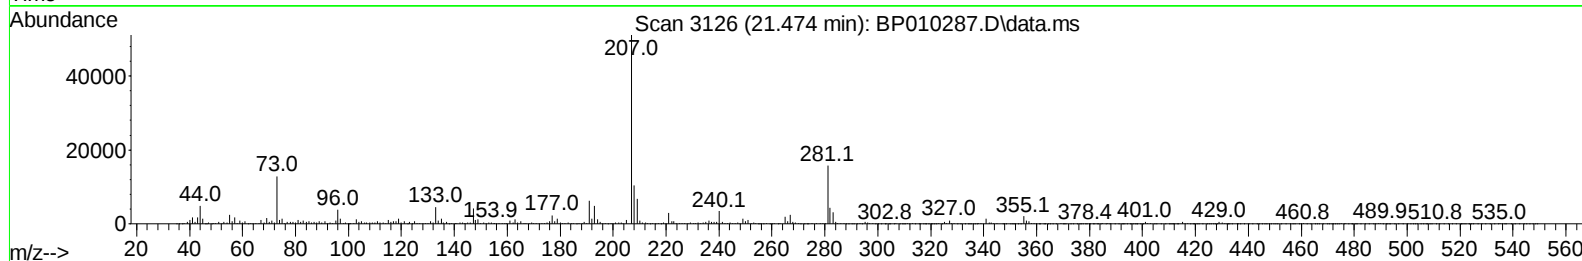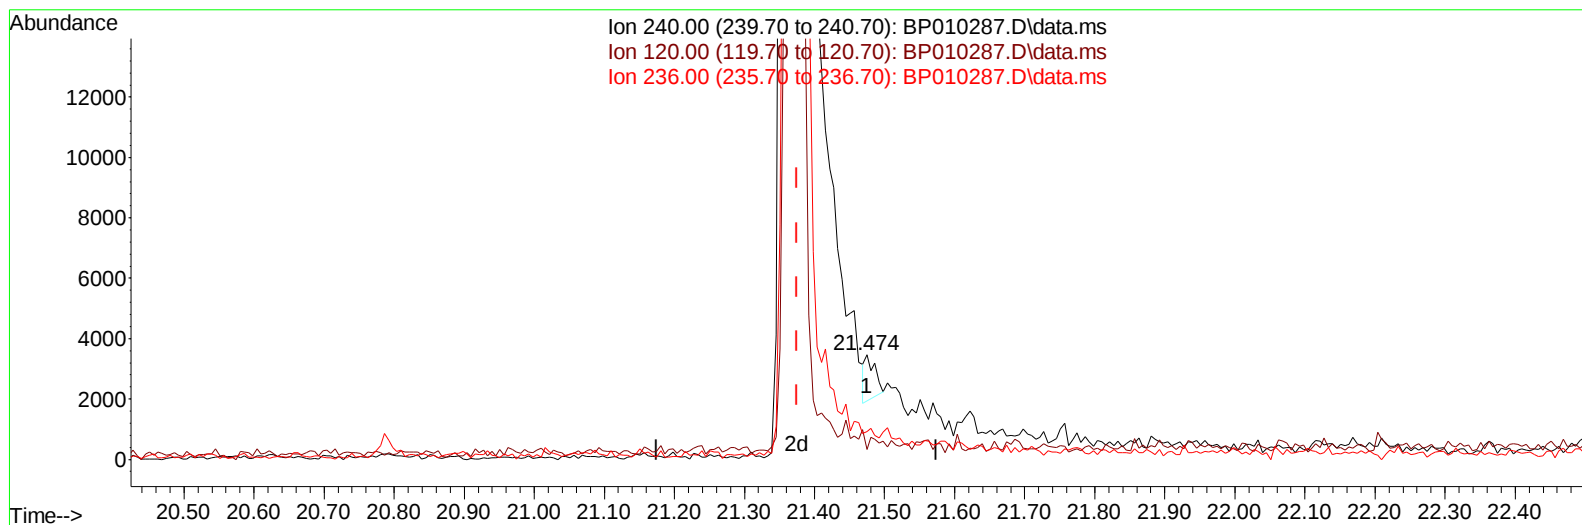

TIC: BP010287.D\data.ms

(79) Chrysene-d12 (I)

21.474min (+ 0.100) 20.00 ng/u1

response 1462

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	9.62
236.00	31.60	26.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010287.D
 Acq On : 11 May 2022 13:43
 Operator : CG/JU
 Sample : N2632-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:12:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

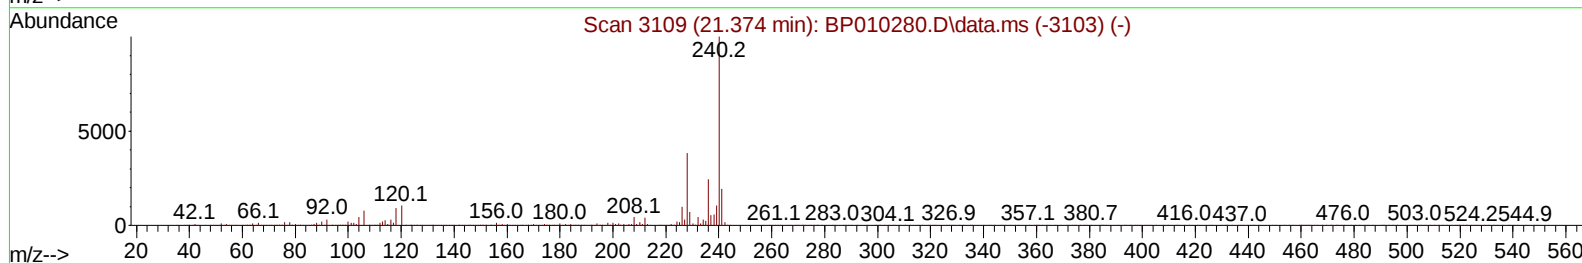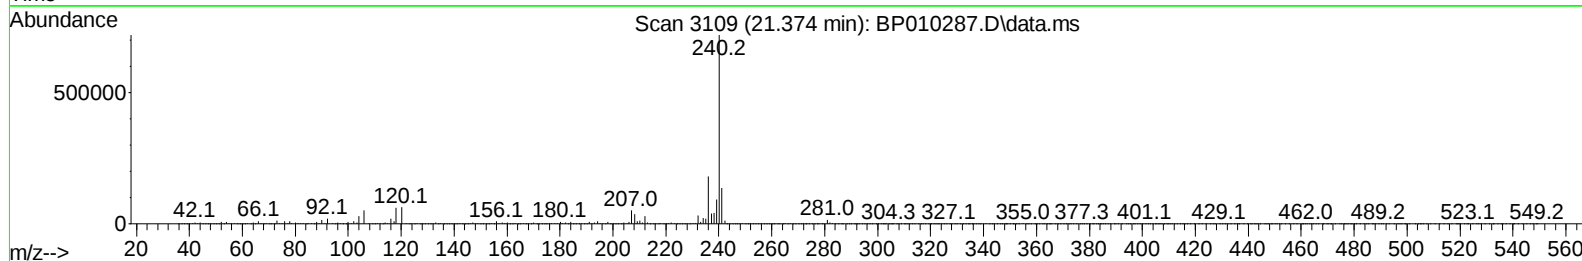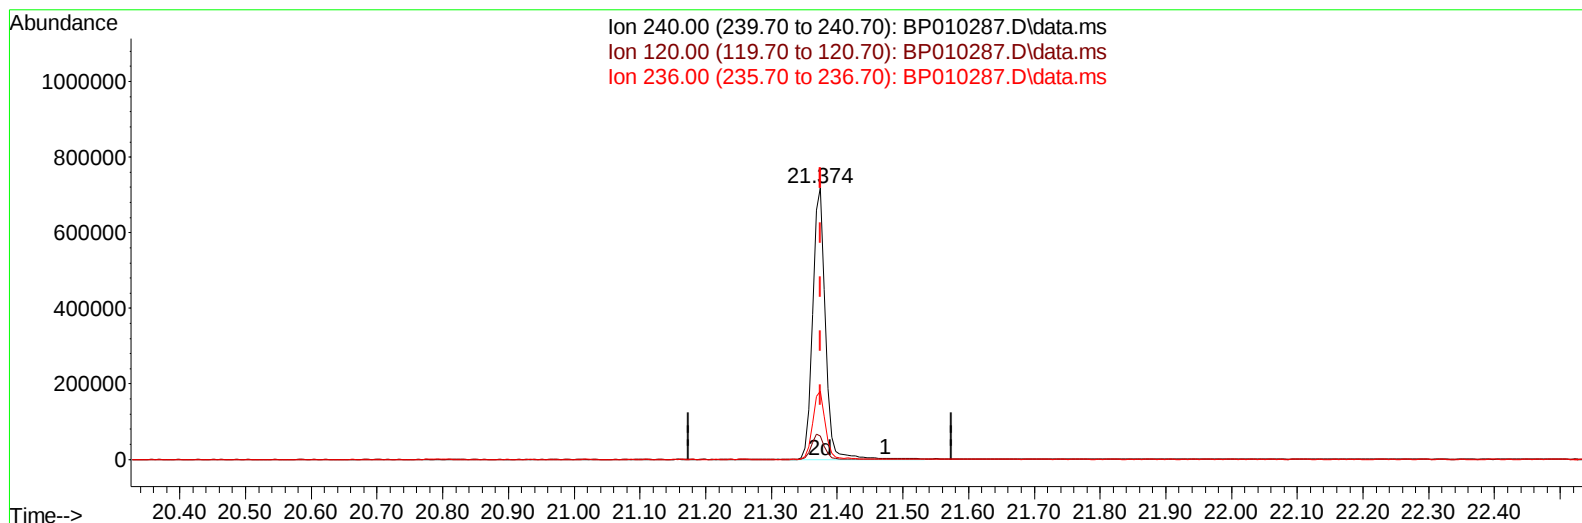

TIC: BP010287.D\data.ms

(79) Chrysene-d12 (I)

21.374min (+ 0.000) 20.00 ng/ul m

response 975309

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	8.68
236.00	31.60	25.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010287.D
 Acq On : 11 May 2022 13:43
 Operator : CG/JU
 Sample : N2632-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:12:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	139729	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	633524	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	446394	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	991884	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.374	240	975309m	20.000	ng/ul	0.00
88) Perylene-d12	23.804	264	971189	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	10046m	3.054	ng/uL	0.00
4) Pyridine-d5	3.781	84	27182	2.970	ng/ul	0.01
7) Phenol-d5	7.069	99	192617	14.842	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	136011	16.941	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	155106	16.228	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	155274	14.553	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	79931	15.735	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	87133	15.044	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	160021	15.180	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	187681	12.060	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	601545	16.915	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	664301	15.668	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	70158	10.285	ng/ul	0.00
60) Fluorene-d10	15.534	176	518567	17.275	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	73471	10.817	ng/ul	0.00
73) Anthracene-d10	17.386	188	789580	16.256	ng/ul	0.00
81) Pyrene-d10	19.622	212	1018479	18.897	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.651	264	912450	17.617	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010287.D
Acq On : 11 May 2022 13:43
Operator : CG/JU
Sample : N2632-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:12:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

