




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010290.D
Acq On : 11 May 2022 15:58
Operator : CG/JU
Sample : N2632-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4A8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:13:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

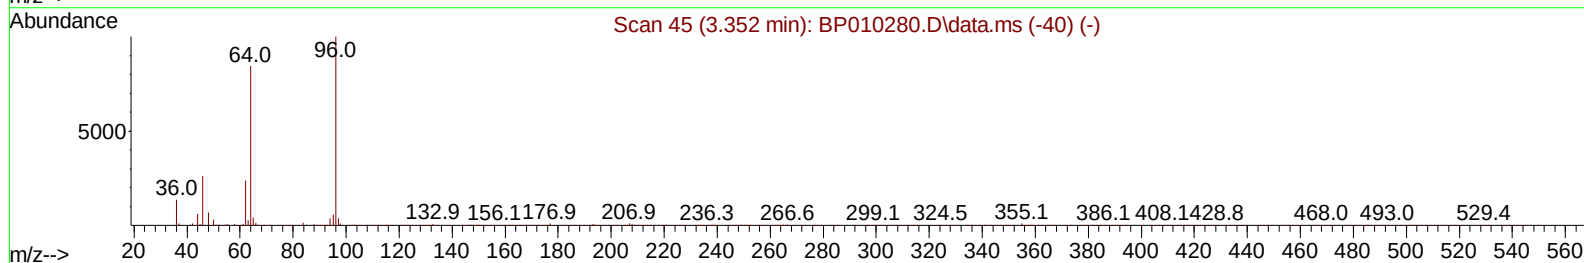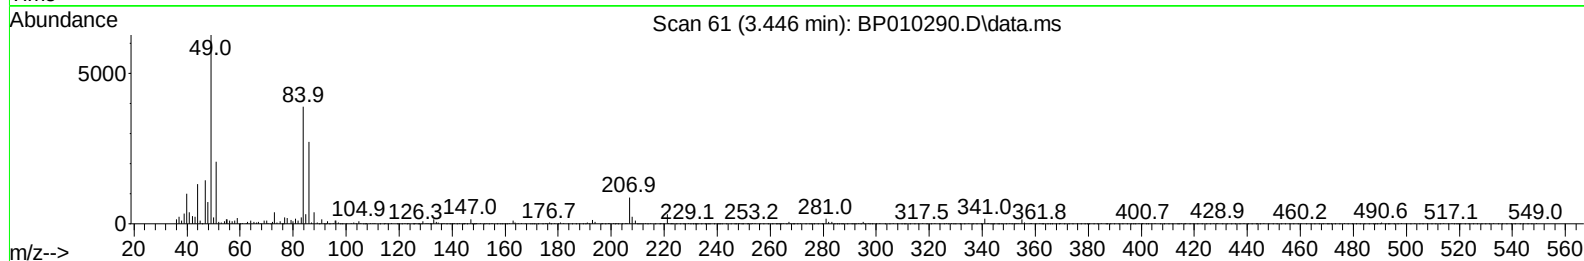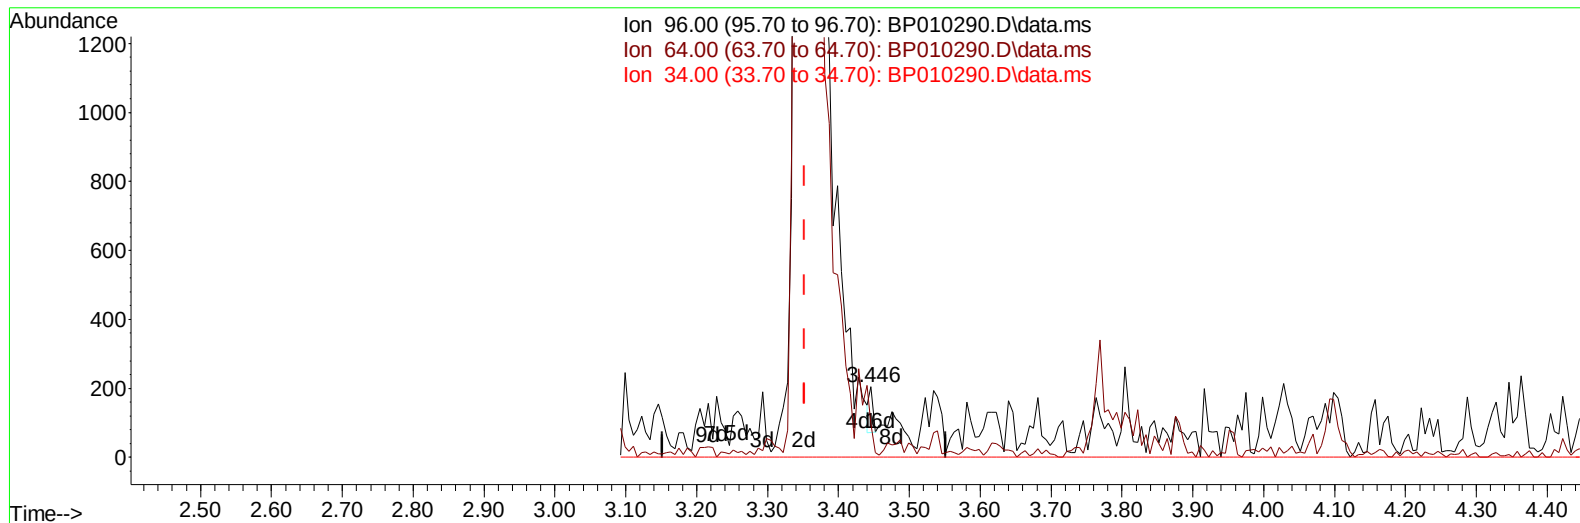

TIC: BP010290.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.446min (+ 0.094) 0.02 ng/uL

response 47

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	47.32
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010290.D
 Acq On : 11 May 2022 15:58
 Operator : CG/JU
 Sample : N2632-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4A8

Manual IntegrationsAPPROVED

Quant Time: May 12 01:13:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

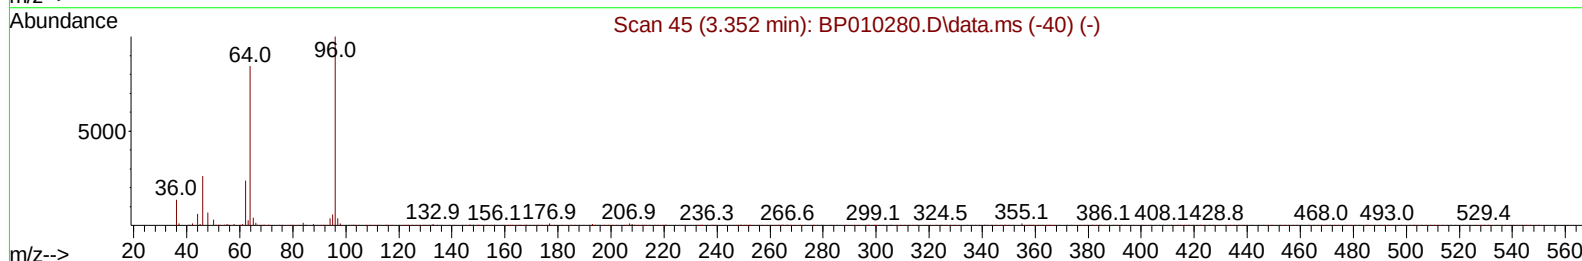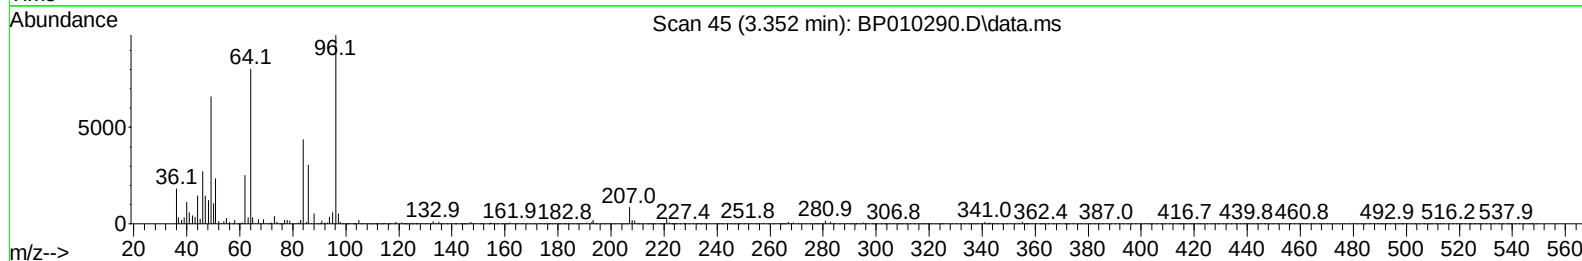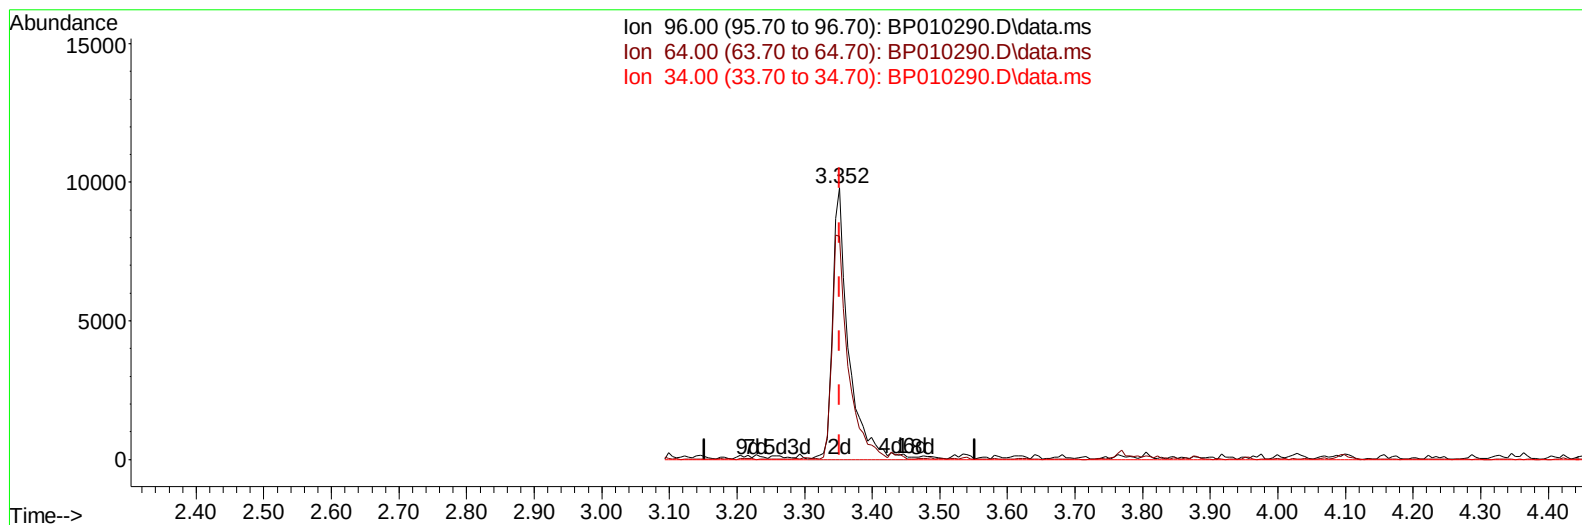

TIC: BP010290.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.76 ng/uL m

response 16184

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	82.14#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010290.D
 Acq On : 11 May 2022 15:58
 Operator : CG/JU
 Sample : N2632-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4A8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:13:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	119379	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	531495	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	379417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	841290	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.374	240	871603	20.000	ng/ul	# 0.00
88) Perylene-d12	23.803	264	892457	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	16184m	5.759	ng/uL	0.00
4) Pyridine-d5	3.769	84	168968	21.607	ng/ul	0.00
7) Phenol-d5	7.069	99	279241	25.185	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	195663	28.526	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	227542	27.865	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	242505	26.603	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	117827	27.648	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	127854	26.313	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	225638	25.514	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	321111	24.595	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	840282	27.799	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	931634	25.851	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143	110439	19.048	ng/ul	0.00
60) Fluorene-d10	15.533	176	719655	28.205	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	113683	19.733	ng/ul	0.00
73) Anthracene-d10	17.386	188	1115879	27.086	ng/ul	0.00
81) Pyrene-d10	19.621	212	1393883	28.939	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	1340919	28.174	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010290.D
Acq On : 11 May 2022 15:58
Operator : CG/JU
Sample : N2632-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4A8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:13:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

