




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010293.D
 Acq On : 11 May 2022 18:50
 Operator : CG/JU
 Sample : PB144661BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK661

Manual IntegrationsAPPROVED

Quant Time: May 12 01:14:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

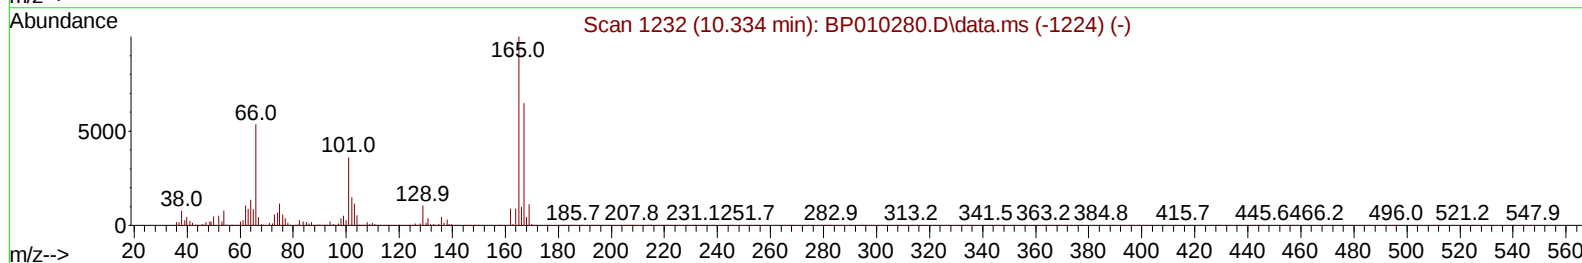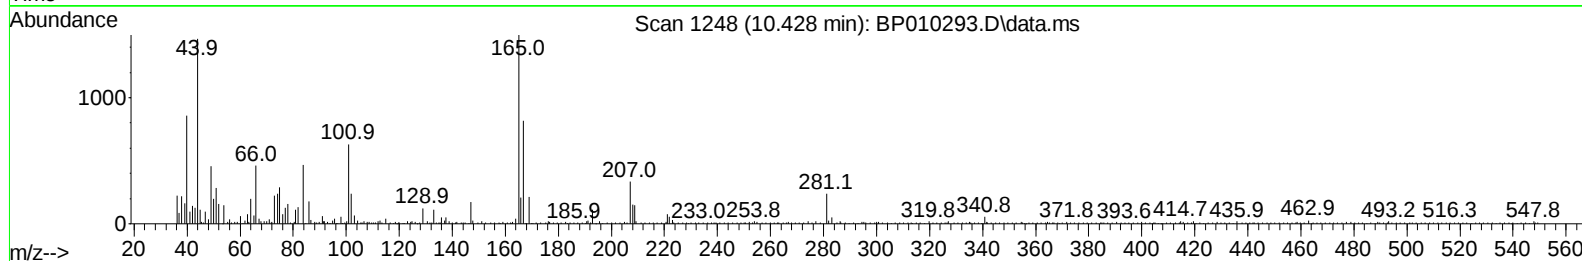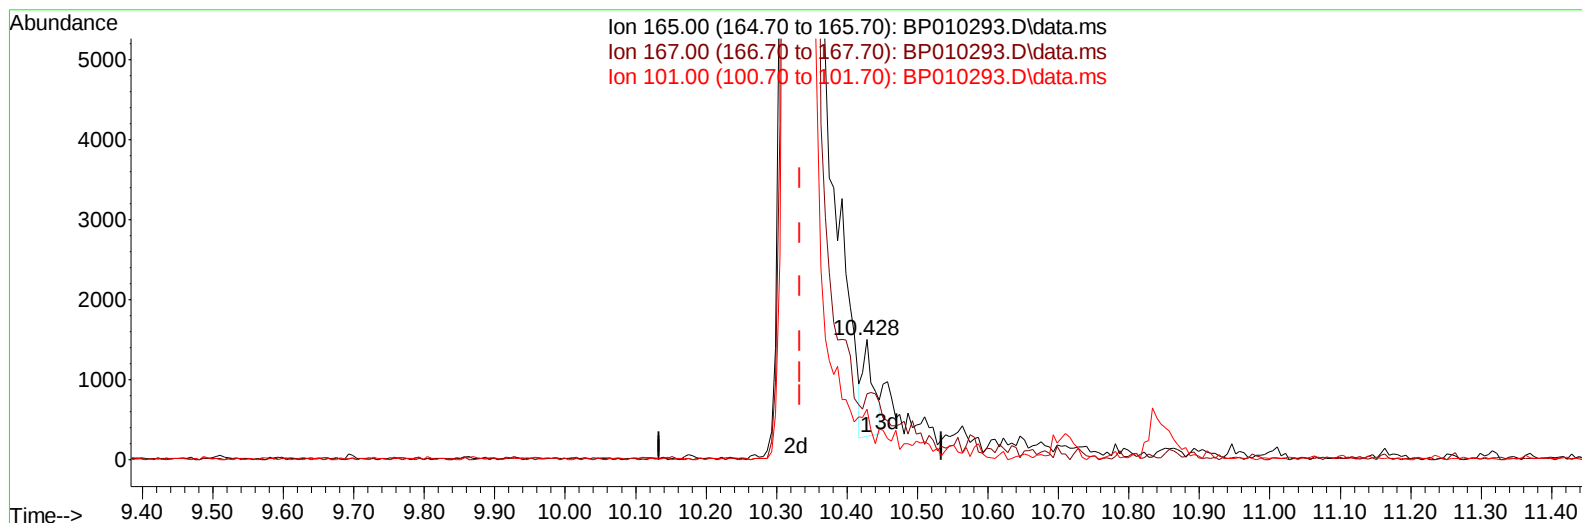

TIC: BP010293.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.428min (+ 0.094) 0.14 ng/ul

response 1301

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	55.07
101.00	49.80	42.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010293.D
 Acq On : 11 May 2022 18:50
 Operator : CG/JU
 Sample : PB144661BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK661

Manual IntegrationsAPPROVED

Quant Time: May 12 01:14:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

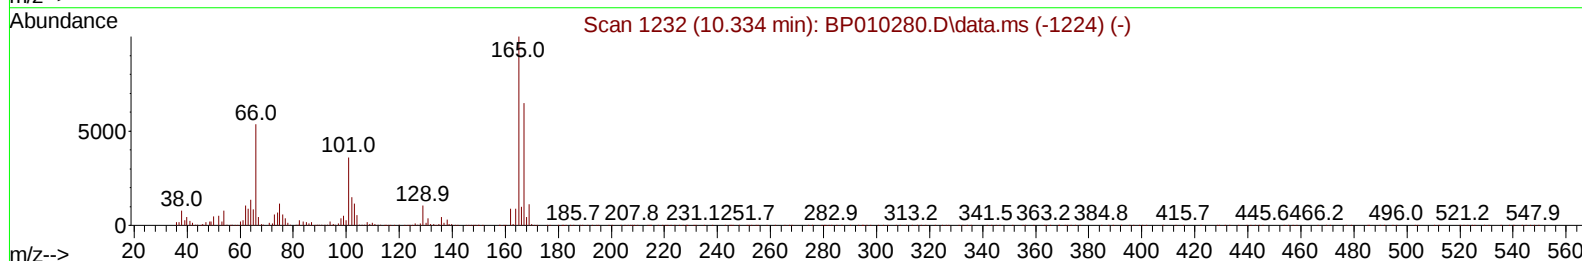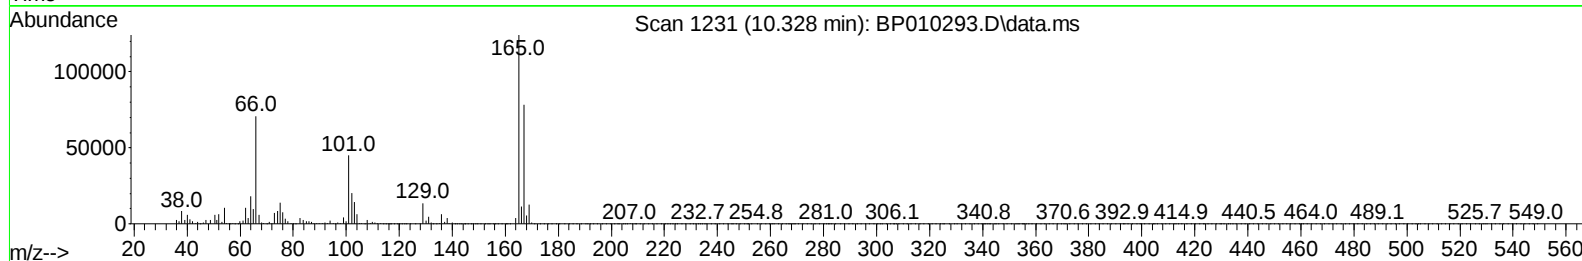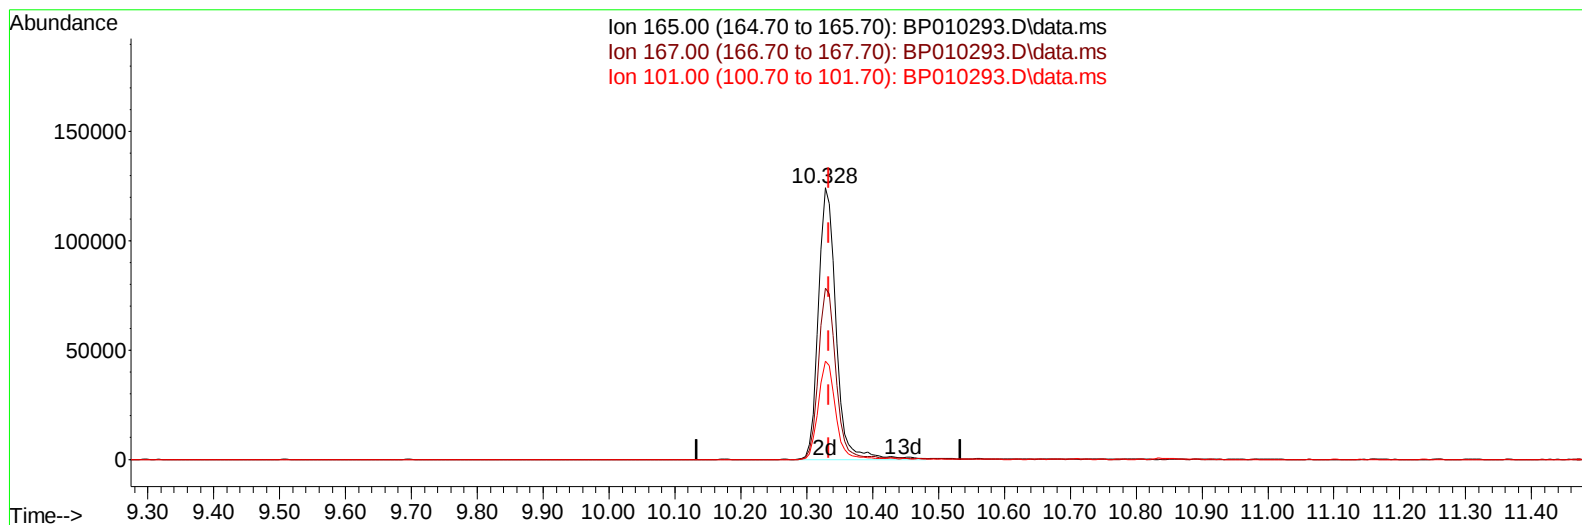

TIC: BP010293.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.328min (-0.006) 24.47 ng/ul m

response 228212

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	63.17
101.00	49.80	36.20#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010293.D
 Acq On : 11 May 2022 18:50
 Operator : CG/JU
 Sample : PB144661BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK661

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:14:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	125403	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	560379	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	406299	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	895397	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	897101	20.000	ng/ul	# 0.00
88) Perylene-d12	23.798	264	897606	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	17020	5.766	ng/uL	0.00
4) Pyridine-d5	3.769	84	219991	26.781	ng/ul	0.00
7) Phenol-d5	7.069	99	277014	23.784	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	201255	27.932	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	227975	26.577	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	241251	25.194	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	123006	27.376	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	130557	25.484	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	228212m	24.475	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	335114	24.344	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	901319	27.846	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	966335	25.040	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	126739	20.413	ng/ul	0.00
60) Fluorene-d10	15.528	176	749612	27.435	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	131232	21.403	ng/ul	0.00
73) Anthracene-d10	17.386	188	1203110	27.438	ng/ul	0.00
81) Pyrene-d10	19.622	212	1471217	29.677	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	1359317	28.396	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010293.D
Acq On : 11 May 2022 18:50
Operator : CG/JU
Sample : PB144661BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK661

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:14:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

