




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010297.D
 Acq On : 11 May 2022 22:13
 Operator : CG/JU
 Sample : N2632-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B6

Manual IntegrationsAPPROVED

Quant Time: May 12 01:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

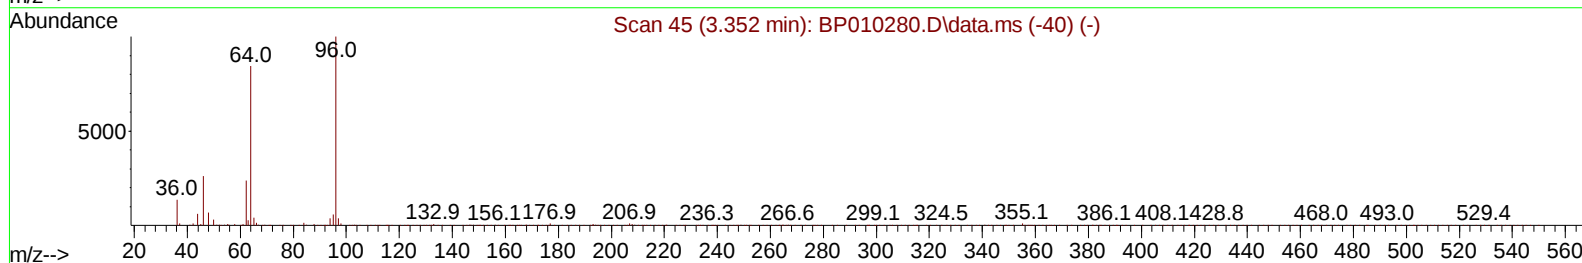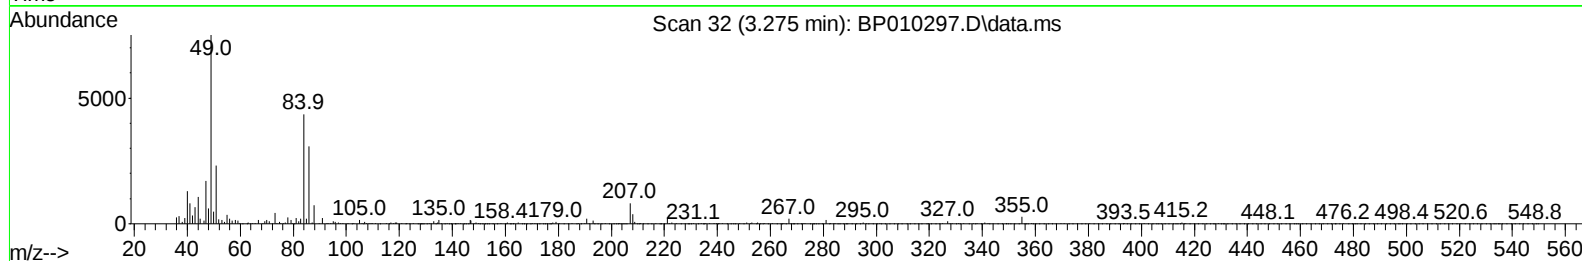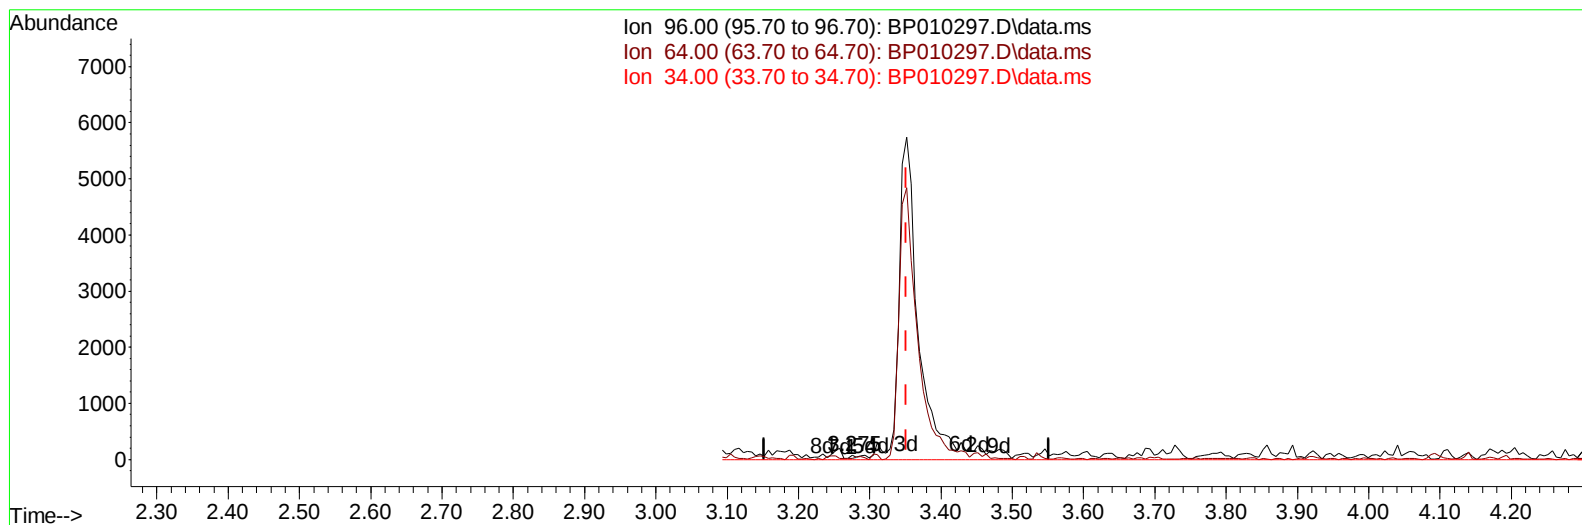

TIC: BP010297.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.275min (-0.076) 0.01 ng/uL

response	32	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	45.95
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010297.D
 Acq On : 11 May 2022 22:13
 Operator : CG/JU
 Sample : N2632-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B6

Manual IntegrationsAPPROVED

Quant Time: May 12 01:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

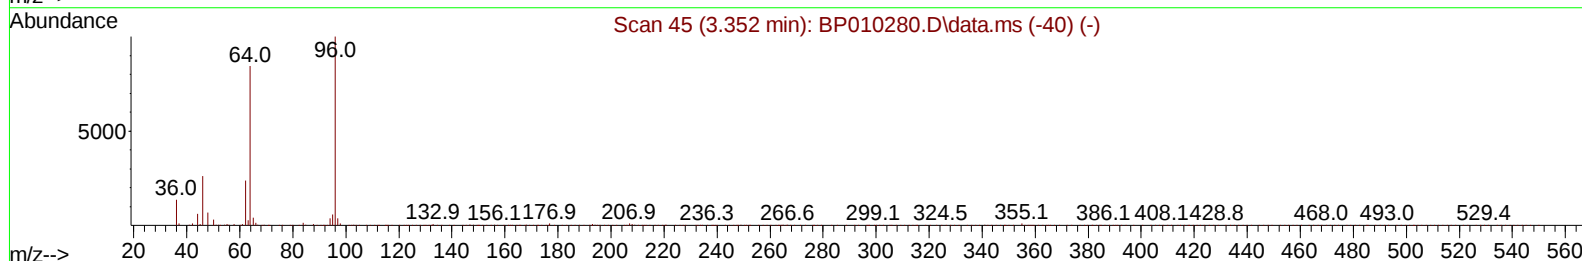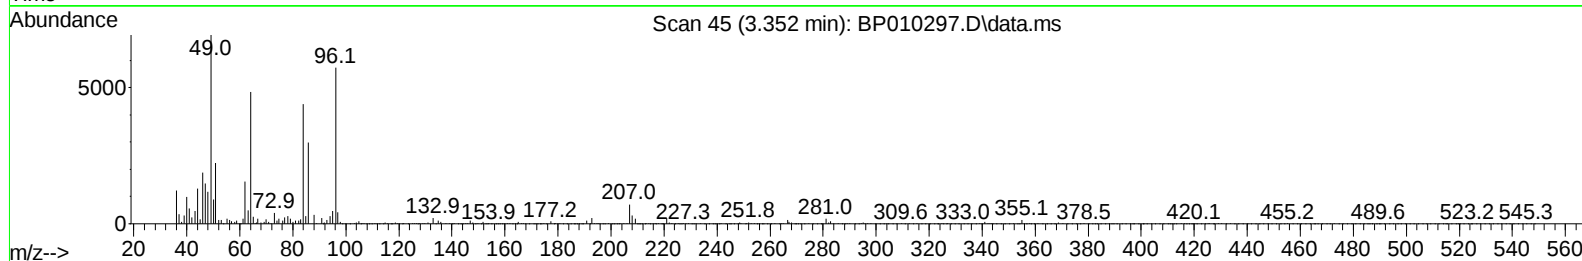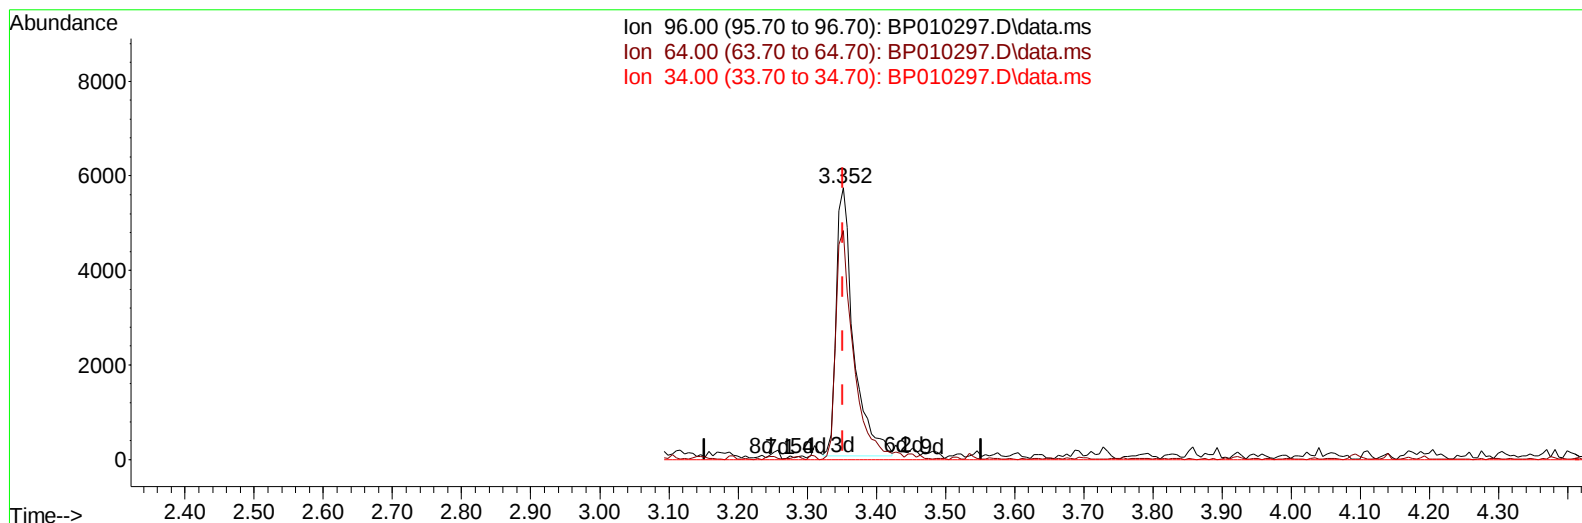

TIC: BP010297.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 2.61 ng/uL m

response 9889

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	84.23#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010297.D
 Acq On : 11 May 2022 22:13
 Operator : CG/JU
 Sample : N2632-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	160967	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	726863	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	514563	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1106100	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	1110013	20.000	ng/ul	# 0.00
88) Perylene-d12	23.804	264	1085960	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	9889m	2.610	ng/uL	0.00
4) Pyridine-d5	3.781	84	41230	3.910	ng/ul	0.01
7) Phenol-d5	7.069	99	204693	13.692	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	144301	15.602	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	163016	14.805	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	161211	13.116	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	88249	15.142	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	91319	13.742	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	166400	13.758	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	214887	12.035	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	642769	15.680	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	694262	14.205	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	79195	10.072	ng/ul	0.00
60) Fluorene-d10	15.528	176	561666	16.232	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	73883	9.754	ng/ul	0.00
73) Anthracene-d10	17.386	188	873894	16.134	ng/ul	0.00
81) Pyrene-d10	19.616	212	1140041	18.586	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	1029196	17.771	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010297.D
Acq On : 11 May 2022 22:13
Operator : CG/JU
Sample : N2632-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:15:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

