




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

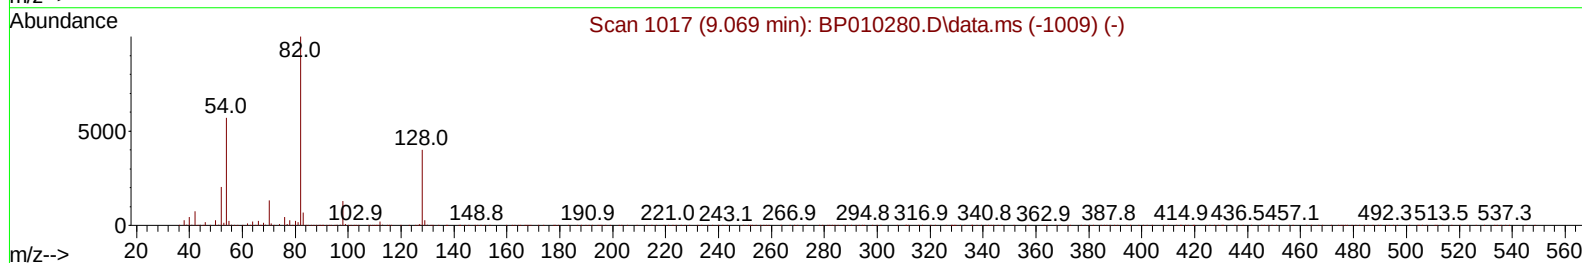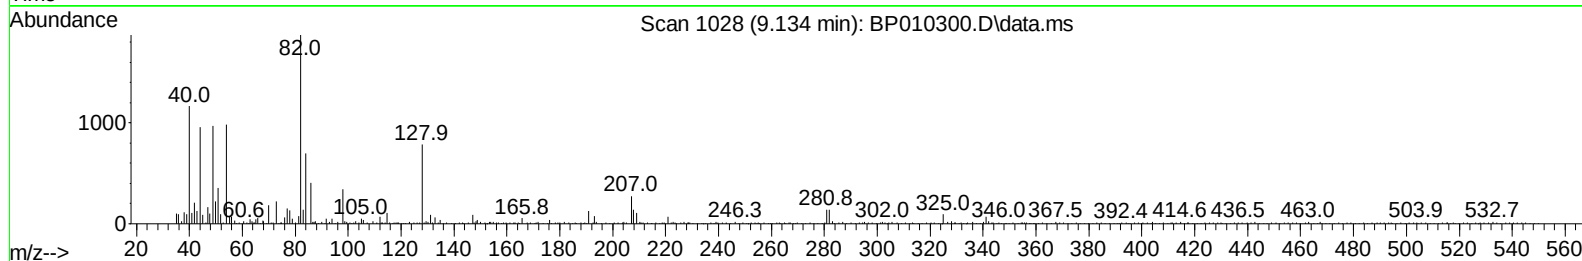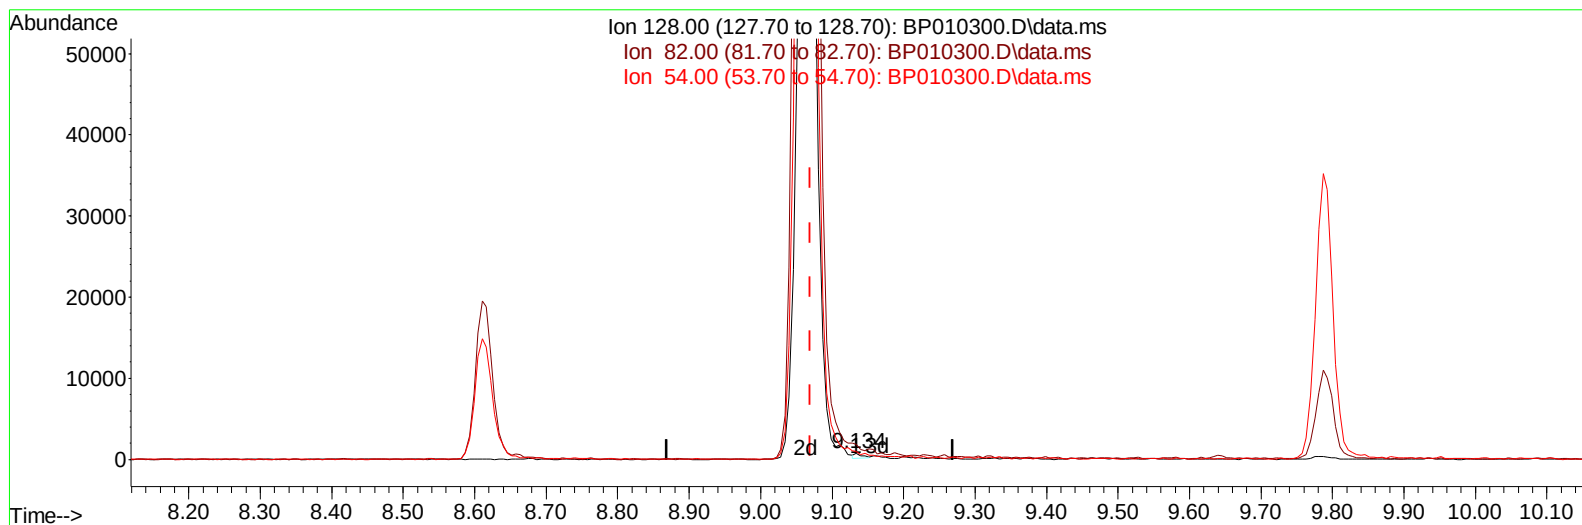

TIC: BP010300.D\data.ms

(21) Nitrobenzene-d5 (S)

9.134min (+ 0.065) 0.09 ng/u1

response 459

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	238.04
54.00	120.20	125.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

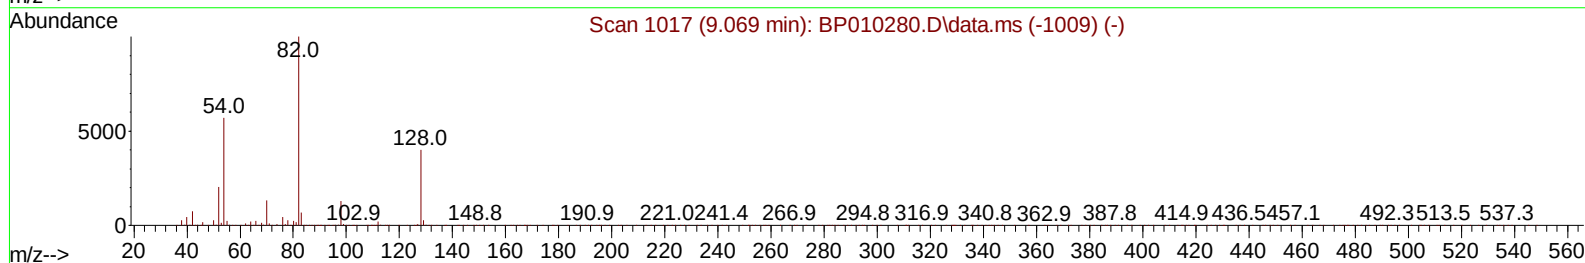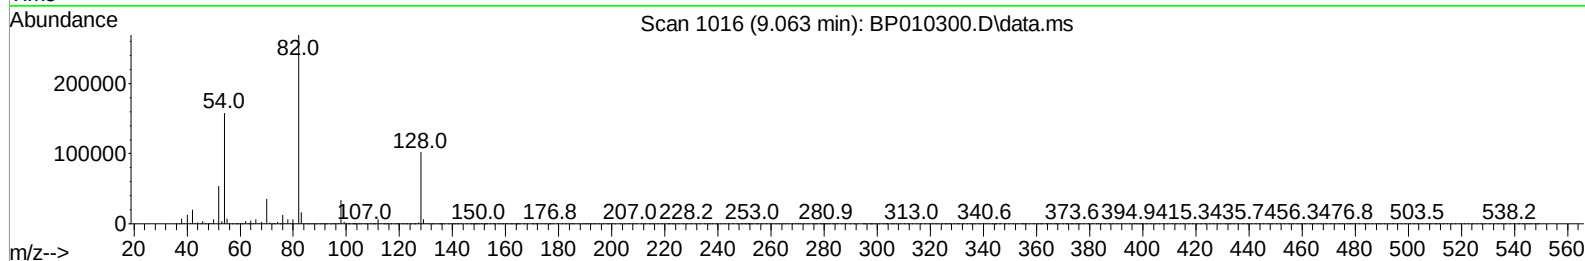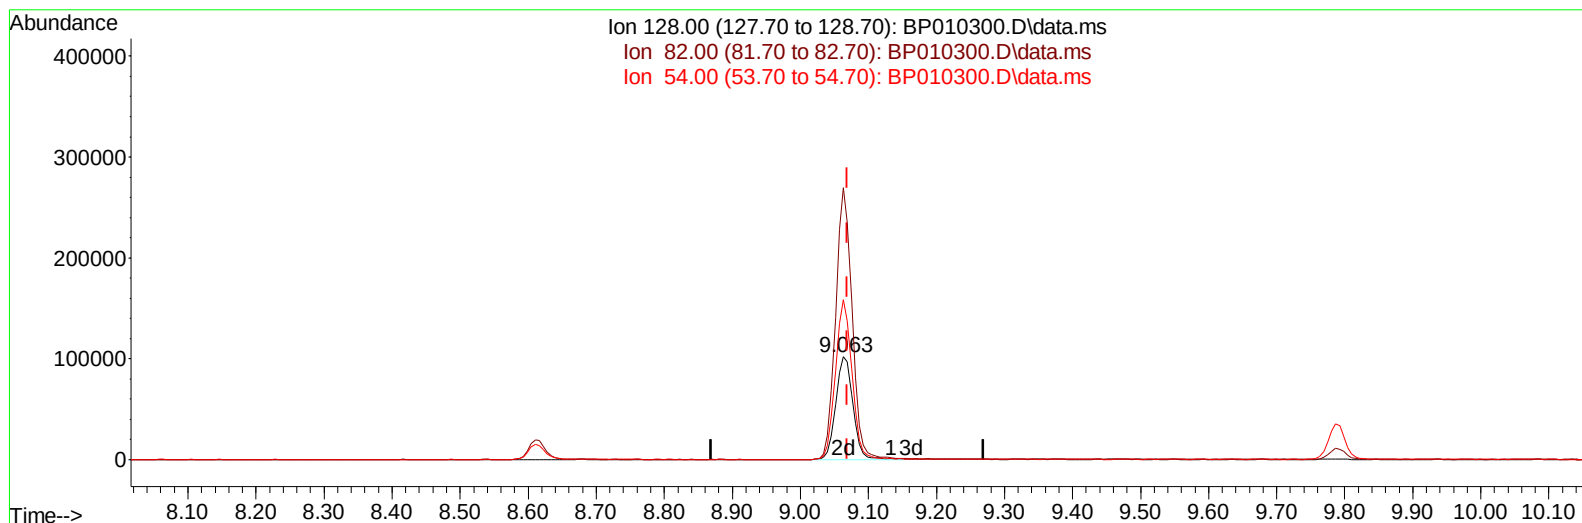

TIC: BP010300.D\data.ms

(21) Nitrobenzene-d5 (S)

9.063min (-0.006) 35.41 ng/ul m

response 178220

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	264.03
54.00	120.20	155.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

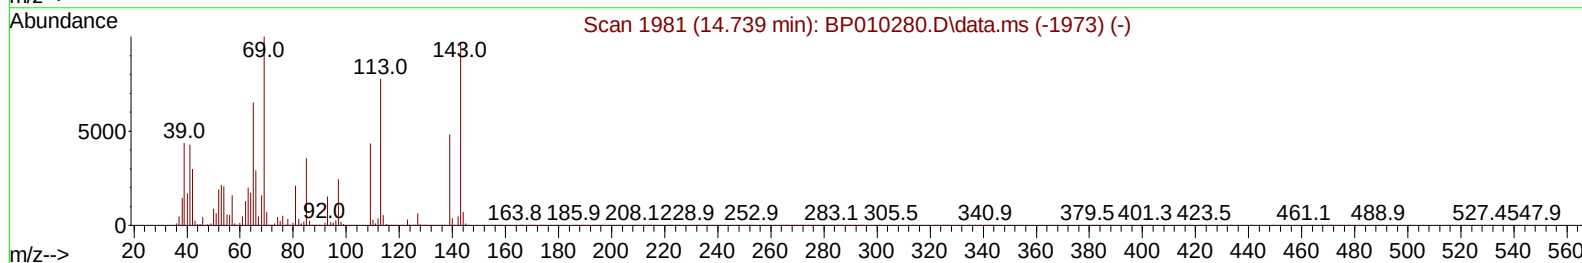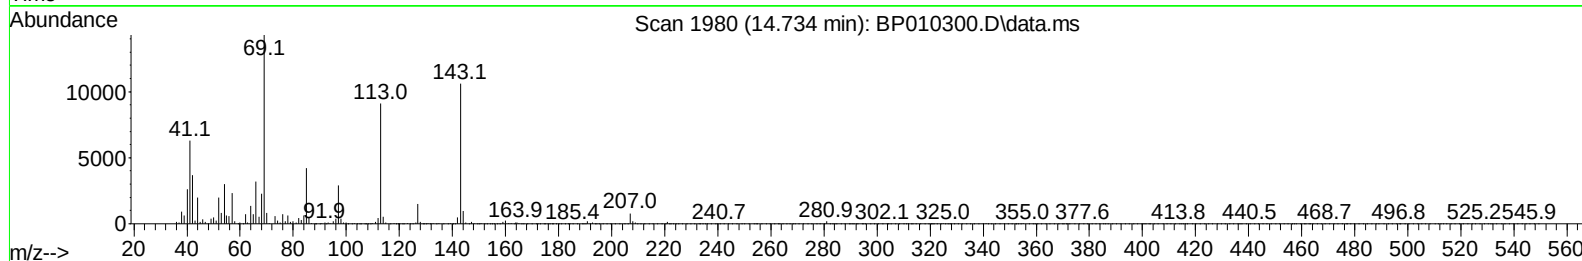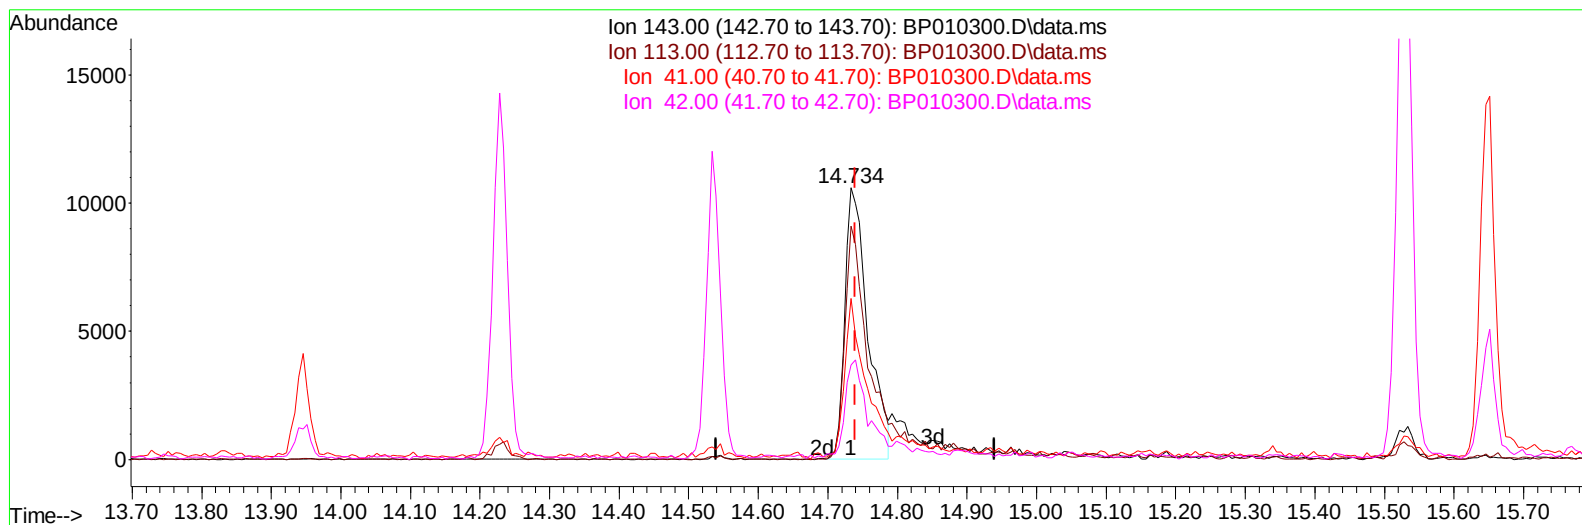

TIC: BP010300.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 3.48 ng/ul

response 24305

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.90#
41.00	23.20	59.24#
42.00	18.00	34.73#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010300.D
Acq On : 11 May 2022 23:54
Operator : CG/JU
Sample : N2707-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:16:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

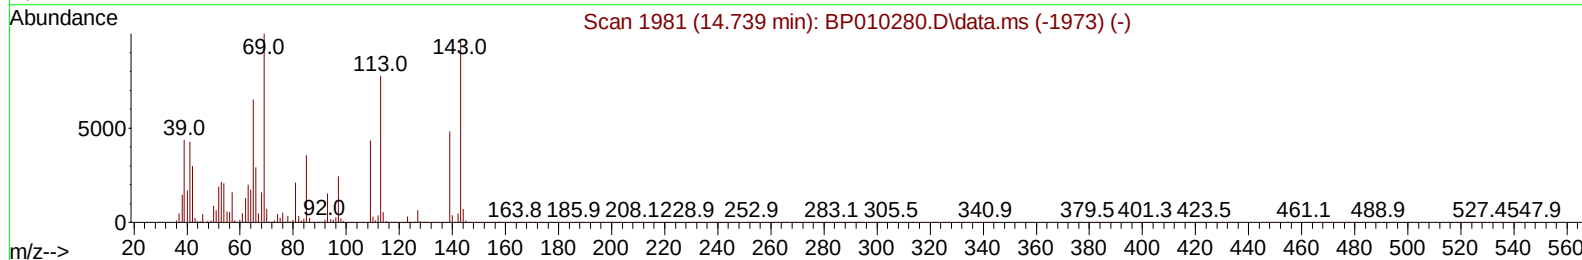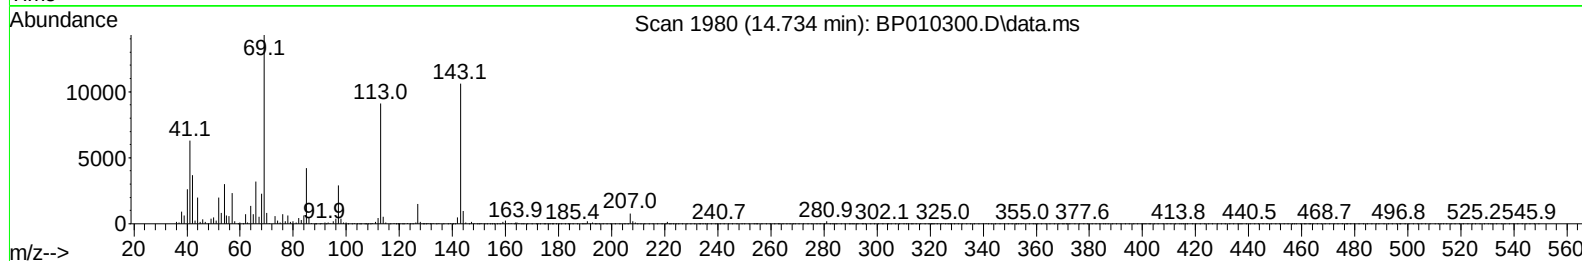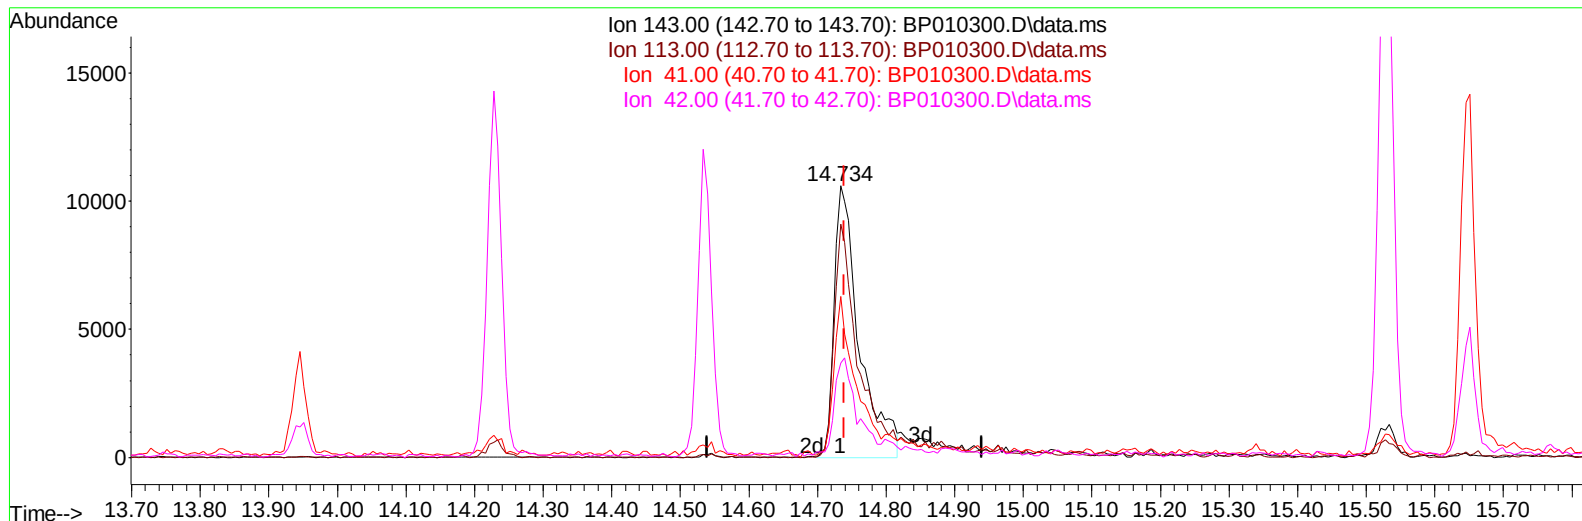

TIC: BP010300.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 3.85 ng/ul m

response 26900

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	85.90#
41.00	23.20	59.24#
42.00	18.00	34.73#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

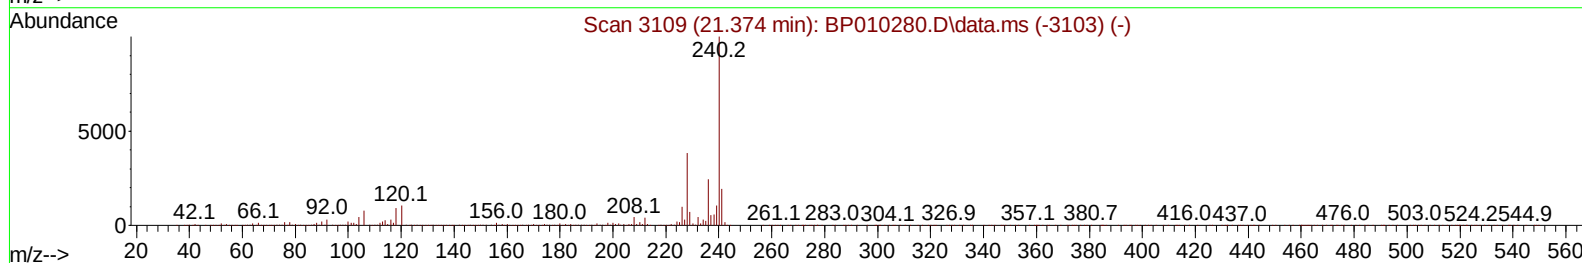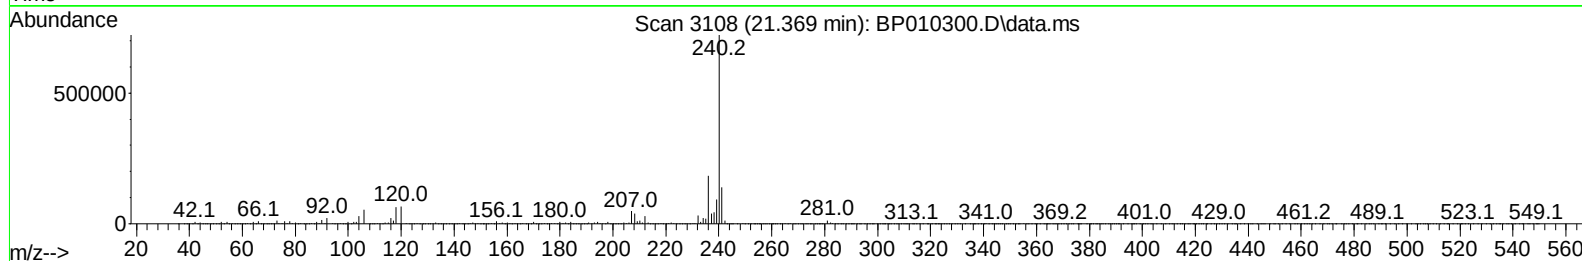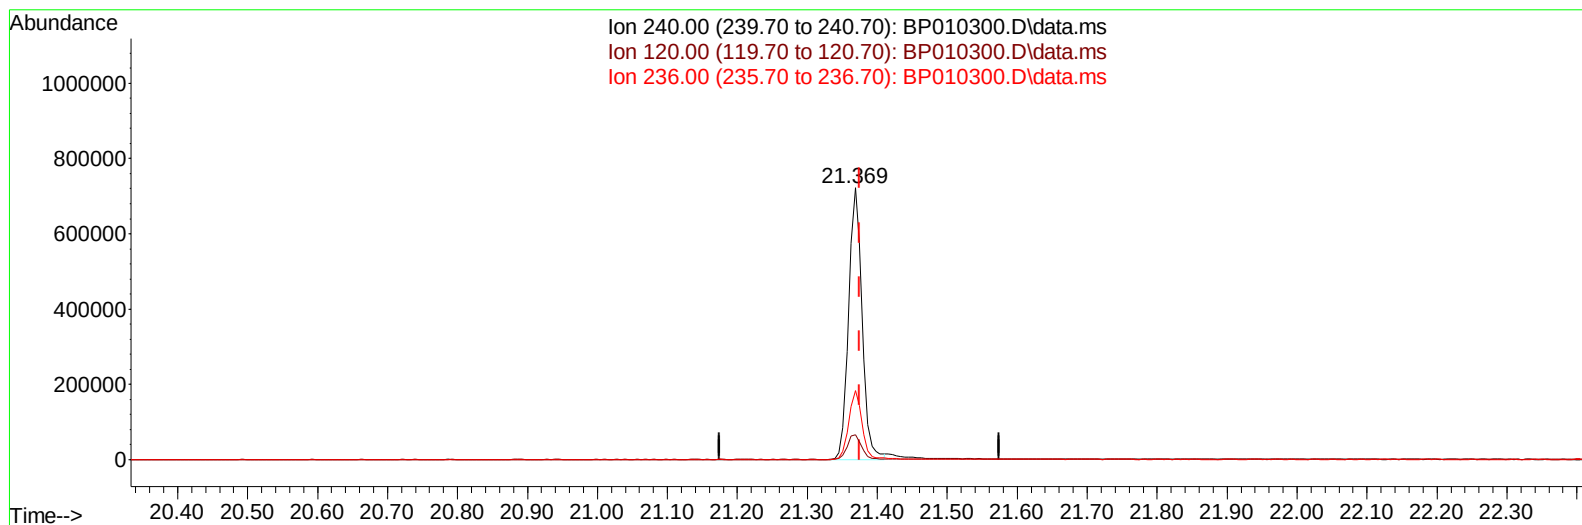

TIC: BP010300.D\data.ms

(79) Chrysene-d12 (I)

21.369min (-0.006) 20.00 ng/ul

response 955166

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	9.21
236.00	31.60	25.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

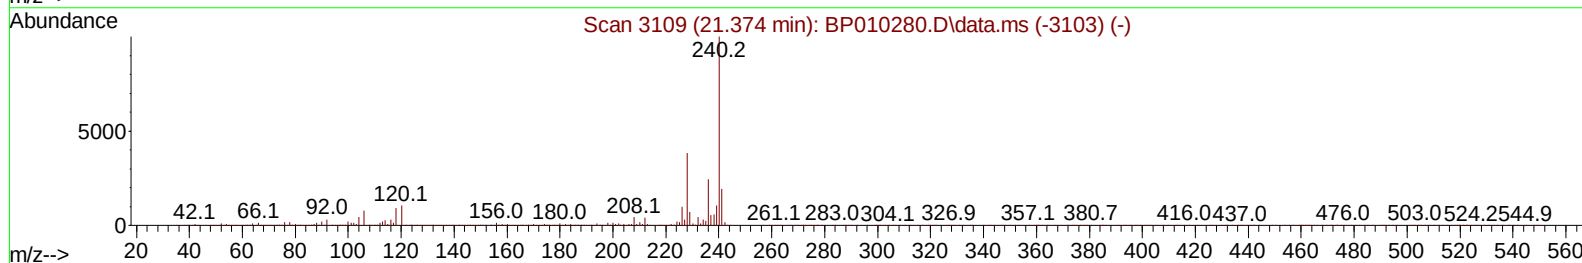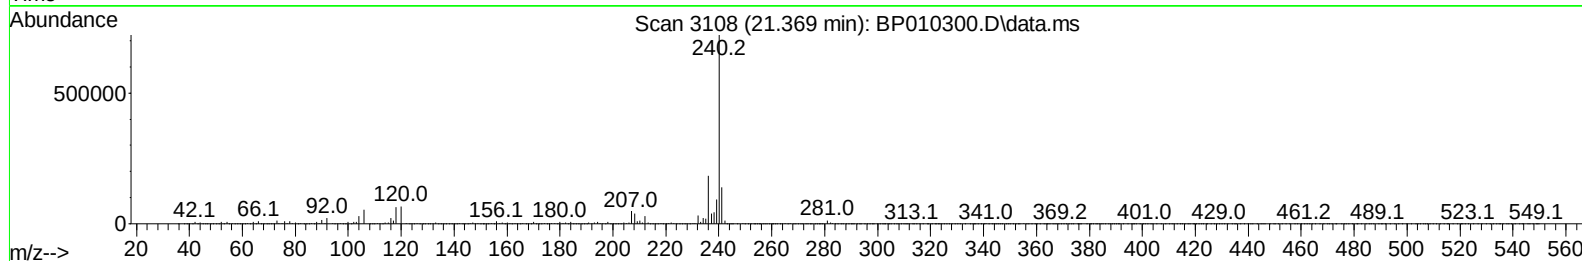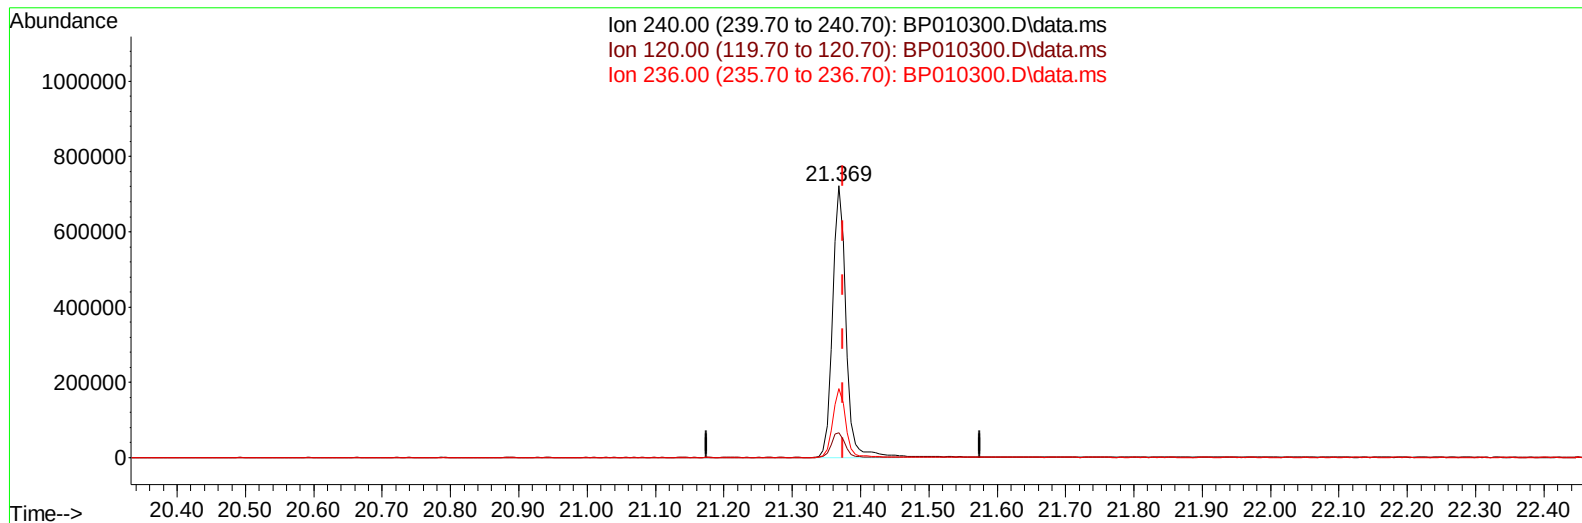

TIC: BP010300.D\data.ms

(79) Chrysene-d12 (I)

21.369min (-0.006) 20.00 ng/ul m

response 979055

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	9.21
236.00	31.60	25.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010300.D
 Acq On : 11 May 2022 23:54
 Operator : CG/JU
 Sample : N2707-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:16:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	139126	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	627759	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	456710	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	993750	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	979055m	20.000	ng/ul	0.00
88) Perylene-d12	23.798	264	937072	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	12823	3.915	ng/uL	0.00
4) Pyridine-d5	3.775	84	54040	5.930	ng/ul	0.00
7) Phenol-d5	7.069	99	68794	5.324	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	287704	35.991	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	234860	24.679	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	153905	14.487	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	178220m	35.407	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	185904	32.393	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	287356	27.510	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	399235	25.889	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1316549	36.184	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1459325	33.641	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	26900m	3.854	ng/ul	0.00
60) Fluorene-d10	15.528	176	1133632	36.911	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	212180	31.179	ng/ul	0.00
73) Anthracene-d10	17.386	188	1889153	38.820	ng/ul	0.00
81) Pyrene-d10	19.622	212	2280694	42.154	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	2088619	41.794	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010300.D
Acq On : 11 May 2022 23:54
Operator : CG/JU
Sample : N2707-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA1

Manual IntegrationsAPPROVED

Quant Time: May 12 01:16:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

