




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

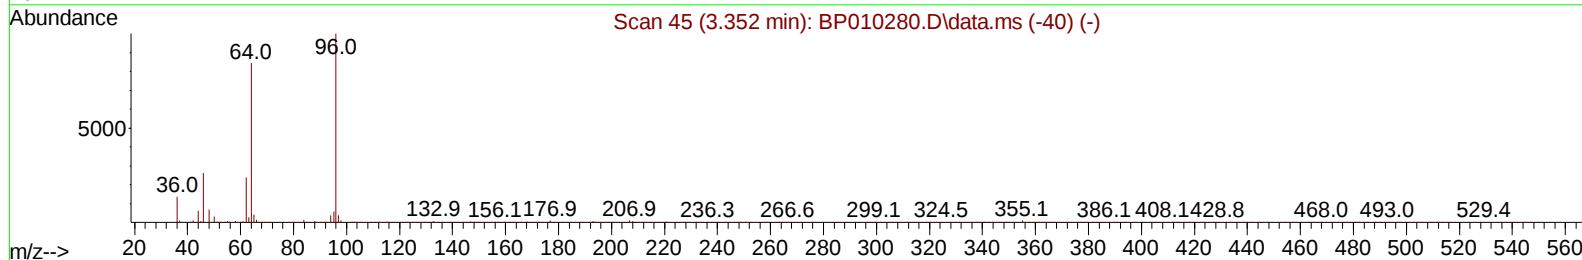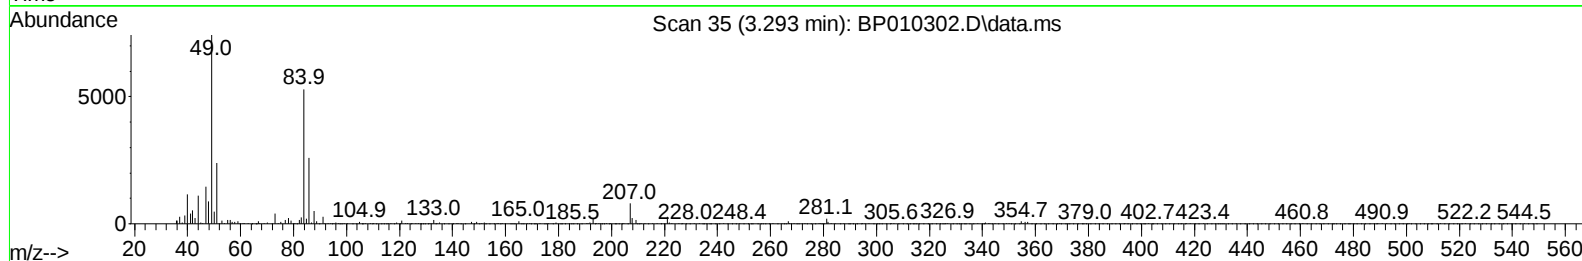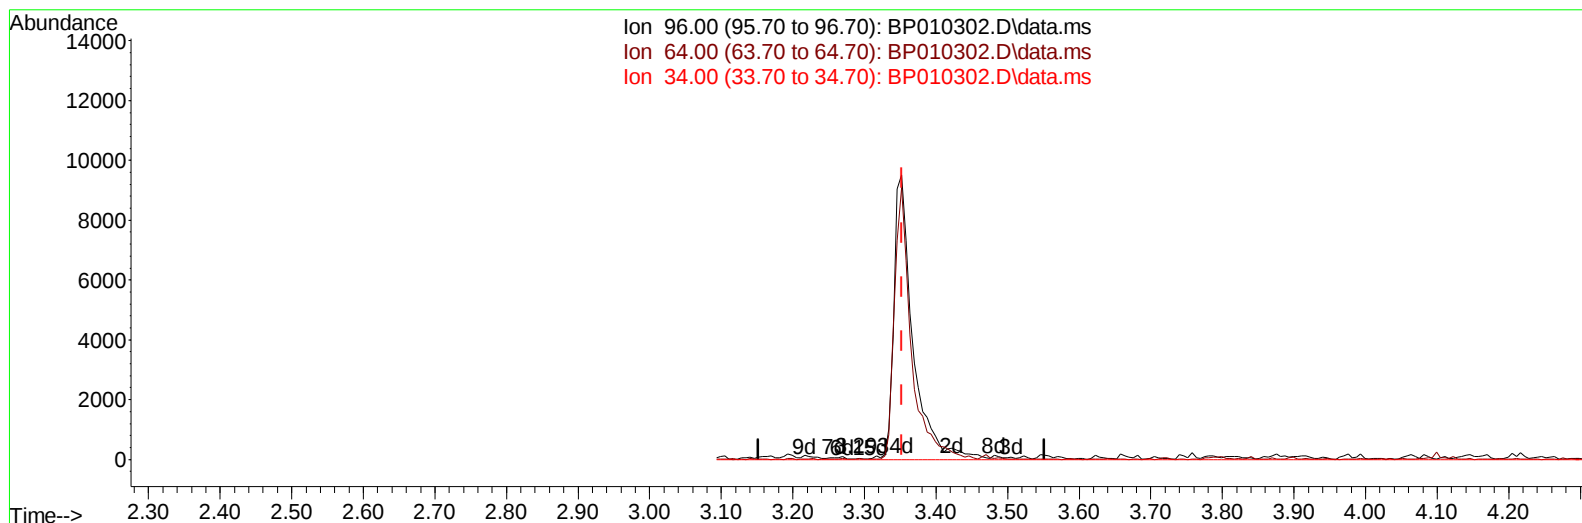

TIC: BP010302.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.059) 0.01 ng/uL

response 22

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	62.50
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

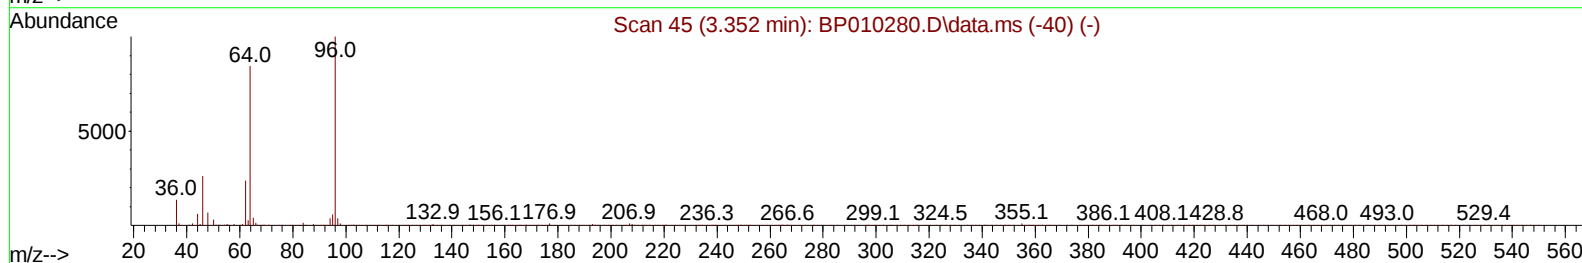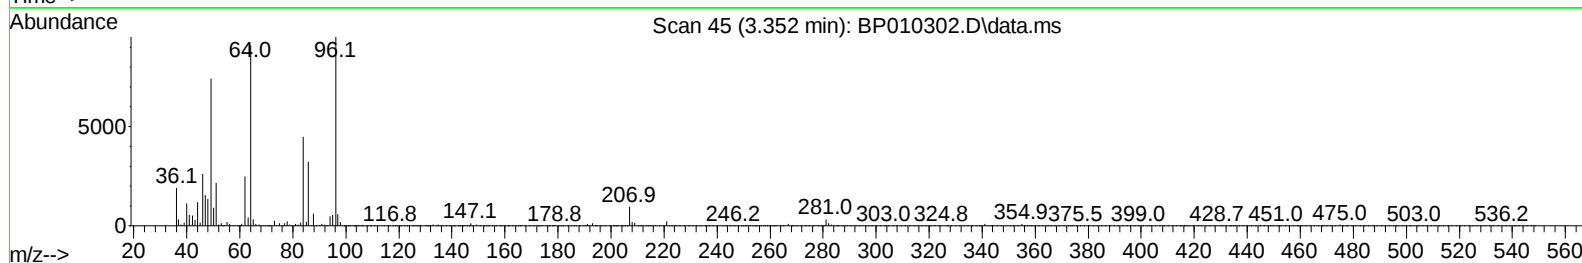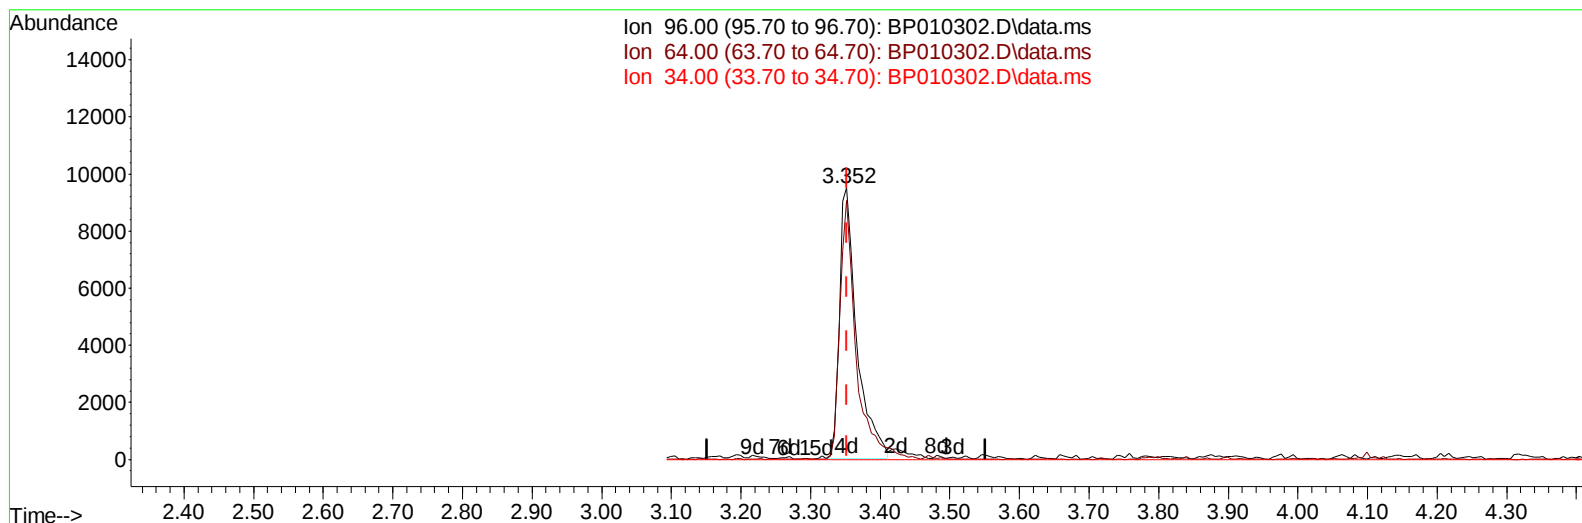

TIC: BP010302.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 4.64 ng/uL m

response 16525

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	95.46#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

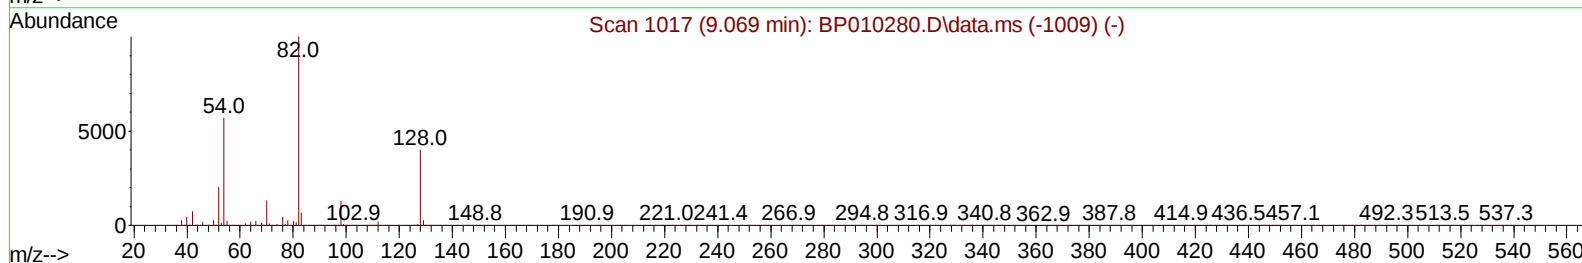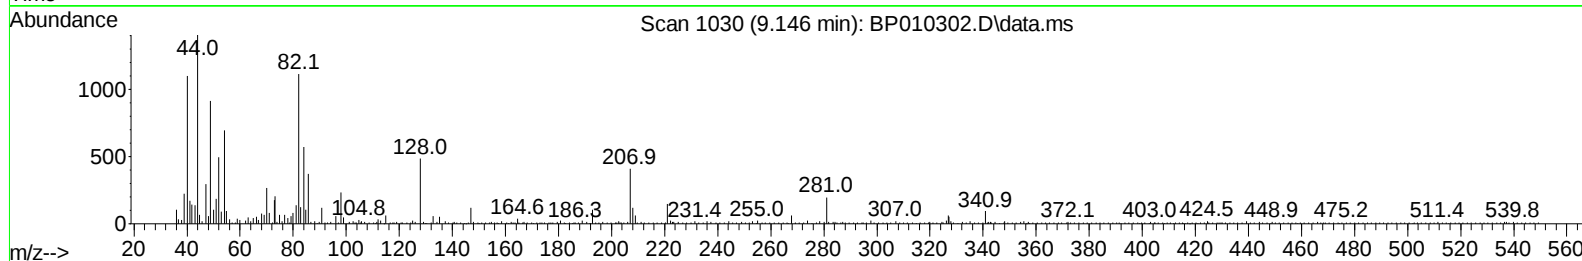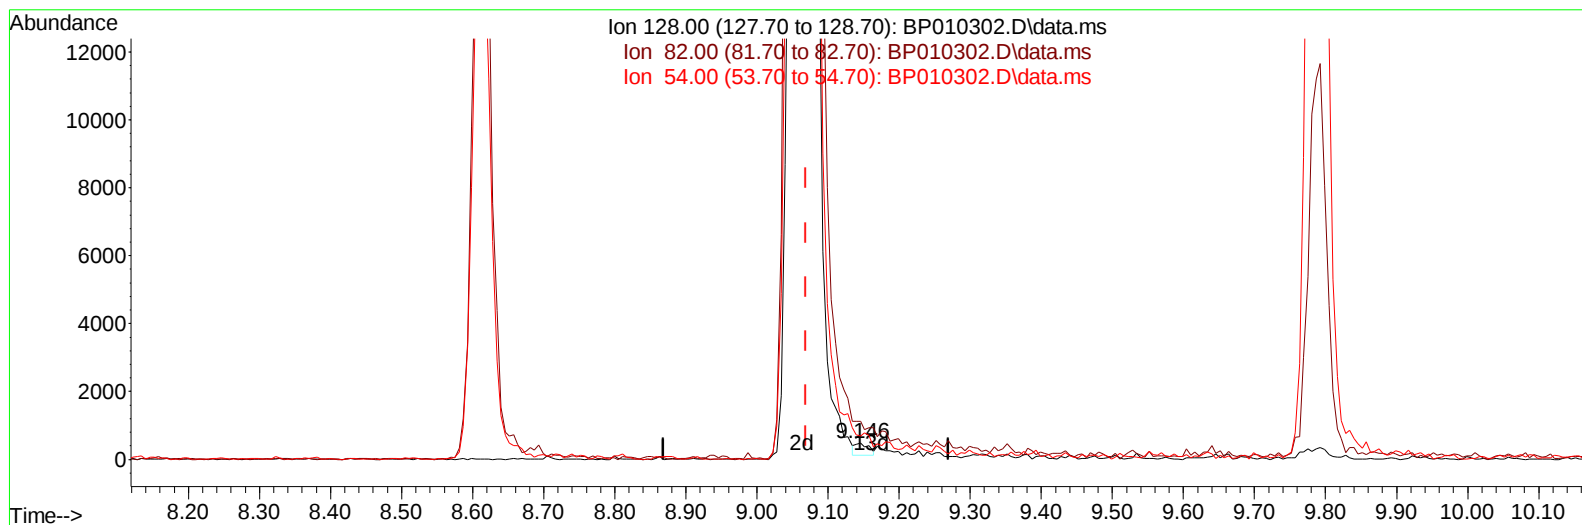

TIC: BP010302.D\data.ms

(21) Nitrobenzene-d5 (S)

9.146min (+ 0.077) 0.08 ng/u1

response 461

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	230.37
54.00	120.20	143.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010302.D
Acq On : 12 May 2022 01:02
Operator : CG/JU
Sample : N2707-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

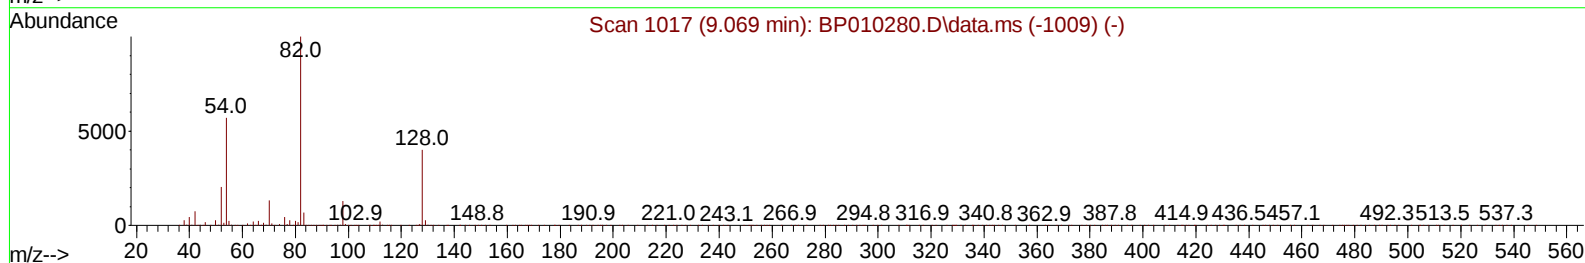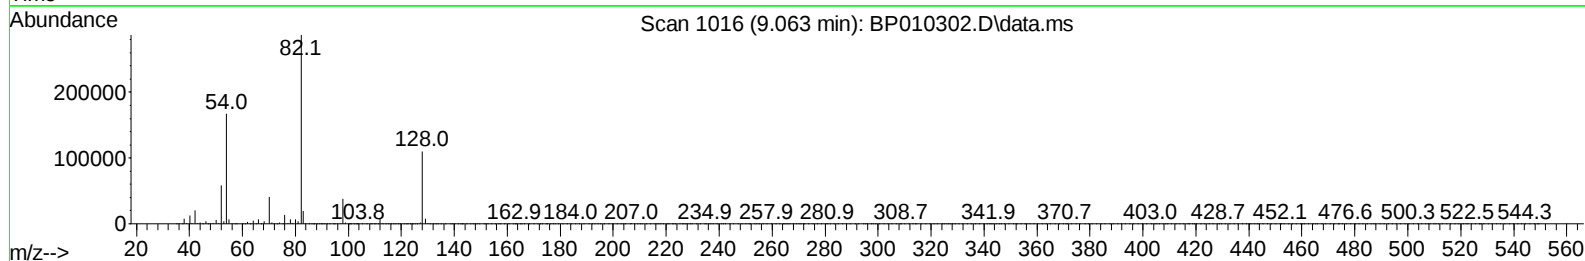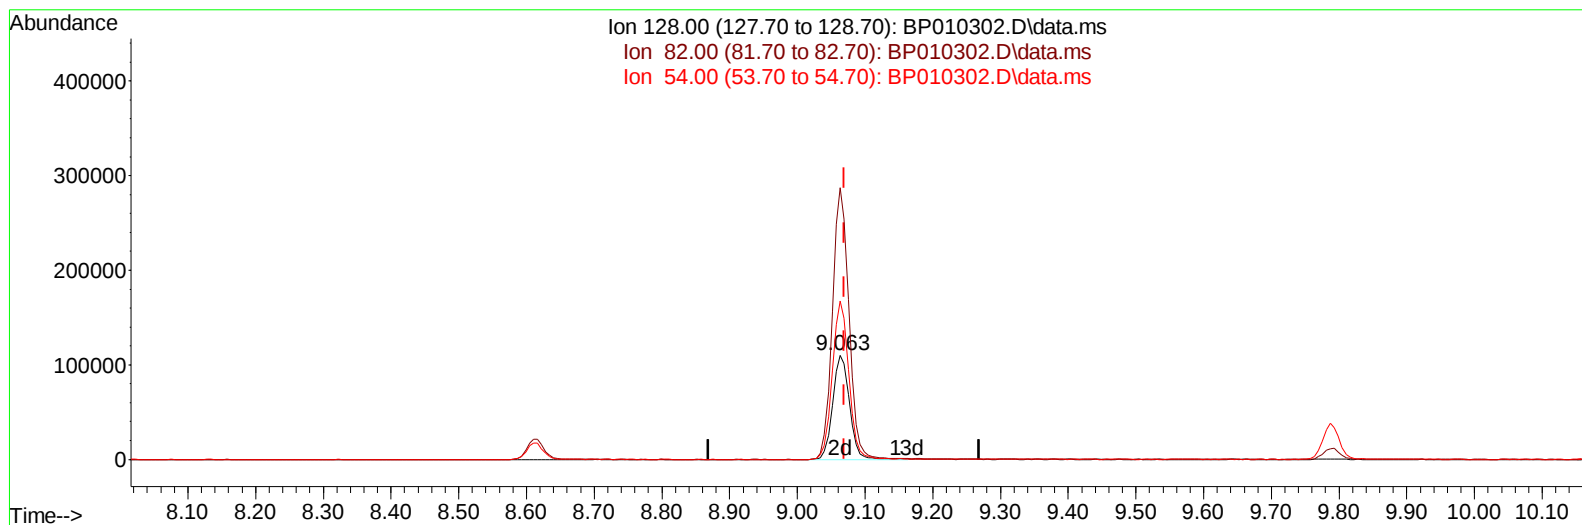

TIC: BP010302.D\data.ms

(21) Nitrobenzene-d5 (S)

9.063min (-0.006) 34.59 ng/u1 m

response 189059

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	287.30	260.53
54.00	120.20	152.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

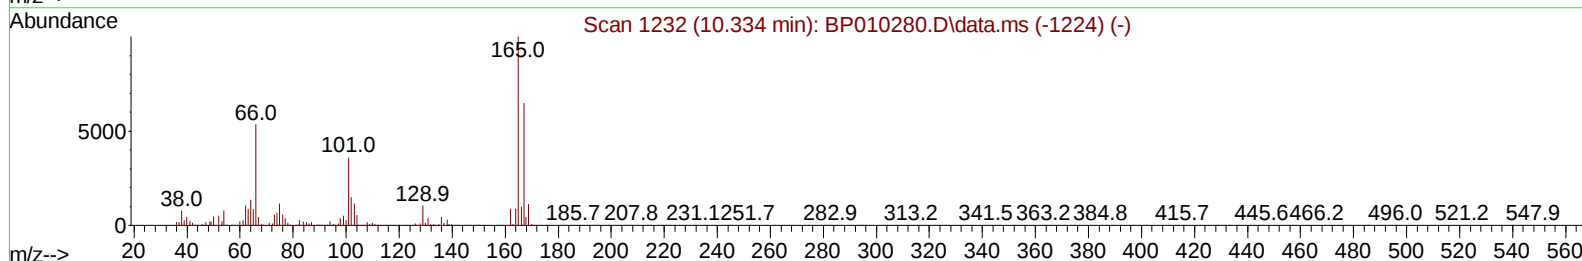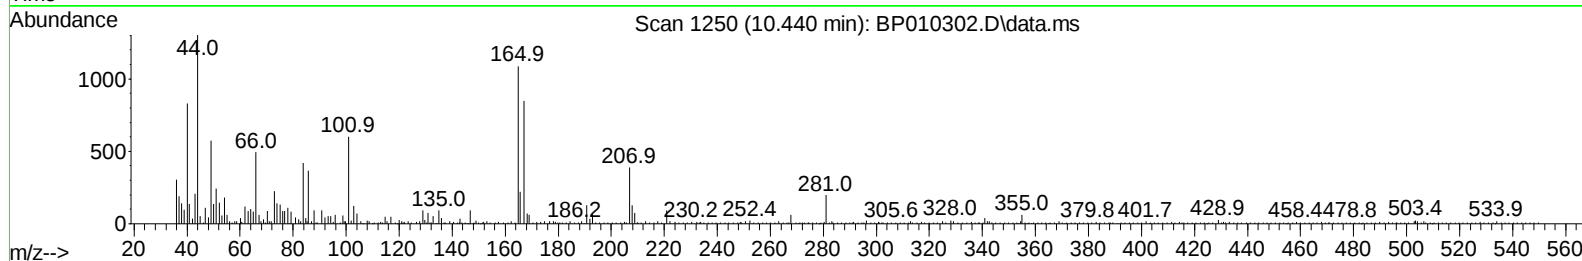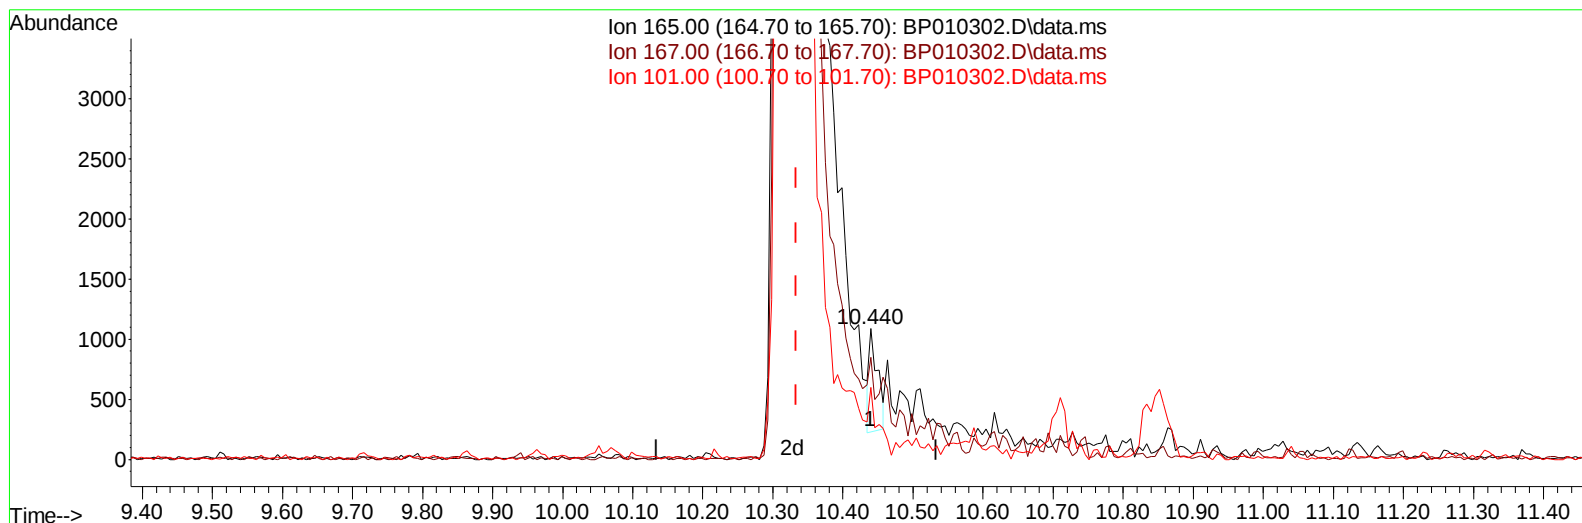

TIC: BP010302.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.440min (+ 0.106) 0.07 ng/u1

response 738

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	64.86
101.00	49.80	45.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

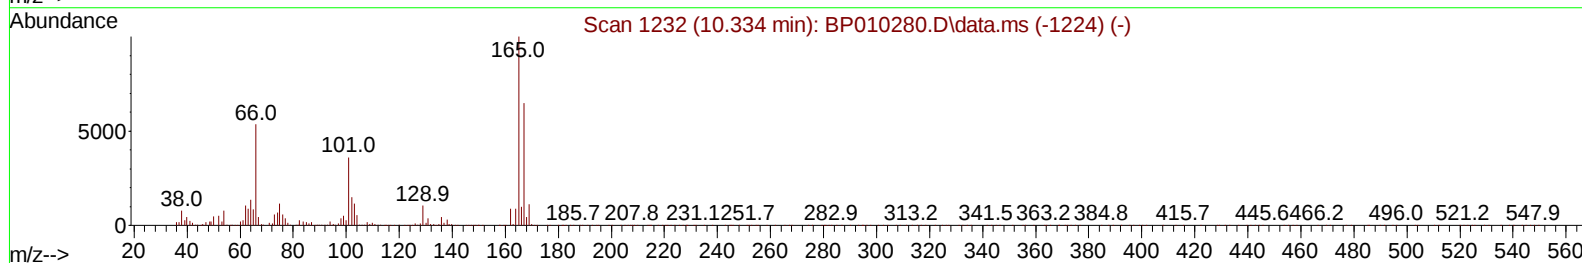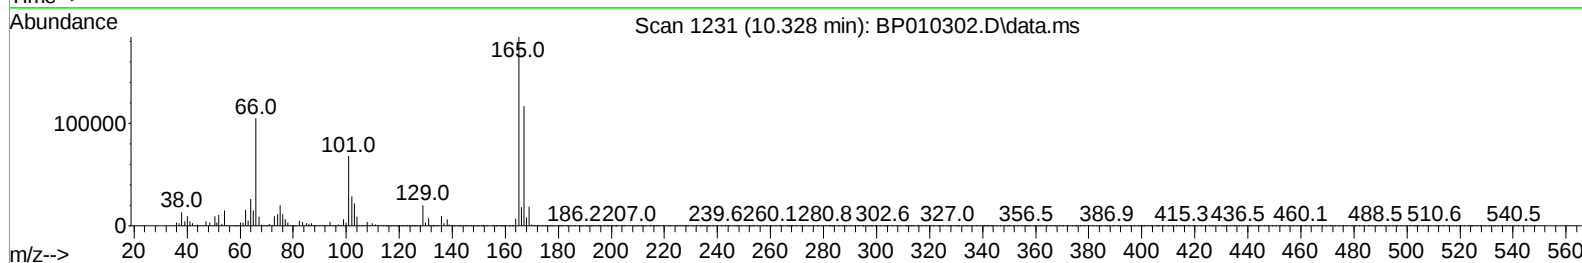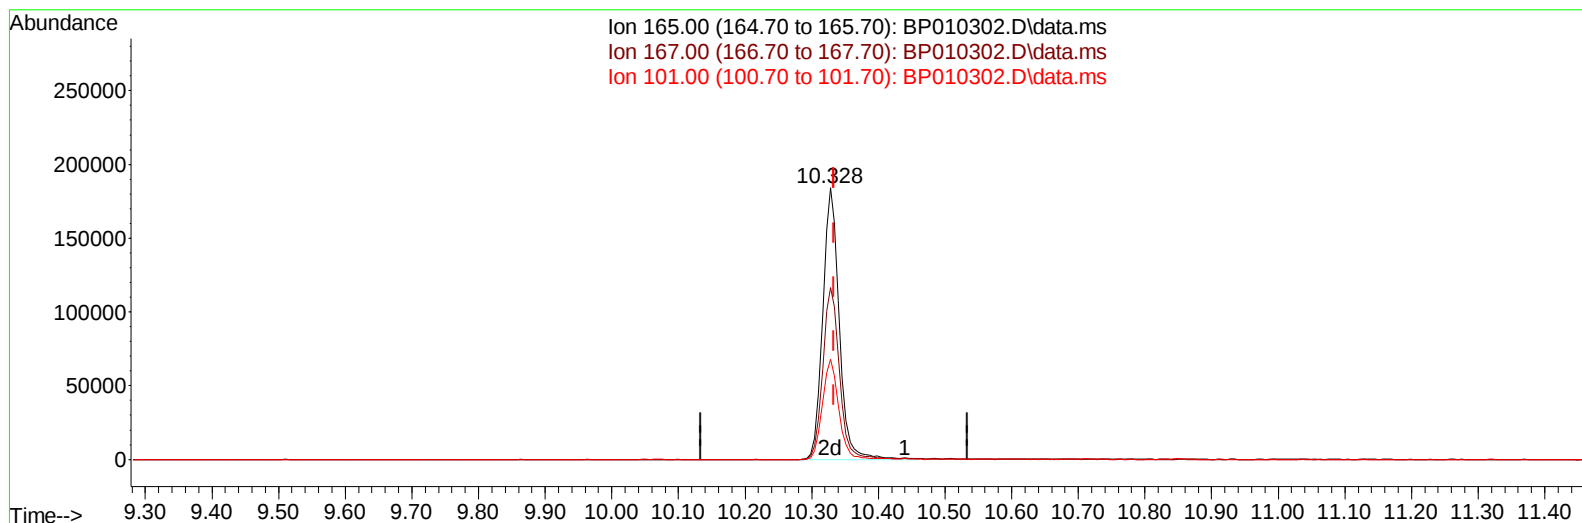

TIC: BP010302.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.328min (-0.006) 28.01 ng/ul m

response 317721

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	63.41
101.00	49.80	36.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

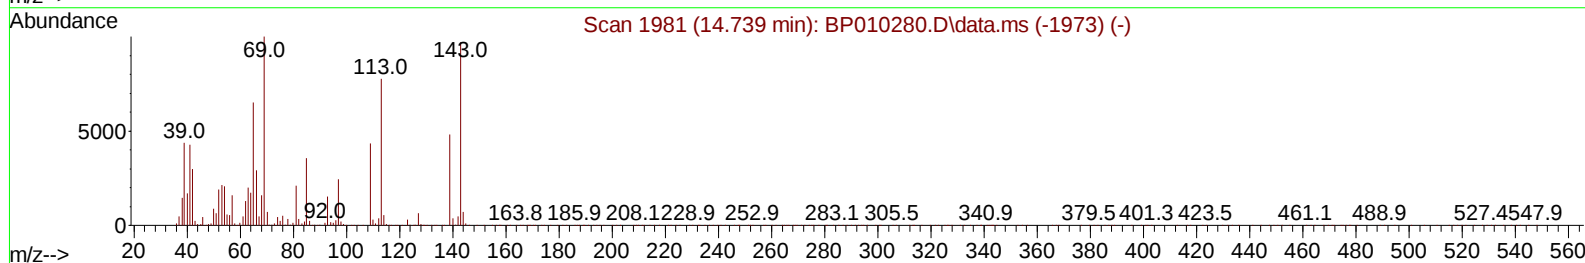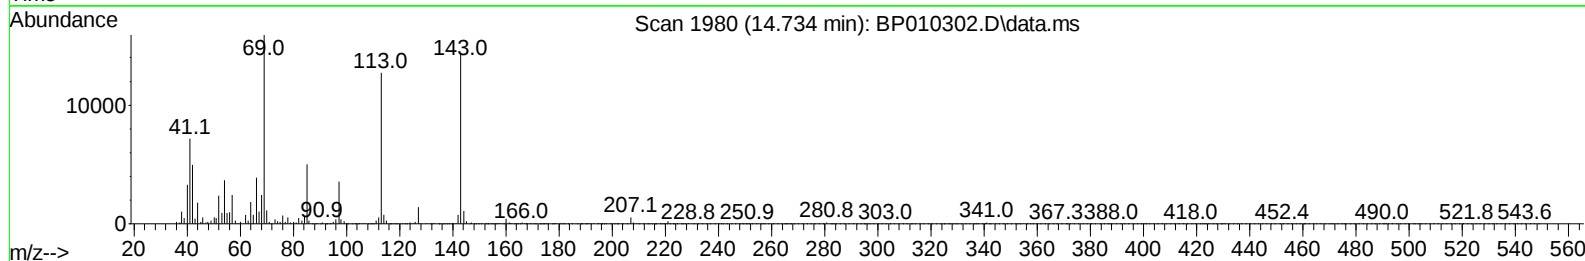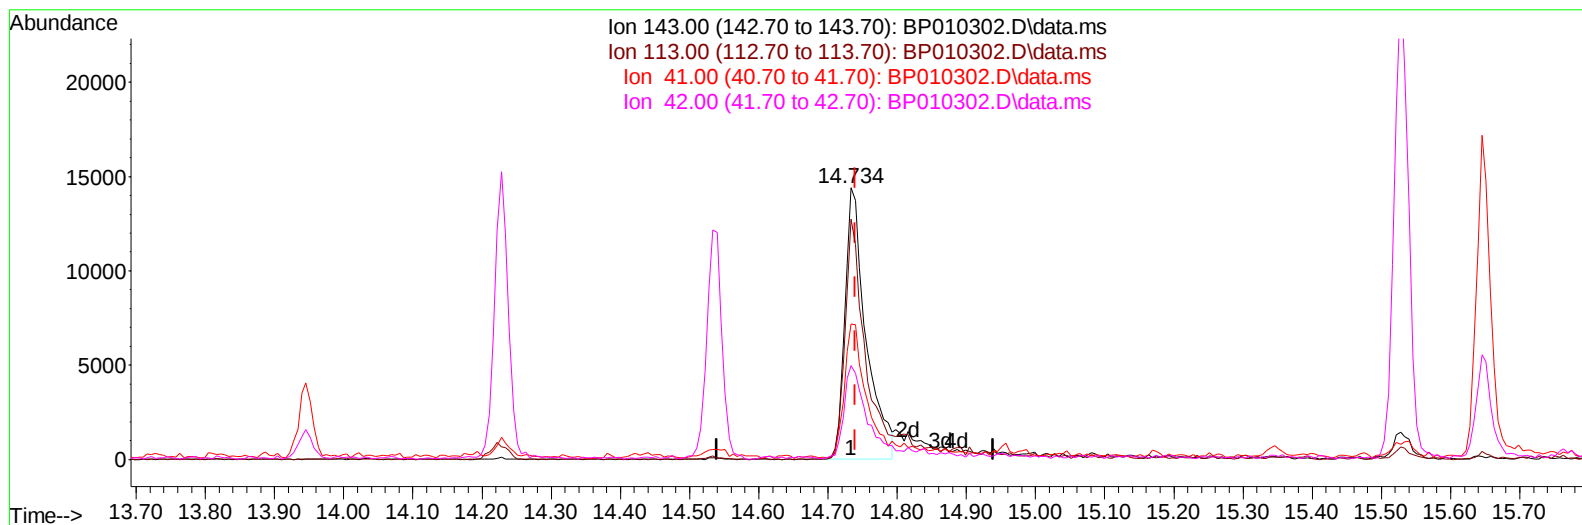

TIC: BP010302.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 4.10 ng/u1

response 30426

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	88.47#
41.00	23.20	49.78#
42.00	18.00	34.54#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

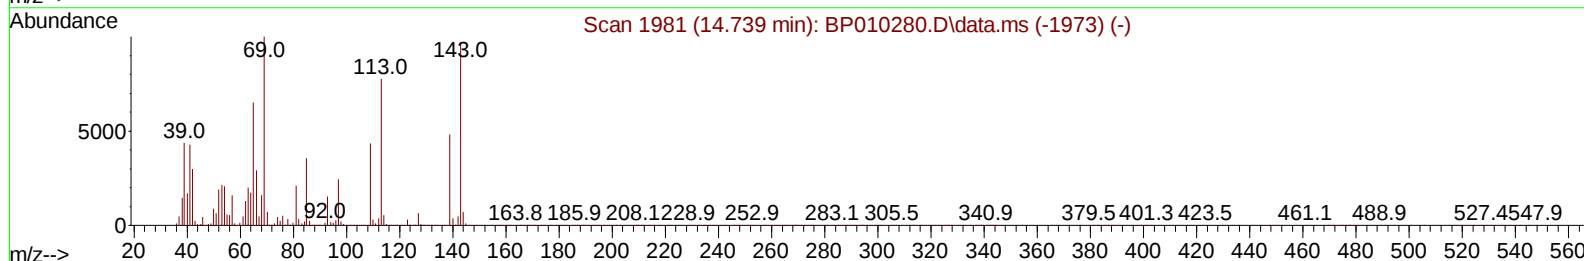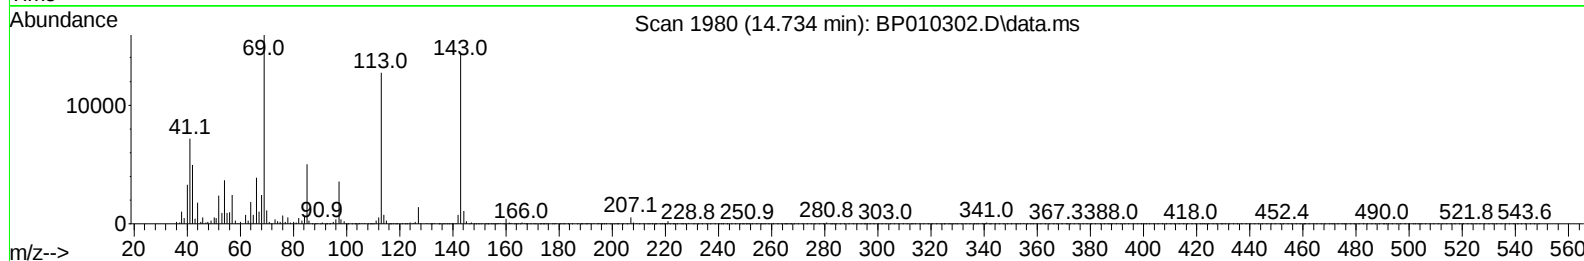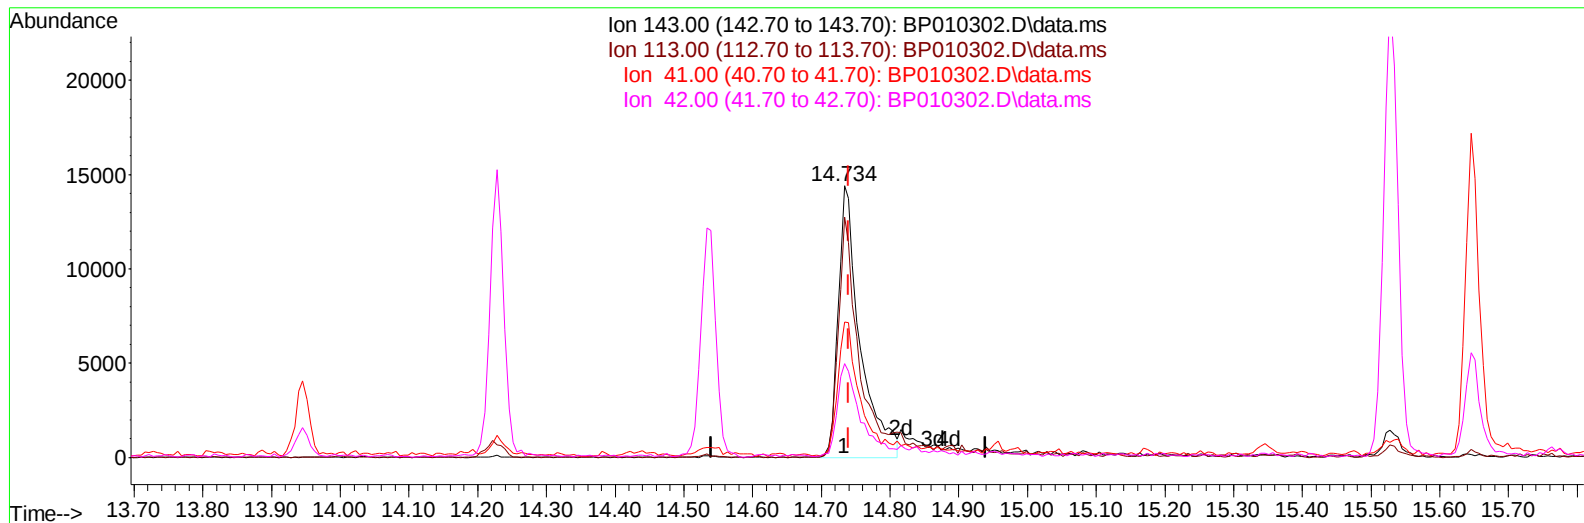

TIC: BP010302.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 4.29 ng/ul m

response 31847

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	88.47#
41.00	23.20	49.78#
42.00	18.00	34.54#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Manual IntegrationsAPPROVED

Quant Time: May 12 02:59:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	151138	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	681609	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	485919	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1066586	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	1053254	20.000	ng/ul	# 0.00
88) Perylene-d12	23.798	264	1008313	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	16525m	4.645	ng/uL	0.00
4) Pyridine-d5	3.781	84	52610	5.314	ng/ul	0.01
7) Phenol-d5	7.069	99	81193	5.784	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	305798	35.214	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	262647	25.405	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	176046	15.254	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	189059m	34.593	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	197711	31.729	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	317721m	28.014	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	414960	24.783	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1367343	35.321	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1500520	32.511	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	31847m	4.289	ng/ul	0.00
60) Fluorene-d10	15.528	176	1182947	36.201	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	233655	31.990	ng/ul	0.00
73) Anthracene-d10	17.386	188	1998433	38.261	ng/ul	0.00
81) Pyrene-d10	19.622	212	2451970	42.127	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	2246936	41.785	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010302.D
Acq On : 12 May 2022 01:02
Operator : CG/JU
Sample : N2707-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 02:59:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

