




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010306.D
Acq On : 12 May 2022 03:16
Operator : CG/JU
Sample : N2707-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL86

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 05:33:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

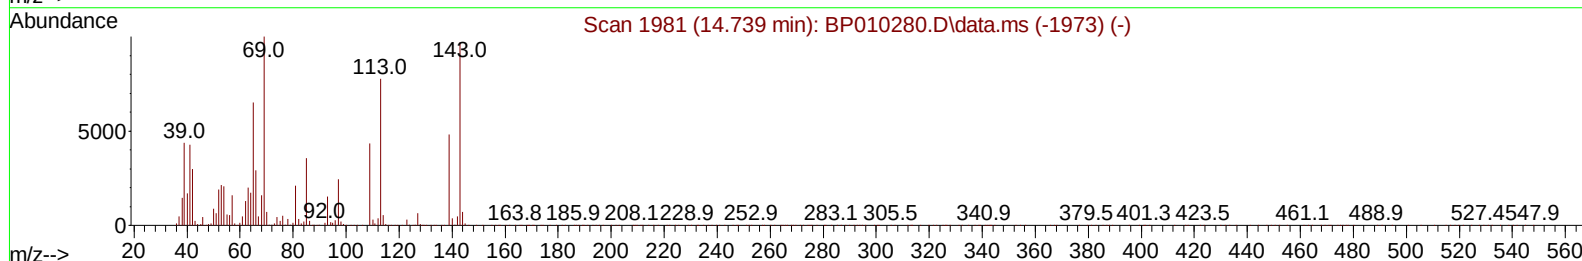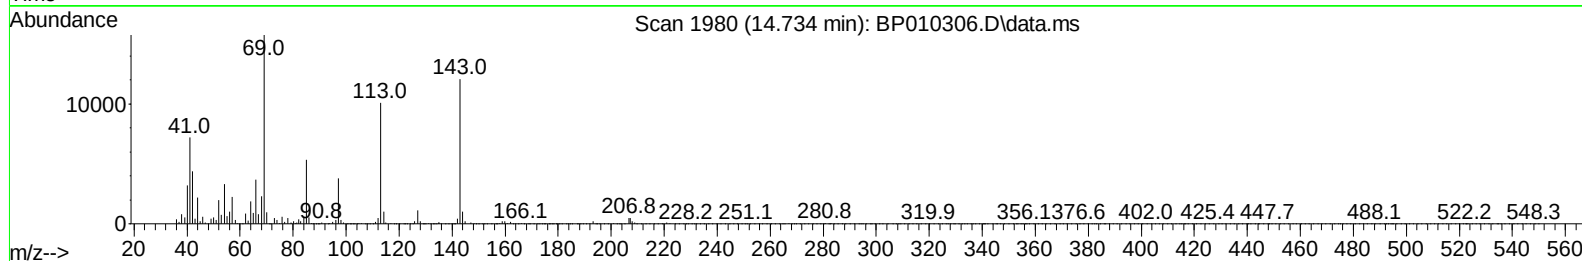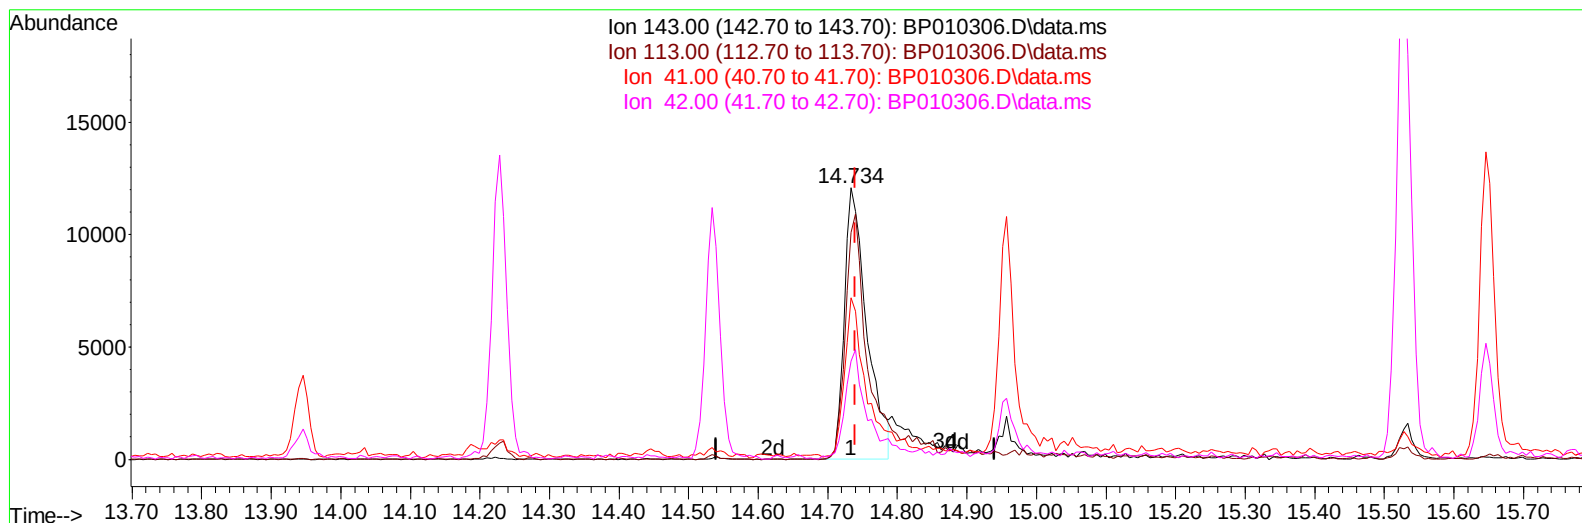

TIC: BP010306.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 4.11 ng/u1

response 26907

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.68#
41.00	23.20	59.61#
42.00	18.00	36.31#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010306.D
Acq On : 12 May 2022 03:16
Operator : CG/JU
Sample : N2707-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL86

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 05:33:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

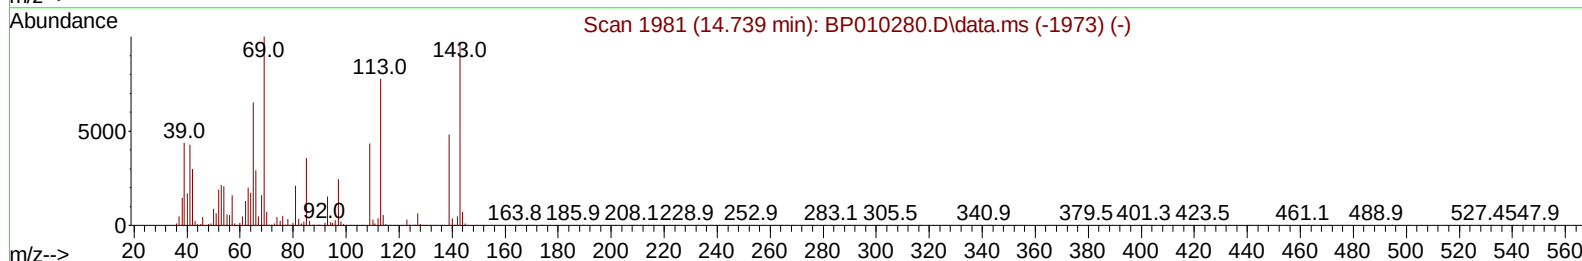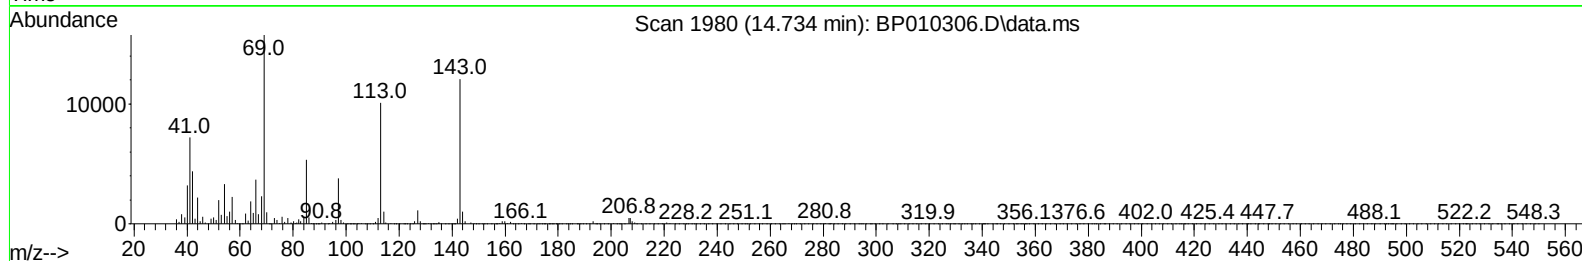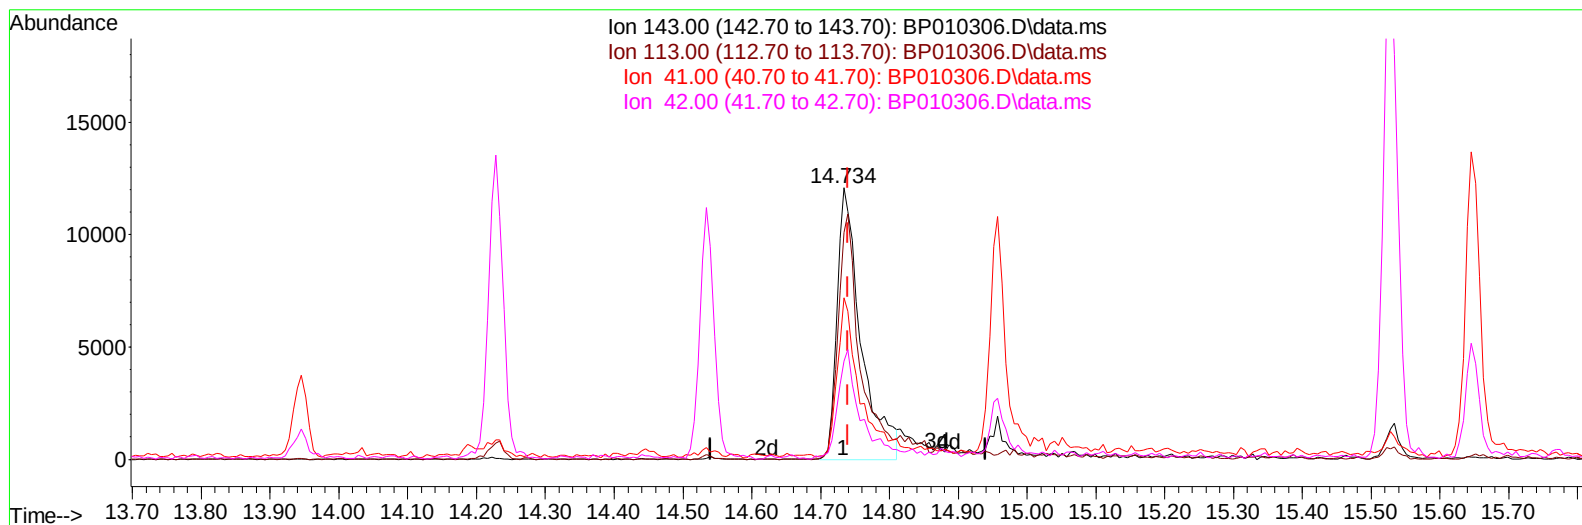

TIC: BP010306.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.734min (-0.006) 4.45 ng/ul m

response 29177

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	83.68#
41.00	23.20	59.61#
42.00	18.00	36.31#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010306.D
 Acq On : 12 May 2022 03:16
 Operator : CG/JU
 Sample : N2707-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL86

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 05:33:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	137406	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	599183	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.534	164	428866	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	948028	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	951702	20.000	ng/ul	# 0.00
88) Perylene-d12	23.798	264	934817	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	14502	4.484	ng/uL	0.00
4) Pyridine-d5	3.776	84	51335	5.703	ng/ul	0.00
7) Phenol-d5	7.069	99	73974	5.796	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	265111	33.580	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	228835	24.347	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	154328	14.709	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	163174	33.964	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	170061	31.046	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	286179	28.704	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	307388	20.884	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	1240598	36.311	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1342918	32.967	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	29177m	4.452	ng/ul	0.00
60) Fluorene-d10	15.528	176	1076391	37.322	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	195614	30.131	ng/ul	0.00
73) Anthracene-d10	17.387	188	1853366	39.922	ng/ul	0.00
81) Pyrene-d10	19.616	212	2262774	43.025	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.645	264	2109027	42.304	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010306.D
Acq On : 12 May 2022 03:16
Operator : CG/JU
Sample : N2707-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL86

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 05:33:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

