




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010310.D
 Acq On : 12 May 2022 06:05
 Operator : CG/JU
 Sample : PB144607BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK607

Manual IntegrationsAPPROVED

Quant Time: May 12 07:39:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

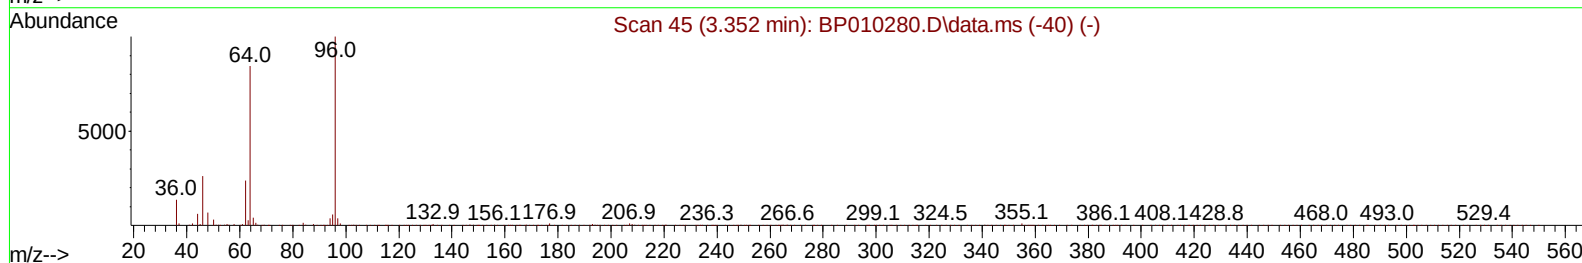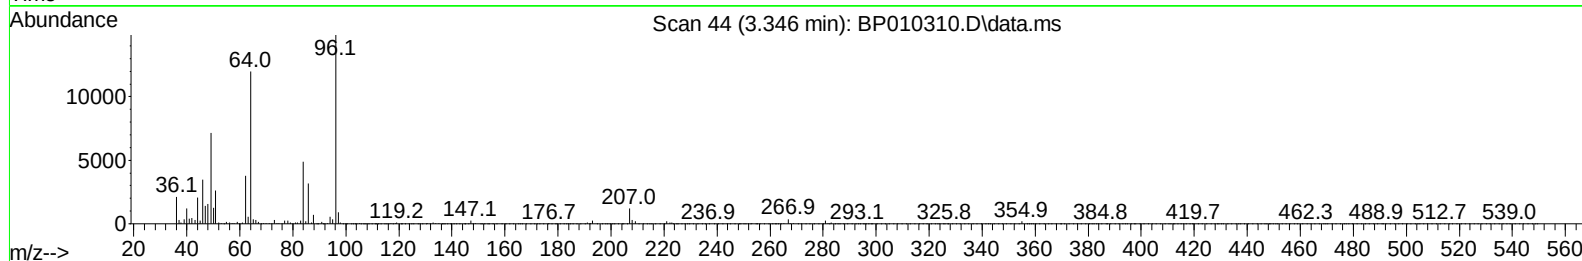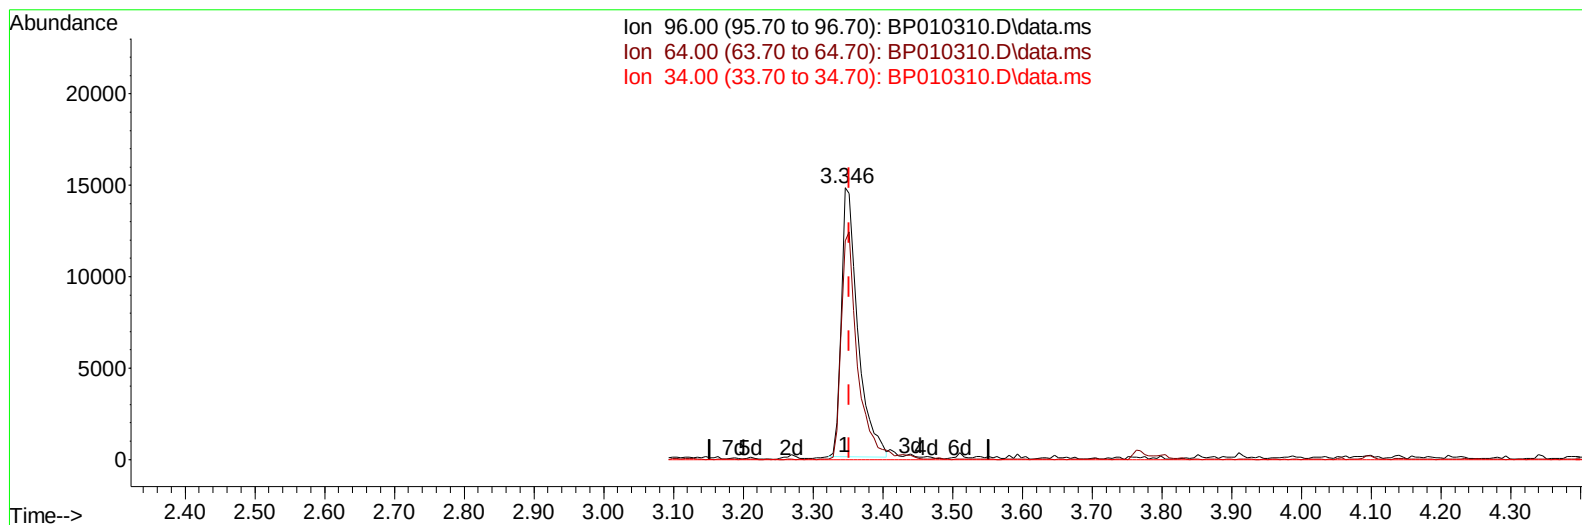

TIC: BP010310.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.006) 6.25 ng/uL

response 24106

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	80.57#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010310.D
Acq On : 12 May 2022 06:05
Operator : CG/JU
Sample : PB144607BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK607

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 07:39:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

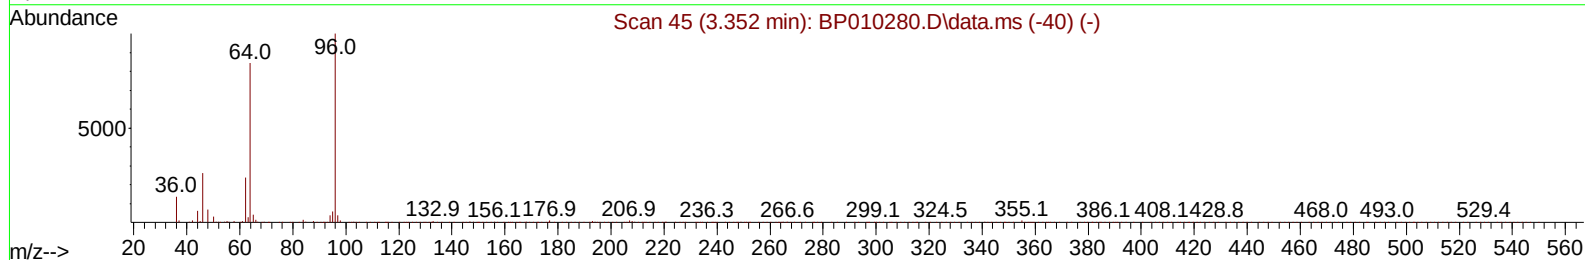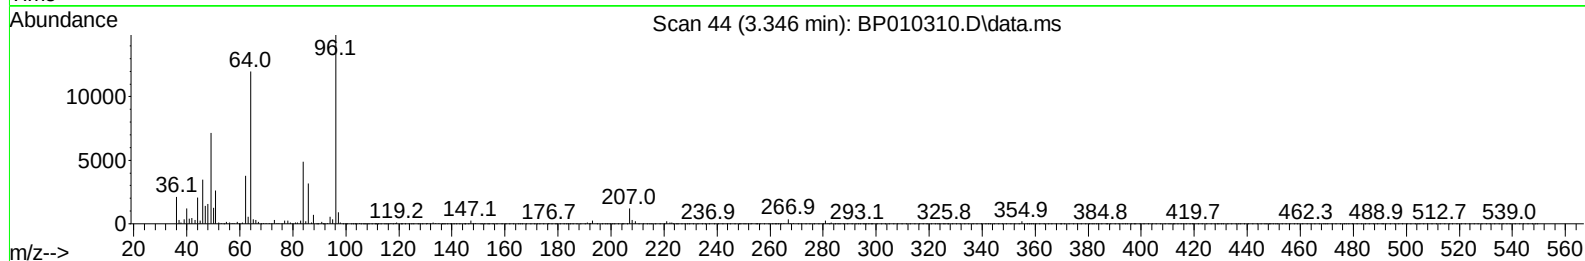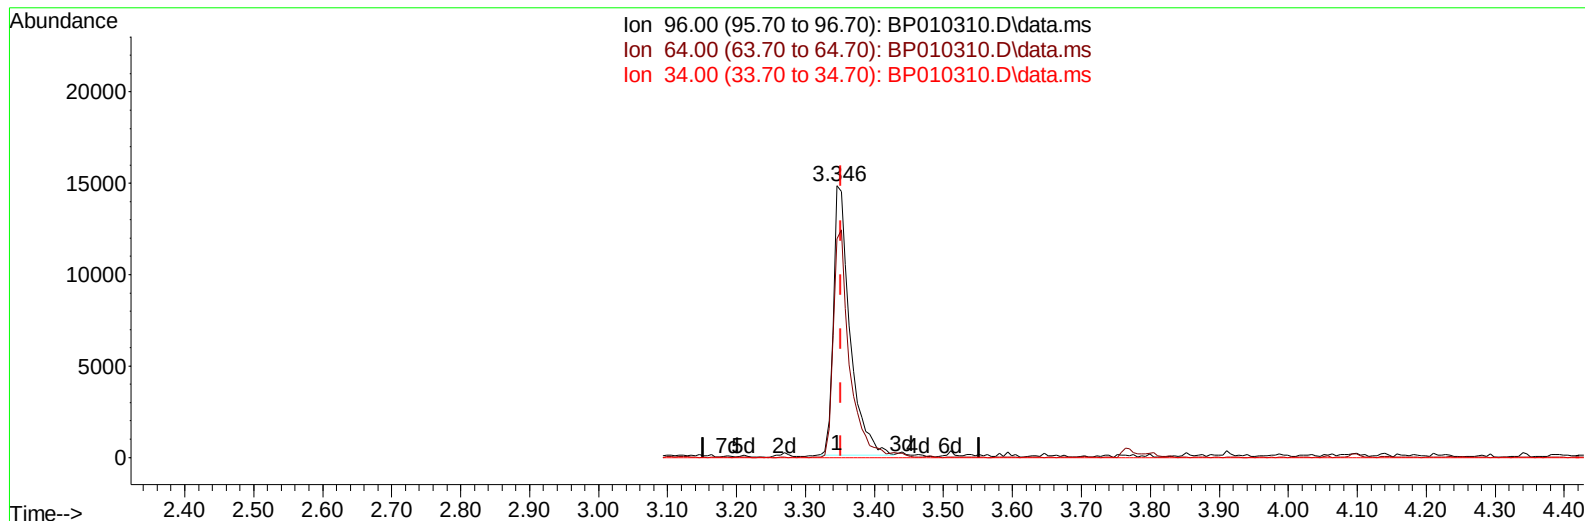

TIC: BP010310.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.006) 6.37 ng/uL m

response 24546

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	80.57#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010310.D
 Acq On : 12 May 2022 06:05
 Operator : CG/JU
 Sample : PB144607BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK607

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 07:39:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	163744	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	749233	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	529190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1144419	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	1108706	20.000	ng/ul	# 0.00
88) Perylene-d12	23.798	264	984725	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	24546m	6.368	ng/uL	0.00
4) Pyridine-d5	3.764	84	340939	31.786	ng/ul	0.00
7) Phenol-d5	7.069	99	426240	28.027	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	304858	32.403	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	348033	31.073	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	367406	29.385	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	184902	30.779	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	204781	29.897	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	344617	27.643	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	518444	28.169	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1328879	31.521	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1452210	28.892	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	194524	24.055	ng/ul	-0.01
60) Fluorene-d10	15.528	176	1111929	31.245	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	200204	25.546	ng/ul	0.00
73) Anthracene-d10	17.386	188	1770334	31.589	ng/ul	0.00
81) Pyrene-d10	19.616	212	2143456	34.985	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1779242	33.880	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010310.D
Acq On : 12 May 2022 06:05
Operator : CG/JU
Sample : PB144607BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK607

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 07:39:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

