




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010320.D
 Acq On : 12 May 2022 12:23
 Operator : CG/JU
 Sample : N2714-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Quant Time: May 13 00:00:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

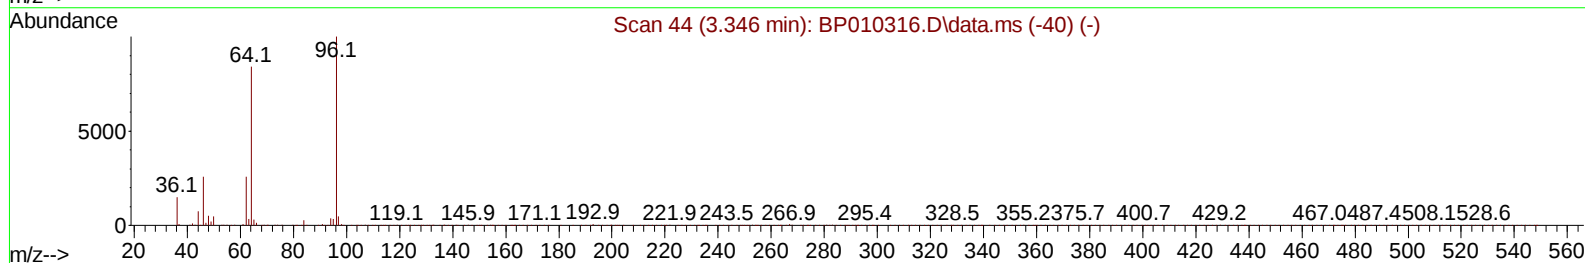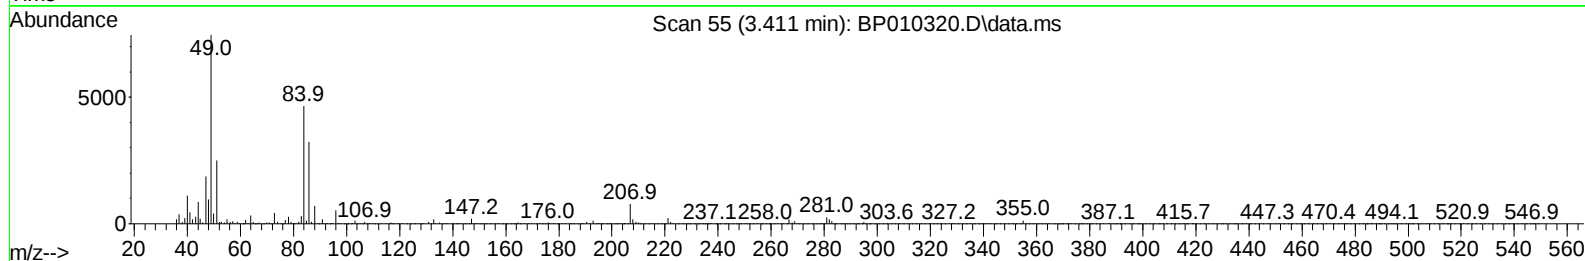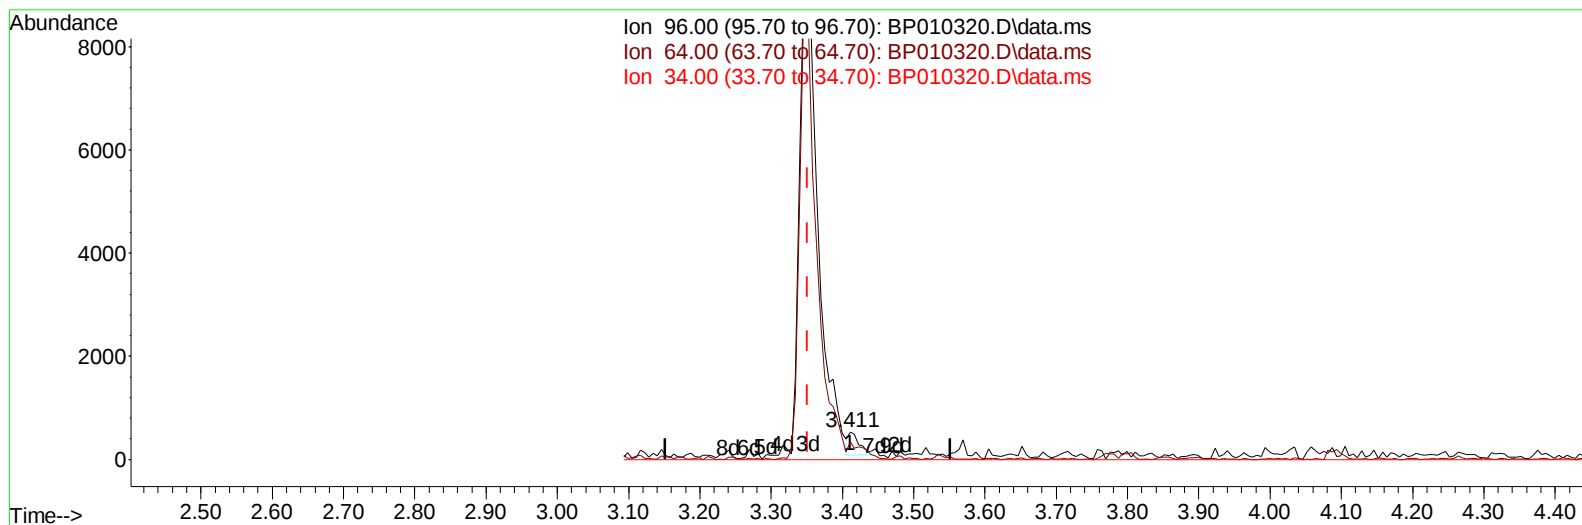

TIC: BP010320.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.411min (+ 0.059) 0.14 ng/uL

response 481

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	64.22
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010320.D
 Acq On : 12 May 2022 12:23
 Operator : CG/JU
 Sample : N2714-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Quant Time: May 13 00:00:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

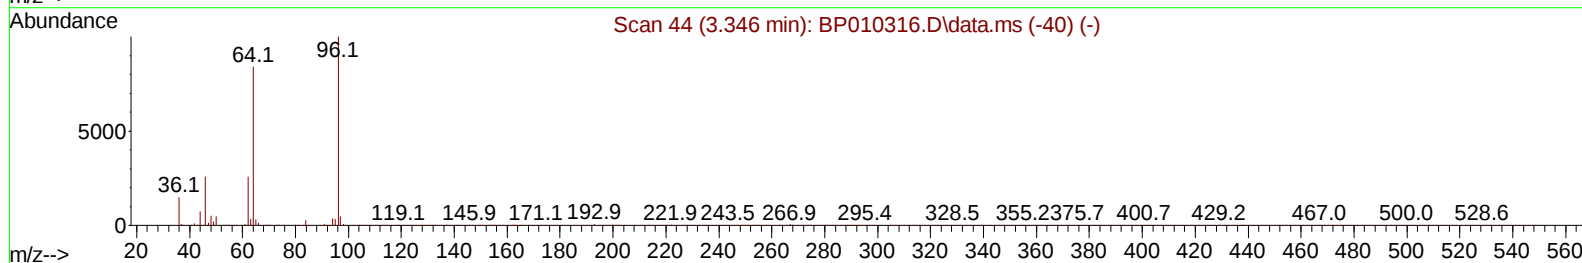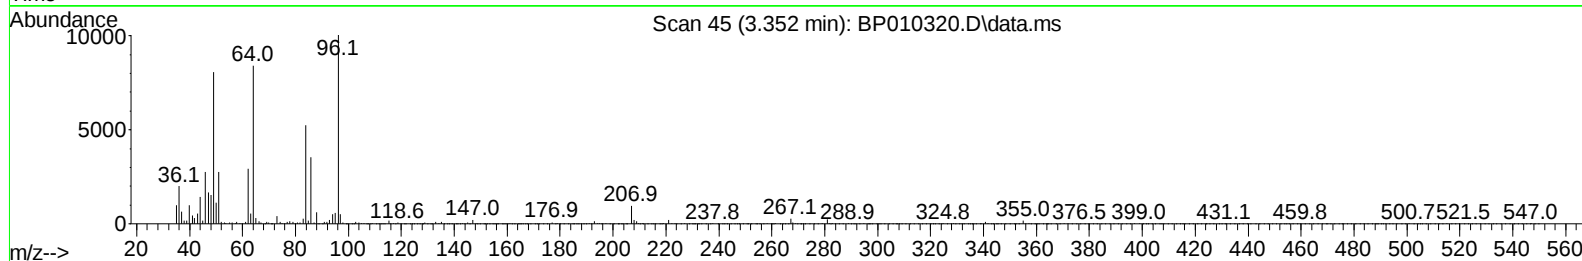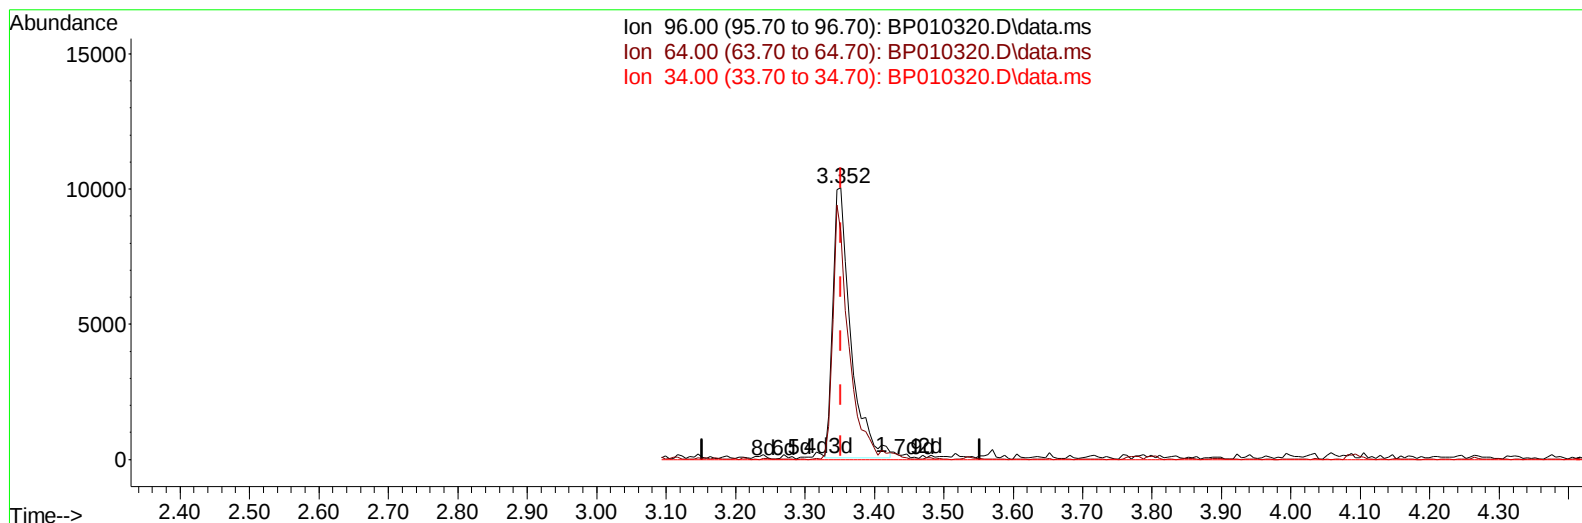

TIC: BP010320.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (+ 0.000) 5.06 ng/uL m

response 17919

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	83.73#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010320.D
 Acq On : 12 May 2022 12:23
 Operator : CG/JU
 Sample : N2714-02
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 00:00:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	150586	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	653101	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	455958	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	993323	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	978538	20.000	ng/ul	# 0.00
88) Perylene-d12	23.798	264	943251	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	17919m	5.055	ng/uL	0.00
4) Pyridine-d5	3.770	84	111632	11.317	ng/ul	0.00
7) Phenol-d5	7.069	99	331432	23.697	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	237084	27.401	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	269295	26.144	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	290239	25.241	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	141252	26.974	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	153125	25.646	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	267969	24.658	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	362761	22.611	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	995812	27.414	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1097437	25.340	ng/ul	0.00
54) 4-Nitrophenol-d4	14.728	143	127819	18.345	ng/ul	-0.01
60) Fluorene-d10	15.528	176	858412	27.996	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	132351	19.457	ng/ul	-0.01
73) Anthracene-d10	17.387	188	1360423	27.967	ng/ul	0.00
81) Pyrene-d10	19.616	212	1708804	31.601	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1554092	30.894	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010320.D
Acq On : 12 May 2022 12:23
Operator : CG/JU
Sample : N2714-02
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW2X5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 00:00:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

