




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010325.D
 Acq On : 12 May 2022 15:45
 Operator : CG/JU
 Sample : N2714-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X8

Manual IntegrationsAPPROVED

Quant Time: May 13 00:01:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

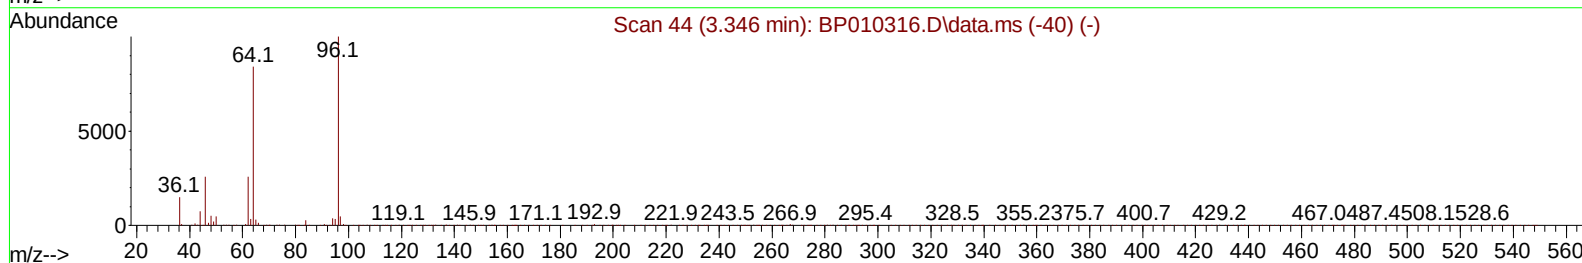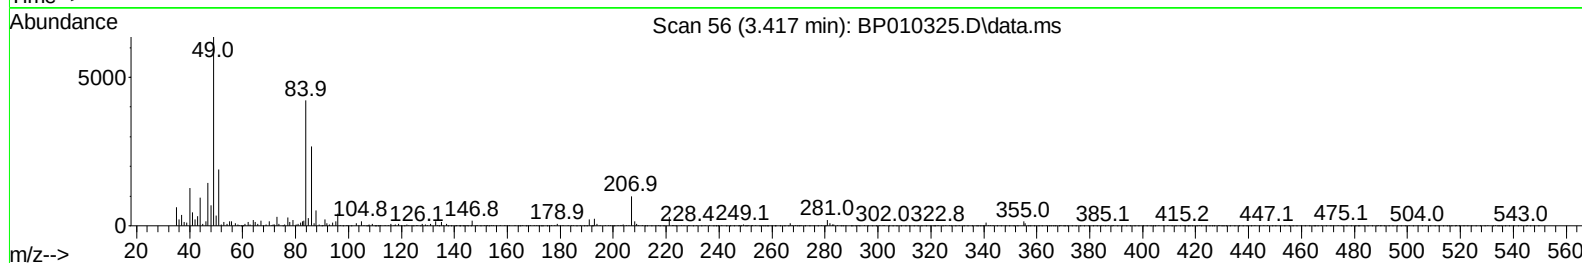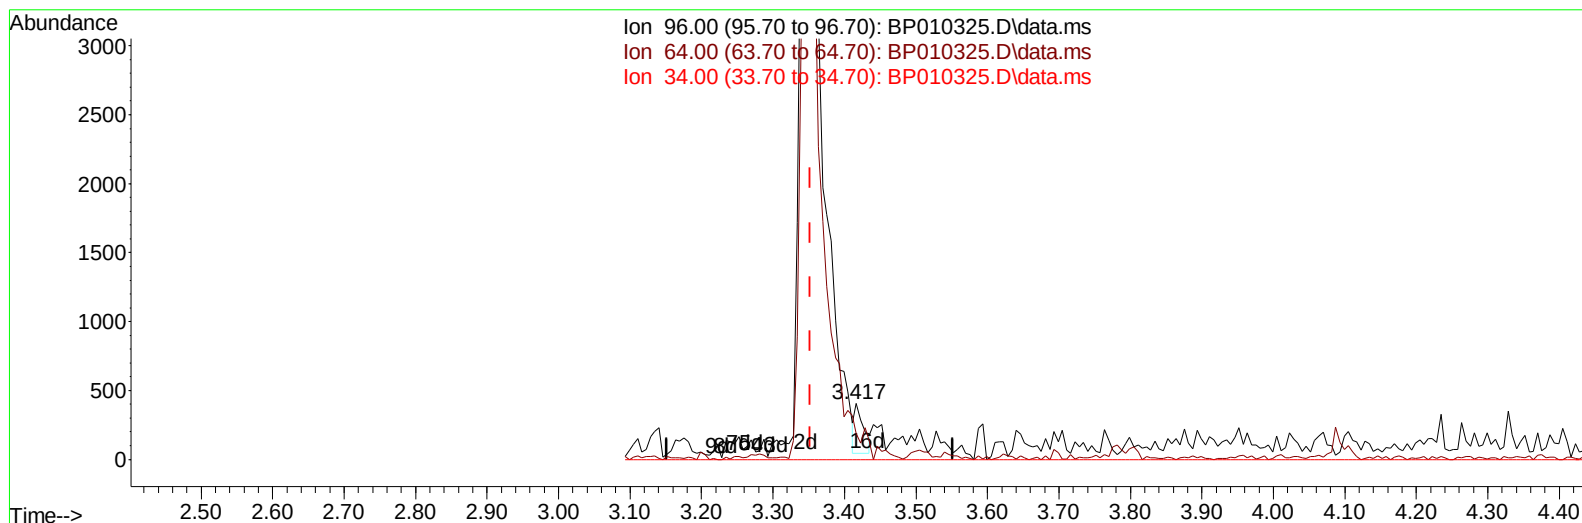

TIC: BP010325.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.417min (+ 0.065) 0.10 ng/uL

response 311

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	46.55
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010325.D
 Acq On : 12 May 2022 15:45
 Operator : CG/JU
 Sample : N2714-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X8

Manual IntegrationsAPPROVED

Quant Time: May 13 00:01:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

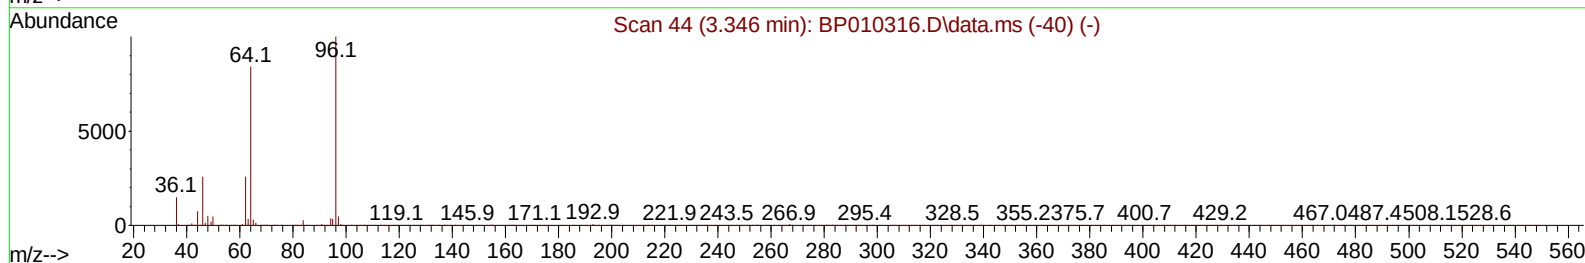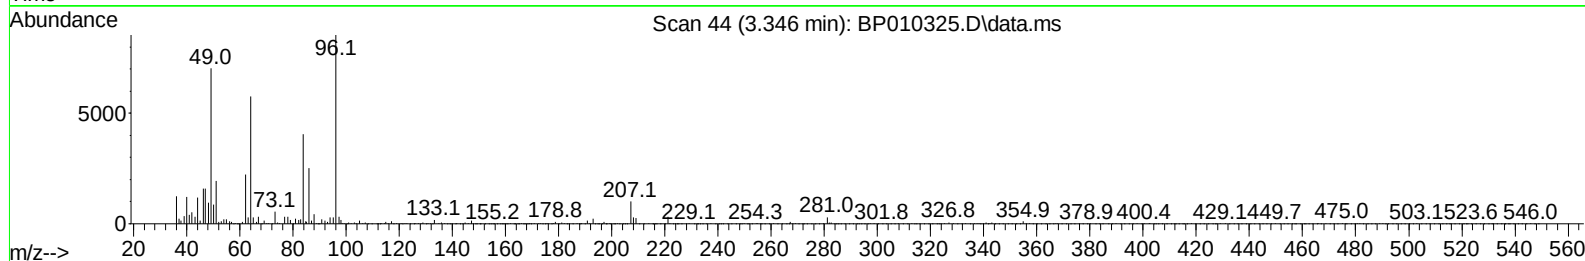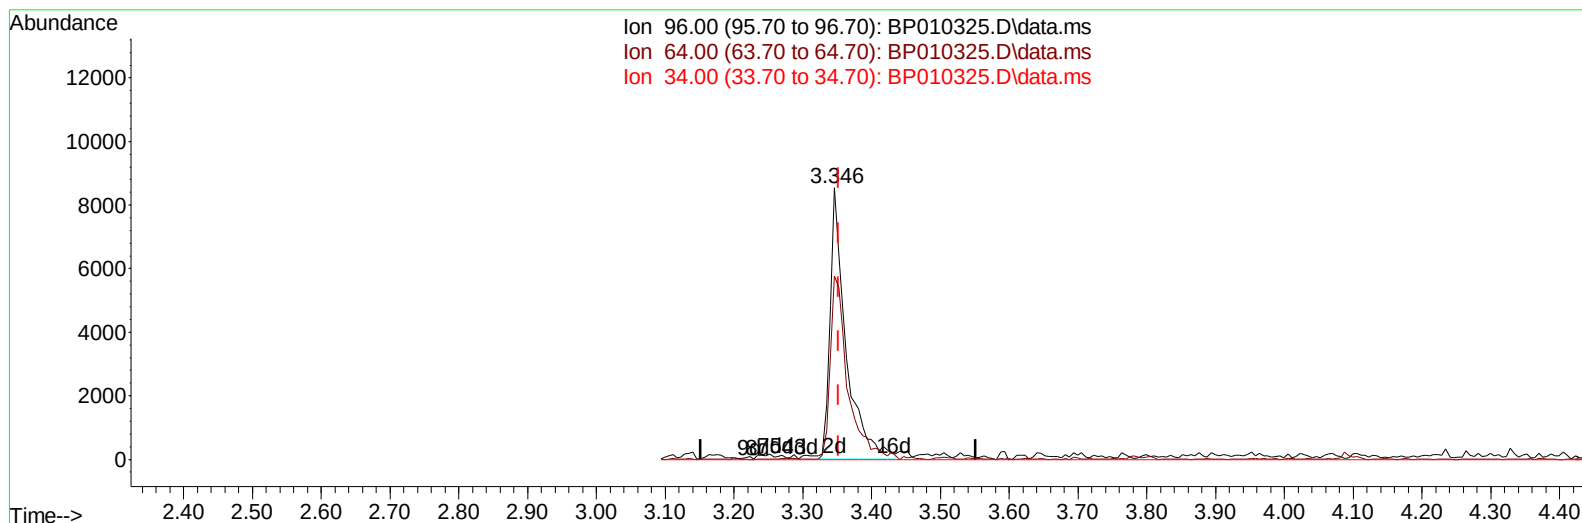

TIC: BP010325.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.346min (-0.006) 4.26 ng/uL m

response 13551

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	67.50#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010325.D
 Acq On : 12 May 2022 15:45
 Operator : CG/JU
 Sample : N2714-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW2X8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 00:01:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.905	152	135013	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	604565	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.534	164	428061	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	938917	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.369	240	938134	20.000	ng/ul	0.00
88) Perylene-d12	23.792	264	971267	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	13551m	4.264	ng/uL	0.00
4) Pyridine-d5	3.775	84	51603	5.835	ng/ul	0.00
7) Phenol-d5	7.069	99	249427	19.891	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	173978	22.427	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	201053	21.770	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	218807	21.224	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	105239	21.710	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	114731	20.758	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	201353	20.016	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	274287	18.469	ng/ul	0.00
46) Dimethylphthalate-d6	13.946	166	781721	22.923	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	848990	20.881	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	100633	15.384	ng/ul	0.00
60) Fluorene-d10	15.528	176	664291	23.077	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	98835	15.372	ng/ul	-0.01
73) Anthracene-d10	17.387	188	1112380	24.193	ng/ul	0.00
81) Pyrene-d10	19.616	212	1429654	27.577	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	1373513	26.517	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010325.D
Acq On : 12 May 2022 15:45
Operator : CG/JU
Sample : N2714-07
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW2X8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 00:01:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

