




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010339.D
 Acq On : 13 May 2022 00:12
 Operator : CG/JU
 Sample : N2801-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

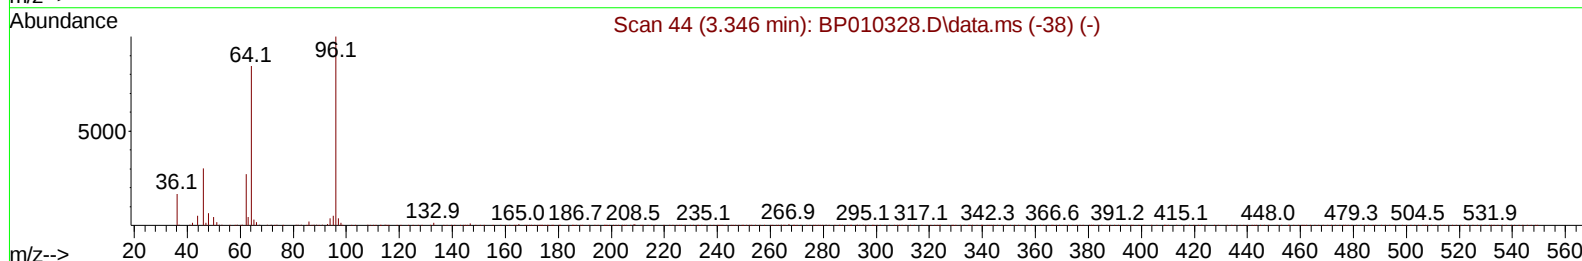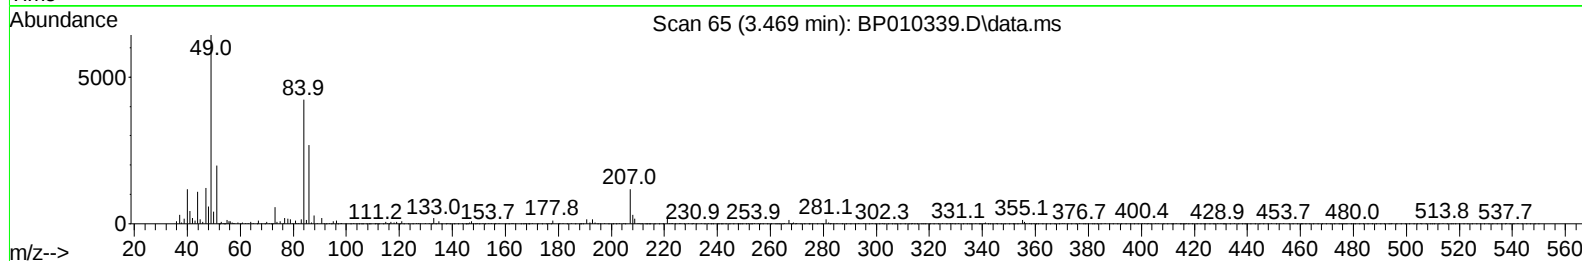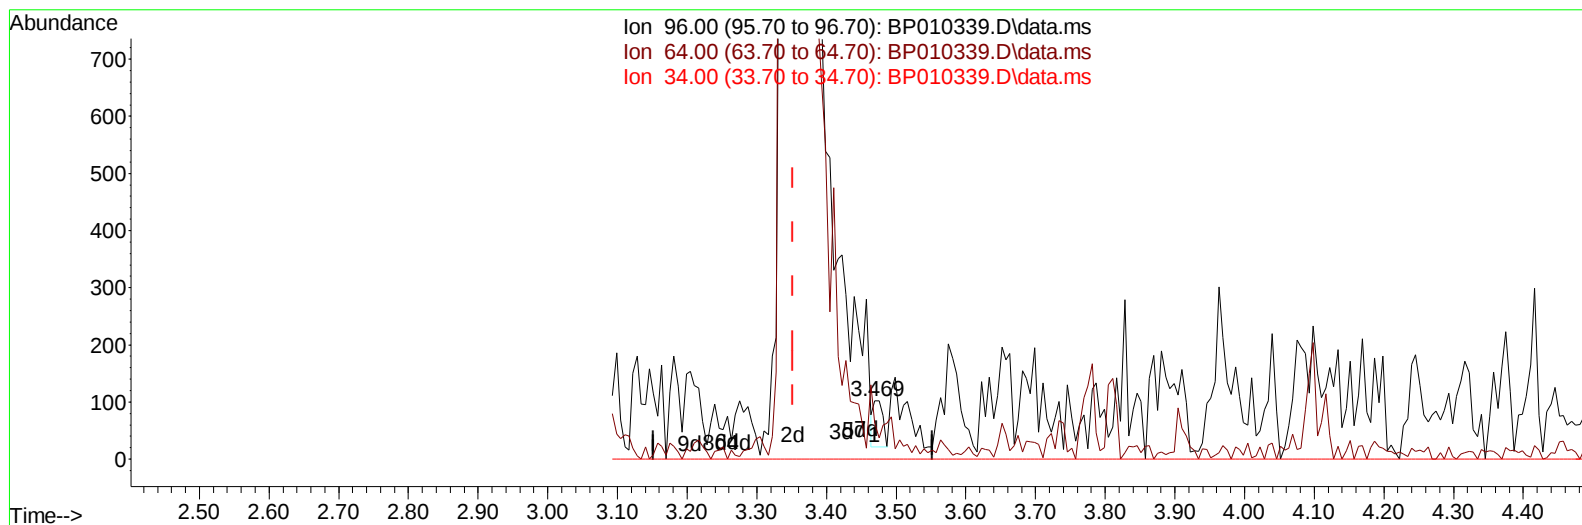

TIC: BP010339.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.469min (+ 0.117) 0.02 ng/uL

response 77

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	61.76
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

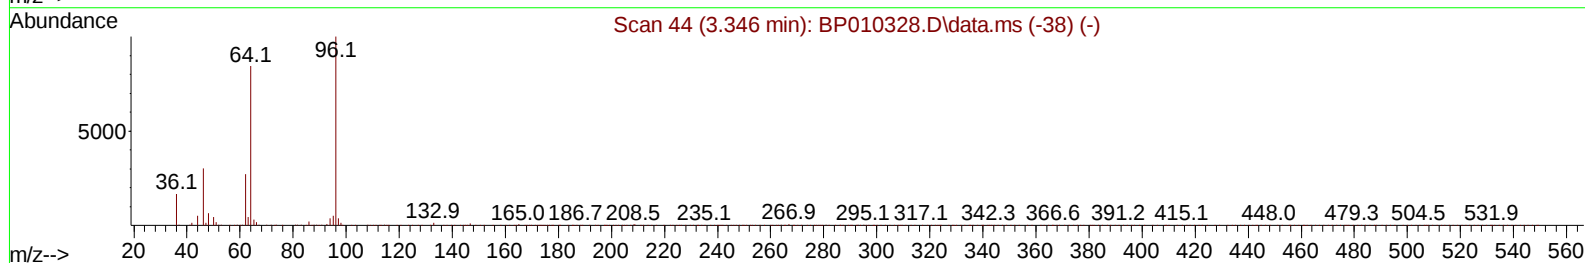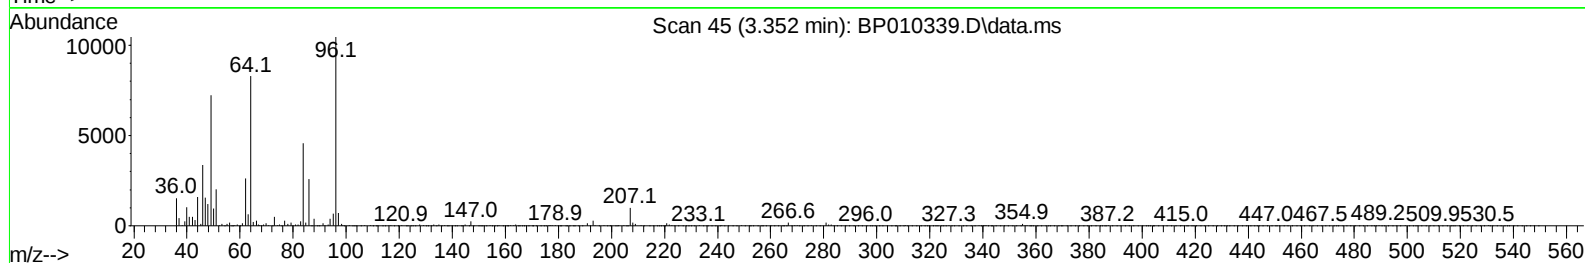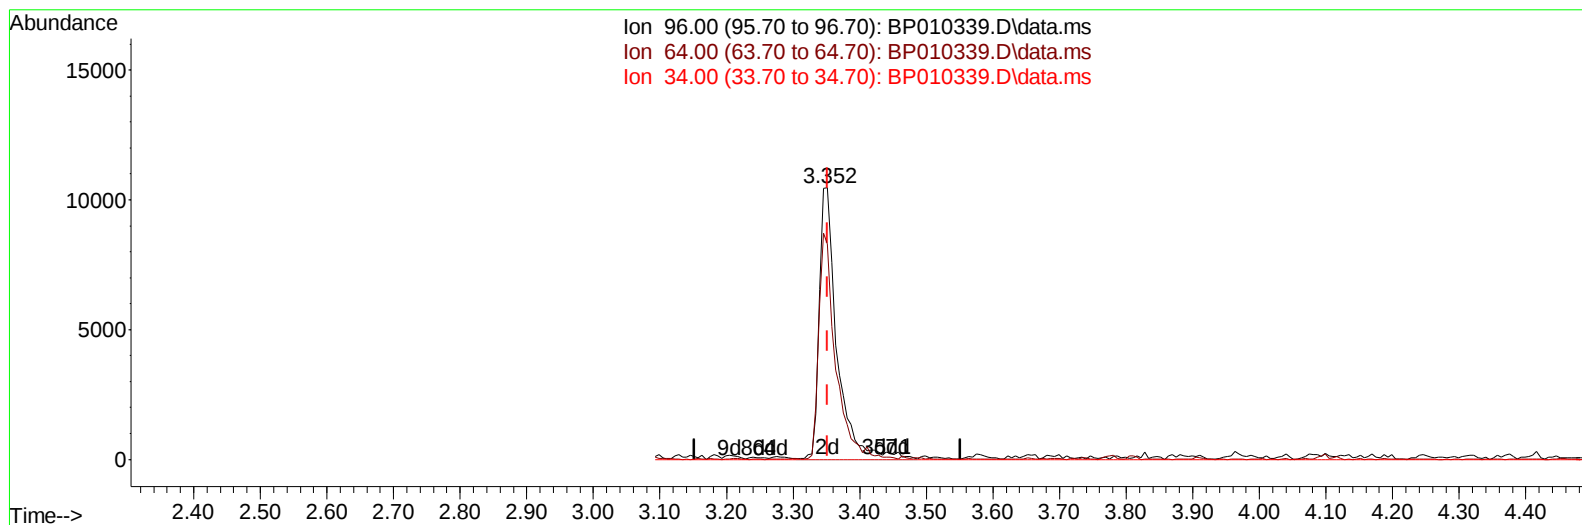

TIC: BP010339.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.352min (-0.000) 5.10 ng/uL m

response 19413

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	55.40	79.28#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

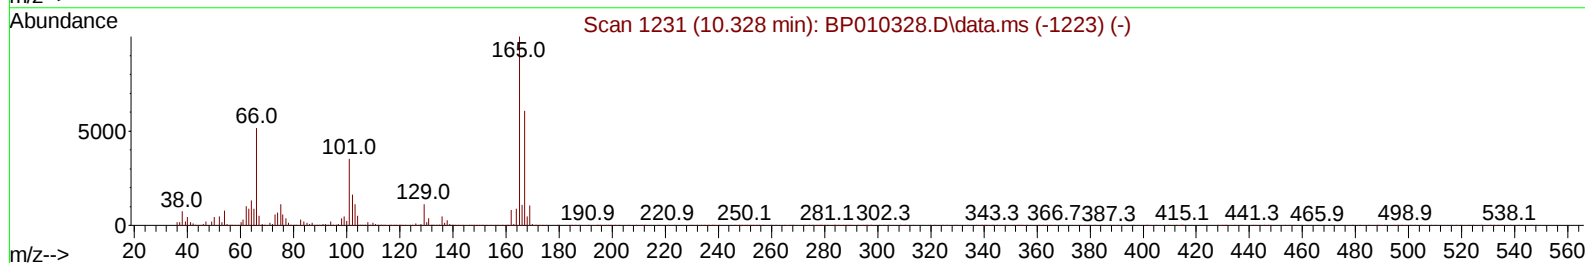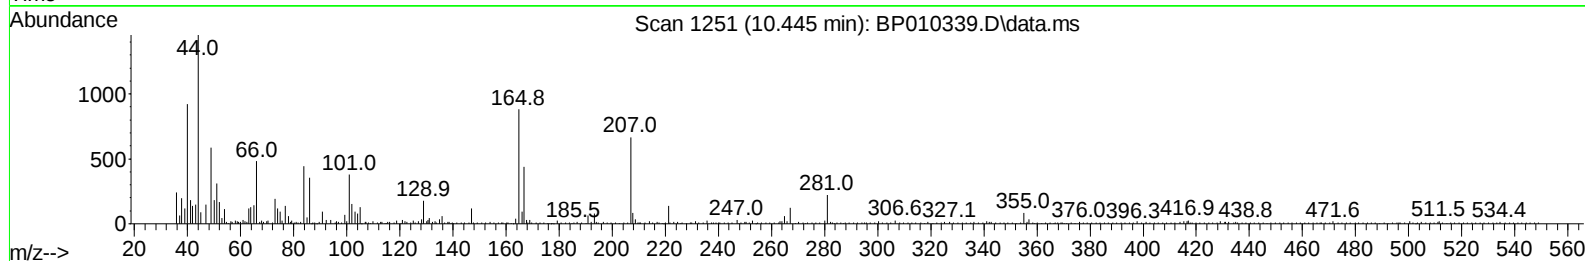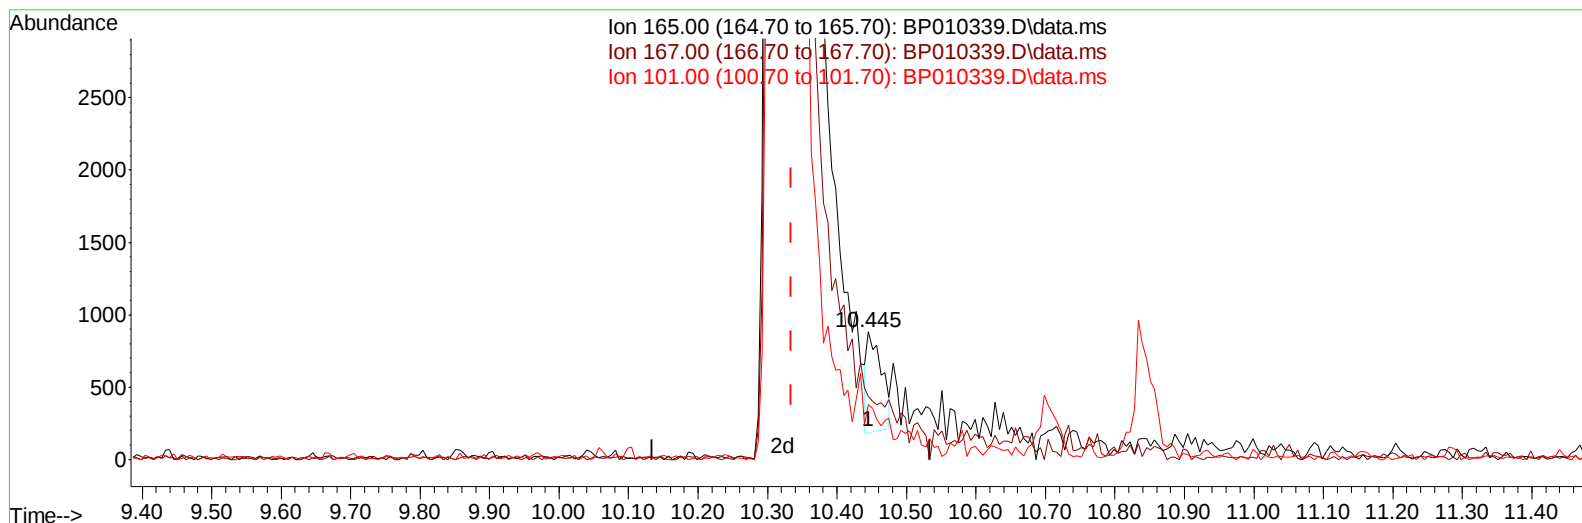

TIC: BP010339.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.445min (+ 0.112) 0.08 ng/u1

response 1009

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	49.72
101.00	49.80	42.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

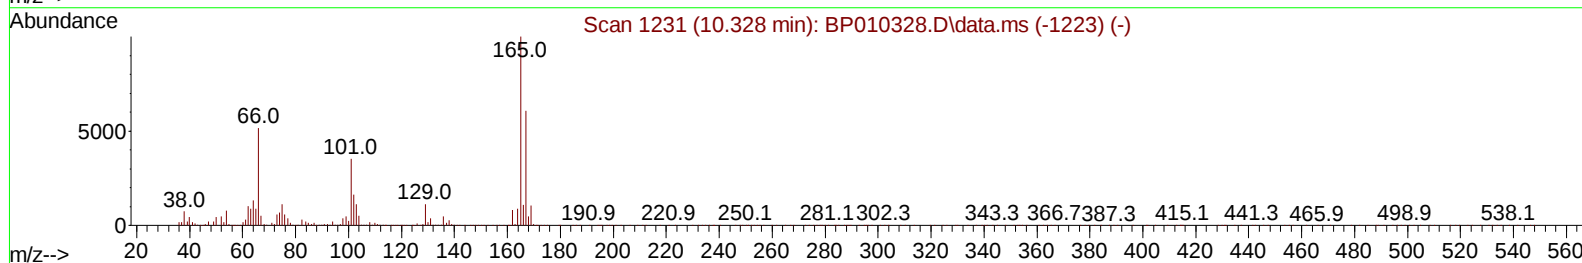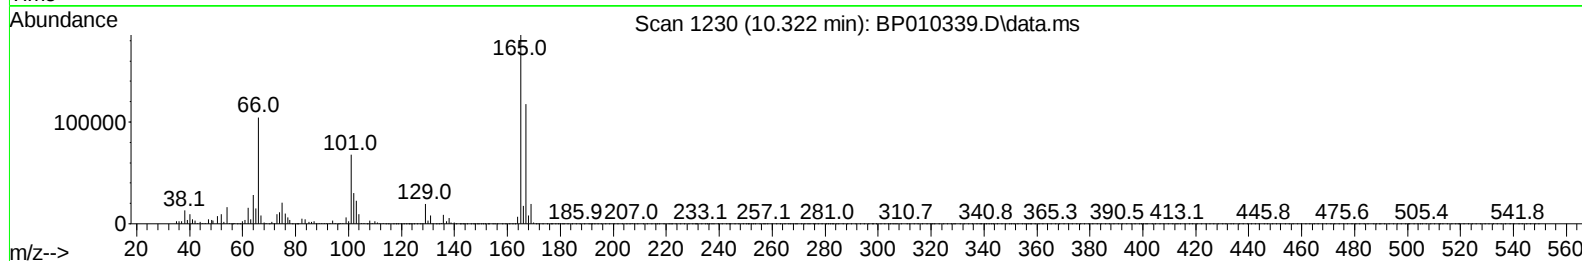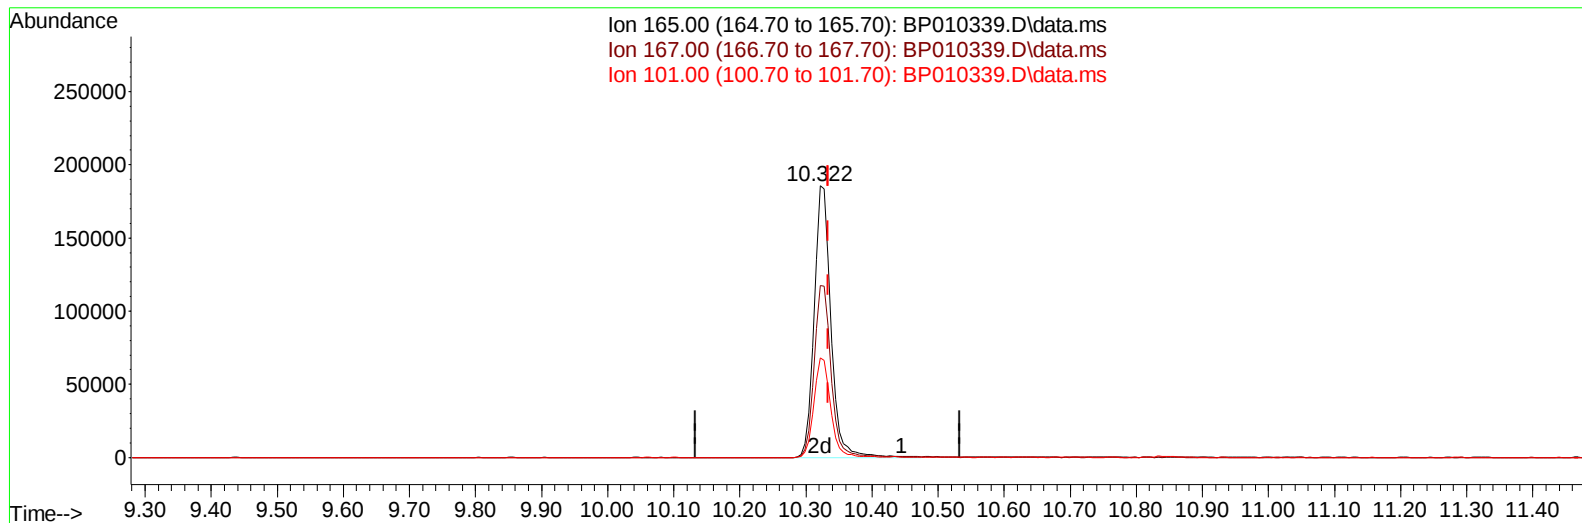

TIC: BP010339.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.322min (-0.012) 27.86 ng/ul m

response 330945

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	57.70	63.44
101.00	49.80	36.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010339.D
 Acq On : 13 May 2022 00:12
 Operator : CG/JU
 Sample : N2801-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

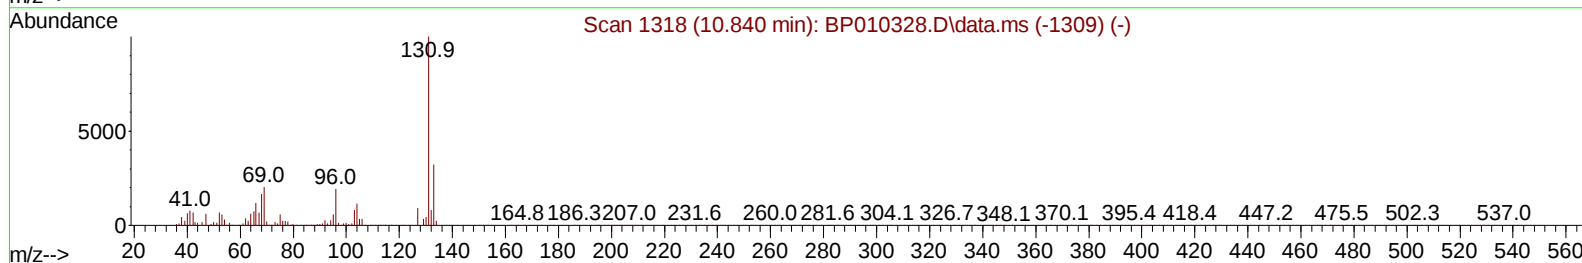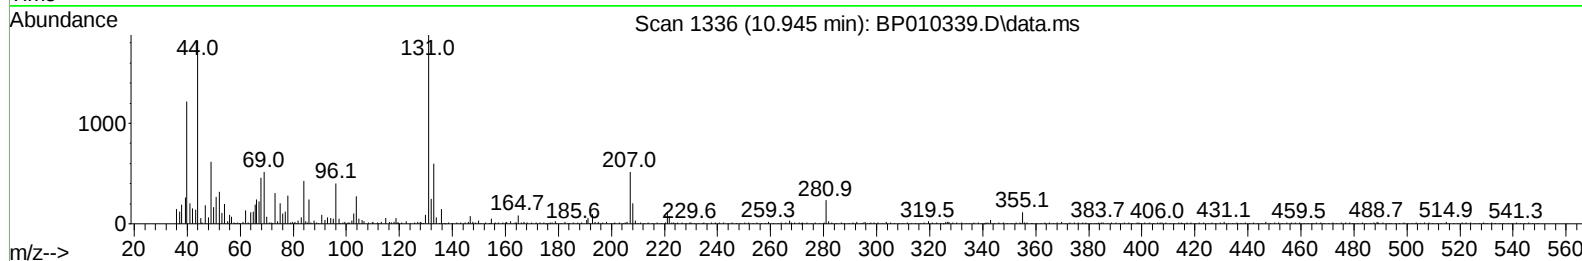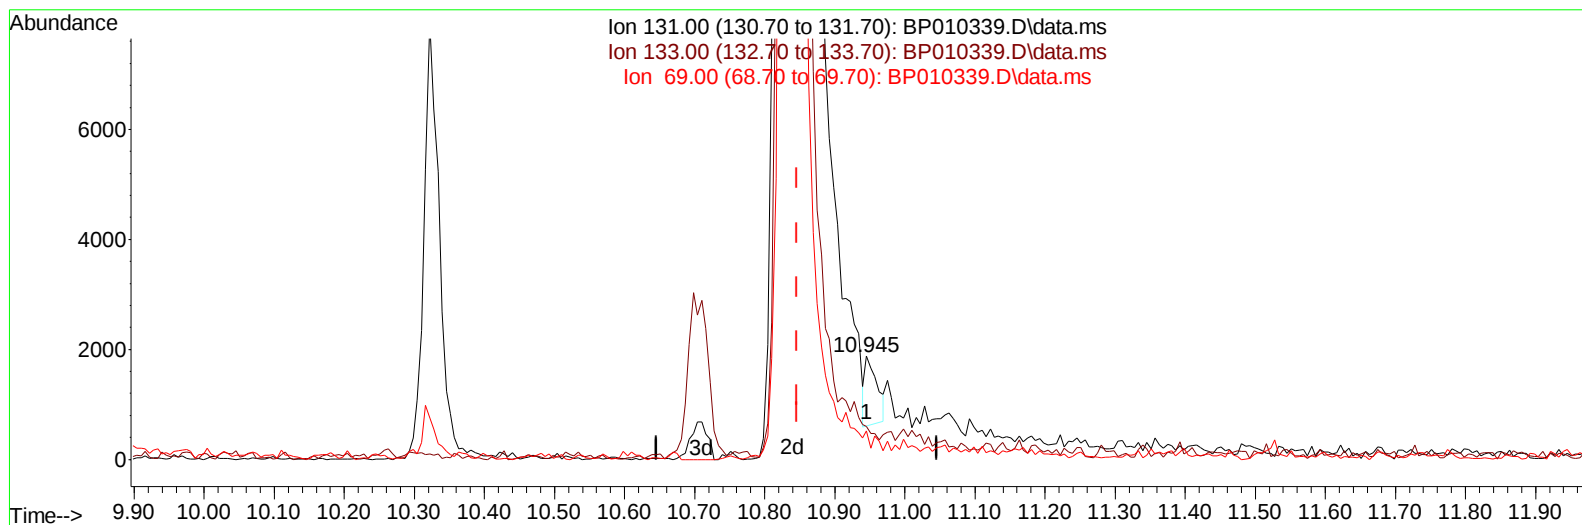

TIC: BP010339.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.945min (+ 0.100) 0.09 ng/ul

response 1509

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	31.83
69.00	26.10	27.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

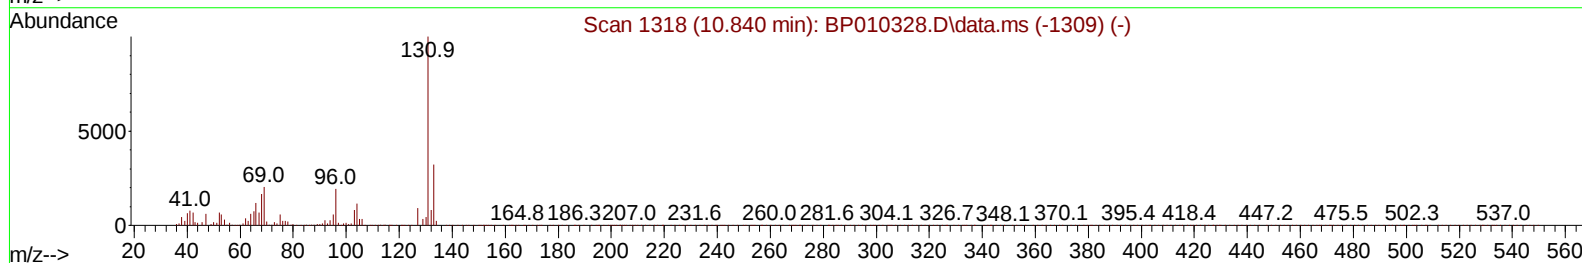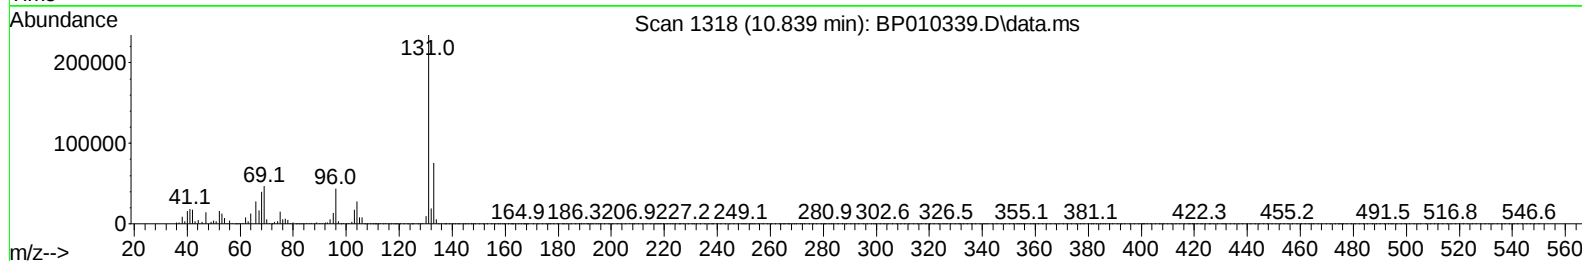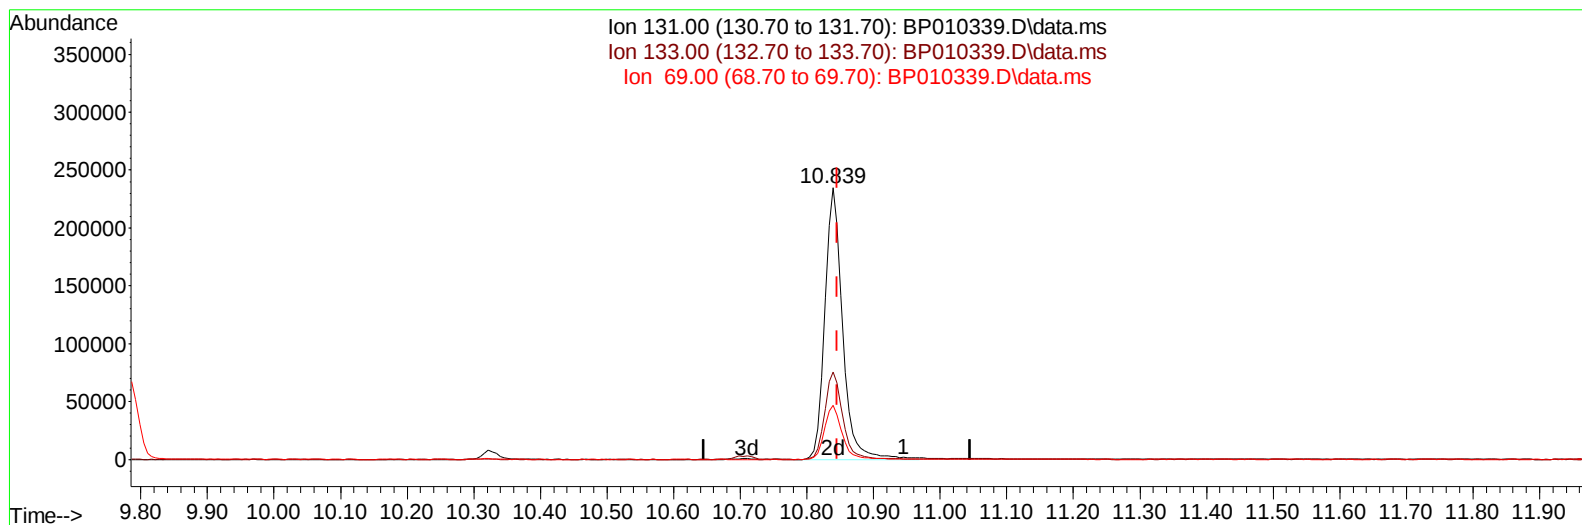

TIC: BP010339.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.839min (-0.006) 24.85 ng/ul m

response 435893

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	29.20	32.17
69.00	26.10	19.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

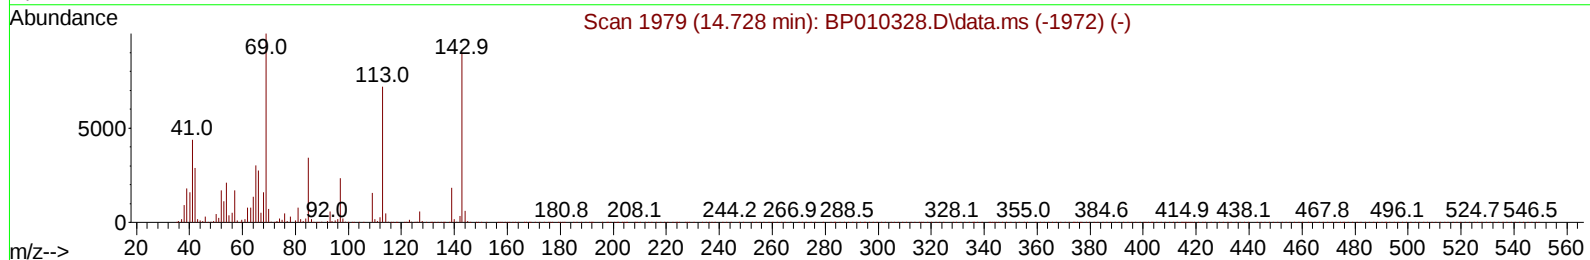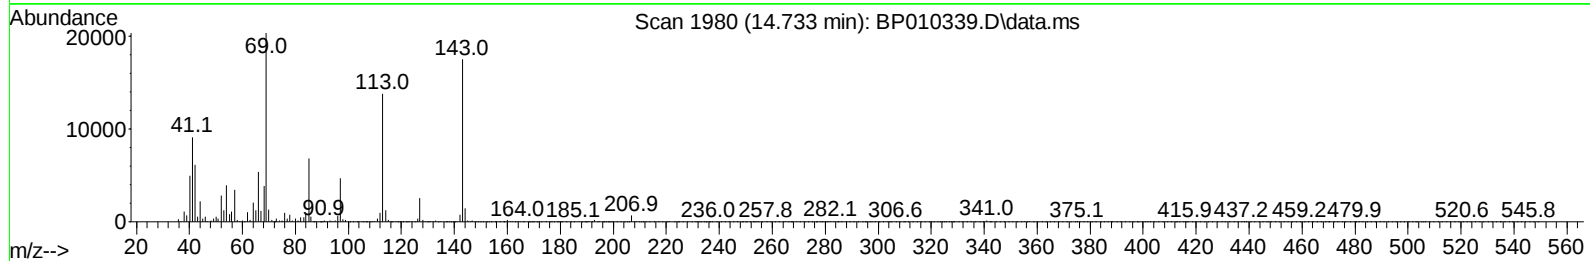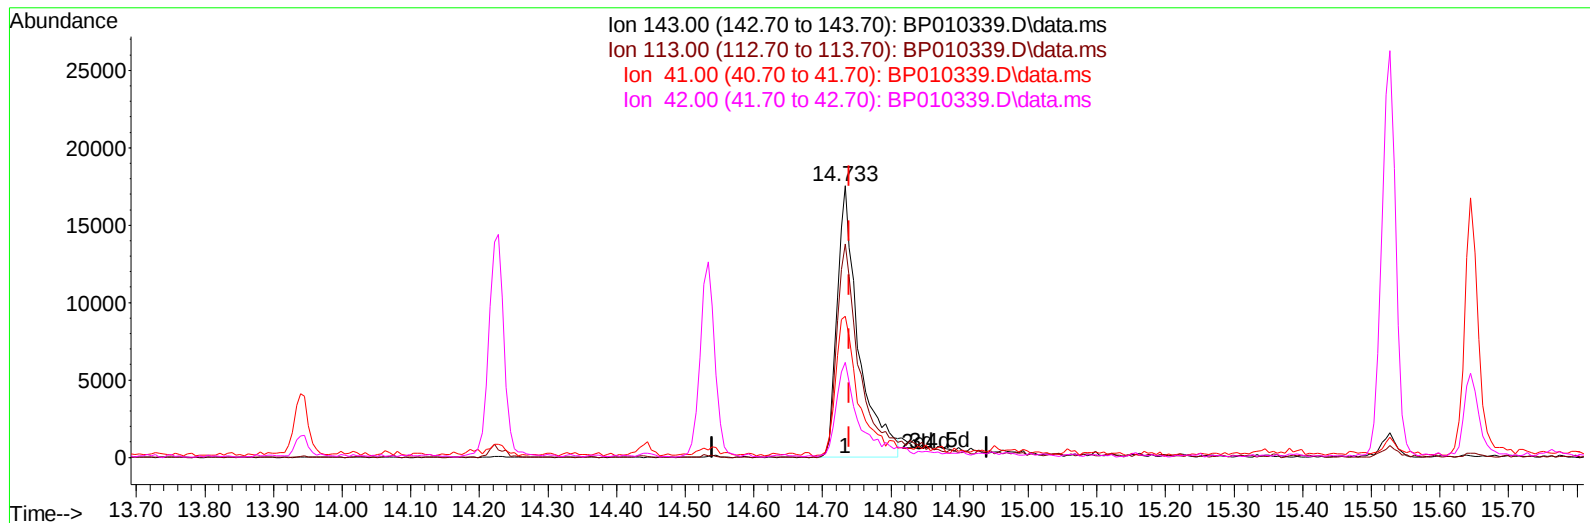

TIC: BP010339.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (-0.006) 4.96 ng/u1

response 38255

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	78.67#
41.00	23.20	52.07#
42.00	18.00	34.92#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010339.D
 Acq On : 13 May 2022 00:12
 Operator : CG/JU
 Sample : N2801-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB6

Manual IntegrationsAPPROVED

Quant Time: May 13 01:56:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

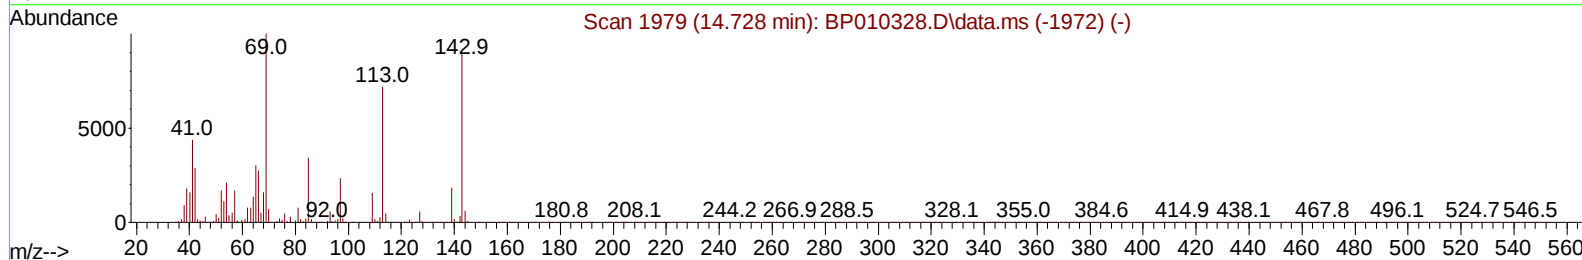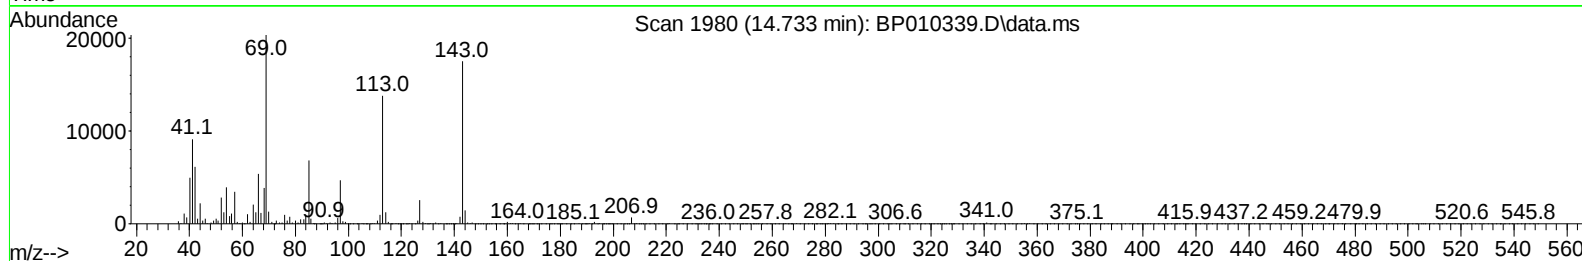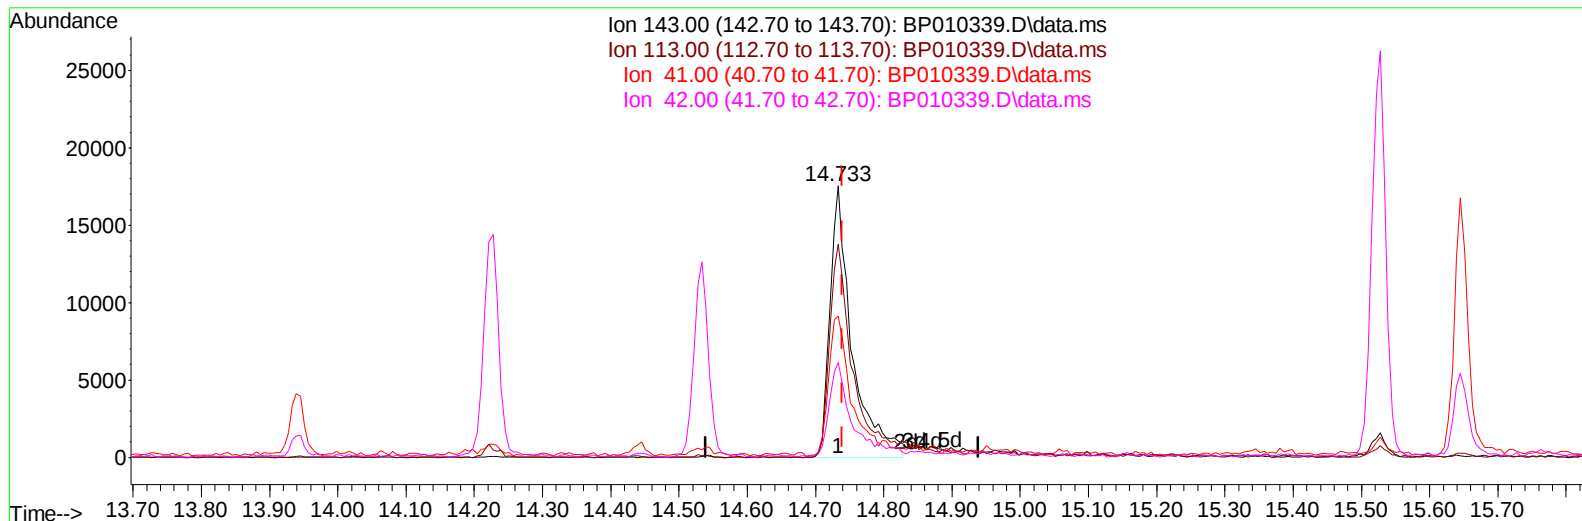

TIC: BP010339.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (-0.006) 5.12 ng/ul m

response 39459

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	132.70	78.67#
41.00	23.20	52.07#
42.00	18.00	34.92#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010339.D
 Acq On : 13 May 2022 00:12
 Operator : CG/JU
 Sample : N2801-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 01:56:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	161597	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	713977	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.533	164	504340	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1090939	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.362	240	1077765	20.000	ng/ul	#-0.01
88) Perylene-d12	23.792	264	988946	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	19413m	5.103	ng/uL	0.00
4) Pyridine-d5	3.769	84	86907	8.210	ng/ul	0.00
7) Phenol-d5	7.069	99	95168	6.341	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	300471	32.361	ng/ul	0.00
11) 2-Chlorophenol-d4	7.434	132	266446	24.105	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	190938	15.474	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	187932	32.828	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.787	143	196563	30.114	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	330945m	27.857	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.839	131	435893m	24.853	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1401861	34.890	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1533385	32.010	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143	39459m	5.120	ng/ul	0.00
60) Fluorene-d10	15.527	176	1229476	36.251	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	227084	30.397	ng/ul	-0.01
73) Anthracene-d10	17.386	188	2099507	39.299	ng/ul	0.00
81) Pyrene-d10	19.615	212	2536635	42.591	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.639	264	2181288	41.359	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010339.D
Acq On : 13 May 2022 00:12
Operator : CG/JU
Sample : N2801-03
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 01:56:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

