

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010285.D
 Acq On : 11 May 2022 12:35
 Operator : CG/JU
 Sample : N2632-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4A4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 12 01:12:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 12 01:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.911	152	78087	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	342538	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	244525	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.287	188	547234	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.375	240	572339	20.000	ng/u1	0.00
88) Perylene-d12	23.804	264	615772	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	7659m	4.167	ng/uL	0.00
4) Pyridine-d5	3.787	84	23221	4.540	ng/u1	0.02
7) Phenol-d5	7.069	99	127589	17.592	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	94145	20.983	ng/u1	0.00
11) 2-Chlorophenol-d4	7.440	132	104872	19.634	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	107817	18.082	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	54740	19.931	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	55821	17.826	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	99115m	17.390	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	137129	16.297	ng/u1	0.00
46) Dimethylphthalate-d6	13.946	166	385616	19.795	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	427288	18.397	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	33693	9.017	ng/u1	0.00
60) Fluorene-d10	15.534	176	340623	20.714	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	34123	9.106	ng/u1	0.00
73) Anthracene-d10	17.387	188	545051	20.339	ng/u1	0.00
81) Pyrene-d10	19.622	212	701414	22.177	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.645	264	705604	21.487	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.734	105	9612	1.031	ng/u1#	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010285.D
Acq On : 11 May 2022 12:35
Operator : CG/JU
Sample : N2632-02
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EW4A4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
Supervised By :Yogesh Patel 05/17/2022


Quant Time: May 12 01:12:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 12 01:10:15 2022
Response via : Initial Calibration

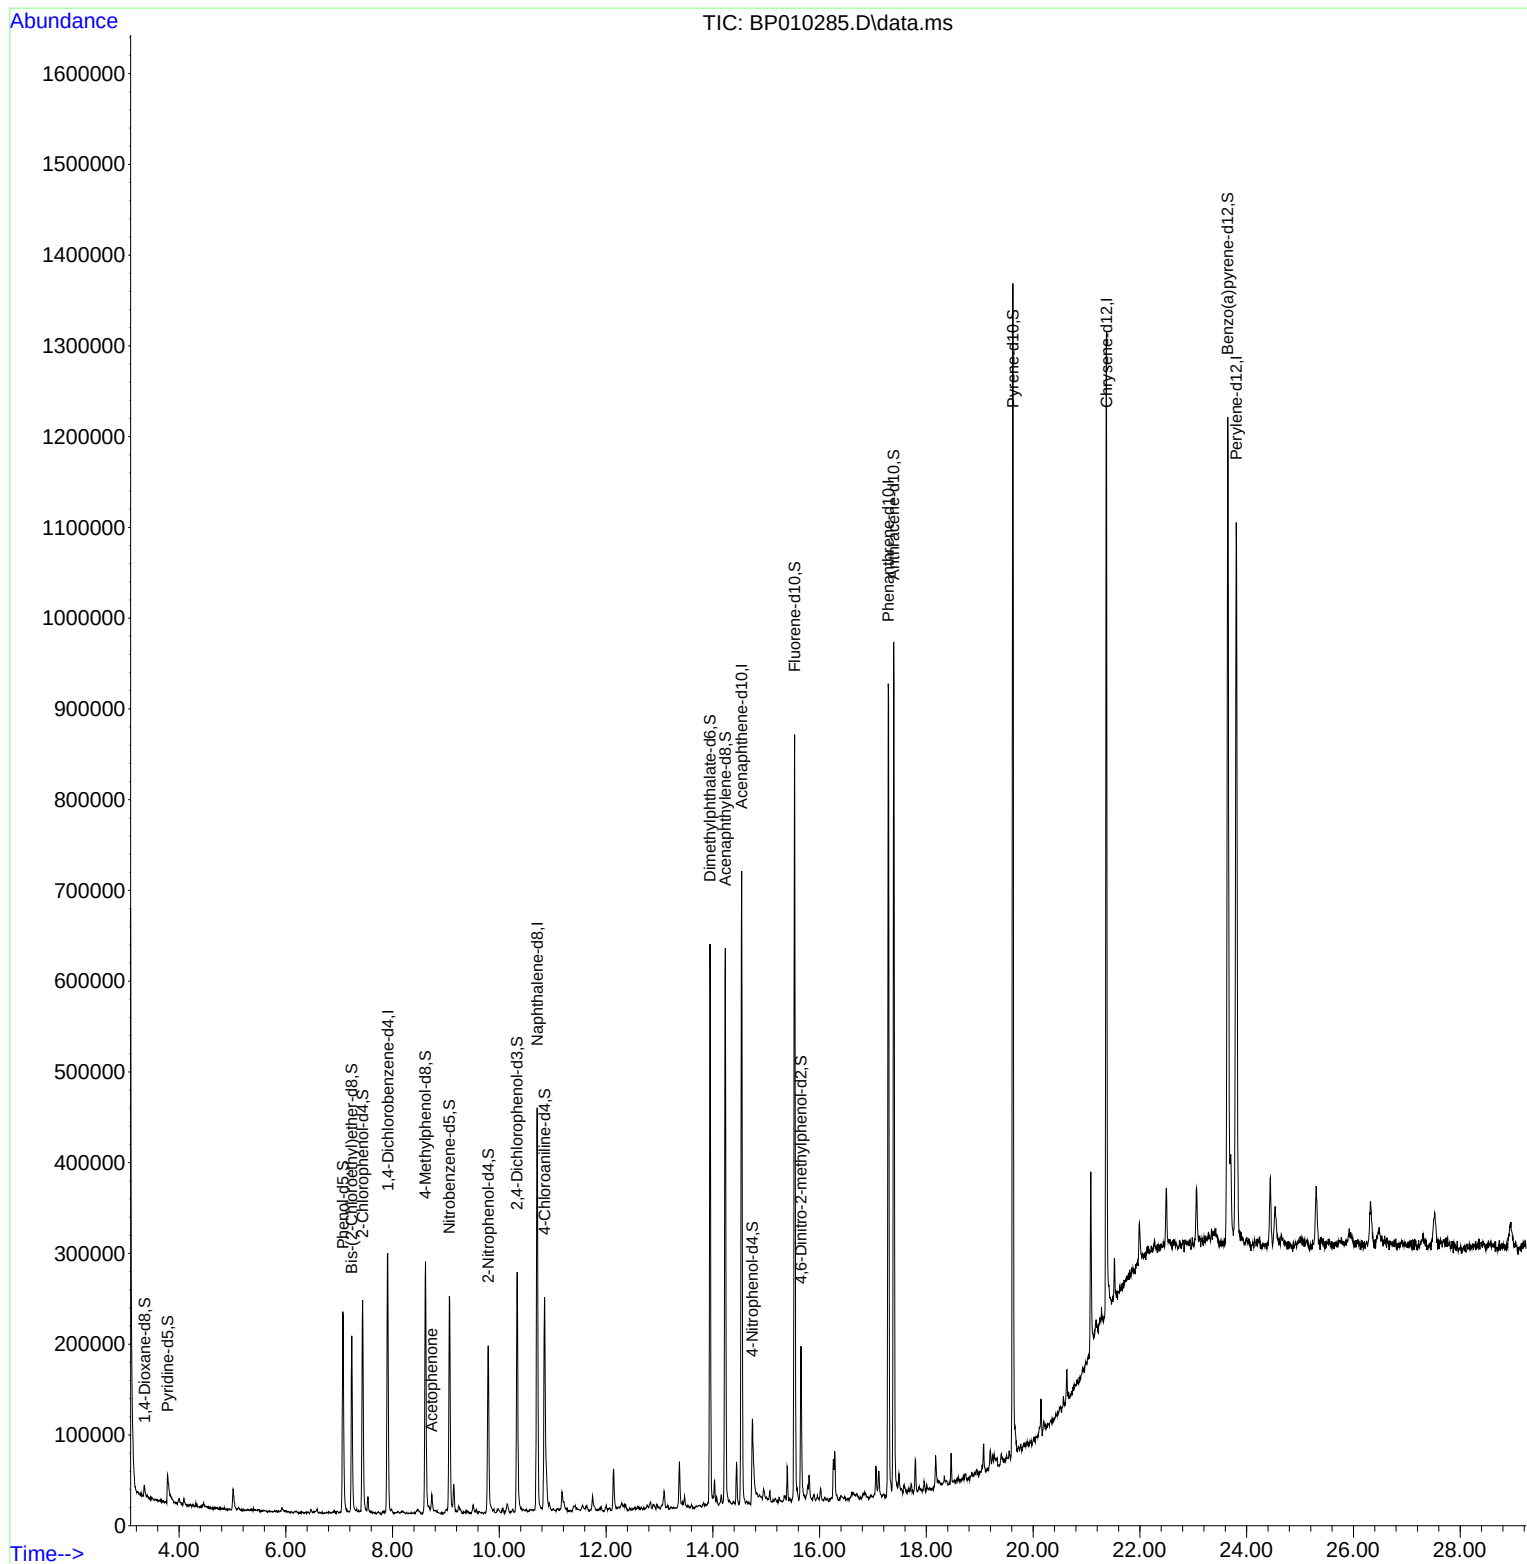

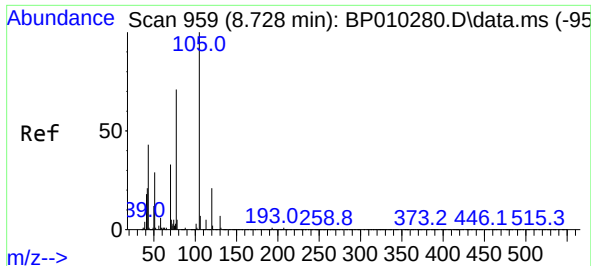

#16
 Acetophenone
 Concen: 1.031 ng/ul
 RT: 8.734 min Scan# 90
 Delta R.T. 0.006 min
 Lab File: BP010285.D
 Acq: 11 May 2022 12:35

Instrument :
 BNA_P
 ClientSampleId :
 EW4A4

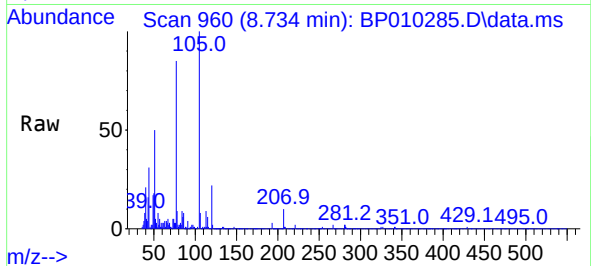

Tgt Ion:105 Resp: 961

Ion	Ratio	Lower	Upper
105	100		
77	85.1	53.4	80.2
51	50.2	13.8	20.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/12/2022
 Supervised By :Yogesh Patel 05/17/2022

