

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010281.D
 Acq On : 11 May 2022 10:21
 Operator : CG/JU
 Sample : PB144607BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK607

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	52	rVB	35623	49921	1.09%	0.111%
2	3.770	112	116	136	rBV	449754	883976	19.38%	1.963%
3	4.093	167	171	176	rBV2	10986	16690	0.37%	0.037%
4	7.069	670	677	693	rBV	611086	1040970	22.82%	2.312%
5	7.234	699	705	717	rBV	524849	851038	18.66%	1.890%
6	7.440	733	740	754	rBV	654612	1074403	23.56%	2.386%
7	7.905	811	819	836	rBV	488199	843741	18.50%	1.874%
8	8.616	931	940	954	rBV	798601	1365832	29.95%	3.034%
9	9.063	1008	1016	1030	rBV	661969	1162814	25.49%	2.583%
10	9.793	1132	1140	1155	rBV	555596	964209	21.14%	2.142%
11	10.328	1223	1231	1247	rBV	734158	1353233	29.67%	3.006%
12	10.710	1288	1296	1308	rBV	768924	1290798	28.30%	2.867%
13	10.846	1311	1319	1343	rBV	761324	1459399	32.00%	3.241%
14	12.304	1563	1567	1578	rBV2	10845	24473	0.54%	0.054%
15	13.522	1767	1774	1779	rBV8	2975	4861	0.11%	0.011%
16	13.951	1839	1847	1859	rBV	1664603	2451459	53.75%	5.445%
17	14.234	1887	1895	1910	rBV	1751827	2611420	57.26%	5.800%
18	14.540	1939	1947	1958	rBV	1247303	1871722	41.04%	4.157%
19	14.734	1973	1980	2009	rBV	622493	1167814	25.60%	2.594%
20	15.534	2108	2116	2129	rBV	2383015	3429080	75.18%	7.616%
21	15.651	2130	2136	2150	rVV	847564	1247557	27.35%	2.771%
22	15.775	2152	2157	2167	rVB	30157	53575	1.17%	0.119%
23	16.316	2245	2249	2254	rVB6	9922	14287	0.31%	0.032%
24	16.975	2357	2361	2367	rVB8	6157	10410	0.23%	0.023%
25	17.075	2373	2378	2383	rBV7	5032	9307	0.20%	0.021%
26	17.292	2408	2415	2425	rBV	1641073	2319243	50.85%	5.151%
27	17.392	2425	2432	2447	rVB	2613344	3818085	83.71%	8.480%
28	18.192	2563	2568	2571	rBV7	4763	9090	0.20%	0.020%
29	19.204	2735	2740	2744	rBV2	37204	51136	1.12%	0.114%
30	19.269	2747	2751	2756	rBV	31372	43031	0.94%	0.096%
31	19.622	2805	2811	2825	rBV	3393019	4560961	100.00%	10.130%
32	21.374	3104	3109	3123	rBV	1851889	2548329	55.87%	5.660%
33	23.657	3489	3497	3504	rBV2	1939794	4083401	89.53%	9.069%
34	23.810	3516	3523	3536	rVB	1125631	2338633	51.28%	5.194%

Sum of corrected areas: 45024898


Instrument :
BNA_P
ClientSampleId :
SBLK607

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010281.D
Acq On : 11 May 2022 10:21
Operator : CG/JU
Sample : PB144607BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK607

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

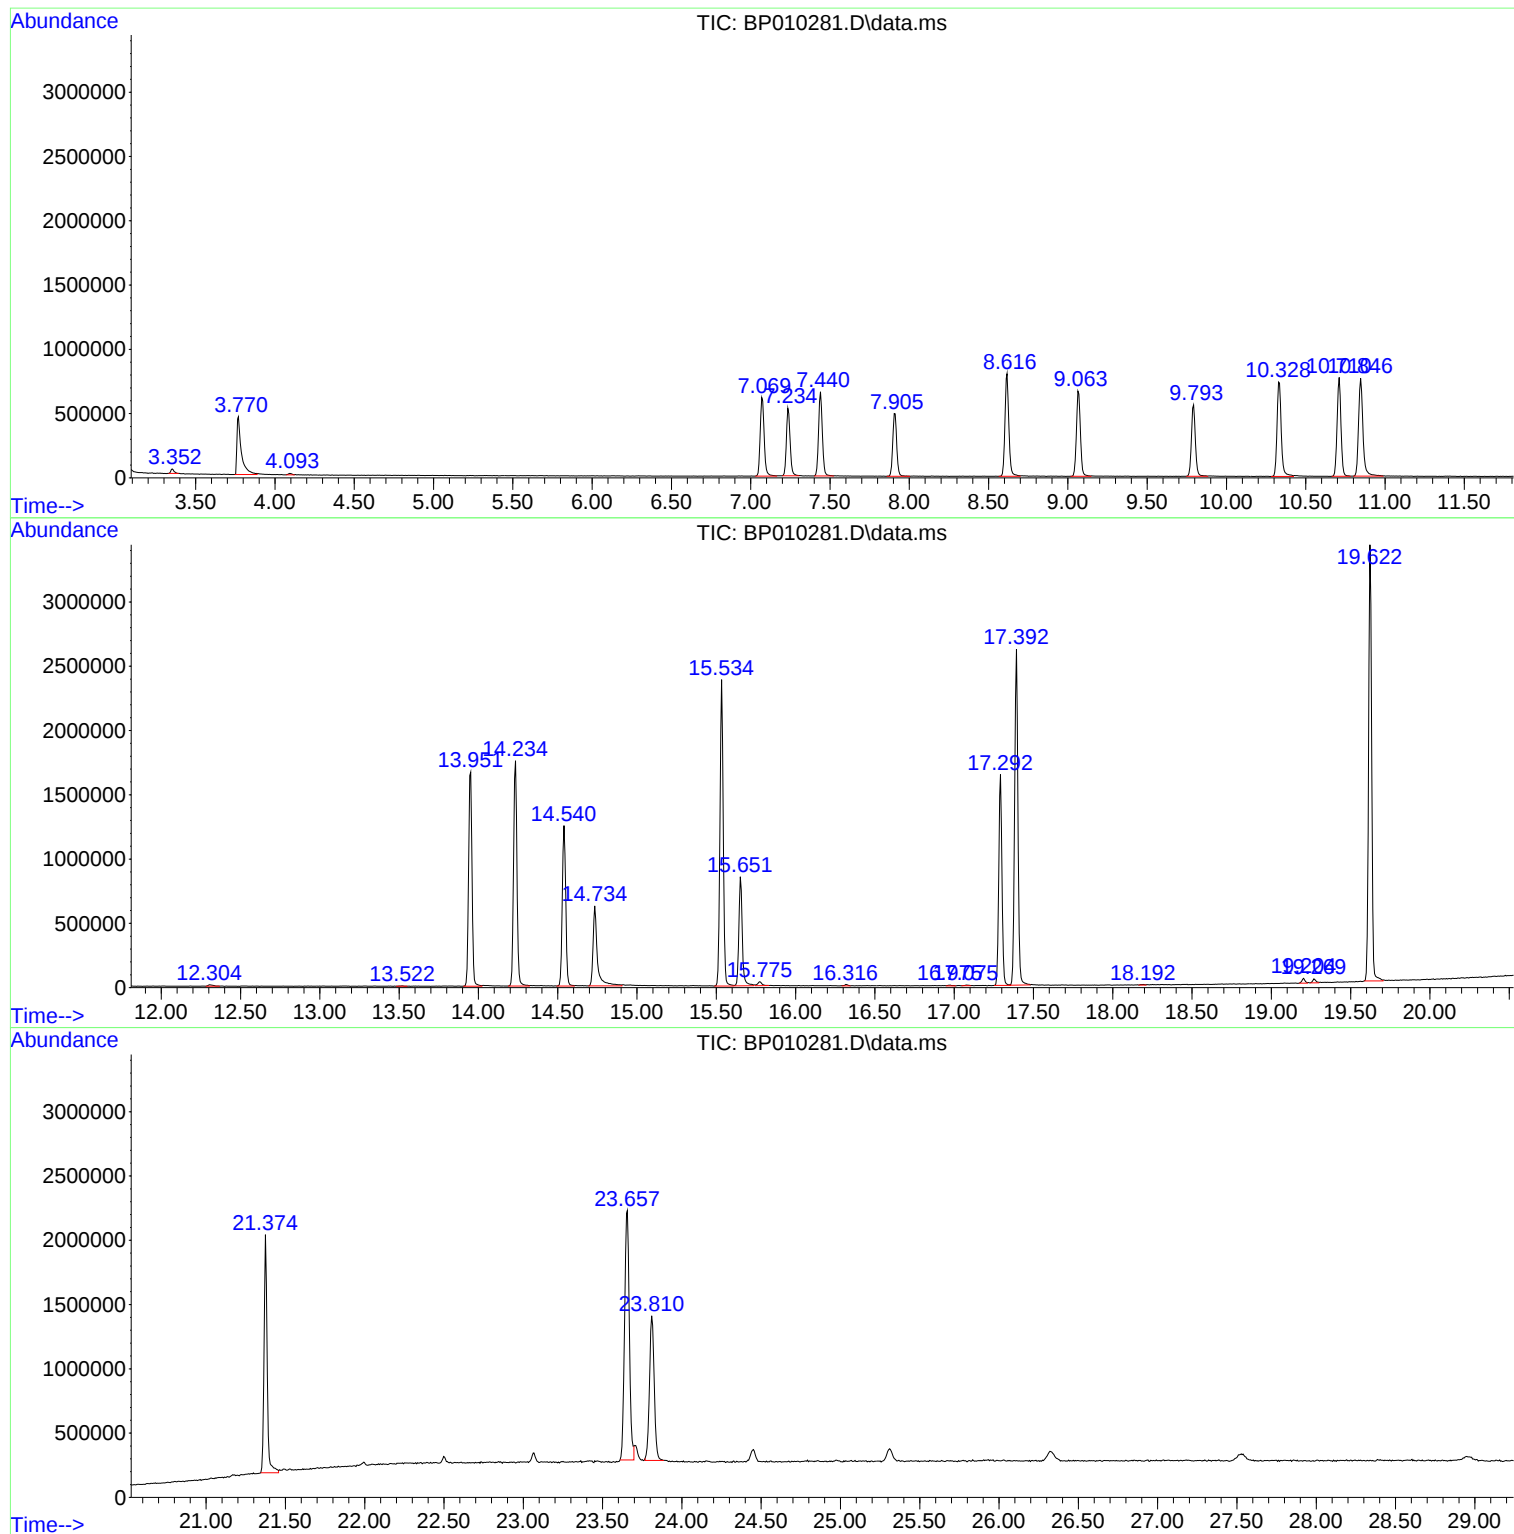

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010281.D
Acq On : 11 May 2022 10:21
Operator : CG/JU
Sample : PB144607BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK607

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010281.D
Acq On : 11 May 2022 10:21
Operator : CG/JU
Sample : PB144607BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK607

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc