

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010284.D
 Acq On : 11 May 2022 12:02
 Operator : CG/JU
 Sample : N2632-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	51	rBV	14259	21596	0.85%	0.078%
2	3.787	115	119	132	rBV2	32839	78525	3.08%	0.284%
3	3.999	151	155	156	rBV3	6813	6808	0.27%	0.025%
4	4.093	167	171	177	rVB4	8902	12765	0.50%	0.046%
5	4.452	228	232	240	rVB4	3743	9817	0.39%	0.036%
6	5.016	322	328	336	rBV2	20836	44006	1.73%	0.159%
7	5.111	340	344	349	rBV8	3715	7795	0.31%	0.028%
8	5.928	479	483	485	rBV5	4792	5709	0.22%	0.021%
9	6.181	521	526	530	rBV7	2486	4997	0.20%	0.018%
10	6.475	571	576	579	rBV5	3901	5312	0.21%	0.019%
11	6.581	587	594	598	rVB6	5611	11131	0.44%	0.040%
12	7.069	670	677	692	rBV	229883	429219	16.84%	1.554%
13	7.234	699	705	719	rBV	209071	343868	13.49%	1.245%
14	7.440	732	740	752	rBV	247656	424625	16.66%	1.537%
15	7.540	753	757	766	rVB4	14645	26538	1.04%	0.096%
16	7.910	812	820	830	rBV	451776	775312	30.42%	2.807%
17	8.469	911	915	920	rVB7	3797	6564	0.26%	0.024%
18	8.616	929	940	948	rBV	302387	524447	20.58%	1.898%
19	8.734	955	960	967	rVB2	19205	33526	1.32%	0.121%
20	9.063	1010	1016	1026	rVV	253337	459465	18.03%	1.663%
21	9.146	1026	1030	1035	rVB	22386	33496	1.31%	0.121%
22	9.240	1041	1046	1057	rVB	7451	19295	0.76%	0.070%
23	9.510	1087	1092	1097	rBV8	5900	11212	0.44%	0.041%
24	9.563	1097	1101	1106	rVB7	3559	6509	0.26%	0.024%
25	9.793	1132	1140	1153	rBV	206123	373561	14.66%	1.352%
26	9.981	1166	1172	1175	rBV6	4804	9445	0.37%	0.034%
27	10.063	1183	1186	1191	rVB5	4535	7292	0.29%	0.026%
28	10.146	1196	1200	1207	rVB9	7801	15106	0.59%	0.055%
29	10.251	1211	1218	1222	rBV10	2848	6131	0.24%	0.022%
30	10.334	1224	1232	1244	rBV	285862	531033	20.83%	1.922%
31	10.710	1287	1296	1307	rBV	689469	1230343	48.27%	4.454%
32	10.846	1312	1319	1332	rBV	271930	556939	21.85%	2.016%
33	11.181	1370	1376	1380	rBV3	16086	33955	1.33%	0.123%
34	11.428	1415	1418	1421	rVV5	3709	4974	0.20%	0.018%
35	11.493	1425	1429	1432	rVB5	3137	4202	0.16%	0.015%
36	11.557	1436	1440	1447	rVV9	4610	9219	0.36%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010284.D
 Acq On : 11 May 2022 12:02
 Operator : CG/JU
 Sample : N2632-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	11.640	1451	1454	1459	rVB6	5796	10028	0.39%	0.036%
38	11.751	1468	1473	1481	rBV3	14847	32060	1.26%	0.116%
39	11.904	1495	1499	1503	rVB7	4687	7508	0.29%	0.027%
40	12.004	1508	1516	1520	rBV7	5910	14629	0.57%	0.053%

41	12.140	1534	1539	1546	rBV	47689	77817	3.05%	0.282%
42	12.298	1560	1566	1570	rBV5	6613	15582	0.61%	0.056%
43	12.357	1574	1576	1582	rVB5	5973	8949	0.35%	0.032%
44	12.451	1589	1592	1598	rVB8	3604	5678	0.22%	0.021%
45	12.769	1641	1646	1649	rBV7	5670	9096	0.36%	0.033%

46	12.828	1651	1656	1661	rVB8	6137	11565	0.45%	0.042%
47	12.887	1662	1666	1668	rBV5	3158	5511	0.22%	0.020%
48	12.945	1674	1676	1681	rBV6	4113	5686	0.22%	0.021%
49	13.034	1689	1691	1694	rBV4	4431	5874	0.23%	0.021%
50	13.087	1694	1700	1706	rVV4	22558	41814	1.64%	0.151%

51	13.151	1708	1711	1717	rVB7	4945	7806	0.31%	0.028%
52	13.375	1742	1749	1755	rBV	55322	92506	3.63%	0.335%
53	13.469	1762	1765	1769	rVB3	7815	9016	0.35%	0.033%
54	13.604	1784	1788	1792	rVB7	4233	5677	0.22%	0.021%
55	13.816	1820	1824	1827	rBV6	5562	8819	0.35%	0.032%

56	13.945	1840	1846	1854	rVV	688696	991059	38.88%	3.588%
57	14.028	1857	1860	1865	rVV2	30962	46054	1.81%	0.167%
58	14.075	1865	1868	1872	rVB6	11160	14898	0.58%	0.054%
59	14.163	1878	1883	1887	rBV6	6325	8427	0.33%	0.031%
60	14.234	1887	1895	1905	rBV	674009	1056810	41.46%	3.826%

61	14.445	1926	1931	1937	rVB	61846	83526	3.28%	0.302%
62	14.539	1940	1947	1956	rBV	1162461	1719340	67.46%	6.224%
63	14.739	1975	1981	1994	rBV	134275	314187	12.33%	1.137%
64	14.957	2013	2018	2023	rBV9	12052	23093	0.91%	0.084%
65	15.069	2034	2037	2044	rVB6	13608	21528	0.84%	0.078%

66	15.245	2064	2067	2071	rBV4	4669	6143	0.24%	0.022%
67	15.351	2079	2085	2088	rBV8	8173	15411	0.60%	0.056%
68	15.398	2088	2093	2097	rVV	45933	56867	2.23%	0.206%
69	15.534	2109	2116	2130	rVV	1003868	1463716	57.43%	5.298%
70	15.651	2130	2136	2149	rVV	216847	348866	13.69%	1.263%

71	15.804	2152	2162	2172	rVB4	37331	98901	3.88%	0.358%
72	15.898	2172	2178	2181	rBV8	8678	15623	0.61%	0.057%
73	15.963	2185	2189	2192	rVV5	7693	13006	0.51%	0.047%
74	16.022	2196	2199	2205	rVB6	13655	20207	0.79%	0.073%
75	16.257	2235	2239	2241	rBV	58721	73866	2.90%	0.267%

76	16.286	2241	2244	2248	rVB2	62663	86110	3.38%	0.312%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010284.D
 Acq On : 11 May 2022 12:02
 Operator : CG/JU
 Sample : N2632-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

77	16.404	2261	2264	2266	rBV3	4690	6228	0.24%	0.023%
78	16.610	2293	2299	2301	rBV7	9313	18514	0.73%	0.067%
79	16.898	2346	2348	2352	rVB5	3793	4202	0.16%	0.015%
80	17.057	2370	2375	2380	rBV	43265	65550	2.57%	0.237%
81	17.110	2380	2384	2391	rVB2	36280	55341	2.17%	0.200%
82	17.292	2408	2415	2424	rBV	1439322	2130541	83.59%	7.712%
83	17.386	2425	2431	2440	rBV2	1119669	1658458	65.07%	6.003%
84	17.486	2445	2448	2453	rVB7	16985	26223	1.03%	0.095%
85	17.716	2485	2487	2493	rVB6	8591	12509	0.49%	0.045%
86	17.792	2496	2500	2506	rVV	45247	59703	2.34%	0.216%
87	18.010	2533	2537	2542	rBV6	8778	15569	0.61%	0.056%
88	18.175	2561	2565	2572	rBV3	60896	92191	3.62%	0.334%
89	18.463	2610	2614	2618	rBV	44140	52986	2.08%	0.192%
90	19.075	2715	2718	2726	rVB	44468	51767	2.03%	0.187%
91	19.204	2736	2740	2743	rVB4	17029	21680	0.85%	0.078%
92	19.410	2771	2775	2779	rBV7	17118	29395	1.15%	0.106%
93	19.622	2805	2811	2826	rBV	1702226	2331087	91.46%	8.438%
94	20.151	2898	2901	2906	rVB	39997	48244	1.89%	0.175%
95	20.516	2960	2963	2967	rVB	34687	42944	1.68%	0.155%
96	20.633	2980	2983	2989	rVB	41911	53199	2.09%	0.193%
97	21.080	3055	3059	3069	rBV	514832	754245	29.59%	2.730%
98	21.374	3104	3109	3120	rBV	1771538	2405925	94.39%	8.709%
99	23.651	3489	3496	3502	rBV2	1096910	2201773	86.38%	7.970%
100	23.810	3516	3523	3535	rVB2	1237721	2548846	100.00%	9.227%


Sum of corrected areas: 27625116

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010284.D
Acq On : 11 May 2022 12:02
Operator : CG/JU
Sample : N2632-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

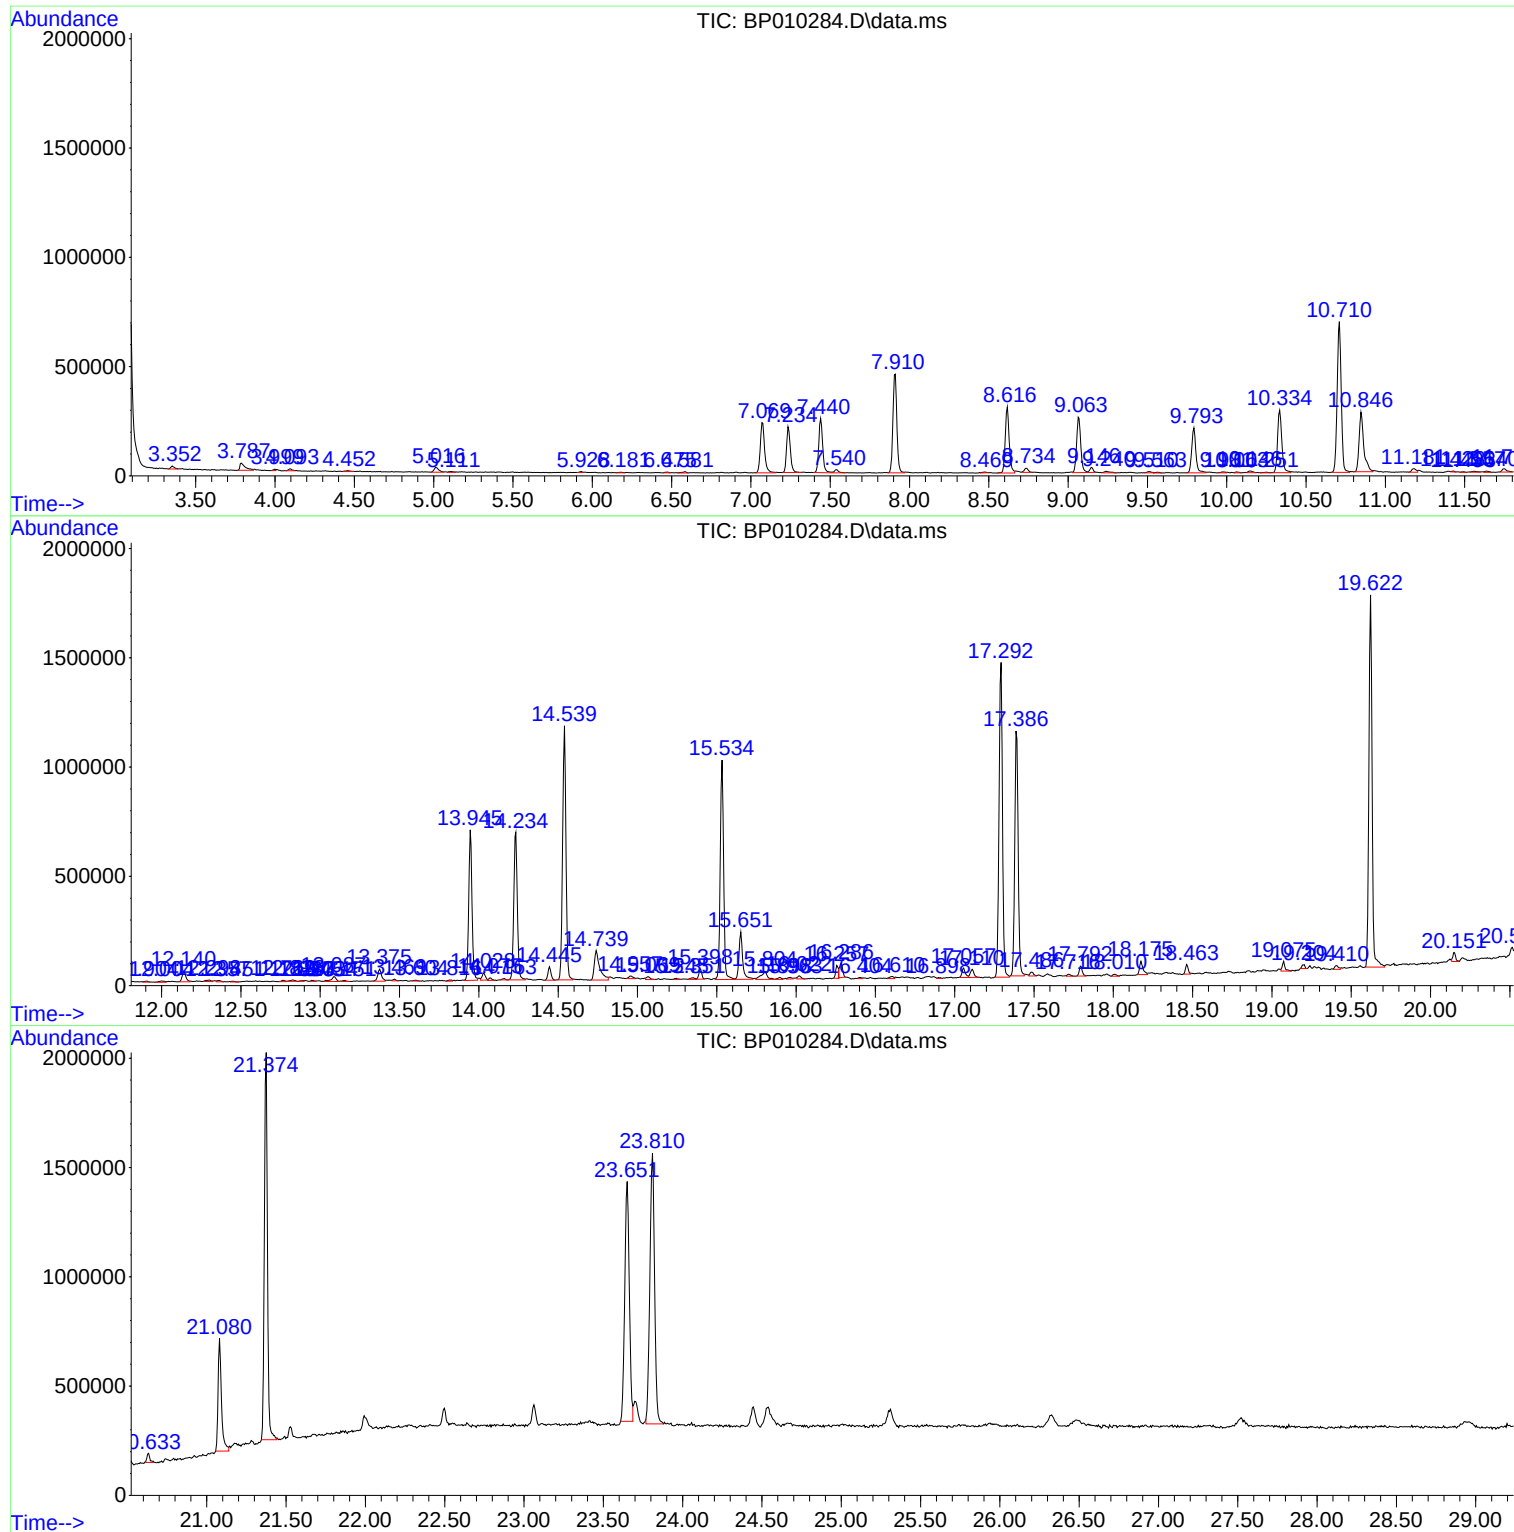

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010284.D
Acq On : 11 May 2022 12:02
Operator : CG/JU
Sample : N2632-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.080	6.27 ng/ul	754245	Chrysene-d12	21.374

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Docosene			308	C22H44	001599-67-3	99
2	2- Chloropropionic acid, octadec...			360	C21H41ClO2	088104-31-8	95
3	Heptafluorobutyric acid, pentade...			424	C19H31F7O2	959261-23-5	94
4	Heptadecyl trifluoroacetate			352	C19H35F3O2	1010351-87-0	94
5	Pentafluoropropionic acid, octad...			416	C21H37F5O2	959261-25-7	91

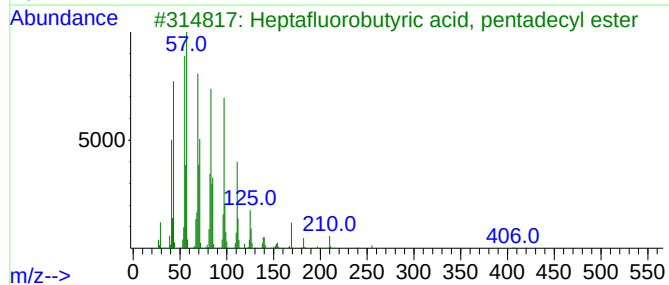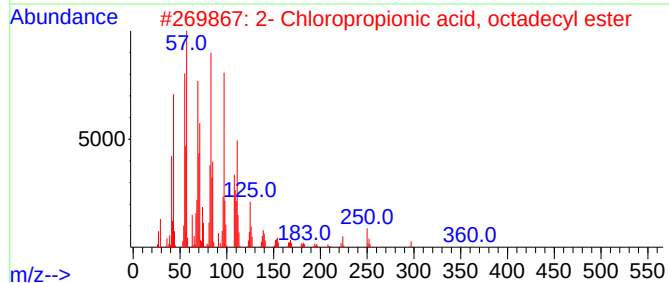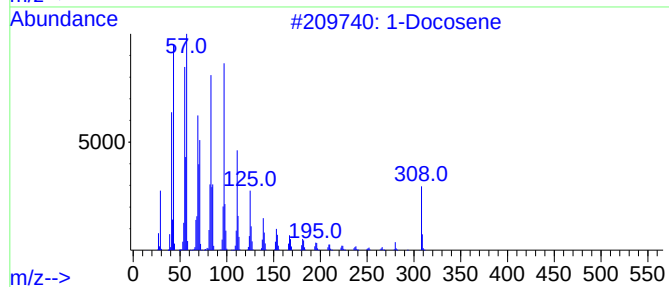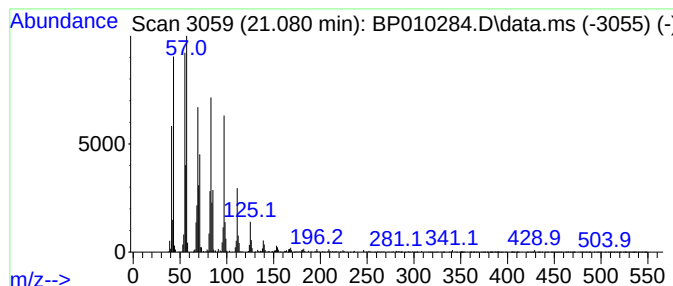

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010284.D
Acq On : 11 May 2022 12:02
Operator : CG/JU
Sample : N2632-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.080	6.3	ng/u1	754245	5	21.374	2405930	20.0